

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070822\
 Data File : PD070761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 13:00
 Operator : AR\AJ
 Sample : N3214-07
 Misc : PEST LOD 2.5PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 13:19:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 15:26:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	4.124	42422217	508.9E6	17.377	19.677
28)	SA Decachlor...	8.268	9.315	47294247	168.1E6	19.074	20.434

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070822\
Data File : PD070761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 13:00
Operator : AR\AJ
Sample : N3214-07
Misc : PEST LOD 2.5PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 13:19:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 15:26:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

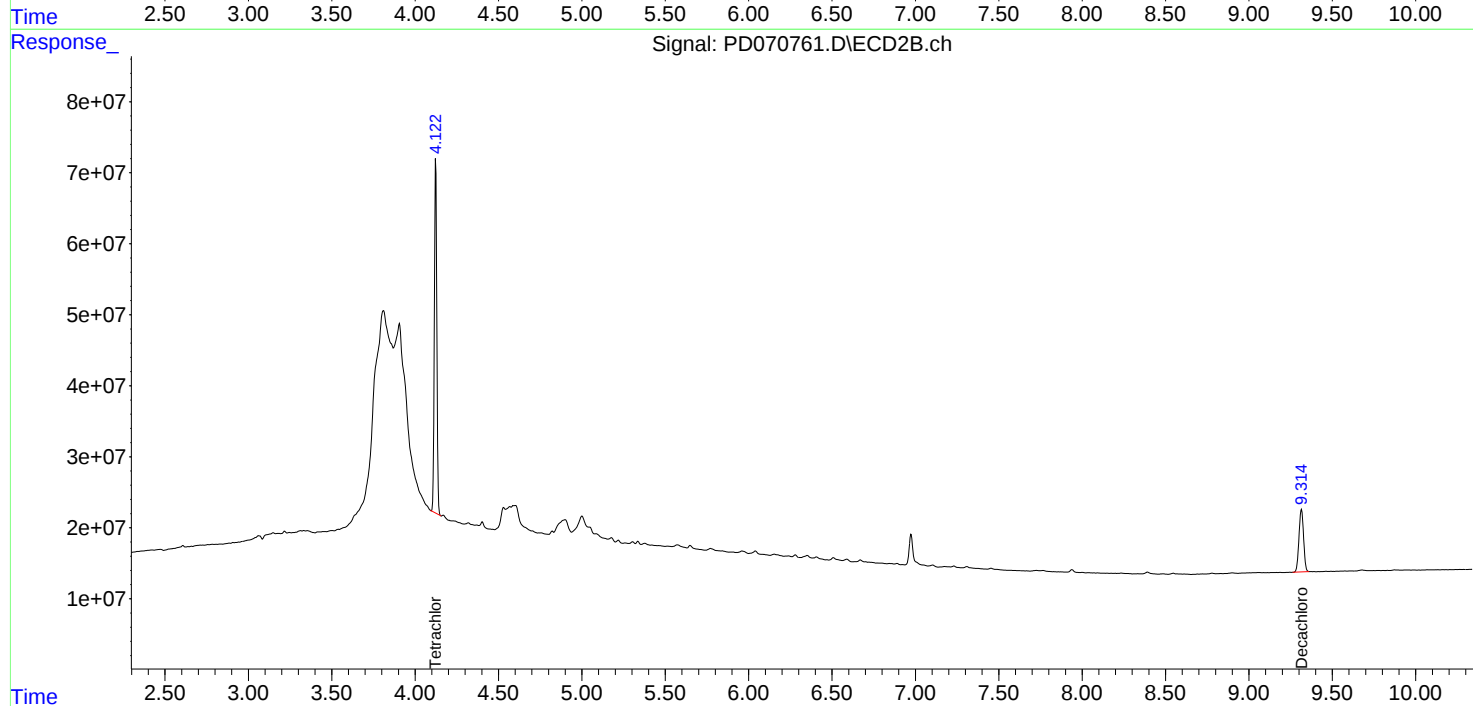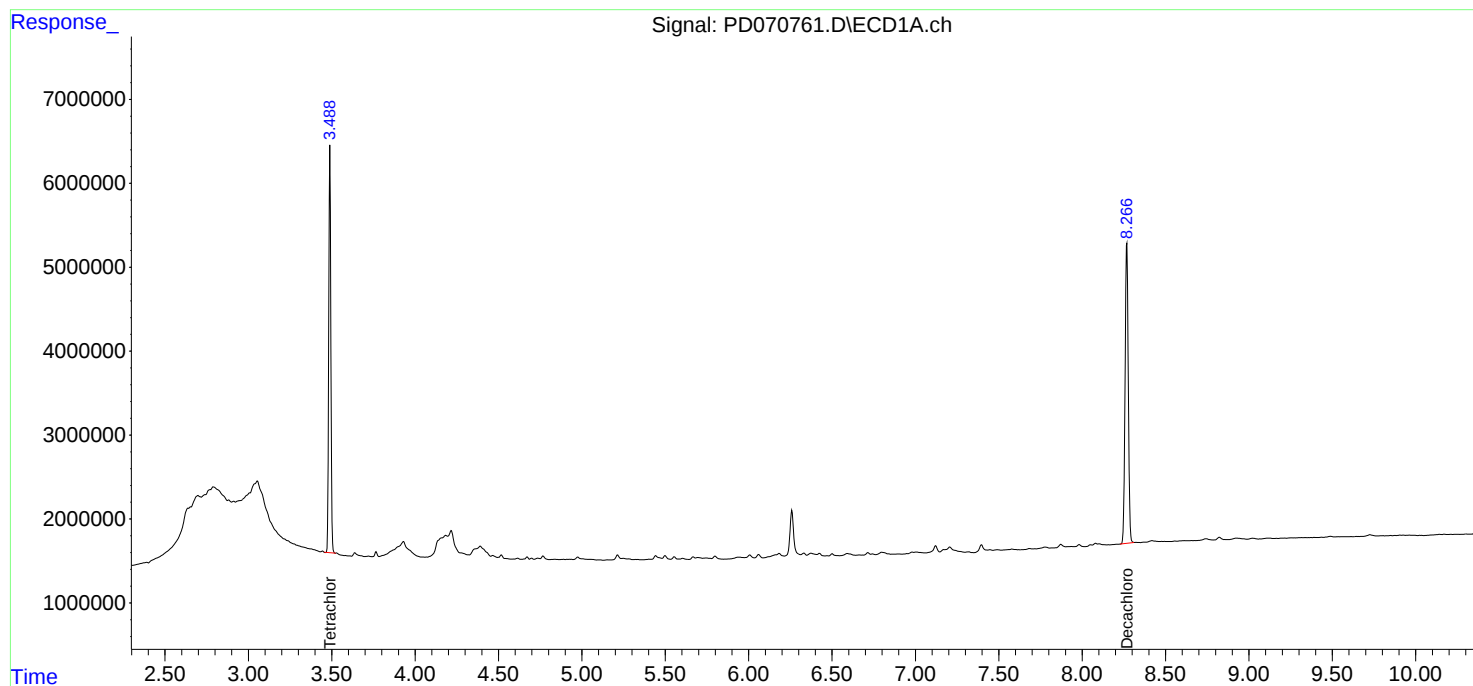


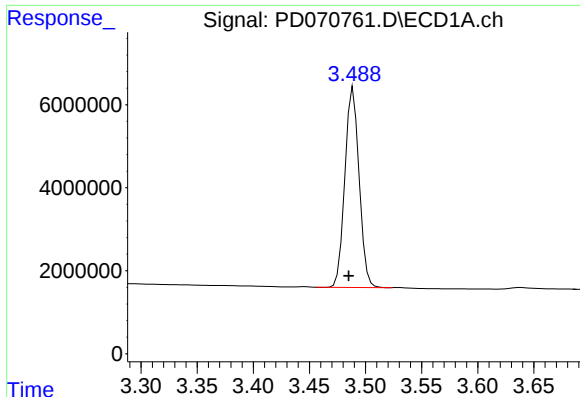

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.004 min
Response: 42422217
Conc: 17.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

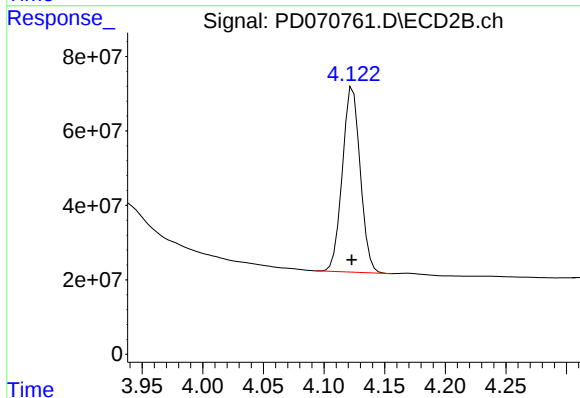


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 508869433
Conc: 19.68 ng/ml

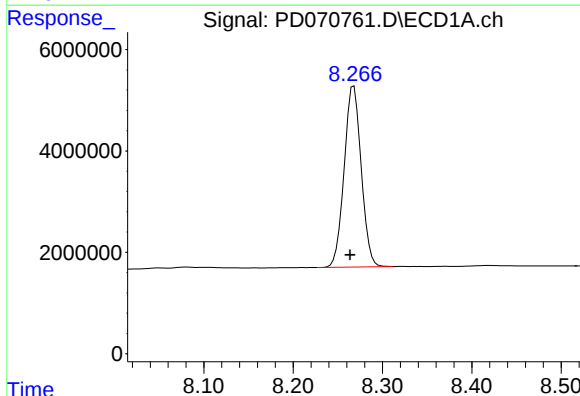

#28 Decachlorobiphenyl

R.T.: 8.268 min
Delta R.T.: 0.004 min
Response: 47294247
Conc: 19.07 ng/ml

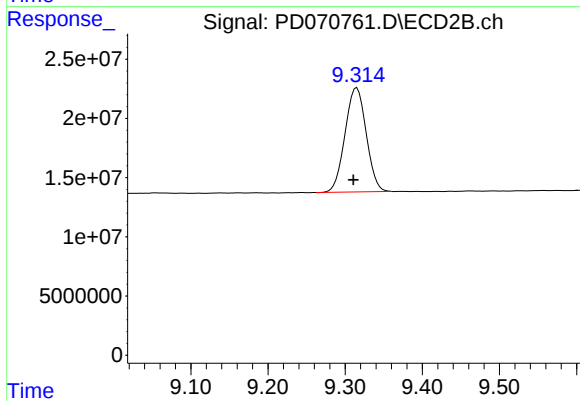

#28 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: 0.004 min
Response: 168109641
Conc: 20.43 ng/ml