

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
 Data File : PD058527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 17:50
 Operator : AJ\MA
 Sample : L3183-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:24:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.866	31696922	43061715	17.384	17.428
28)	SA Decachlor...	7.845	8.861	32722768	41080523	18.121	18.842
Target Compounds							
10)	B gamma-Chl...	0.000	5.934	0	1773662	N.D.	0.610 #
25)	Chlordane-3	0.000	5.934	0	1773662	N.D.	4.769 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
Data File : PD058527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 17:50
Operator : AJ\MA
Sample : L3183-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:24:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

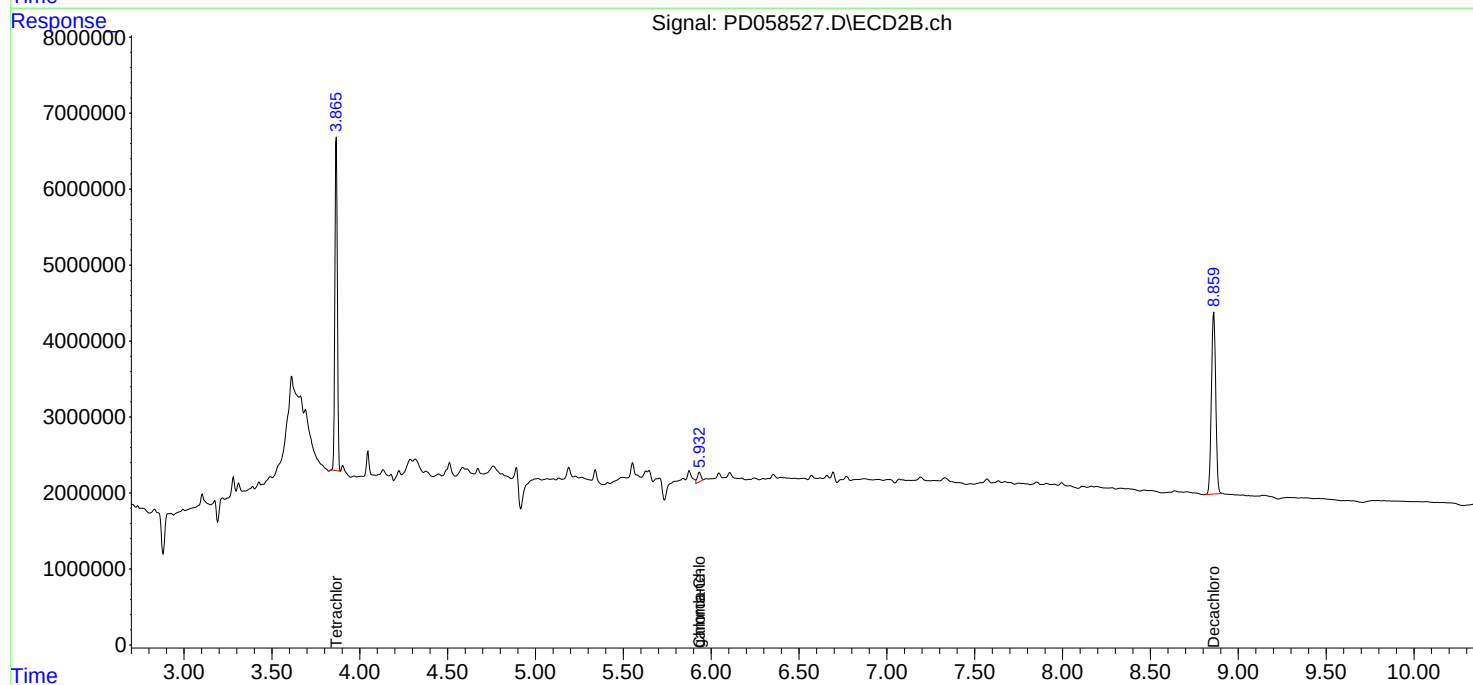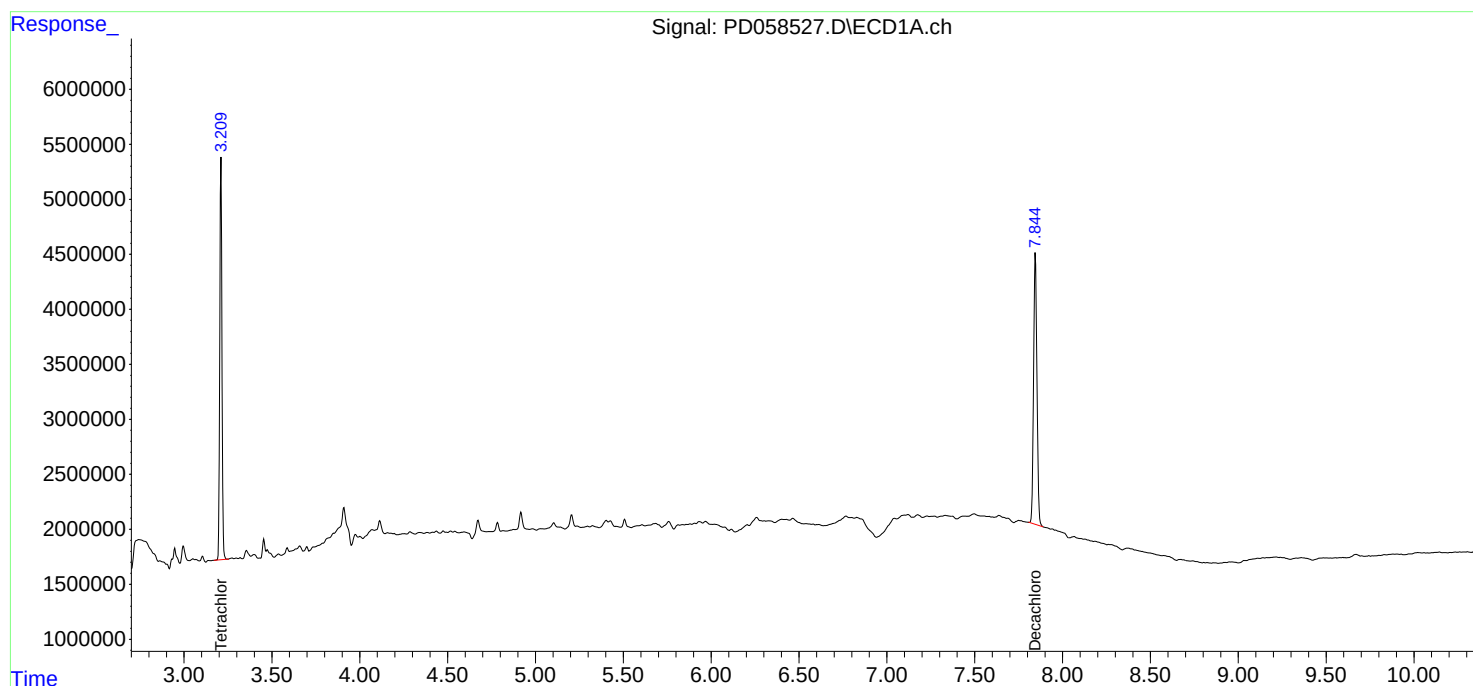


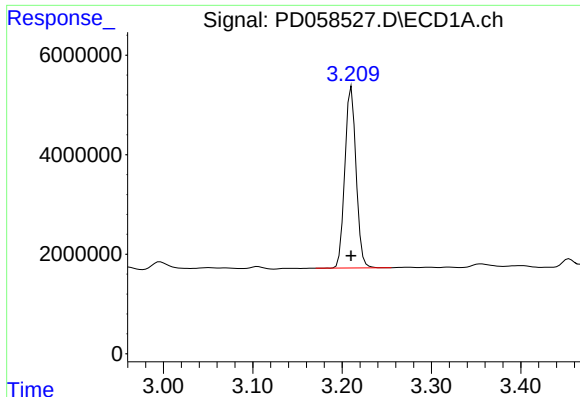

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 31696922
Conc: 17.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

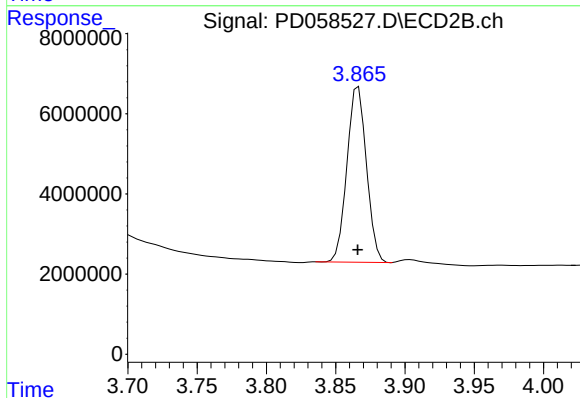


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 43061715
Conc: 17.43 ng/ml

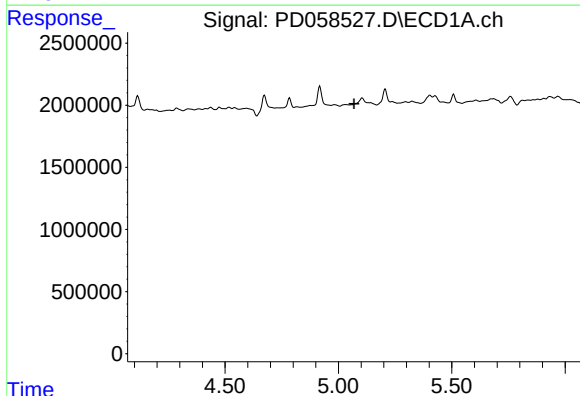


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

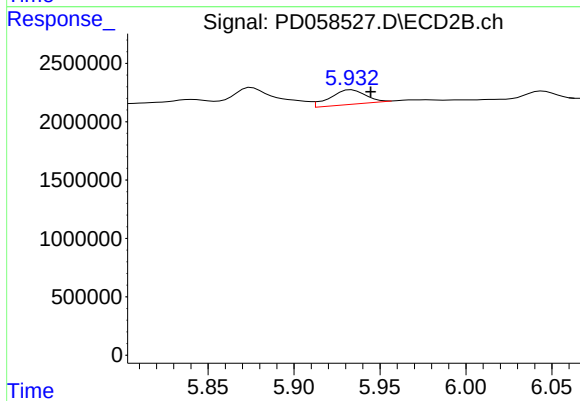

#10 gamma-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.011 min
Response: 1773662
Conc: 0.61 ng/ml

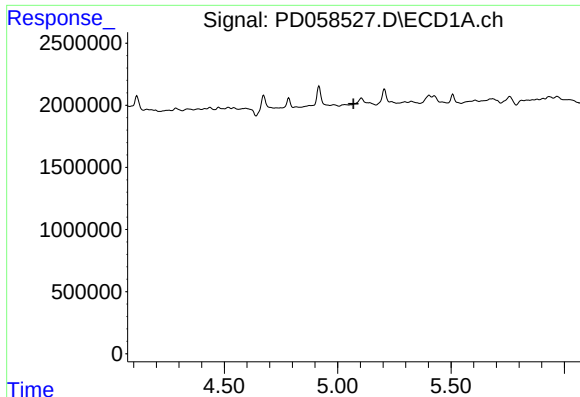

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

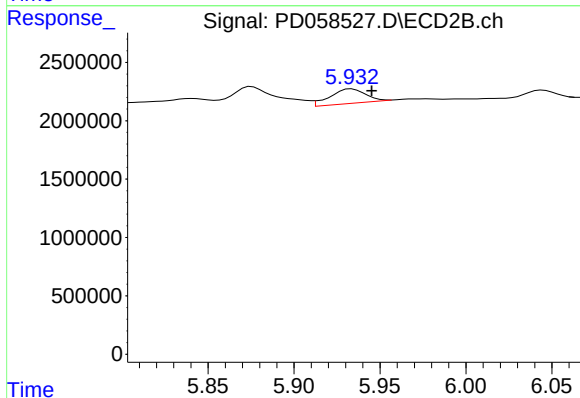


#25 Chlordane-3

R.T.: 5.934 min
Delta R.T.: -0.012 min
Response: 1773662
Conc: 4.77 ng/ml

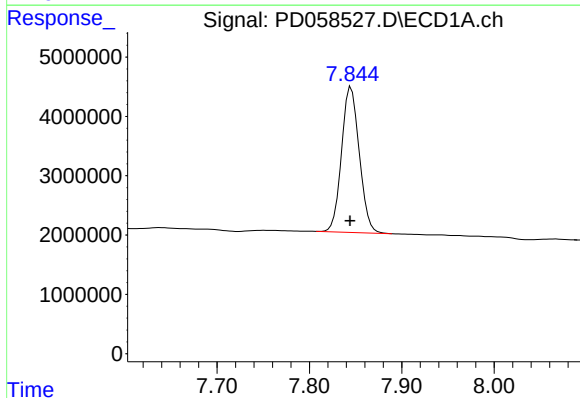

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.001 min
Response: 32722768
Conc: 18.12 ng/ml

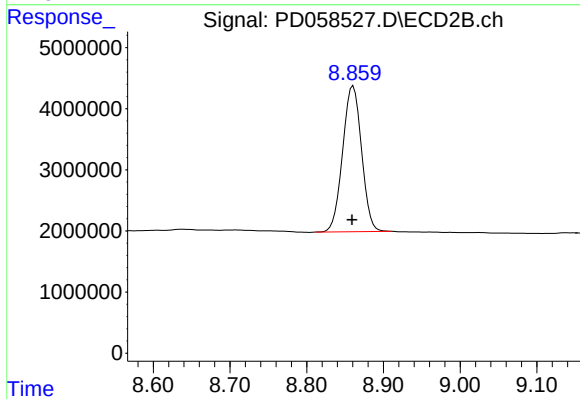

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.001 min
Response: 41080523
Conc: 18.84 ng/ml