

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
 Data File : PD058520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 16:07
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Ankita
 7/10/2020 12:32:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:34:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 13:55:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.210	3.866	79854864	110.5E6	43.656	44.663
7) SA Decachlor...	7.846	8.860	80487810	99216563	46.199	47.877
Target Compounds						
2) Toxaphene-1	5.594	6.412	8604303	11638008	472.408	458.960m
3) Toxaphene-2	5.970	6.704	13381601	12736363	462.578	453.568
4) Toxaphene-3	6.211	6.992	13369056	28491042	482.854	459.358
5) Toxaphene-4	6.348	7.075	5861882	17670690	496.160	472.873
6) Toxaphene-5	6.629	7.486	5294199	13154654	504.840	481.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
Data File : PD058520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 16:07
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:34:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 13:55:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

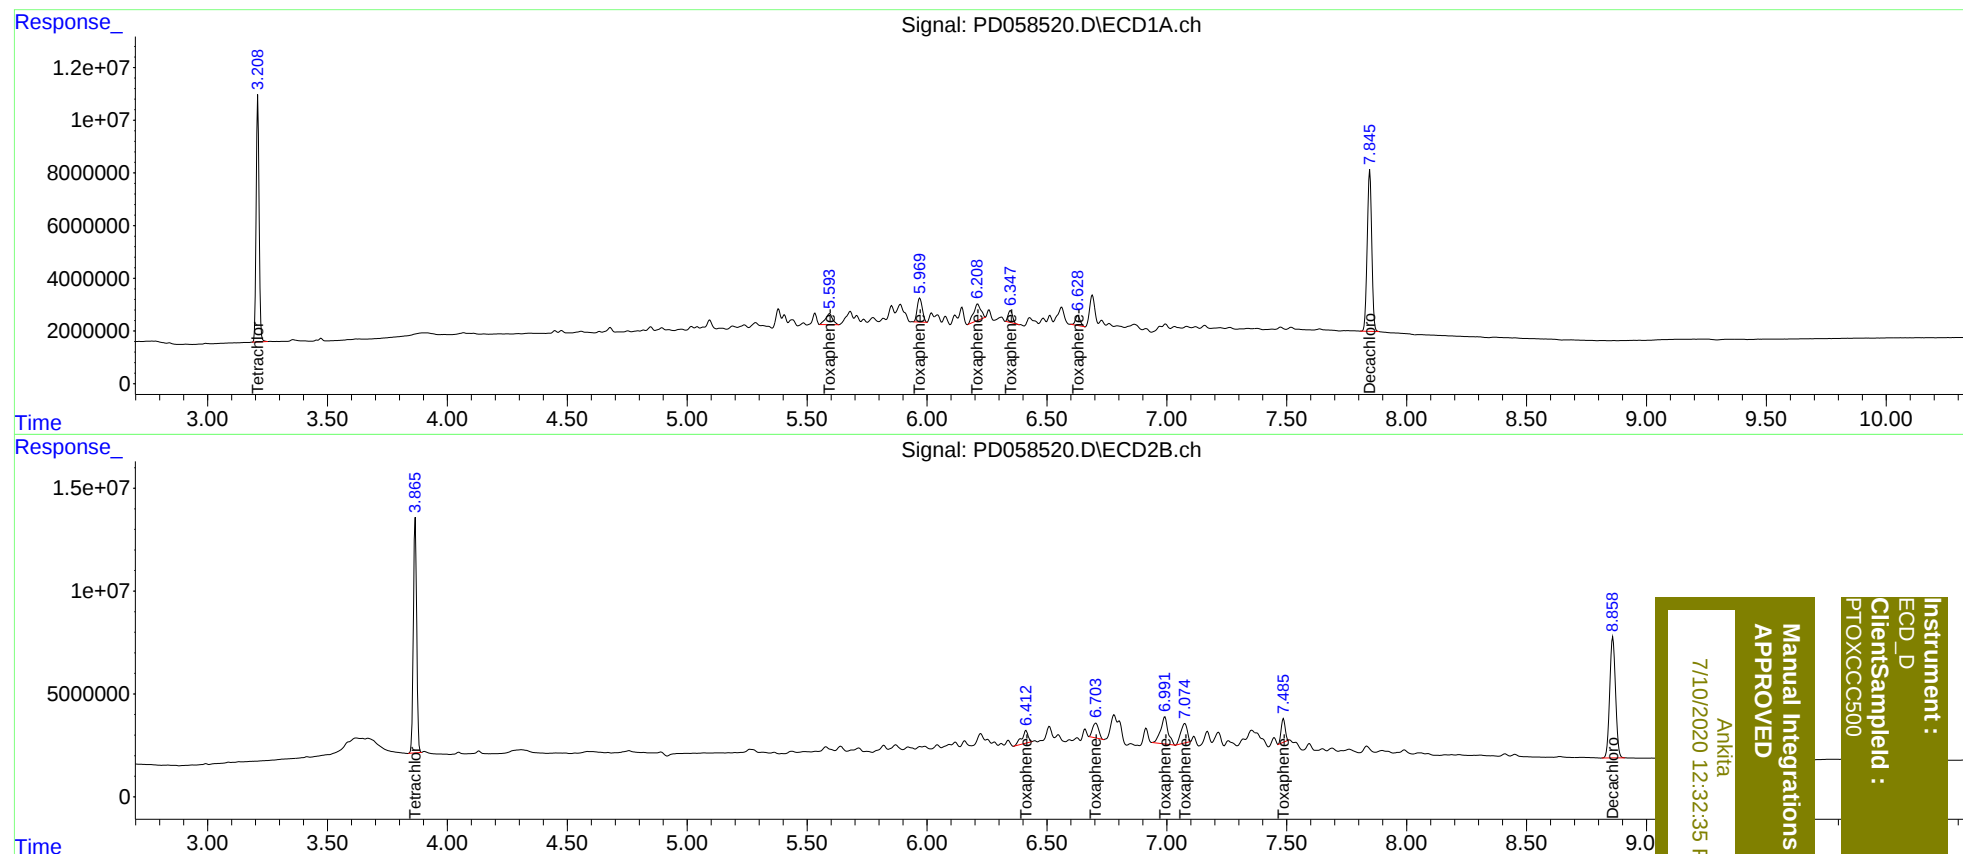

Manual Integrations
APPROVED

Ankita

7/10/2020 12:32:35 PM

Instrument :
ECD_D
ClientSampled :
PTOXCCC500