

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
 Data File : PD058503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 11:55
 Operator : AJ\MA
 Sample : L3216-07
 Misc : LOD 1 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:18:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	30039913	41649412	16.475	16.857
28)	SA Decachlor...	7.847	8.860	30793130	38645490	17.052	17.725

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
Data File : PD058503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 11:55
Operator : AJ\MA
Sample : L3216-07
Misc : LOD 1 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT3-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:18:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

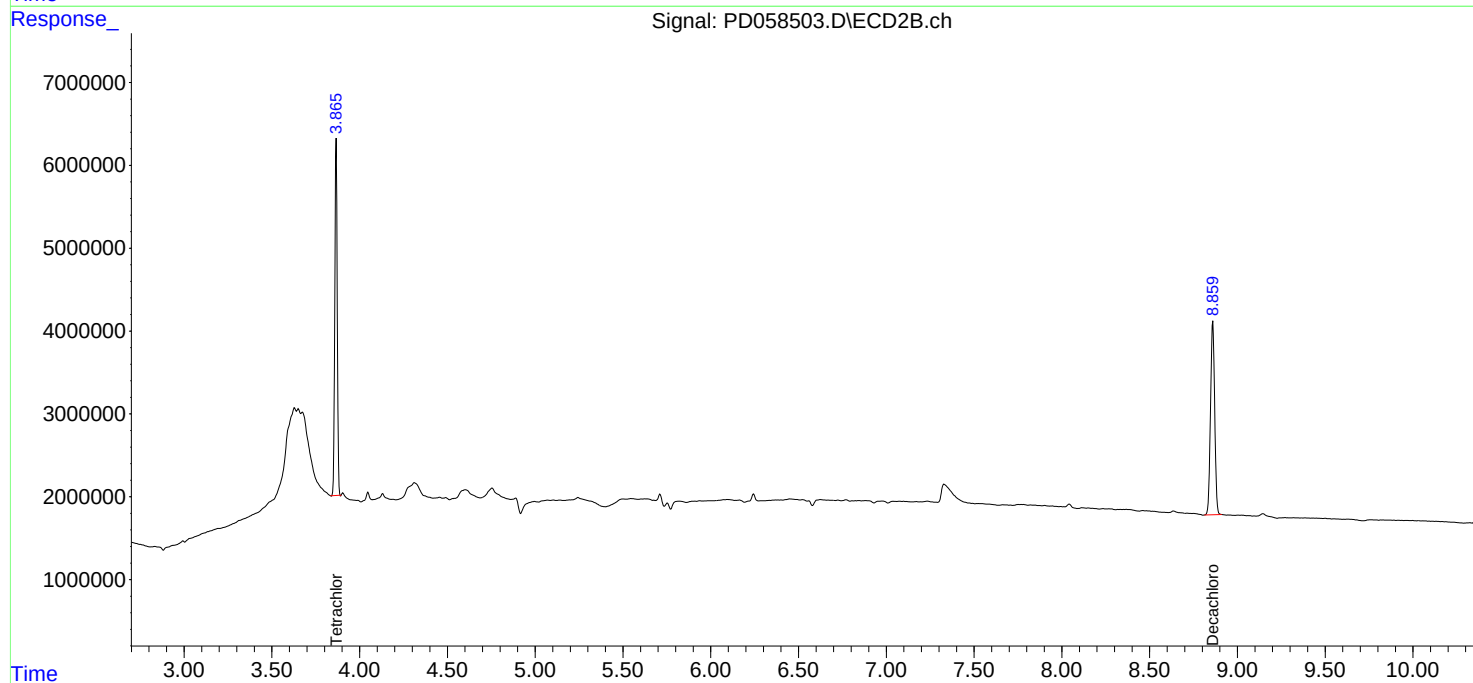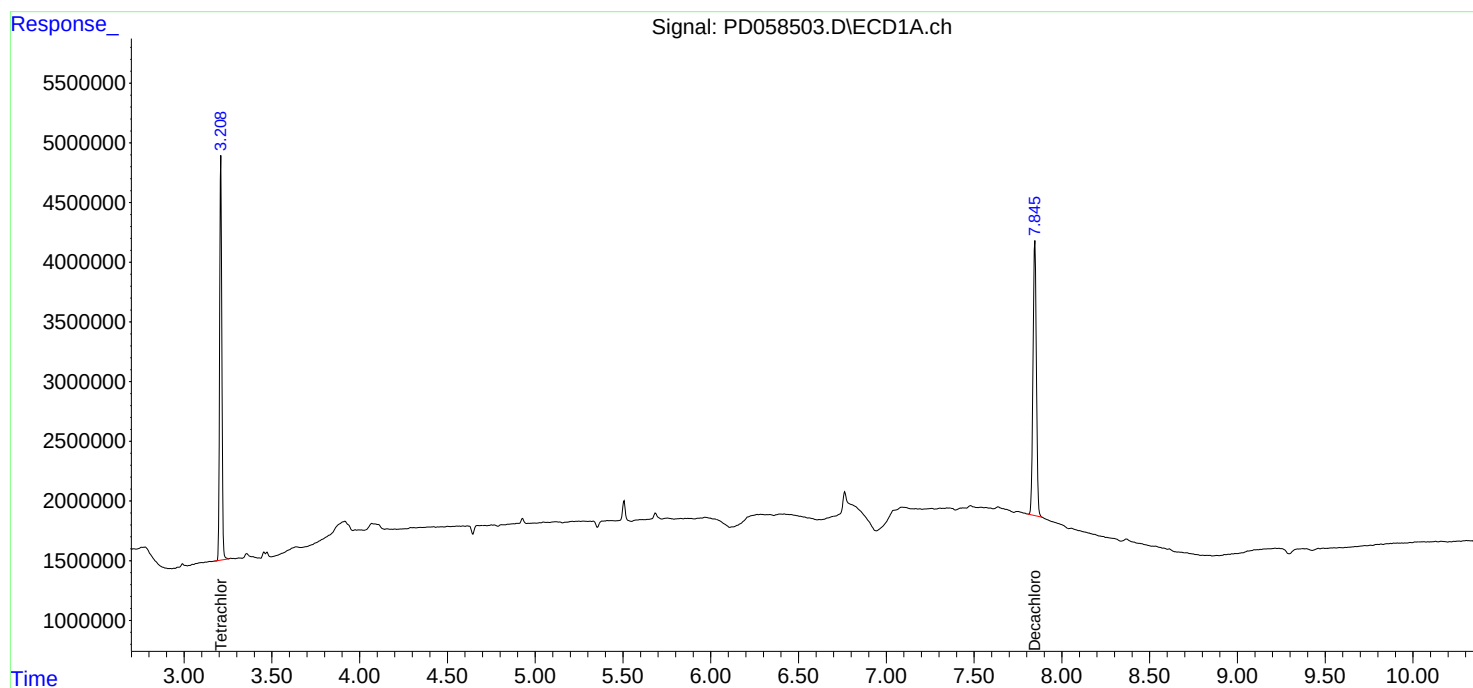


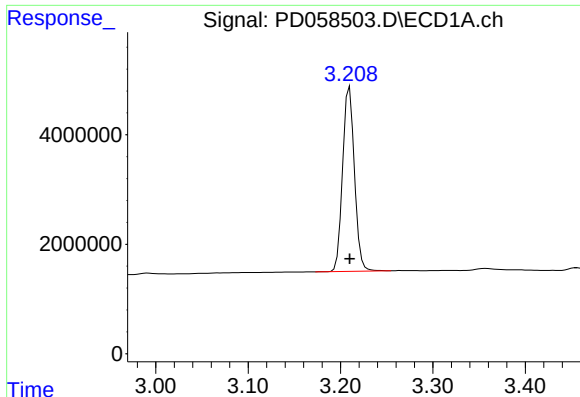

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 30039913
Conc: 16.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT3-2020

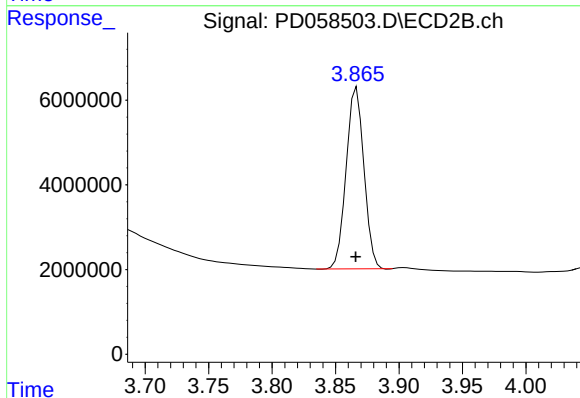


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 41649412
Conc: 16.86 ng/ml

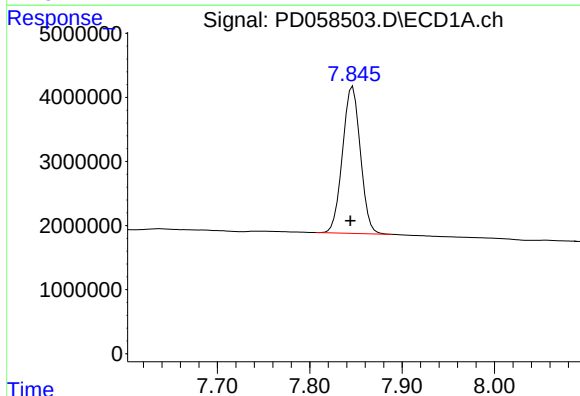

#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.002 min
Response: 30793130
Conc: 17.05 ng/ml

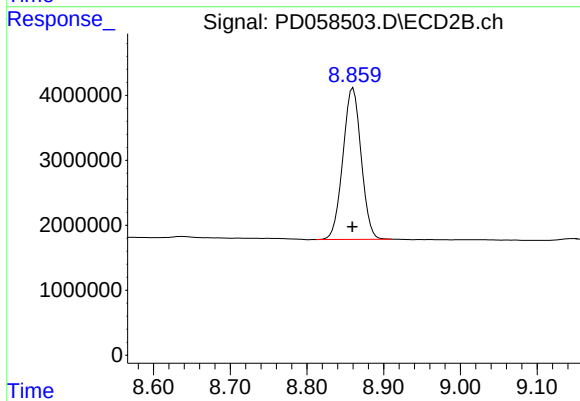

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 38645490
Conc: 17.72 ng/ml