

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
 Data File : PD058508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 13:08
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:20:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	85059374	106.2E6	46.651	42.985
28)	SA Decachlor...	7.846	8.859	76052404	91828350	42.115	42.118
Target Compounds							
23)	Chlordane-1	4.037	4.843	24667397	38575225	422.728	433.424
24)	Chlordane-2	4.522	5.305	27178450	40733561	420.454	412.341
25)	Chlordane-3	5.070	5.945	88552746	165.7E6	432.612	445.453
26)	Chlordane-4	5.125	6.018	81916810	194.3E6	429.269	446.731
27)	Chlordane-5	5.941	6.815	27946493	34936186	454.769	438.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
Data File : PD058508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 13:08
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:20:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

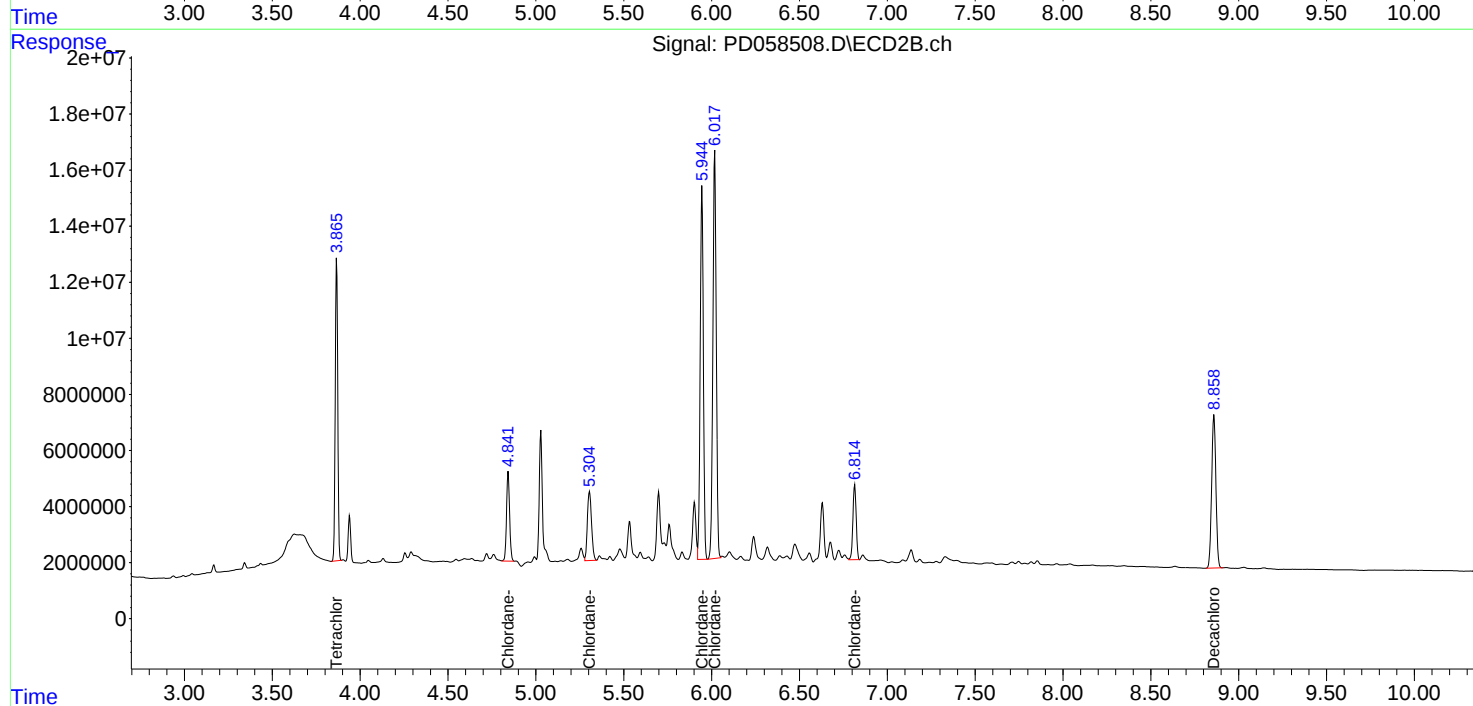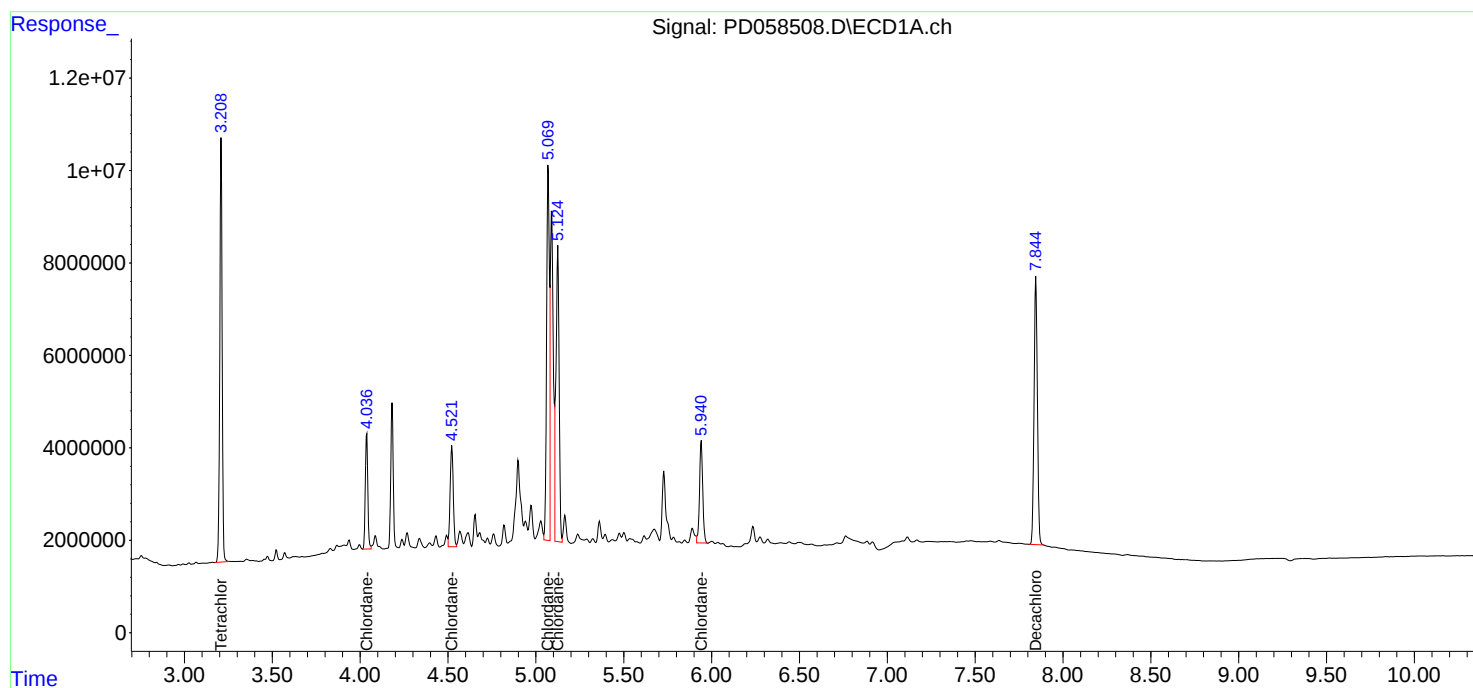


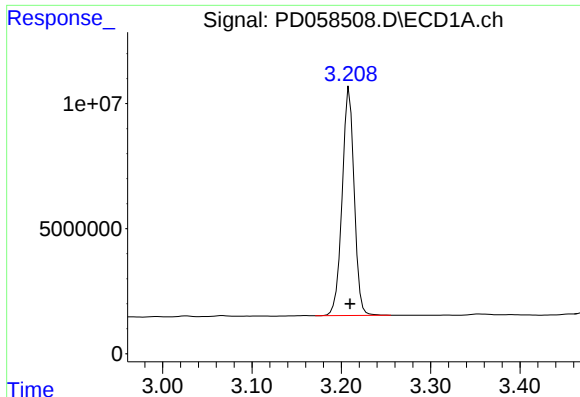

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 85059374
Conc: 46.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

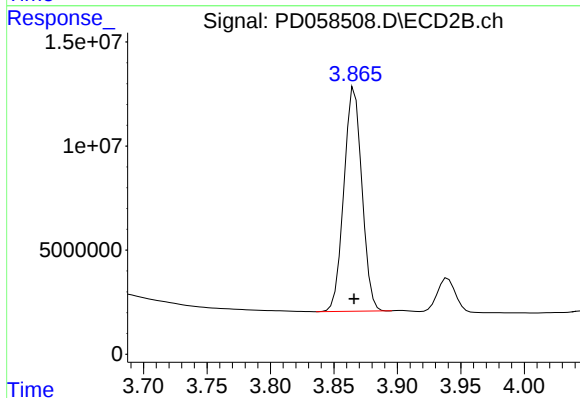


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 106205634
Conc: 42.98 ng/ml

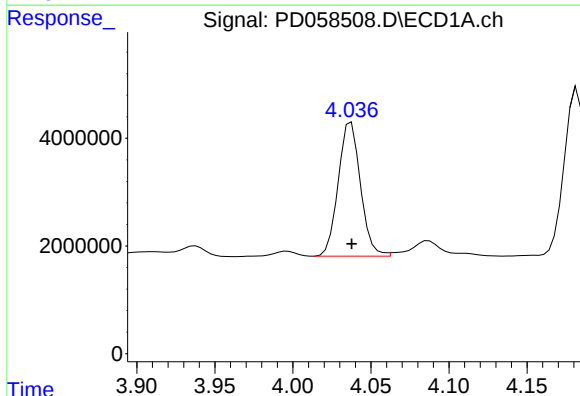


#23 Chlordane-1

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 24667397
Conc: 422.73 ng/ml

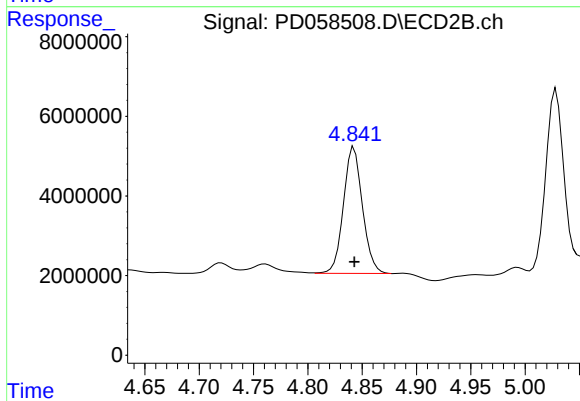

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 38575225
Conc: 433.42 ng/ml

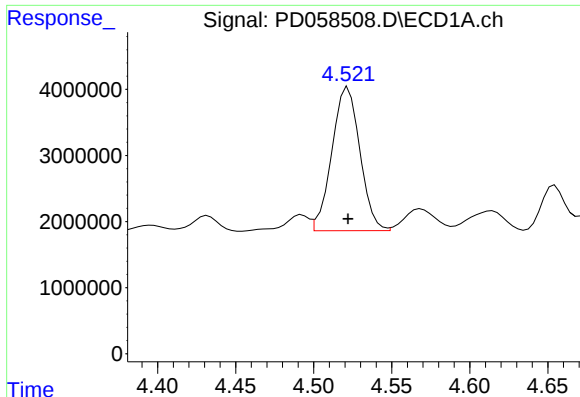

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 27178450
Conc: 420.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

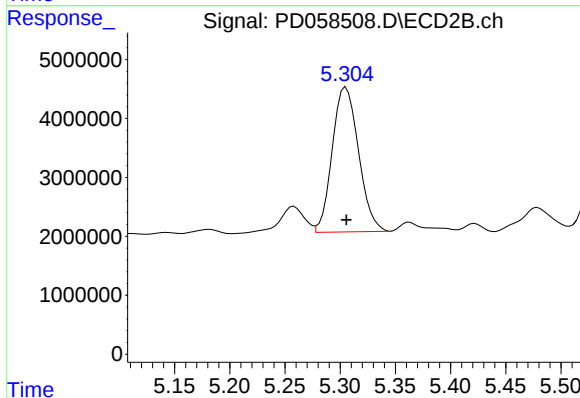


#24 Chlordane-2

R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 40733561
Conc: 412.34 ng/ml

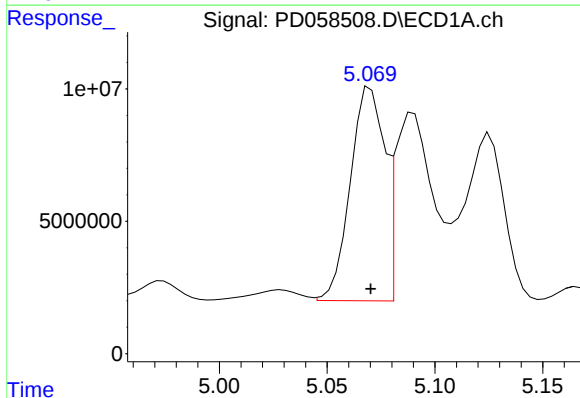


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 88552746
Conc: 432.61 ng/ml

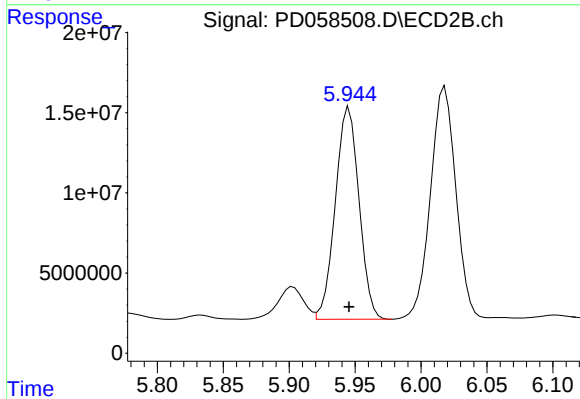

#25 Chlordane-3


R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 165684253
Conc: 445.45 ng/ml

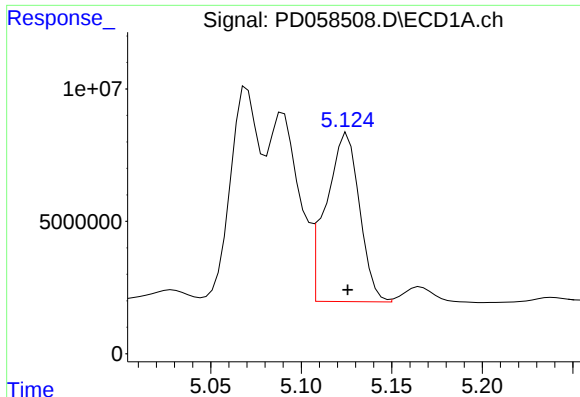

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 81916810
Conc: 429.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

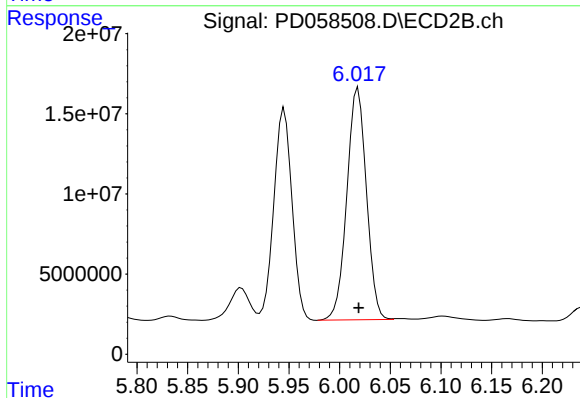


#26 Chlordane-4

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 194328161
Conc: 446.73 ng/ml

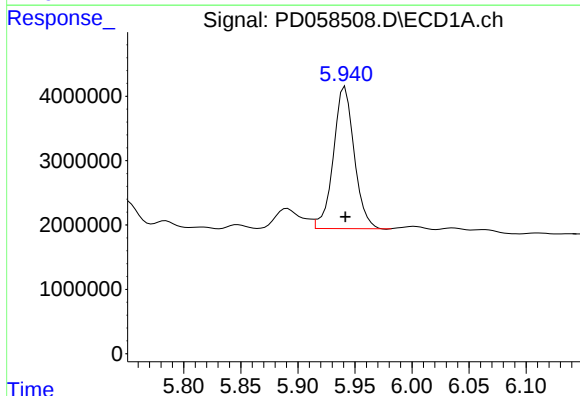


#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 27946493
Conc: 454.77 ng/ml

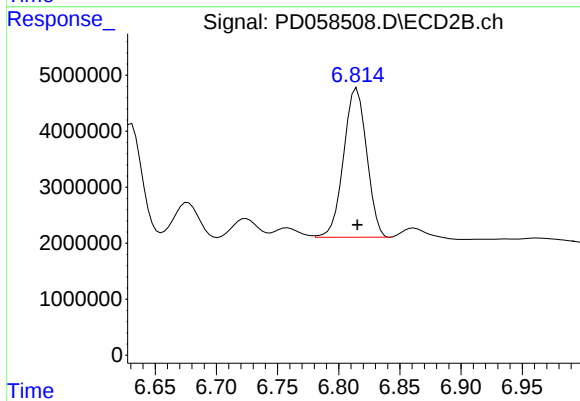

#27 Chlordane-5


R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 34936186
Conc: 438.46 ng/ml

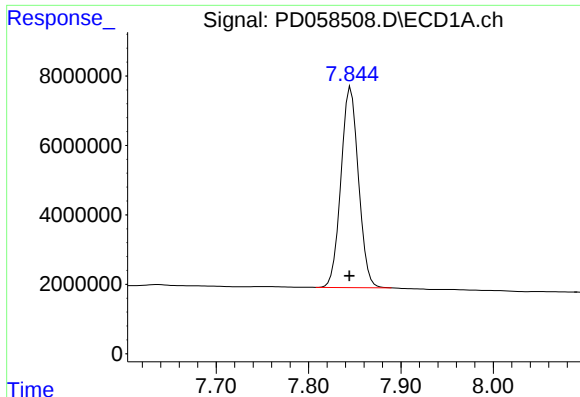

#28 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.002 min
Response: 76052404
Conc: 42.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

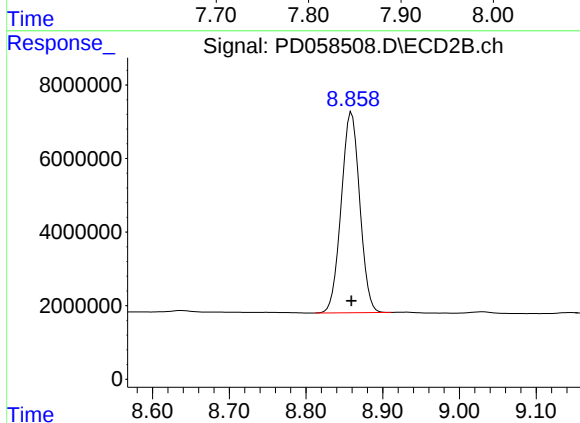

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 91828350
Conc: 42.12 ng/ml