

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
 Data File : PD058533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 19:18
 Operator : AJ\MA
 Sample : L3186-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-02-070820

Manual Integrations
 APPROVED

Ankita
 7/10/2020 12:32:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:25:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	31642248	43083018	17.354m	17.437
28)	SA Decachlor...	7.847	8.862	34631128	43041422	19.177	19.741

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070920\
Data File : PD058533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 19:18
Operator : AJ\MA
Sample : L3186-05
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OR-02-070820


Manual Integrations
APPROVED

Ankita
7/10/2020 12:32:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:25:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

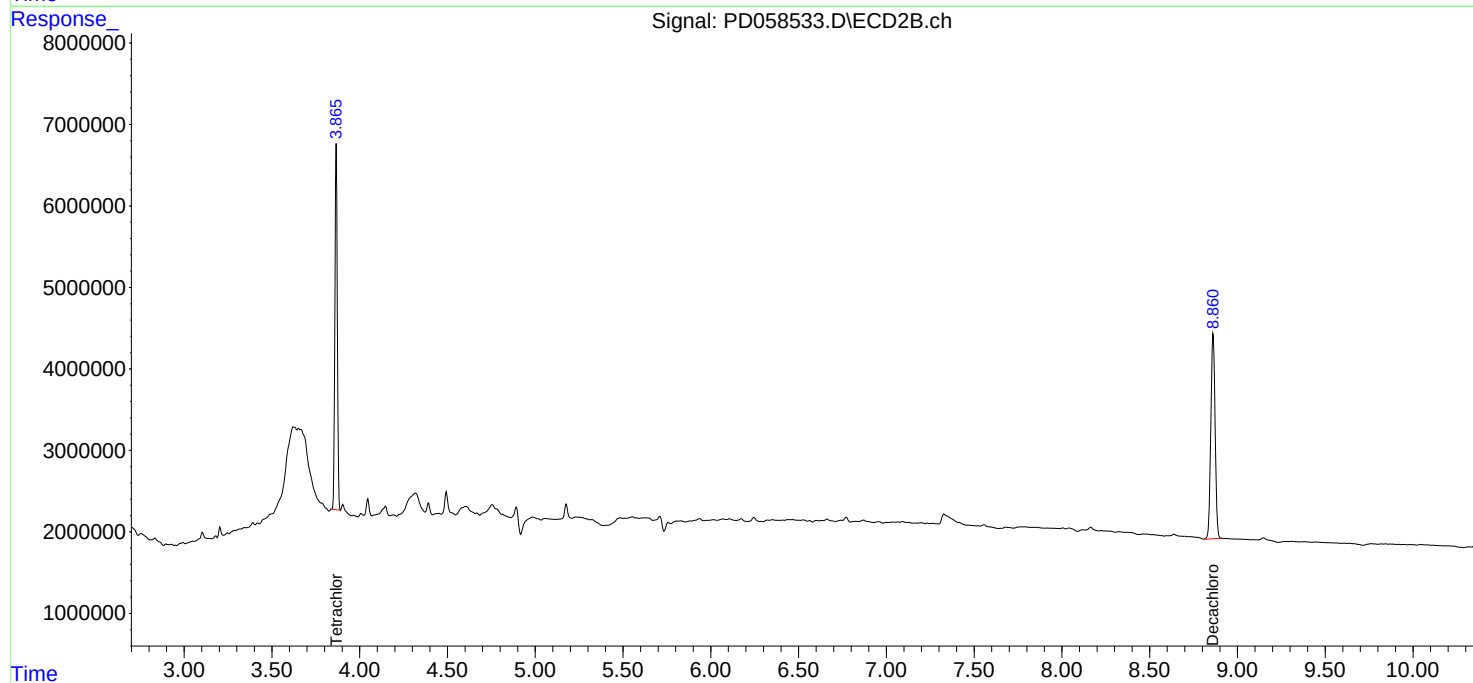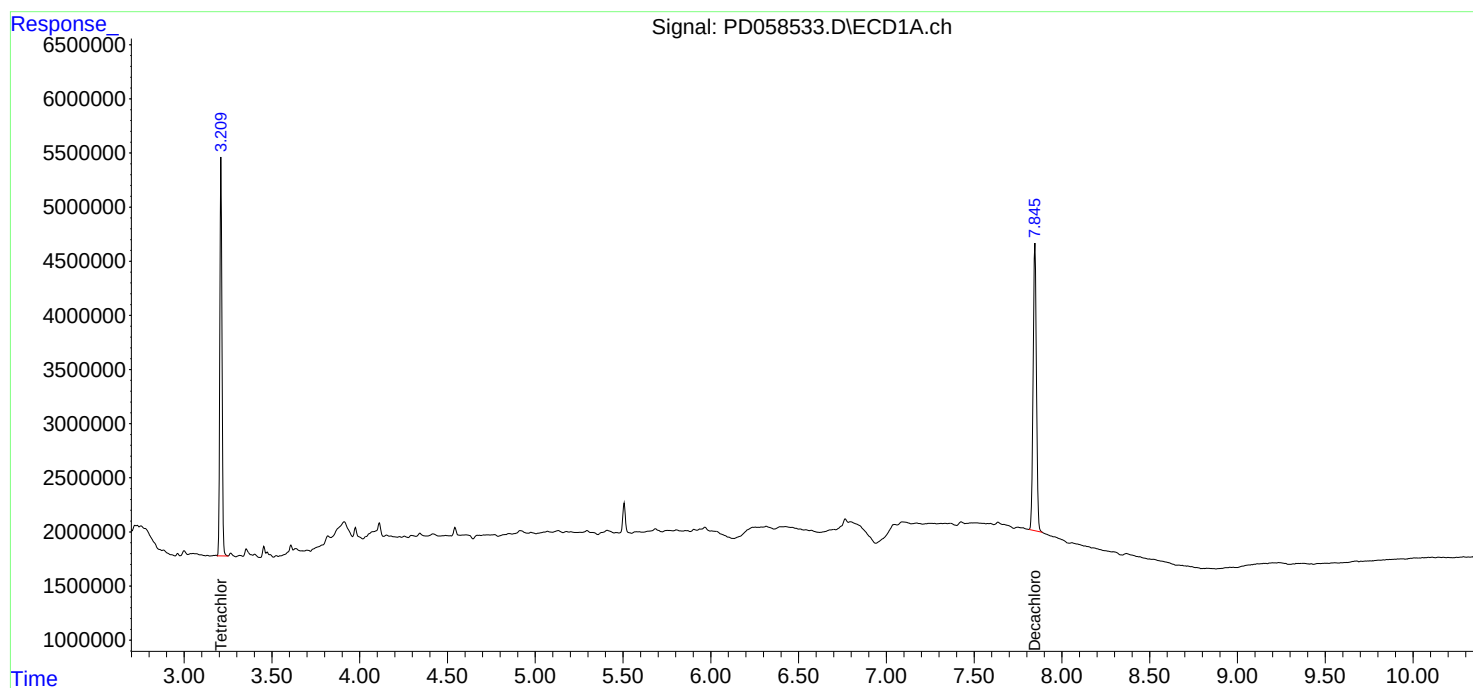

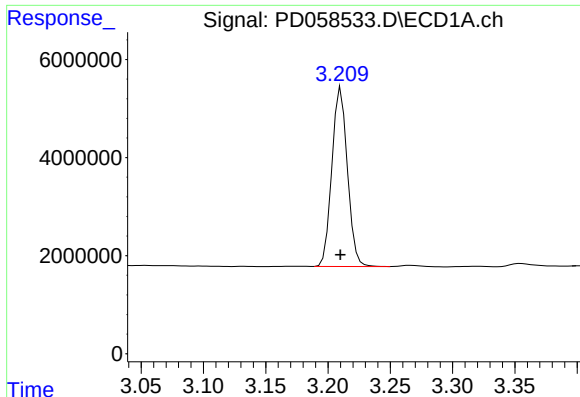


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 31642248
Conc: 17.35 ng/ml m

Instrument :
ECD_D
ClientSampleId :
OR-02-070820


Manual Integrations
APPROVED

Ankita
7/10/2020 12:32:51 PM

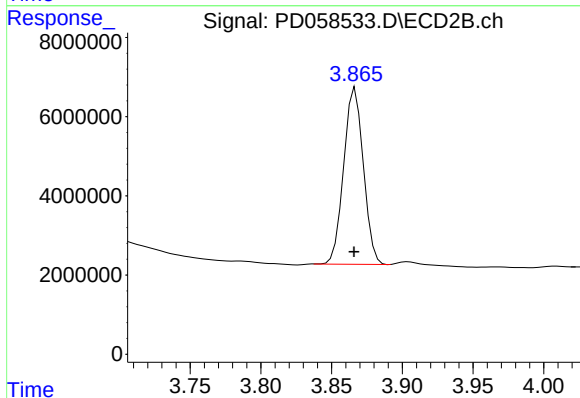


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 43083018
Conc: 17.44 ng/ml

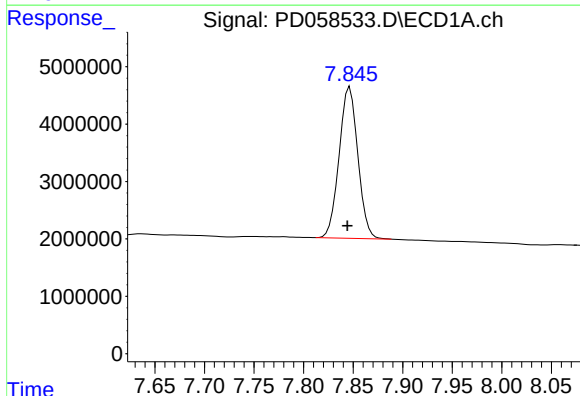

#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.003 min
Response: 34631128
Conc: 19.18 ng/ml

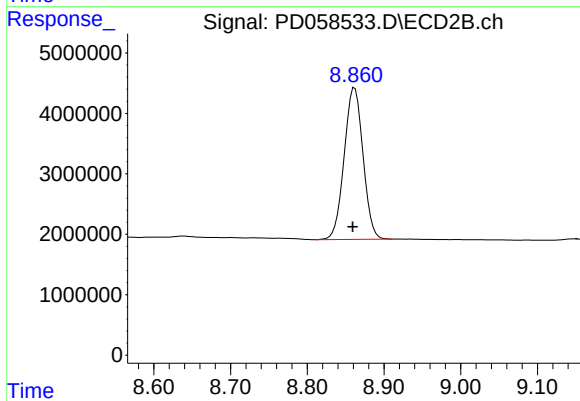

#28 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.003 min
Response: 43041422
Conc: 19.74 ng/ml