

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 13:37
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:46:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 15:45:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.045	3.513	7252746	58235257	5.413	5.908
27)	SA Decachlor...	9.214	8.259	11207384	57296955	10.170	10.885
Target Compounds							
2)	A alpha-BHC	4.447	3.953	9397805	77394869	5.023	5.908
3)	MA gamma-BHC...	4.739	4.235	9438443	72962671	5.305	6.199
4)	MA Heptachlor	5.250	4.535	9902219	65188293	5.719	5.779
9)	A Endosulfan I	6.317	5.563	7997609	47762501	5.958	5.716
13)	MA Dieldrin	6.579	5.806	16244664	94569655	11.648	11.170
14)	MA Endrin	6.801	6.063	13356754	81289683	11.774	11.266
16)	A 4,4'-DDD	6.926	6.185	12749813	73100405	11.643	10.912
17)	MA 4,4'-DDT	7.226	6.426	12744497	75023548	11.501	10.749
20)	A Methoxychlor	7.692	6.972	35035943	181.4E6	52.345	59.034


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 13:37
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:46:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 15:45:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

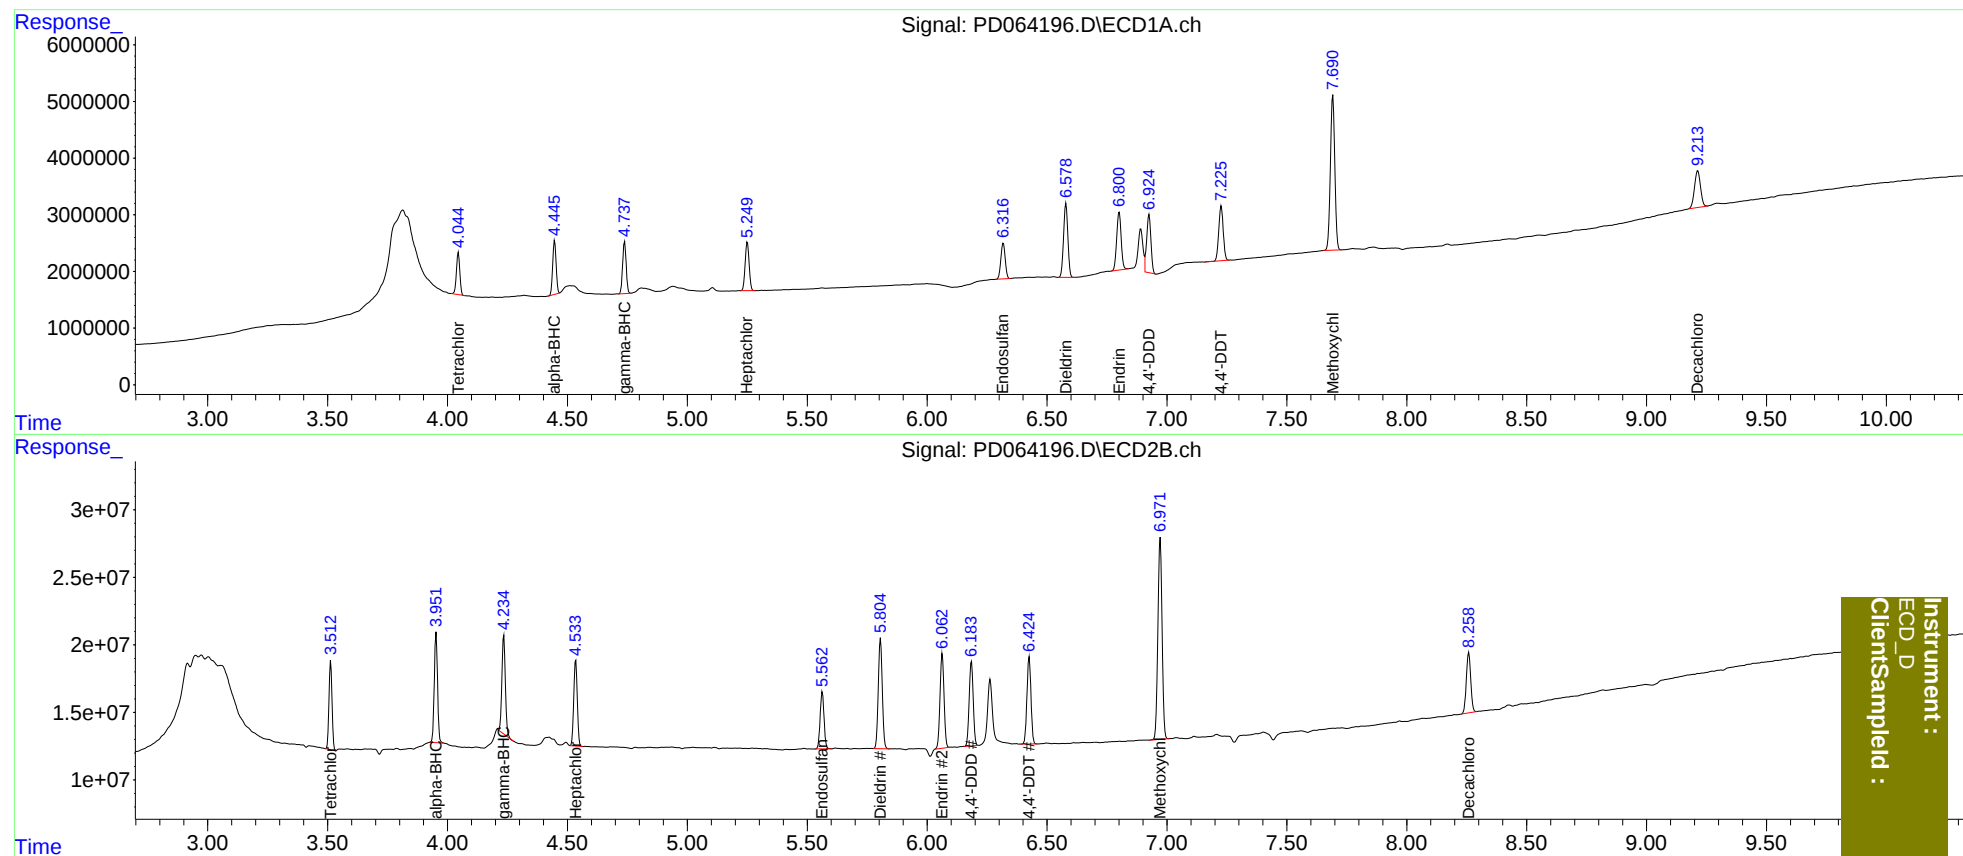


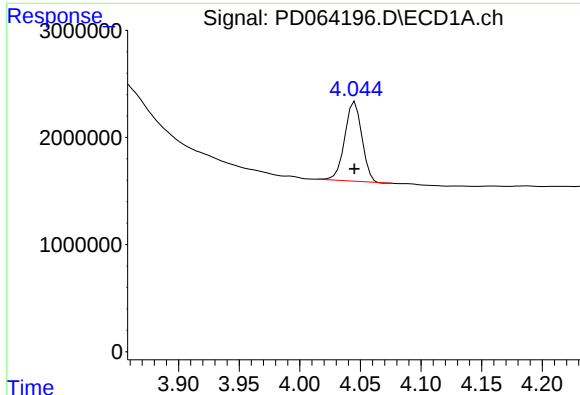

#1 Tetrachloro-m-xylene


R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 7252746
Conc: 5.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

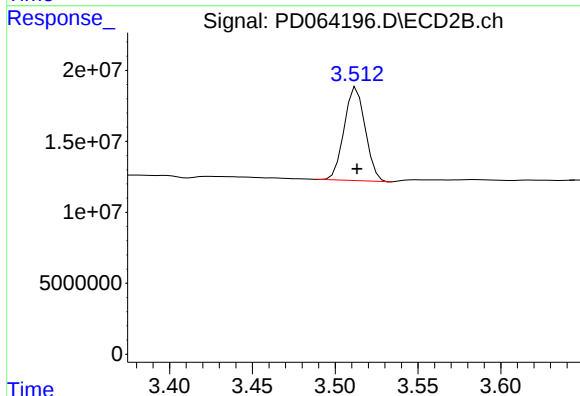


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 58235257
Conc: 5.91 ng/ml

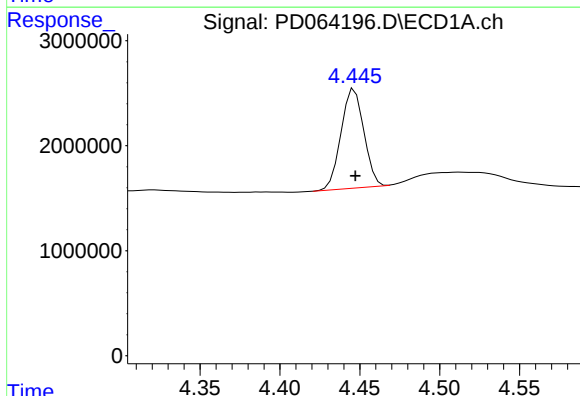


#2 alpha-BHC

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 9397805
Conc: 5.02 ng/ml

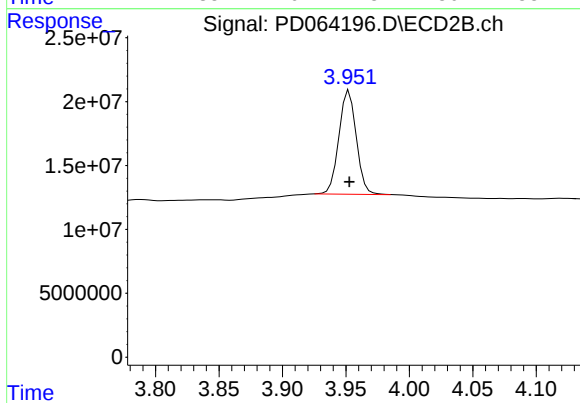

#2 alpha-BHC


R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 77394869
Conc: 5.91 ng/ml

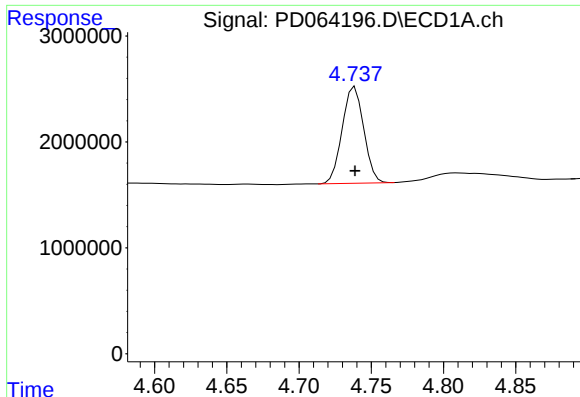

#3 gamma-BHC (Lindane)


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 9438443
Conc: 5.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

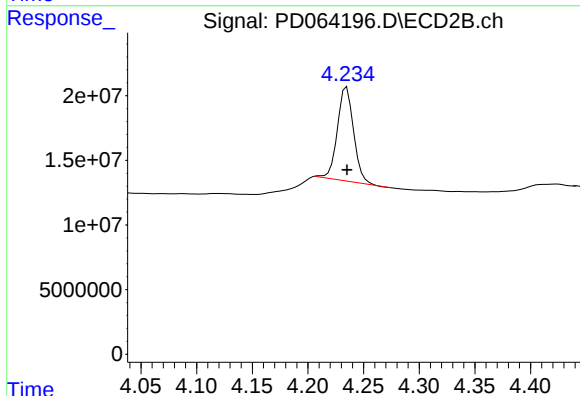


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 72962671
Conc: 6.20 ng/ml

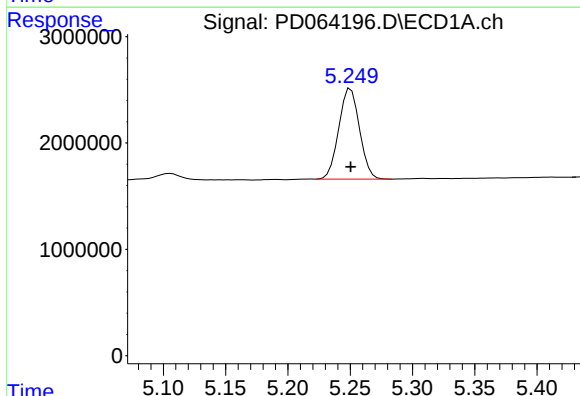


#4 Heptachlor

R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 9902219
Conc: 5.72 ng/ml

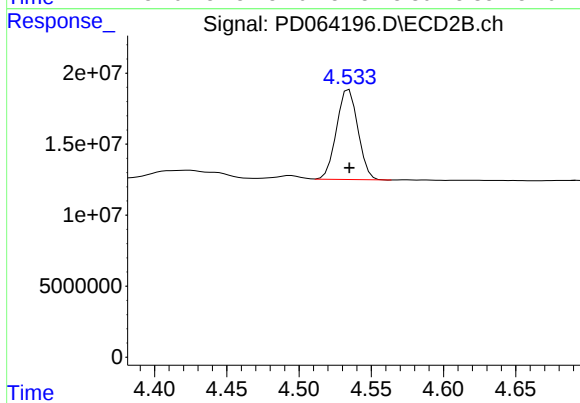

#4 Heptachlor


R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 65188293
Conc: 5.78 ng/ml

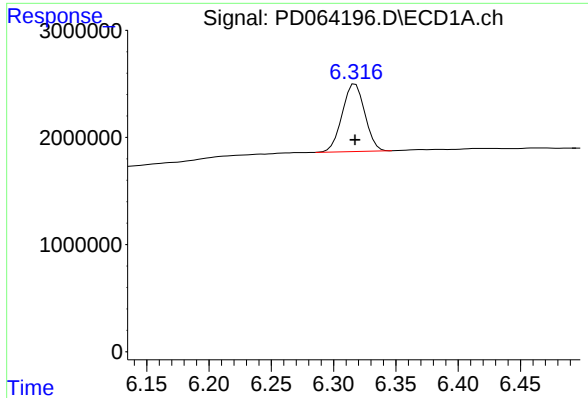

#9 Endosulfan I


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 7997609
Conc: 5.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

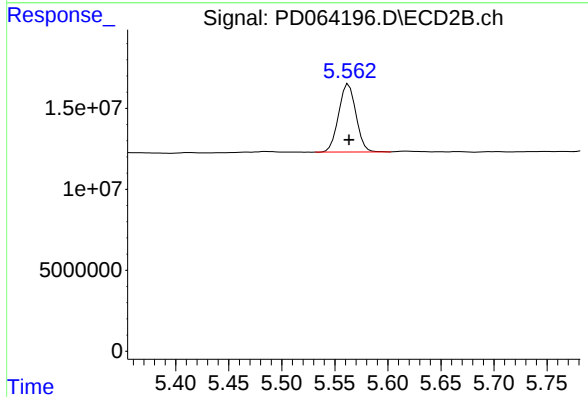


#9 Endosulfan I

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 47762501
Conc: 5.72 ng/ml

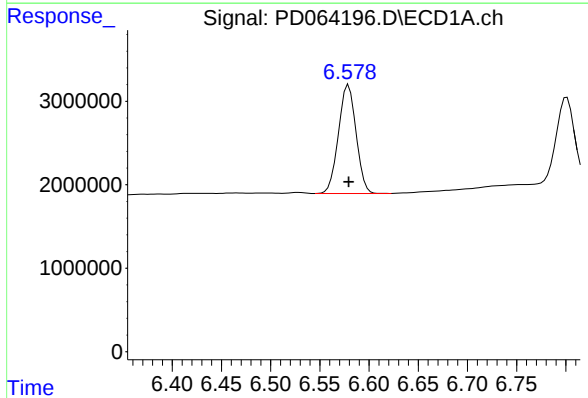


#13 Dieldrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 16244664
Conc: 11.65 ng/ml

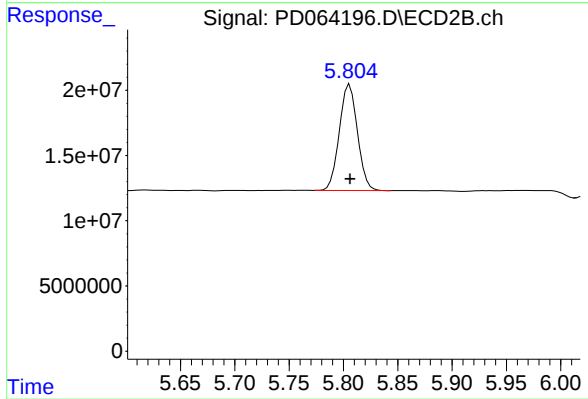

#13 Dieldrin


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 94569655
Conc: 11.17 ng/ml

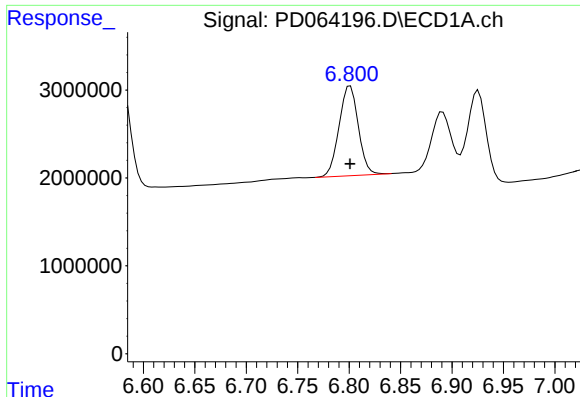

#14 Endrin


R.T.: 6.801 min
Delta R.T.: 0.000 min
Response: 13356754
Conc: 11.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

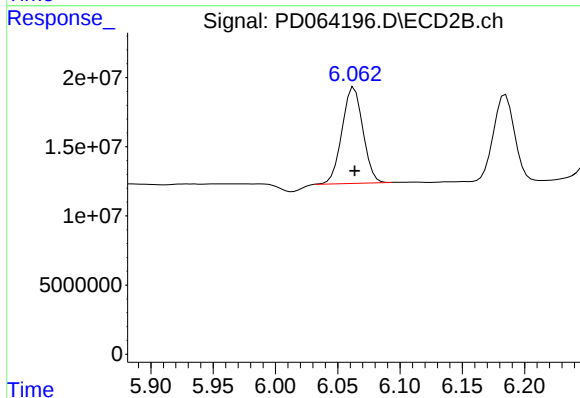


#14 Endrin

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 81289683
Conc: 11.27 ng/ml

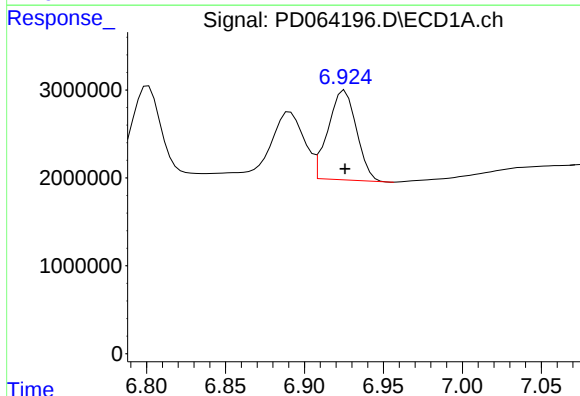


#16 4,4'-DDD

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 12749813
Conc: 11.64 ng/ml

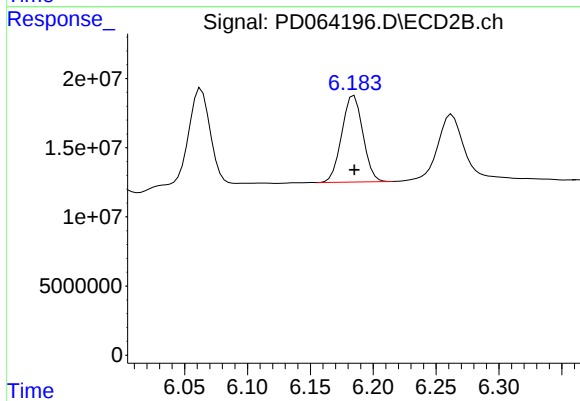

#16 4,4'-DDD


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 73100405
Conc: 10.91 ng/ml

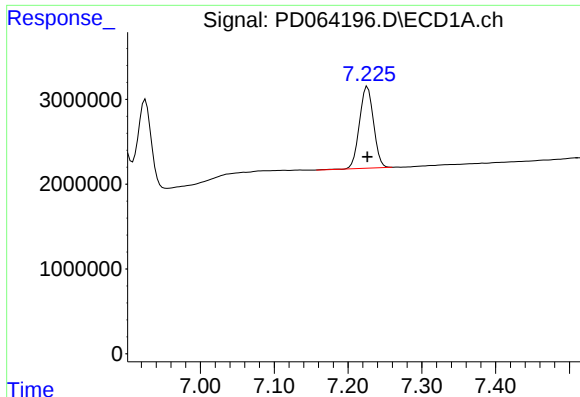

#17 4,4'-DDT


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 12744497
Conc: 11.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

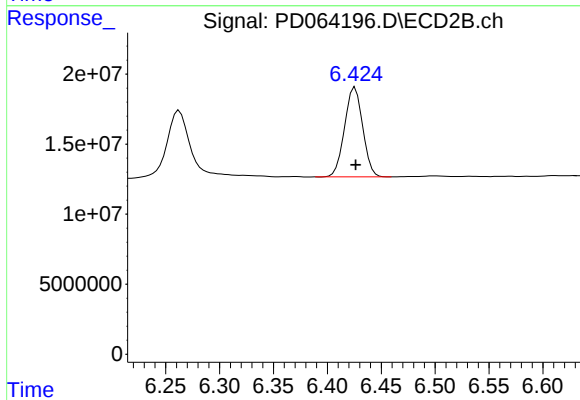


#17 4,4'-DDT

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 75023548
Conc: 10.75 ng/ml

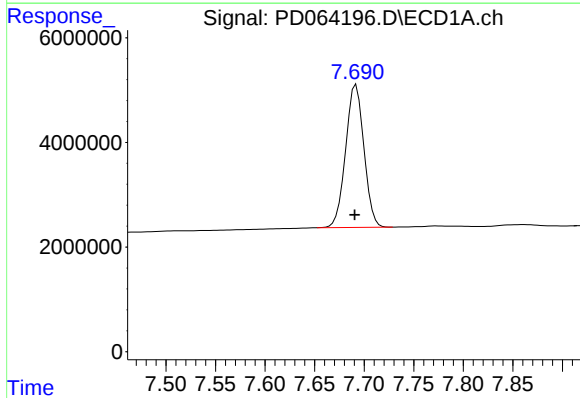


#20 Methoxychlor

R.T.: 7.692 min
Delta R.T.: 0.001 min
Response: 35035943
Conc: 52.34 ng/ml

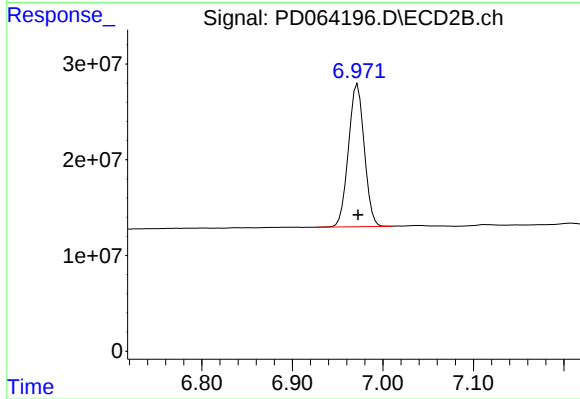

#20 Methoxychlor


R.T.: 6.972 min
Delta R.T.: 0.000 min
Response: 181368071
Conc: 59.03 ng/ml

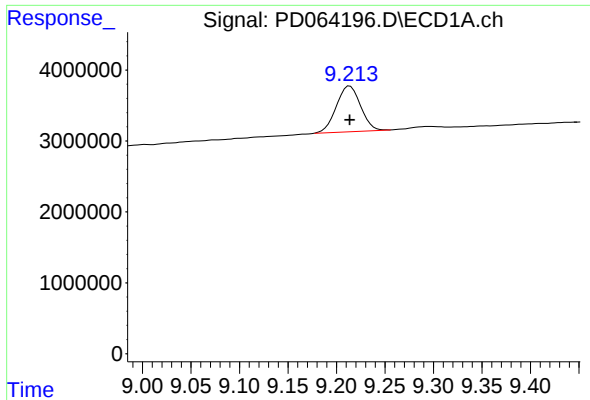

#27 Decachlorobiphenyl

R.T.: 9.214 min
Delta R.T.: 0.000 min
Response: 11207384
Conc: 10.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

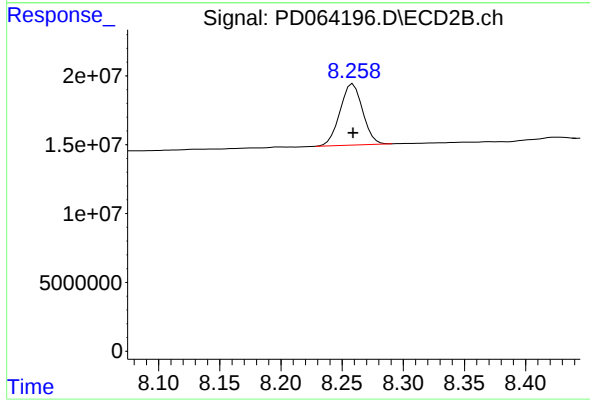

#27 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 57296955
Conc: 10.89 ng/ml