

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 14:32
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:46:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 15:45:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.045	3.513	26798695	197.1E6	20.000	20.000
27)	SA Decachlor...	9.214	8.259	44082036	210.5E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.447	3.953	37419002	262.0E6	20.000	20.000
3)	MA gamma-BHC...	4.739	4.235	35585353	235.4E6	20.000	20.000
4)	MA Heptachlor	5.251	4.535	34626788	225.6E6	20.000	20.000
9)	A Endosulfan I	6.317	5.563	26846376	167.1E6	20.000	20.000
13)	MA Dieldrin	6.579	5.806	55783723	338.6E6	40.000	40.000
14)	MA Endrin	6.801	6.064	45378532	288.6E6	40.000	40.000
16)	A 4,4'-DDD	6.926	6.185	43802509	268.0E6	40.000	40.000
17)	MA 4,4'-DDT	7.226	6.426	44324669	279.2E6	40.000	40.000
20)	A Methoxychlor	7.690	6.973	133.9E6	614.4E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 14:32
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:46:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 15:45:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

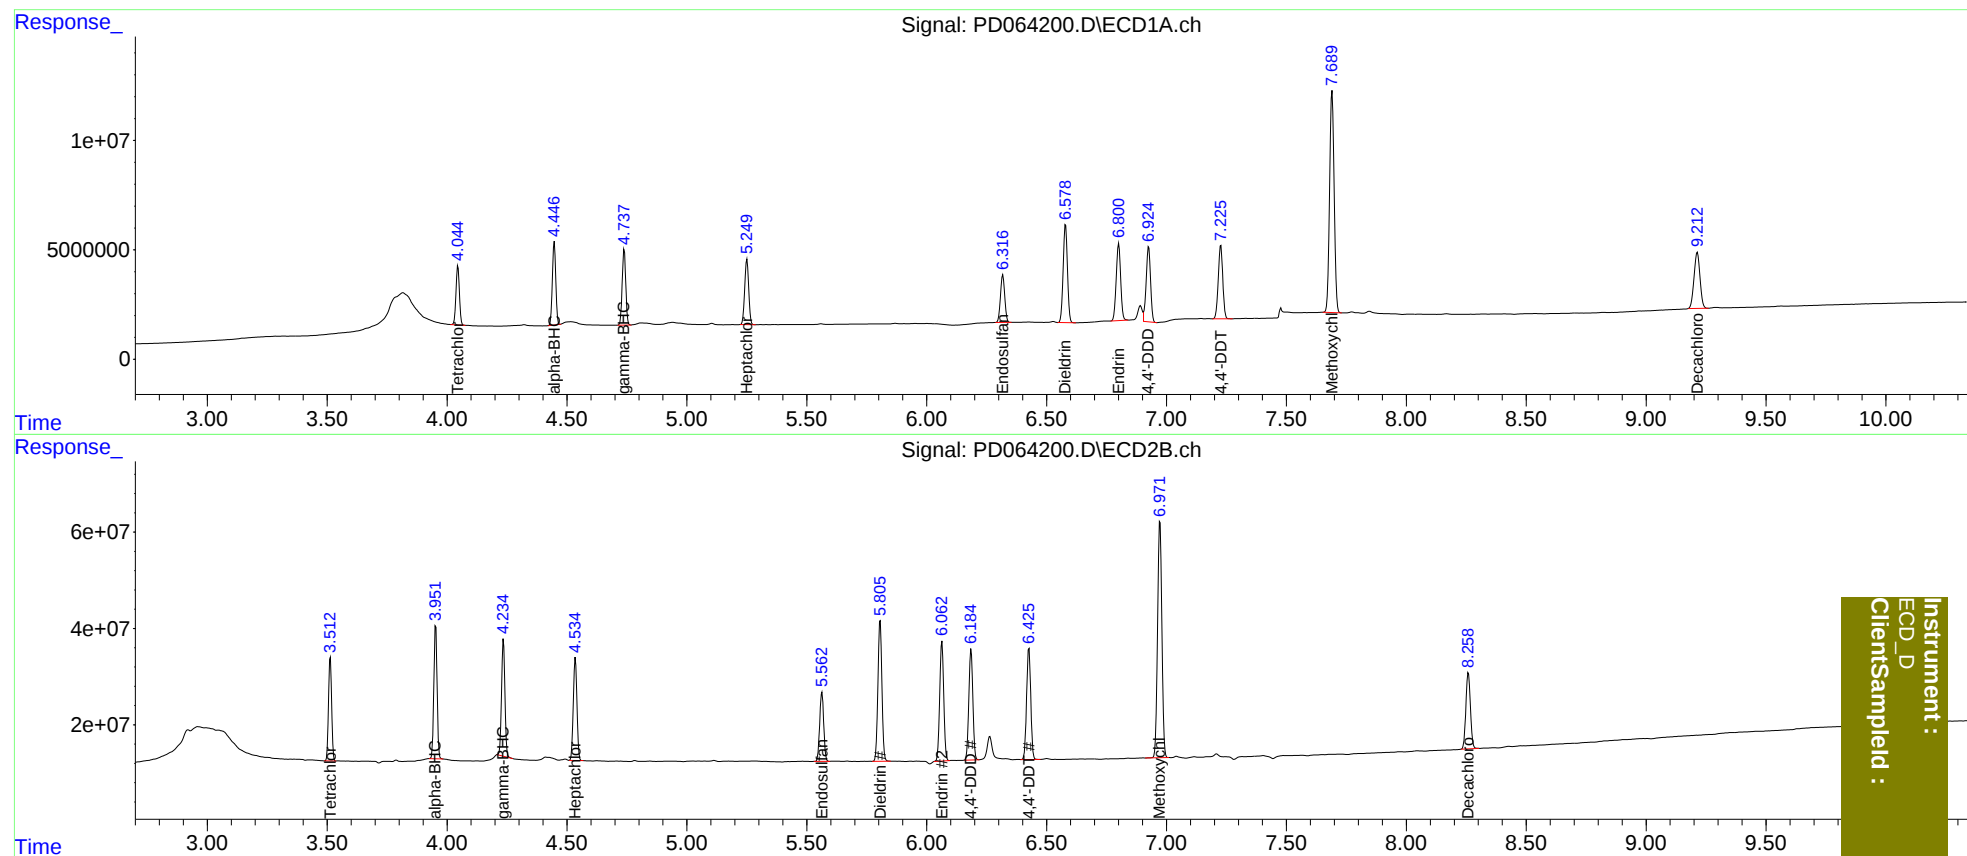


Instrument :
ECD_D
ClientSampled :

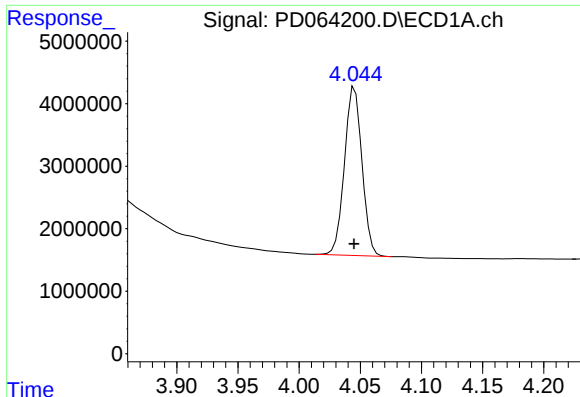

#1 Tetrachloro-m-xylene


R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 26798695
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

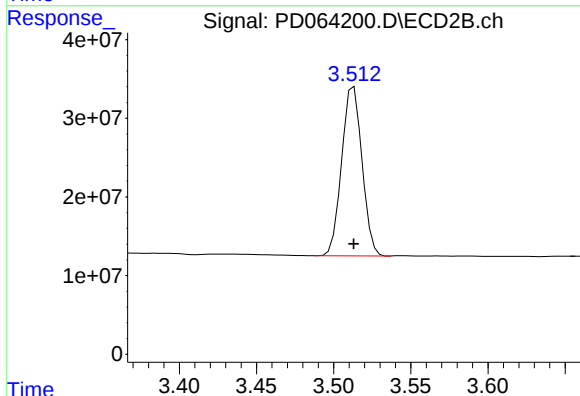


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 197129684
Conc: 20.00 ng/ml

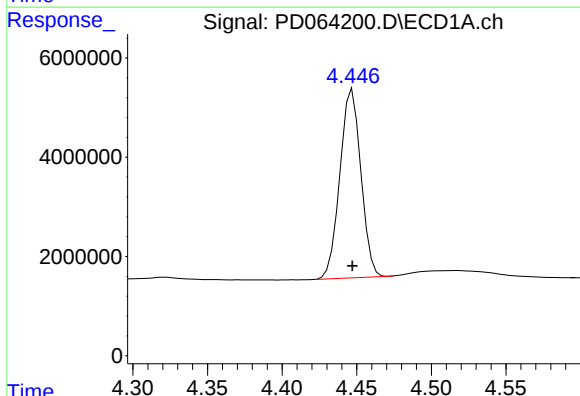


#2 alpha-BHC

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 37419002
Conc: 20.00 ng/ml

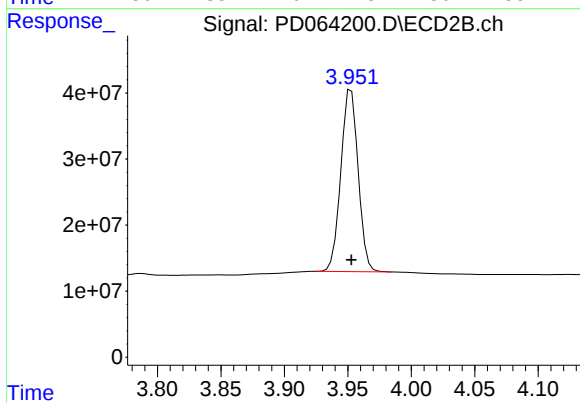

#2 alpha-BHC


R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 261999861
Conc: 20.00 ng/ml

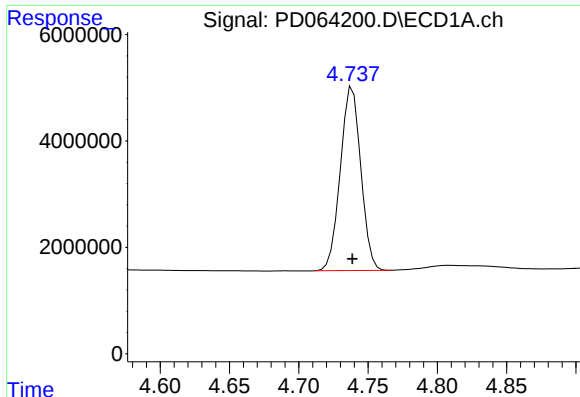

#3 gamma-BHC (Lindane)


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 35585353
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

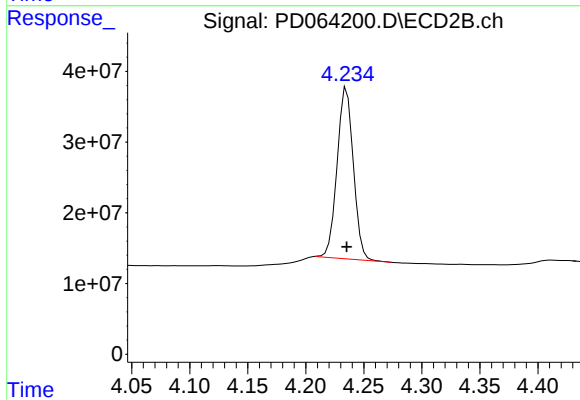


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 235390663
Conc: 20.00 ng/ml

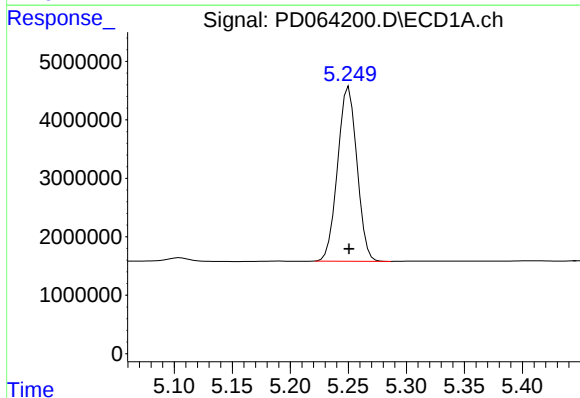


#4 Heptachlor

R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 34626788
Conc: 20.00 ng/ml

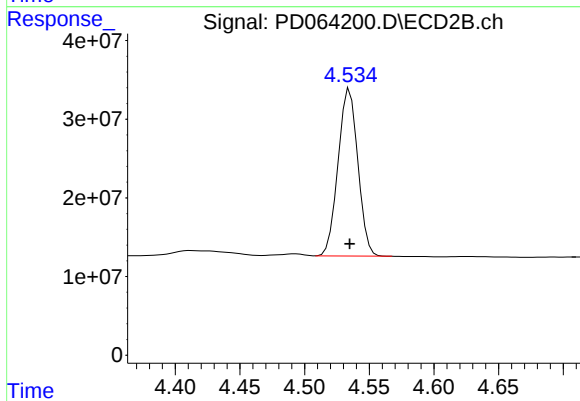

#4 Heptachlor


R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 225607743
Conc: 20.00 ng/ml

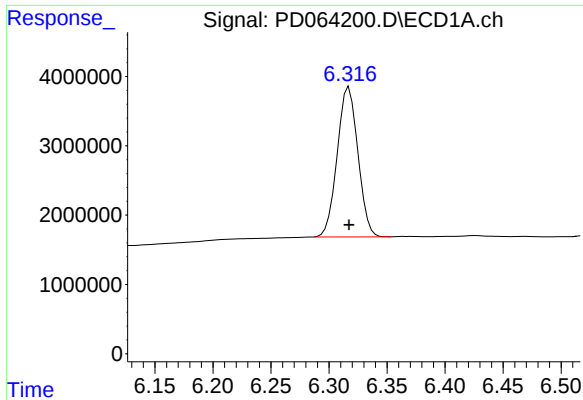

#9 Endosulfan I


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 26846376
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

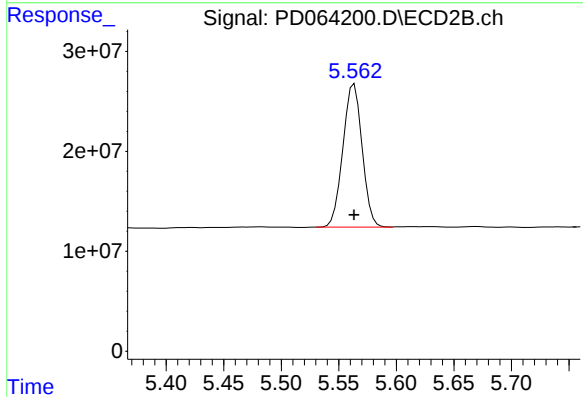


#9 Endosulfan I

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 167120385
Conc: 20.00 ng/ml

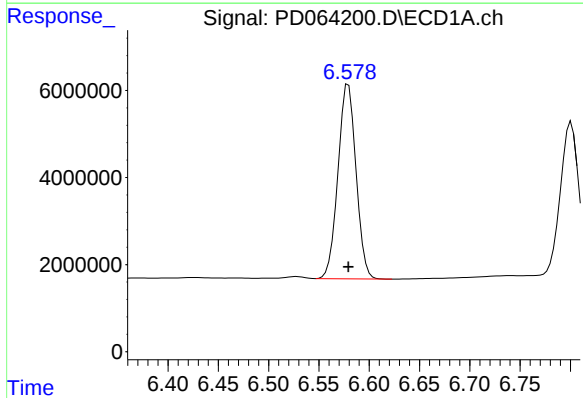


#13 Dieldrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 55783723
Conc: 40.00 ng/ml

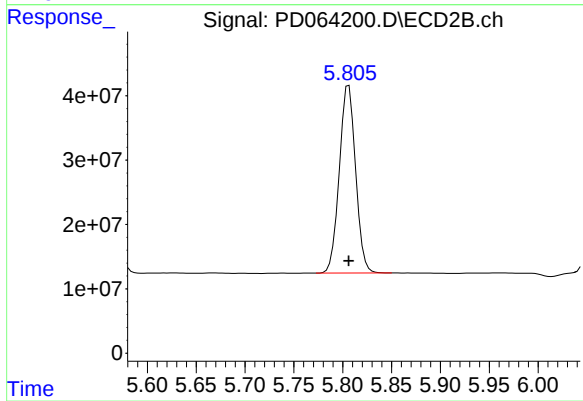

#13 Dieldrin


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 338649697
Conc: 40.00 ng/ml

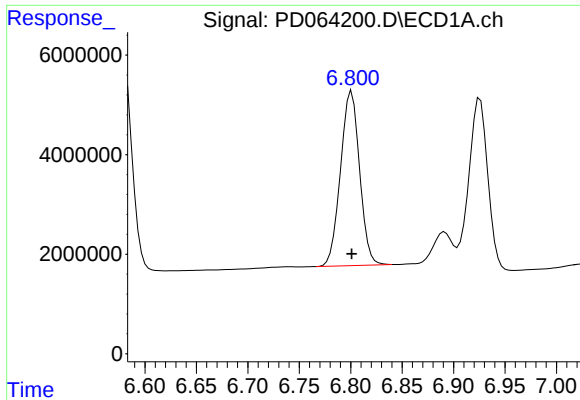

#14 Endrin


R.T.: 6.801 min
Delta R.T.: 0.000 min
Response: 45378532
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

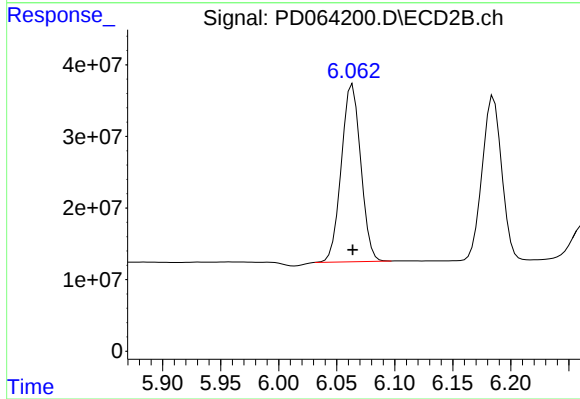


#14 Endrin

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 288626753
Conc: 40.00 ng/ml

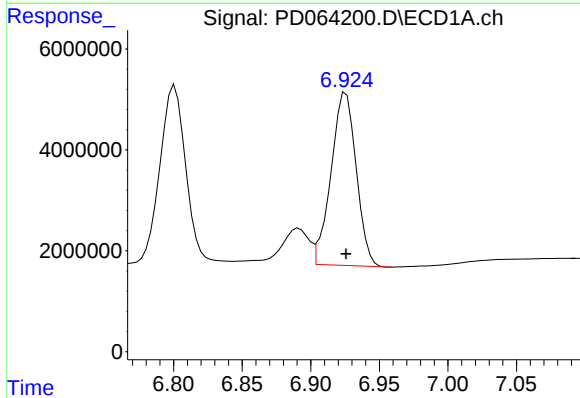


#16 4,4'-DDD

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 43802509
Conc: 40.00 ng/ml

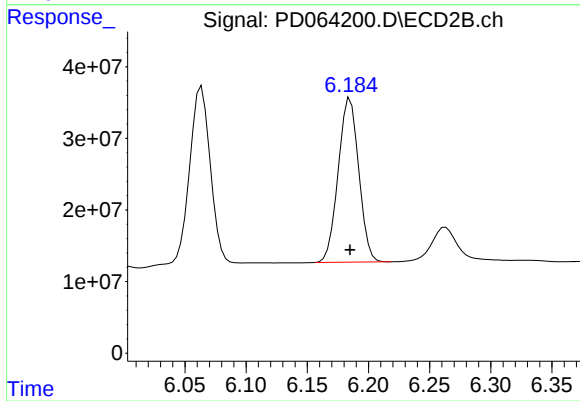

#16 4,4'-DDD


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 267972781
Conc: 40.00 ng/ml

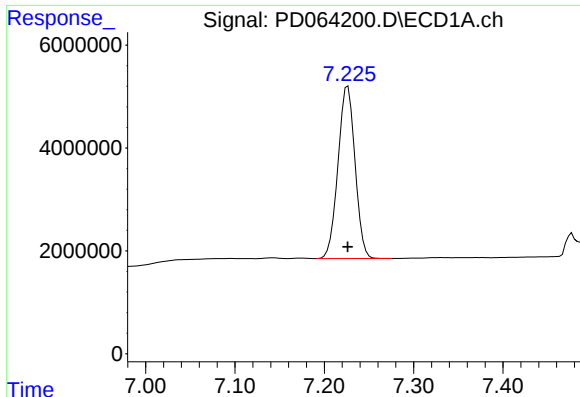

#17 4,4'-DDT


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 44324669
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

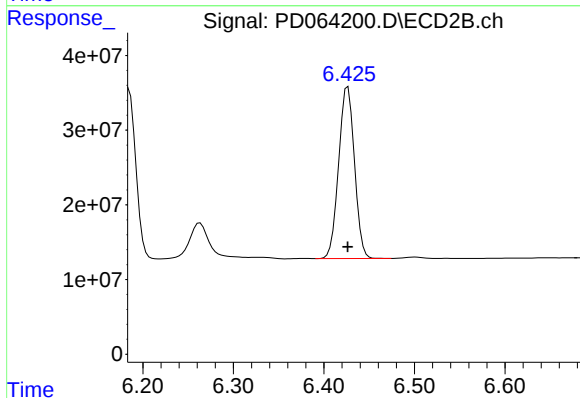


#17 4,4'-DDT

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 279176103
Conc: 40.00 ng/ml

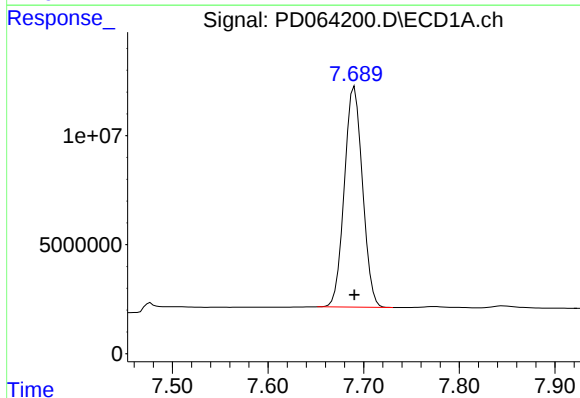


#20 Methoxychlor

R.T.: 7.690 min
Delta R.T.: 0.000 min
Response: 133866048
Conc: 200.00 ng/ml

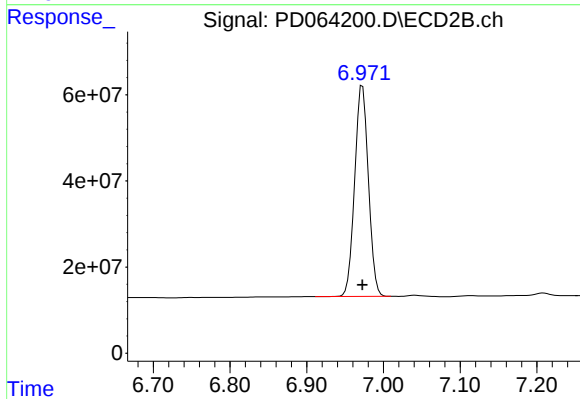

#20 Methoxychlor

R.T.: 6.973 min
Delta R.T.: 0.000 min
Response: 614448002
Conc: 200.00 ng/ml

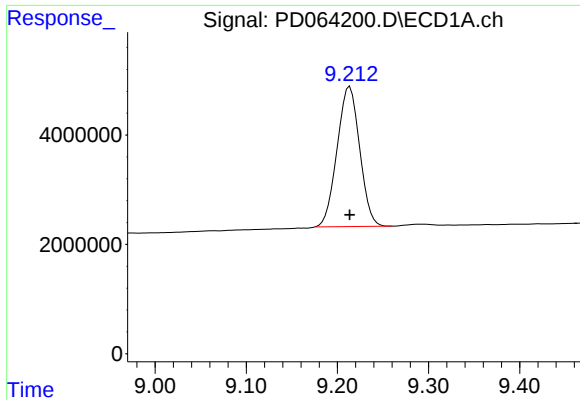

#27 Decachlorobiphenyl


R.T.: 9.214 min

Delta R.T.: 0.000 min

Response: 44082036

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

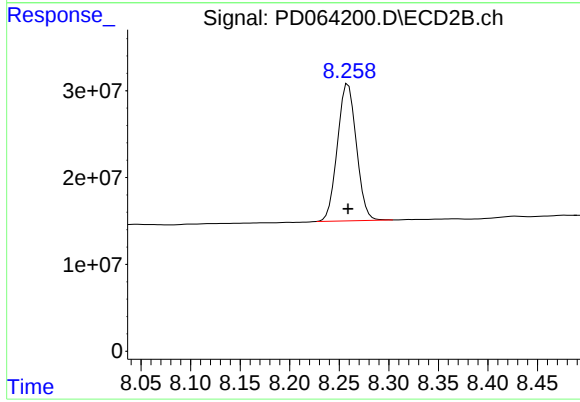

#27 Decachlorobiphenyl

R.T.: 8.259 min

Delta R.T.: 0.000 min

Response: 210546154

Conc: 40.00 ng/ml