

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 15:00
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:46:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 15:45:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.045	3.513	52276057	364.6E6	39.014	36.995
27)	SA Decachlor...	9.211	8.258	81486640	395.2E6	73.941	75.082
Target Compounds							
2)	A alpha-BHC	4.447	3.953	75922331	492.9E6	40.580	37.626
3)	MA gamma-BHC...	4.738	4.235	70119416	440.1E6	39.409	37.391
4)	MA Heptachlor	5.250	4.535	67176095	419.6E6	38.800	37.199
9)	A Endosulfan I	6.317	5.563	52106798	316.6E6	38.818	37.894
13)	MA Dieldrin	6.579	5.806	112.0E6	647.2E6	80.288	76.449
14)	MA Endrin	6.800	6.064	90766446	547.6E6	80.008	75.897
16)	A 4,4'-DDD	6.925	6.185	88153025	512.4E6	80.500	76.486
17)	MA 4,4'-DDT	7.226	6.426	89658122	538.0E6	80.910	77.086
20)	A Methoxychlor	7.690	6.972	228.6E6	1124.6E6	341.472	366.064


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 15:00
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:46:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 15:45:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

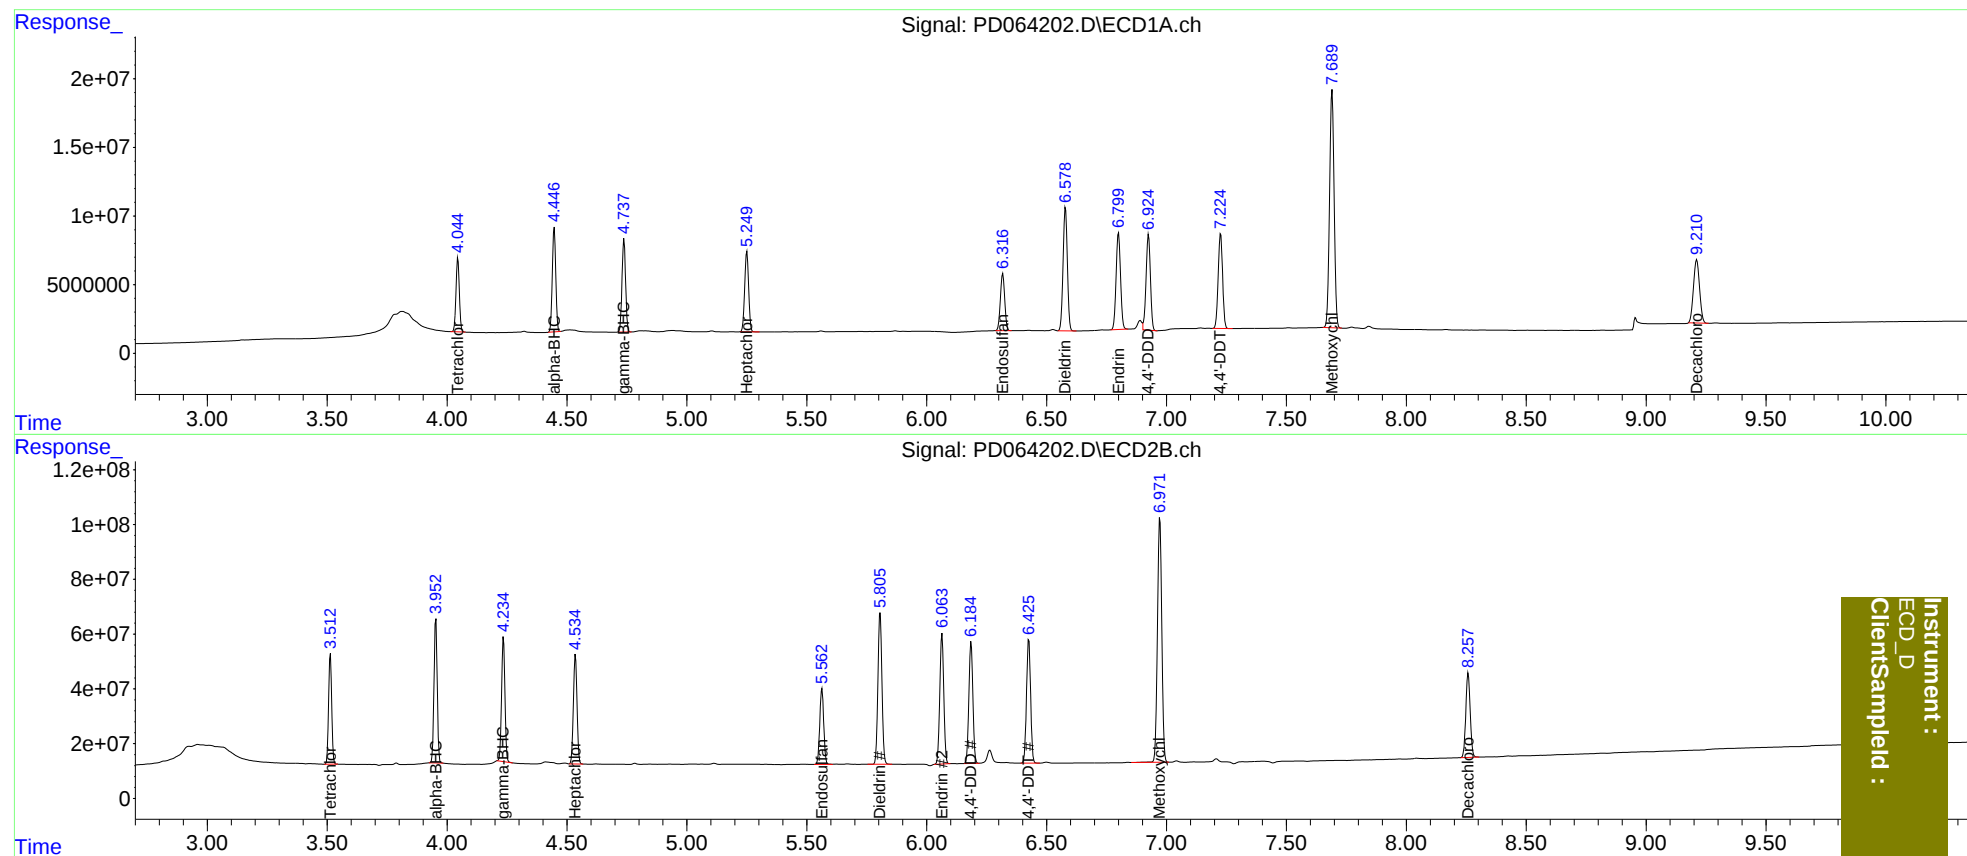


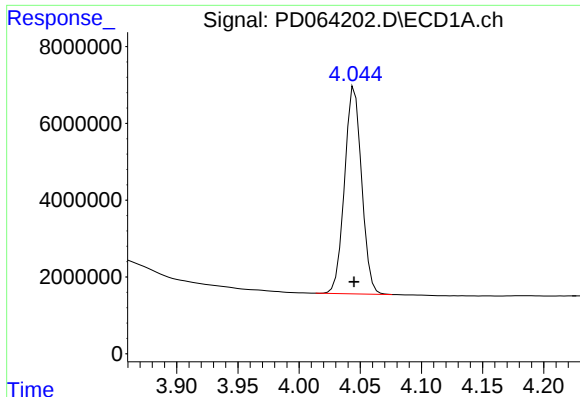

#1 Tetrachloro-m-xylene


R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 52276057
Conc: 39.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

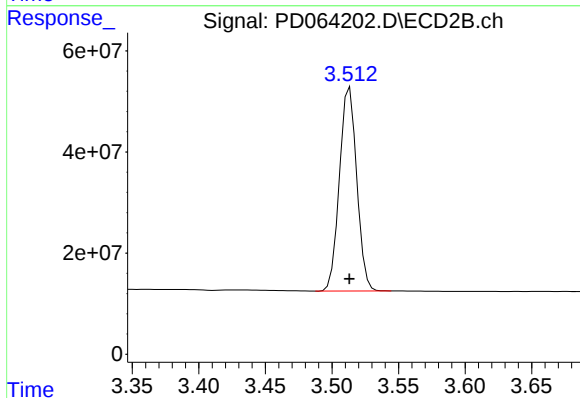


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 364641716
Conc: 37.00 ng/ml

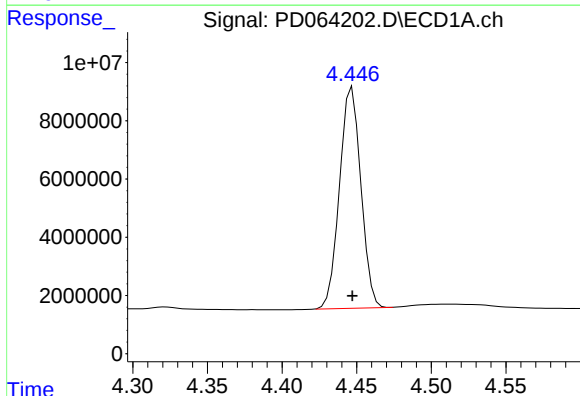


#2 alpha-BHC

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 75922331
Conc: 40.58 ng/ml

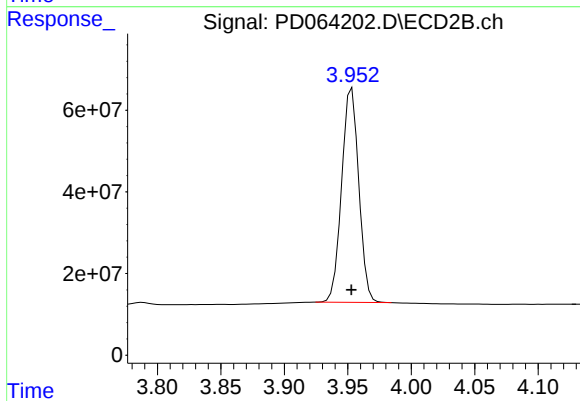

#2 alpha-BHC


R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 492900485
Conc: 37.63 ng/ml

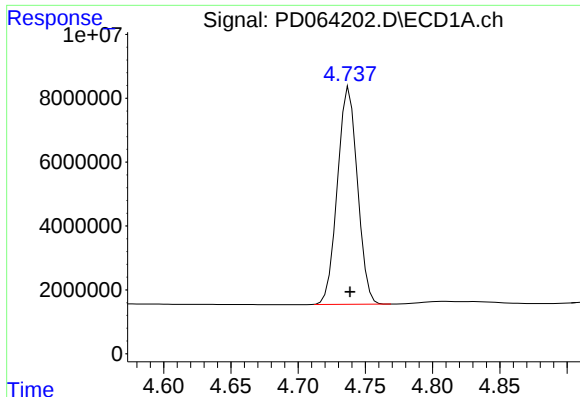

#3 gamma-BHC (Lindane)


R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 70119416
Conc: 39.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

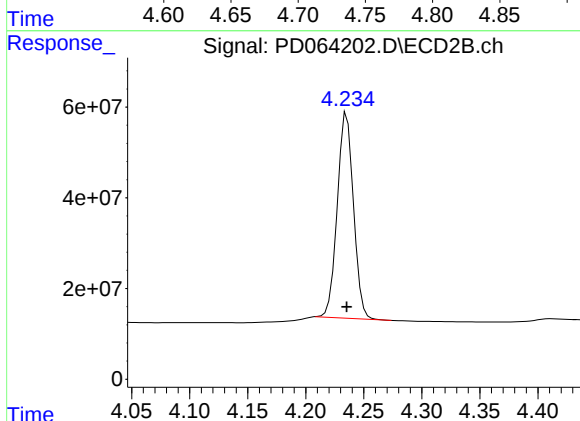


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 440077512
Conc: 37.39 ng/ml

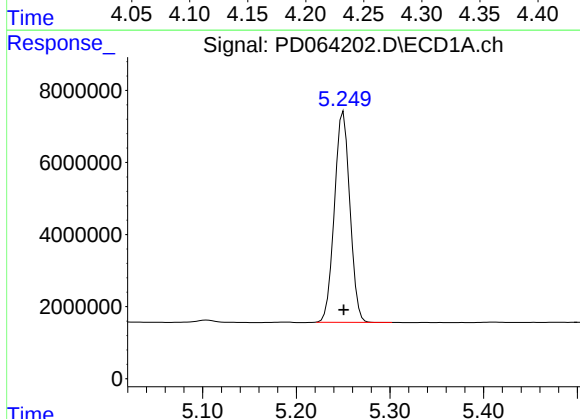


#4 Heptachlor

R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 67176095
Conc: 38.80 ng/ml

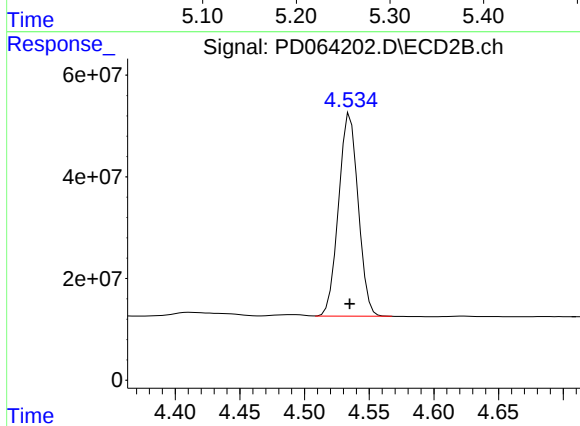

#4 Heptachlor


R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 419619191
Conc: 37.20 ng/ml

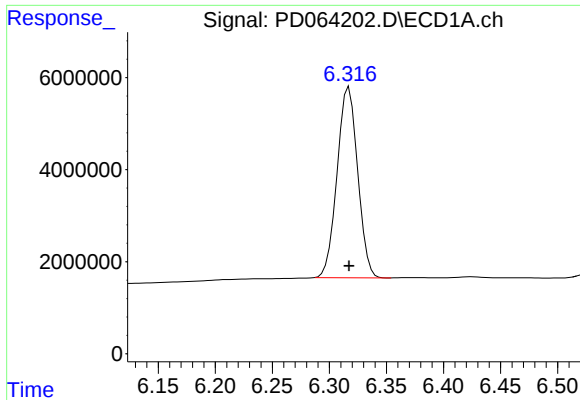

#9 Endosulfan I


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 52106798
Conc: 38.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

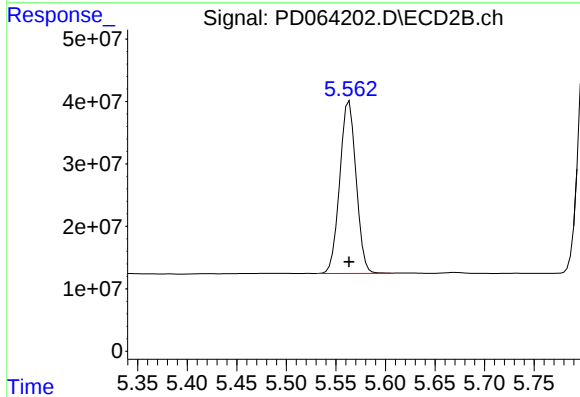


#9 Endosulfan I

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 316642632
Conc: 37.89 ng/ml

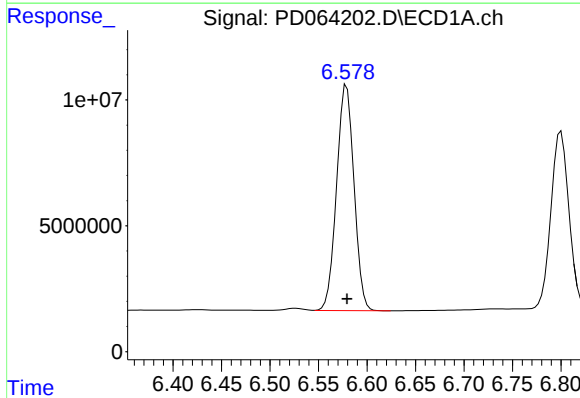


#13 Dieldrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 111968933
Conc: 80.29 ng/ml

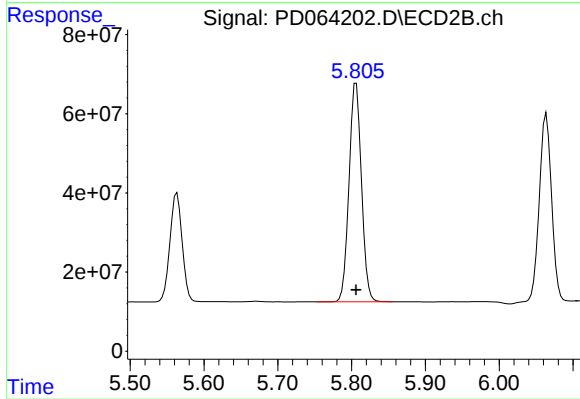

#13 Dieldrin


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 647239208
Conc: 76.45 ng/ml

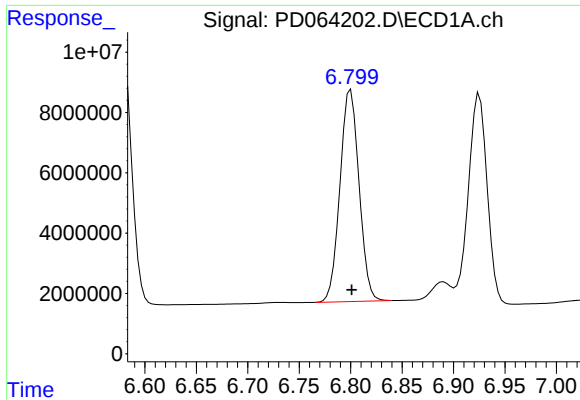

#14 Endrin


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 90766446
Conc: 80.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

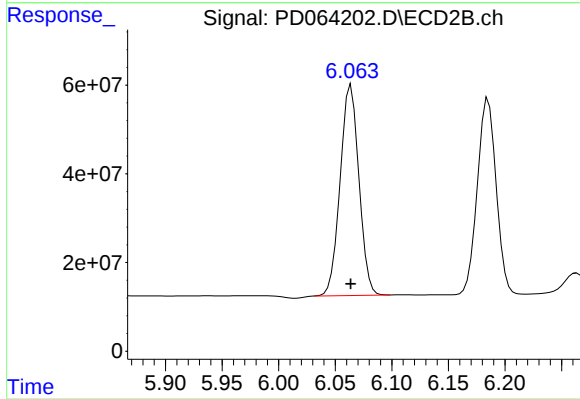


#14 Endrin

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 547646256
Conc: 75.90 ng/ml

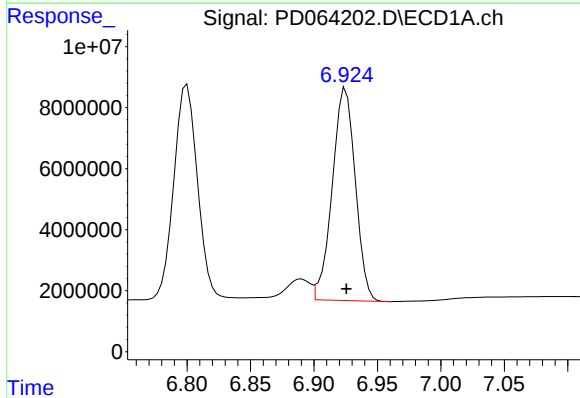


#16 4,4'-DDD

R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 88153025
Conc: 80.50 ng/ml

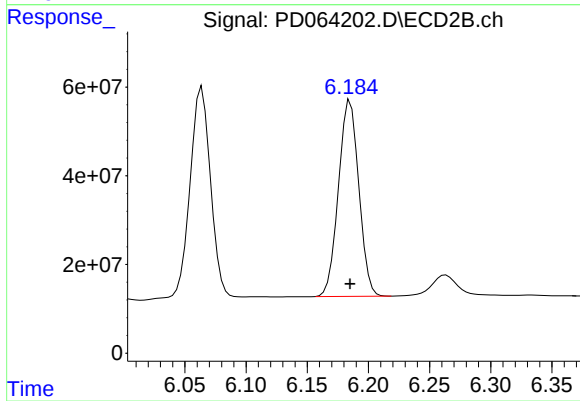

#16 4,4'-DDD


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 512402775
Conc: 76.49 ng/ml

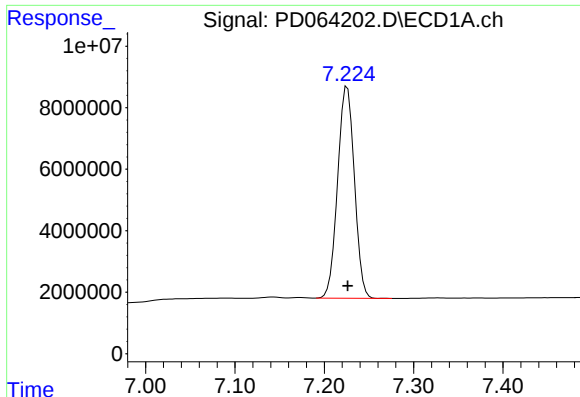

#17 4,4'-DDT


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 89658122
Conc: 80.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

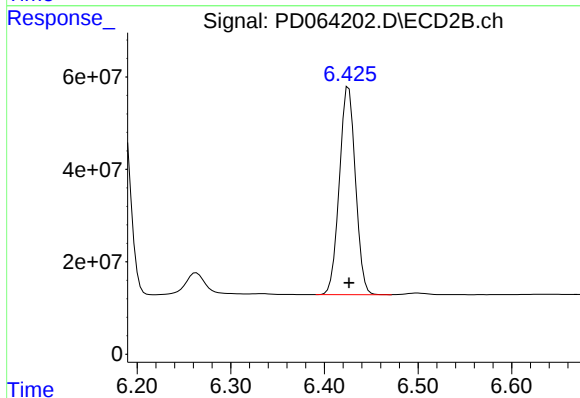


#17 4,4'-DDT

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 538014274
Conc: 77.09 ng/ml

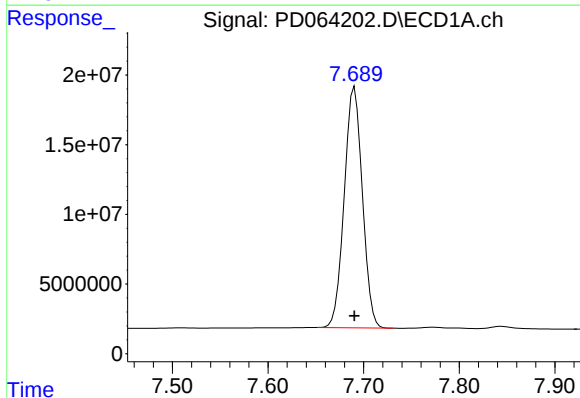


#20 Methoxychlor

R.T.: 7.690 min
Delta R.T.: 0.000 min
Response: 228557306
Conc: 341.47 ng/ml

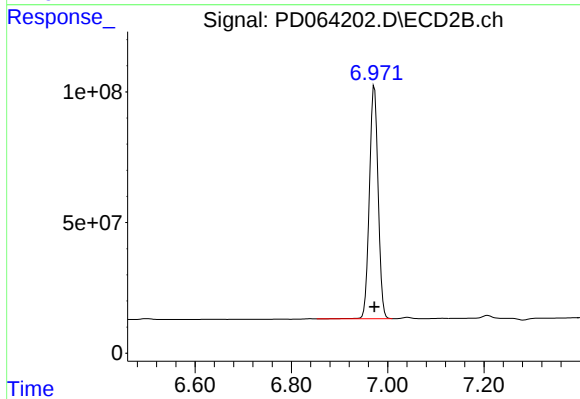

#20 Methoxychlor


R.T.: 6.972 min
Delta R.T.: 0.000 min
Response: 1124636997
Conc: 366.06 ng/ml

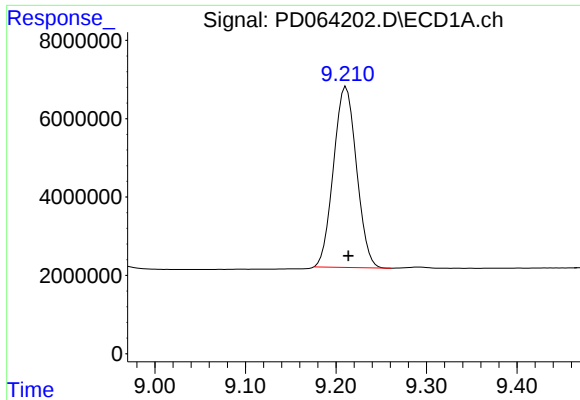

#27 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.002 min
Response: 81486640
Conc: 73.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

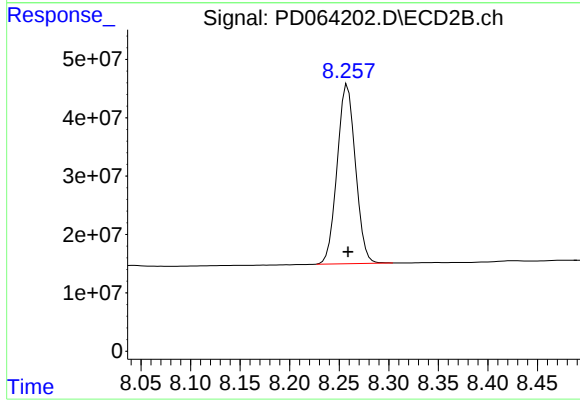

#27 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 395207565
Conc: 75.08 ng/ml