

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 15:14
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 16:11:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 16:10:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.046	3.513	49262083	349.9E6	37.782	36.420
27)	SA Decachlor...	9.212	8.259	78989242	393.3E6	73.156	74.708
Target Compounds							
5)	MB Aldrin	5.561	4.783	59121575	389.2E6	36.993	37.811
6)	B beta-BHC	4.918	4.481	30346641	199.7E6	36.145	36.676
7)	B delta-BHC	5.137	4.686	65257607	410.7E6	38.365	37.927
8)	B Heptachlo...	5.955	5.225	54863341	339.3E6	33.761	37.399
10)	B trans-Chl...	6.192	5.450	56093428	348.1E6	33.548	37.466
11)	B cis-Chlor...	6.265	5.509	54772909	336.8E6	33.421	37.440
12)	B 4,4'-DDE	6.426	5.671	103.7E6	632.2E6	69.615	75.394
15)	B Endosulfa...	7.016	6.335	87126956	491.1E6	68.778	74.852
18)	B Endrin al...	7.142	6.503	74086428	416.9E6	68.862	73.948
19)	B Endosulfa...	7.366	6.715	88110427	460.0E6	68.598	74.037
21)	B Endrin ke...	7.845	7.209	97445754	511.3E6	70.674	74.616

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 15:14
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 16:11:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 16:10:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

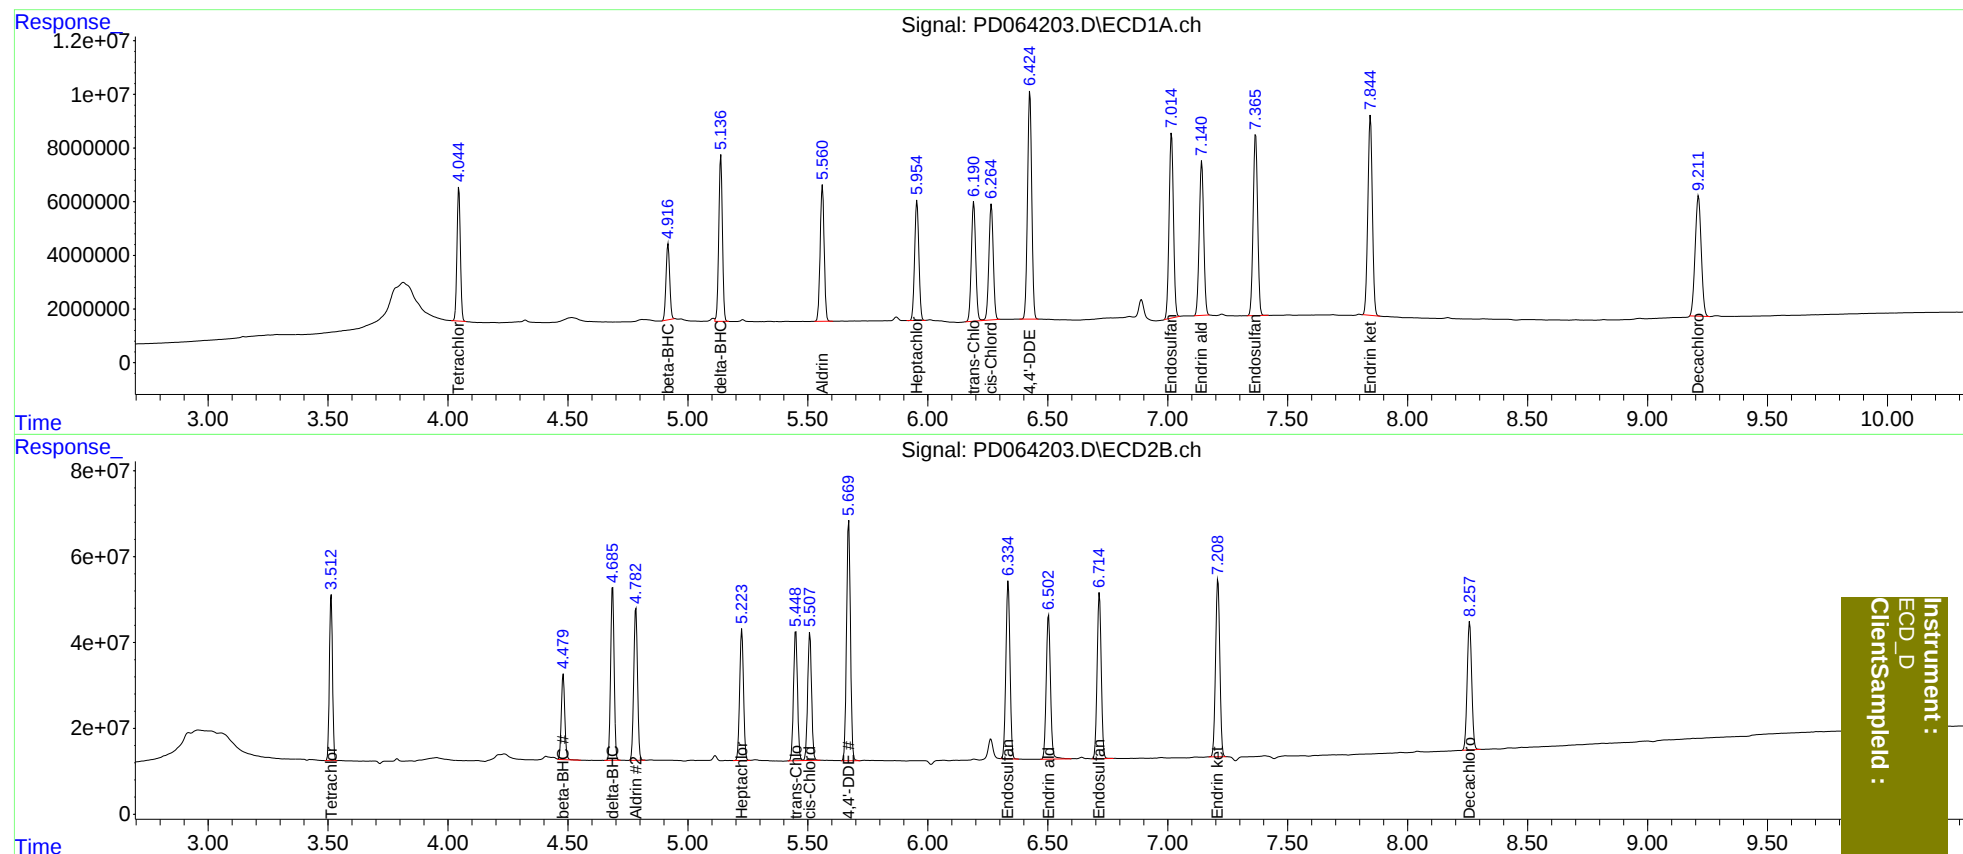


Instrument :
ECD_D
ClientSampled :

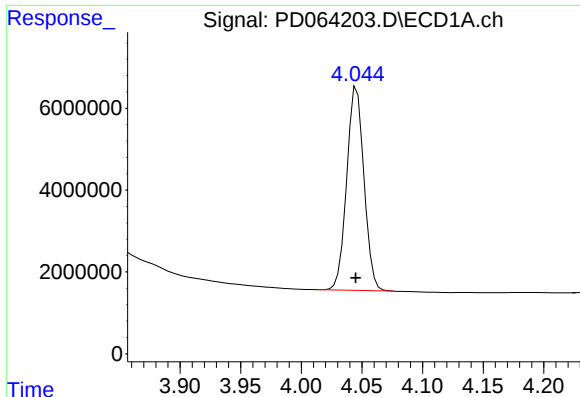

#1 Tetrachloro-m-xylene


R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 49262083
Conc: 37.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

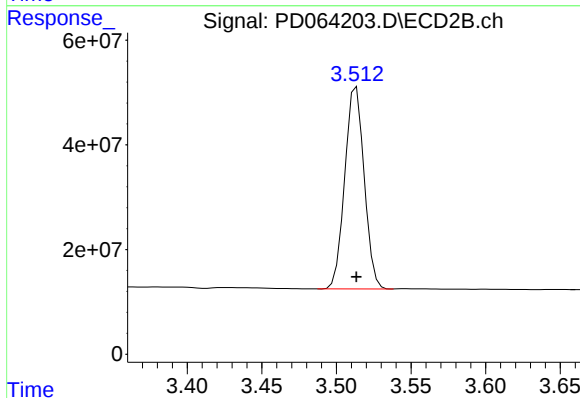


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 349936694
Conc: 36.42 ng/ml

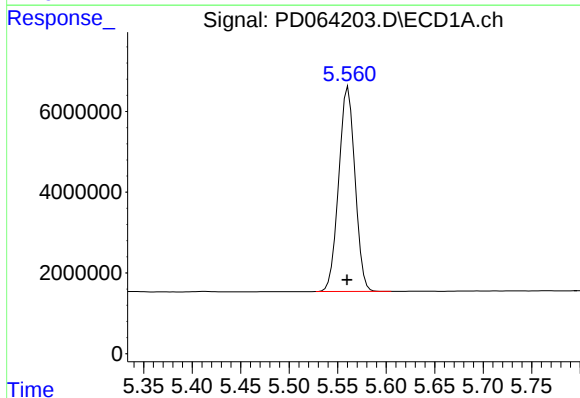


#5 Aldrin

R.T.: 5.561 min
Delta R.T.: 0.001 min
Response: 59121575
Conc: 36.99 ng/ml

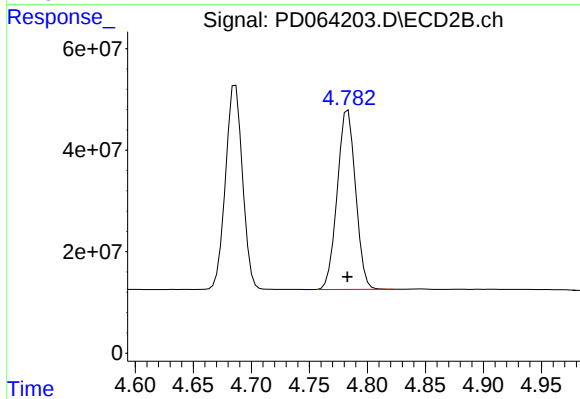

#5 Aldrin


R.T.: 4.783 min
Delta R.T.: 0.000 min
Response: 389234027
Conc: 37.81 ng/ml

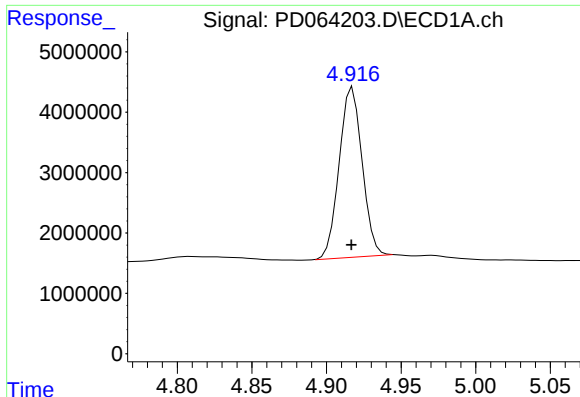

#6 beta-BHC


R.T.: 4.918 min
Delta R.T.: 0.000 min
Response: 30346641
Conc: 36.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

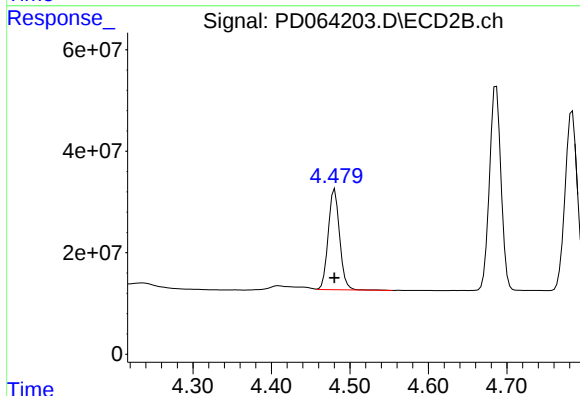


#6 beta-BHC

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 199719137
Conc: 36.68 ng/ml

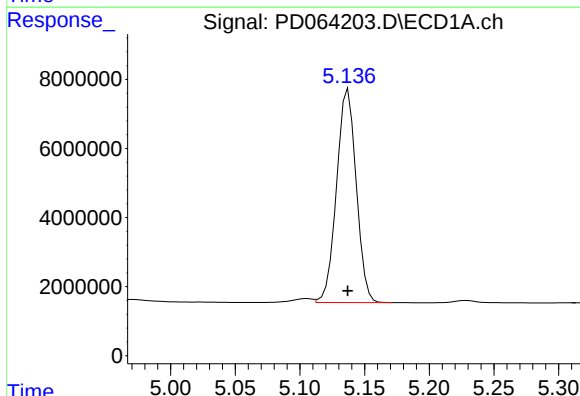


#7 delta-BHC

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 65257607
Conc: 38.37 ng/ml

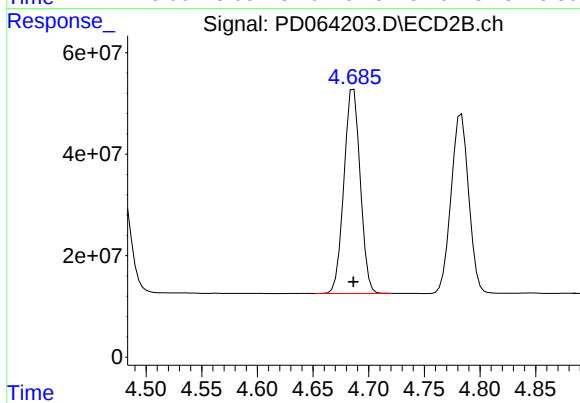

#7 delta-BHC


R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 410664165
Conc: 37.93 ng/ml

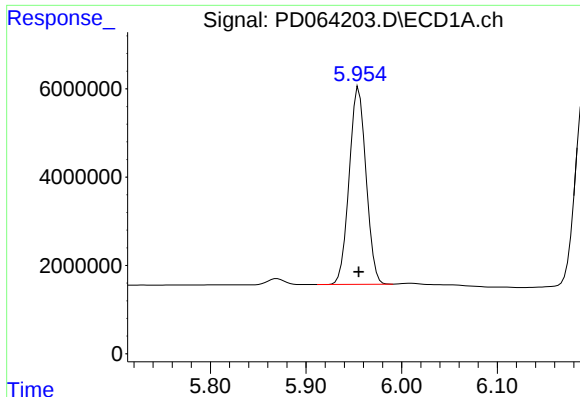

#8 Heptachlor epoxide


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 54863341
Conc: 33.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

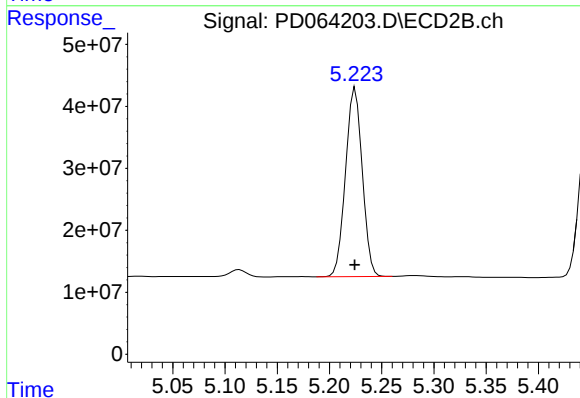


#8 Heptachlor epoxide

R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 339293241
Conc: 37.40 ng/ml

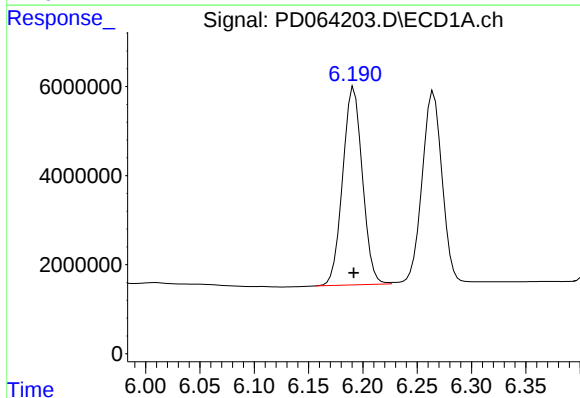


#10 trans-Chlordane

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 56093428
Conc: 33.55 ng/ml

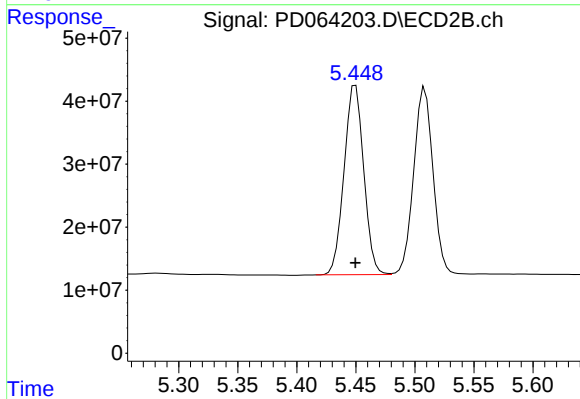

#10 trans-Chlordane


R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 348099562
Conc: 37.47 ng/ml

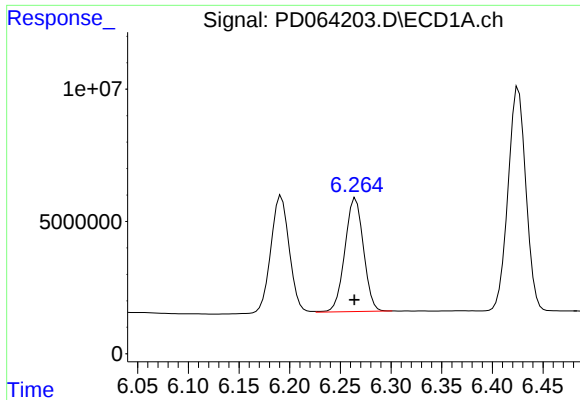

#11 cis-Chlordane


R.T.: 6.265 min
Delta R.T.: 0.001 min
Response: 54772909
Conc: 33.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

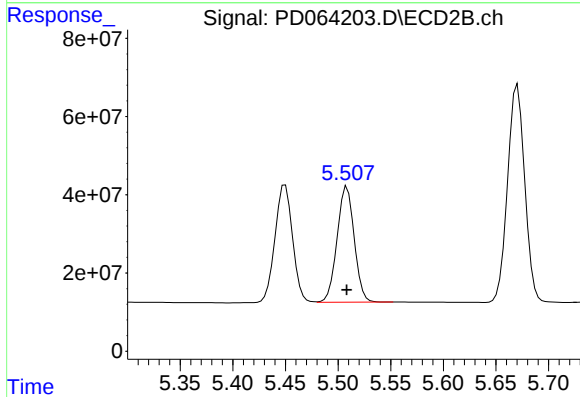


#11 cis-Chlordane

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 336783769
Conc: 37.44 ng/ml

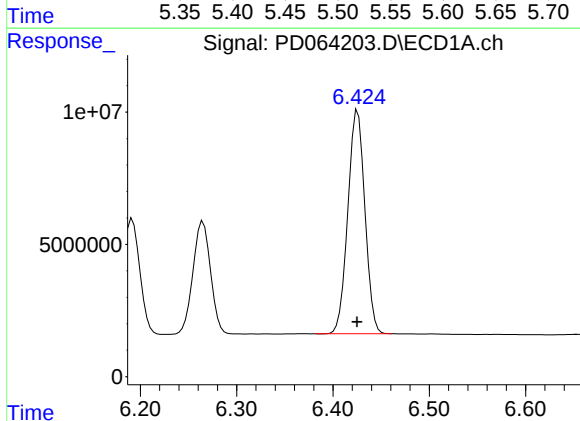


#12 4,4'-DDE

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 103683998
Conc: 69.62 ng/ml

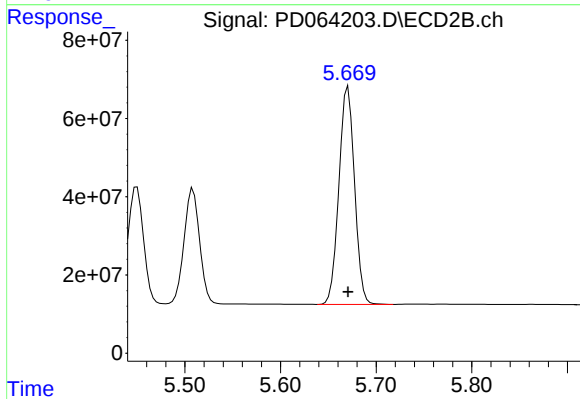

#12 4,4'-DDE


R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 632245229
Conc: 75.39 ng/ml

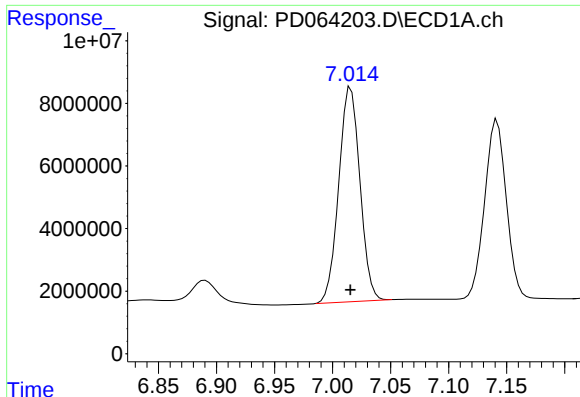

#15 Endosulfan II


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 87126956
Conc: 68.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

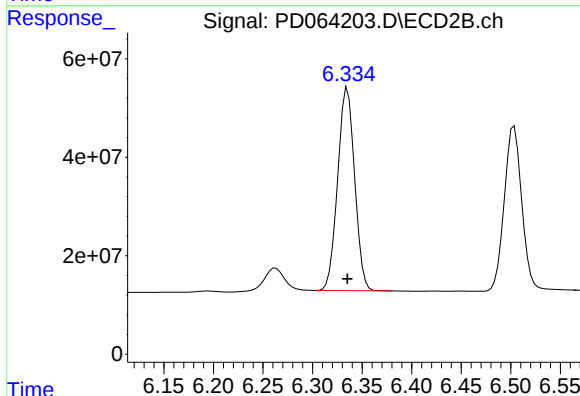


#15 Endosulfan II

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 491101127
Conc: 74.85 ng/ml

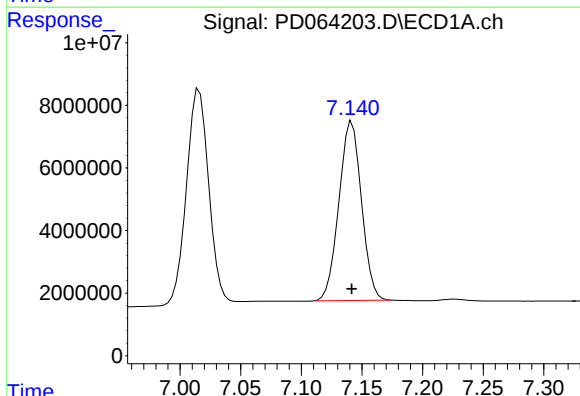


#18 Endrin aldehyde

R.T.: 7.142 min
Delta R.T.: 0.000 min
Response: 74086428
Conc: 68.86 ng/ml

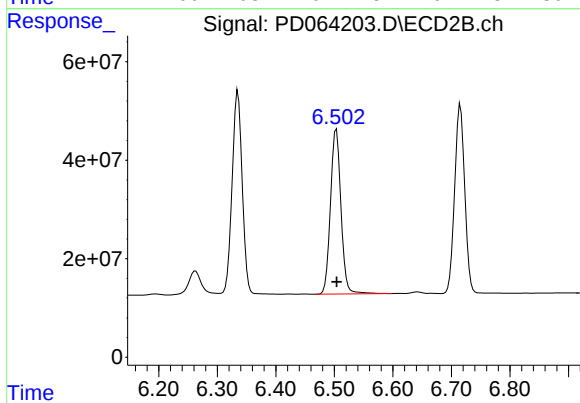

#18 Endrin aldehyde


R.T.: 6.503 min
Delta R.T.: 0.000 min
Response: 416935604
Conc: 73.95 ng/ml

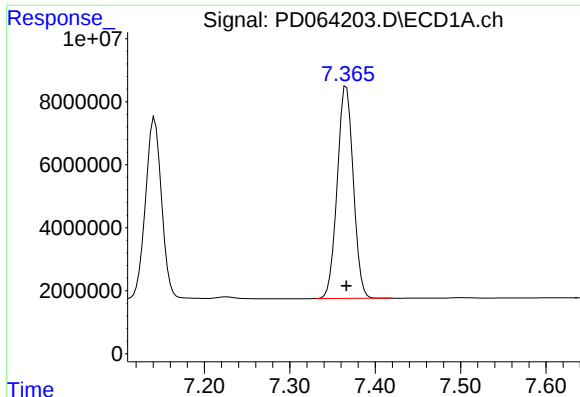

#19 Endosulfan Sulfate


R.T.: 7.366 min
Delta R.T.: 0.000 min
Response: 88110427
Conc: 68.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

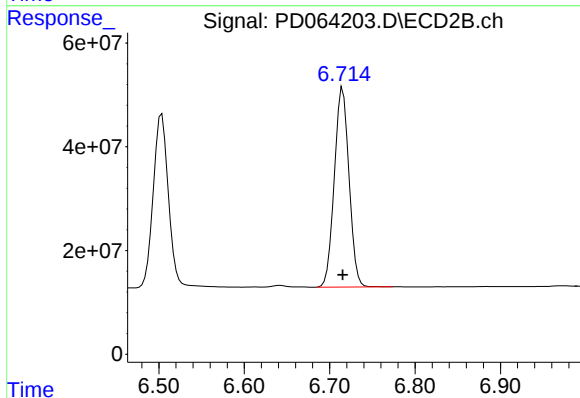


#19 Endosulfan Sulfate

R.T.: 6.715 min
Delta R.T.: 0.000 min
Response: 460012442
Conc: 74.04 ng/ml

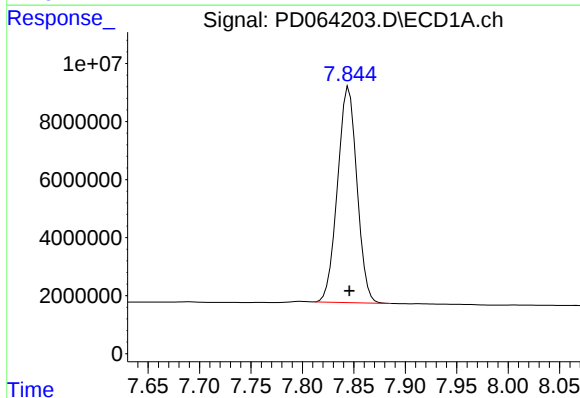


#21 Endrin ketone

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 97445754
Conc: 70.67 ng/ml

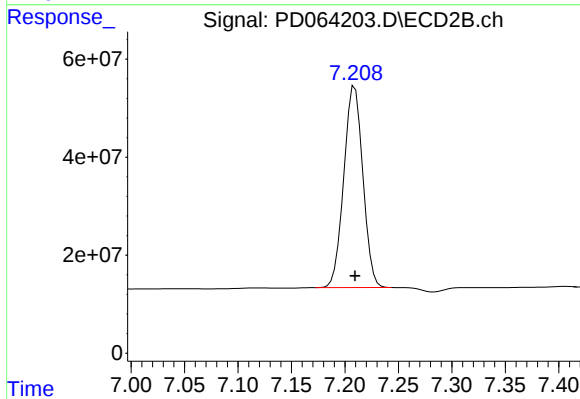

#21 Endrin ketone


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 511287974
Conc: 74.62 ng/ml

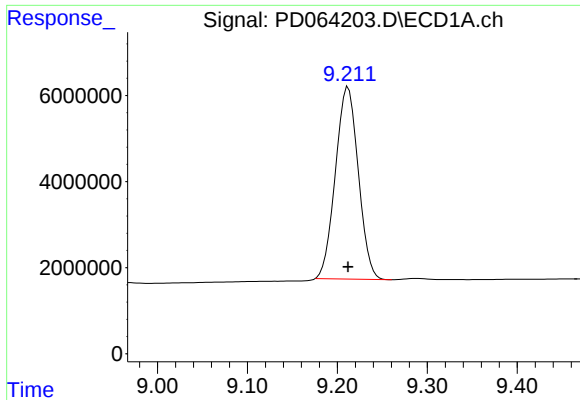

#27 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: 0.000 min
Response: 78989242
Conc: 73.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

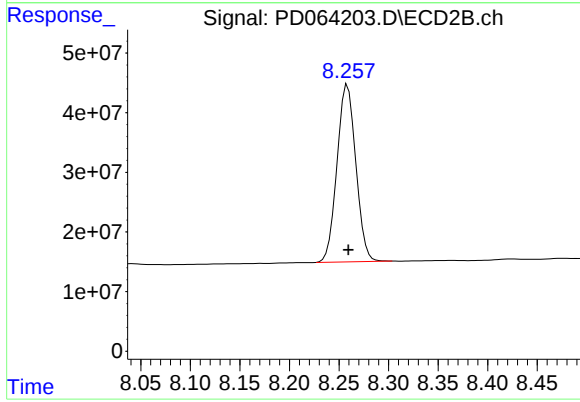

#27 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 393272833
Conc: 74.71 ng/ml