

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 15:27
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:46:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 15:45:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.046	3.513	94038452	666.1E6	70.181	67.576
27)	SA Decachlor...	9.212	8.259	149.8E6	737.2E6	135.939	140.056
Target Compounds							
2)	A alpha-BHC	4.447	3.953	140.7E6	920.9E6	75.218	70.296
3)	MA gamma-BHC...	4.739	4.235	129.6E6	824.2E6	72.866	70.027
4)	MA Heptachlor	5.251	4.535	122.7E6	784.6E6	70.844	69.553
9)	A Endosulfan I	6.318	5.563	98138975	587.9E6	73.112	70.358
13)	MA Dieldrin	6.580	5.806	218.7E6	1218.3E6	156.848	143.902
14)	MA Endrin	6.801	6.064	177.3E6	1021.7E6	156.290	141.600
16)	A 4,4'-DDD	6.926	6.185	172.5E6	971.4E6	157.500	144.999
17)	MA 4,4'-DDT	7.226	6.426	177.6E6	1025.4E6	160.238	146.923
20)	A Methoxychlor	7.691	6.973	444.0E6	2003.8E6	663.297	652.218


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 15:27
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:46:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 15:45:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

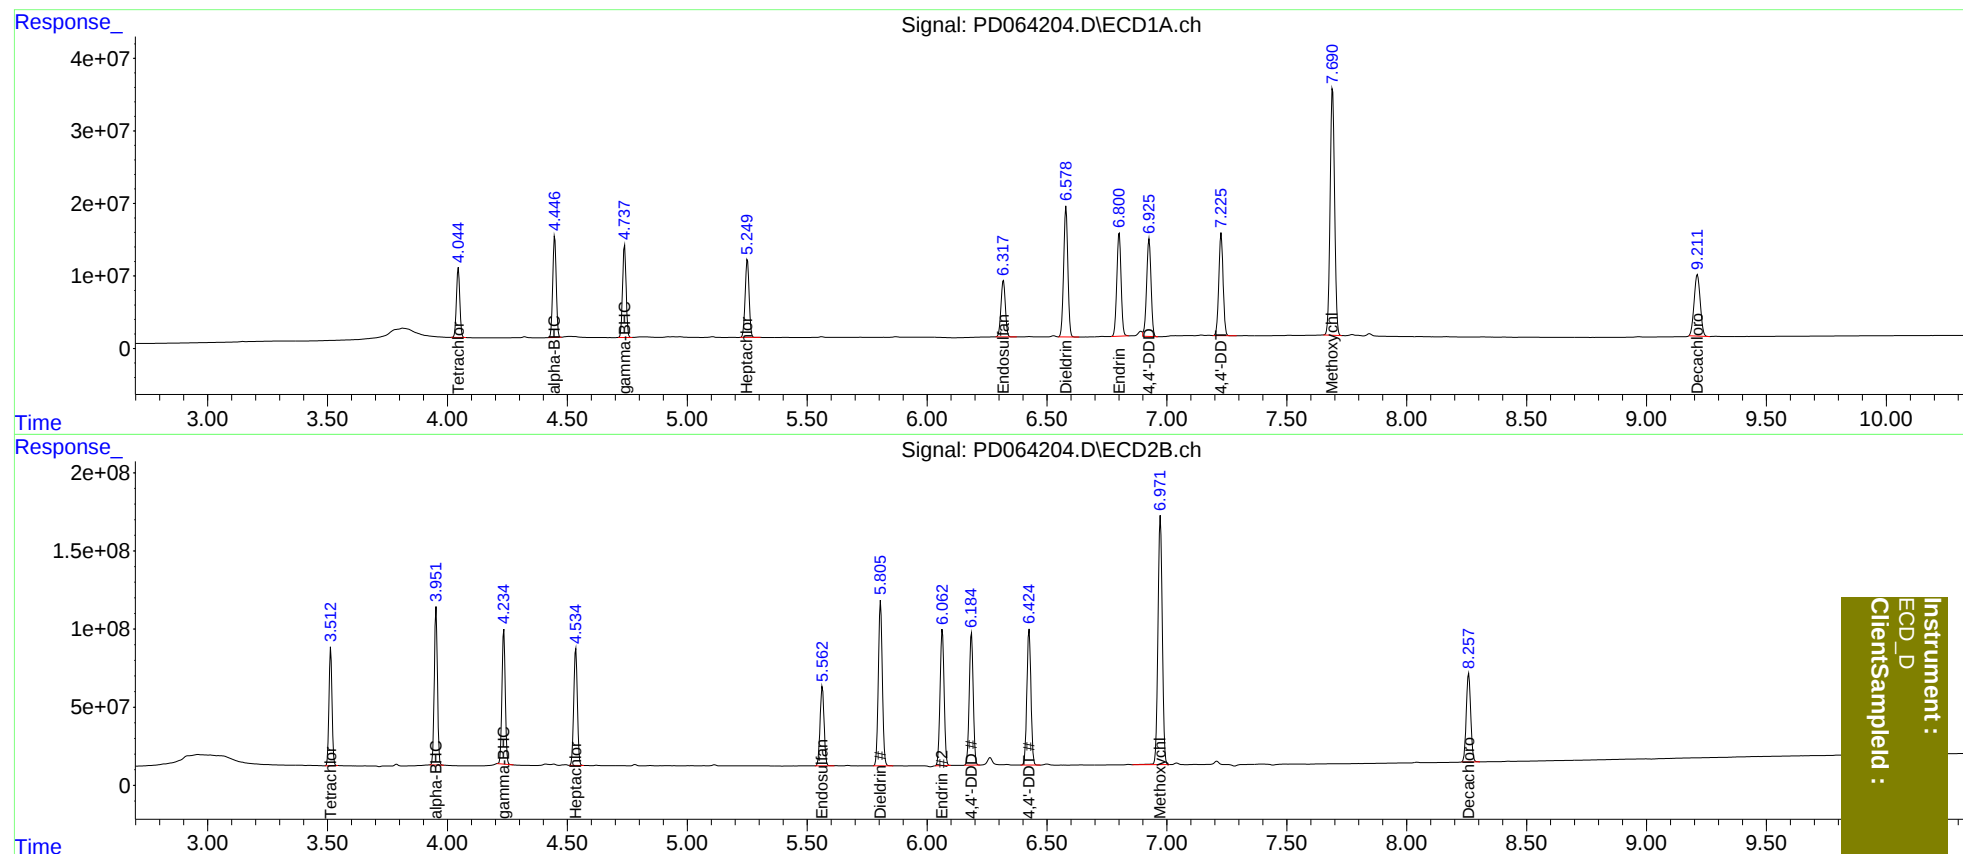


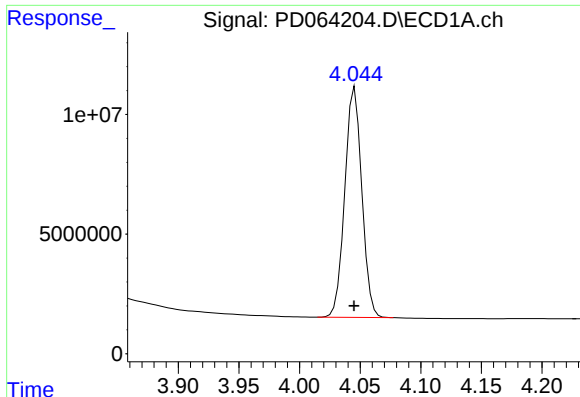

#1 Tetrachloro-m-xylene


R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 94038452
Conc: 70.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

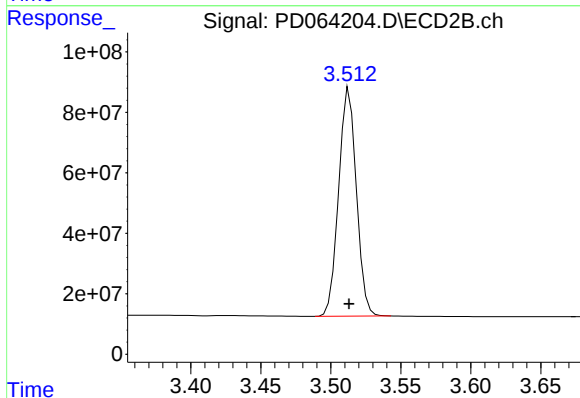


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 666057492
Conc: 67.58 ng/ml

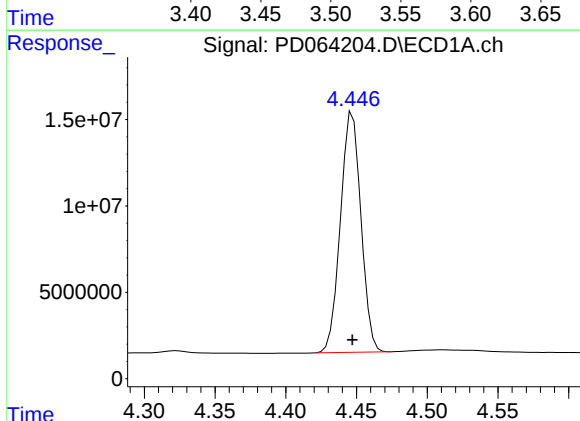


#2 alpha-BHC

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 140728540
Conc: 75.22 ng/ml

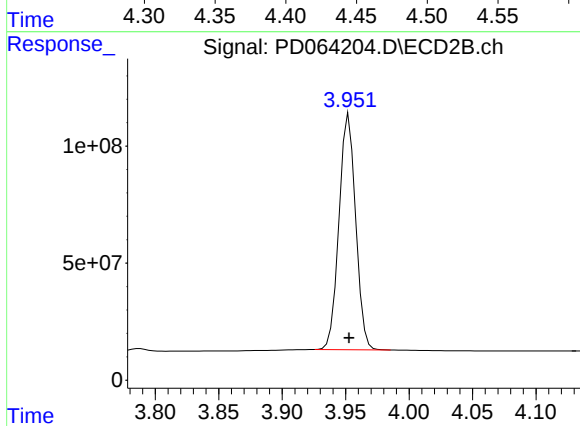

#2 alpha-BHC


R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 920874256
Conc: 70.30 ng/ml

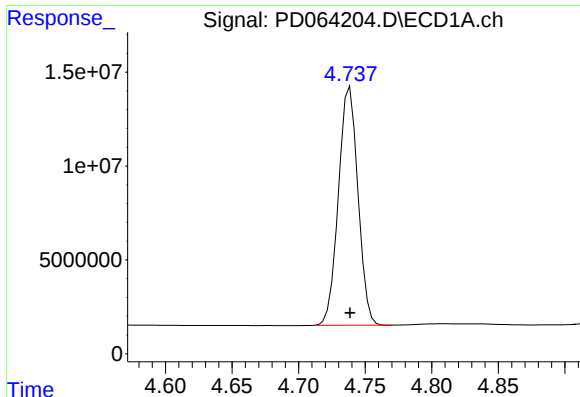

#3 gamma-BHC (Lindane)


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 129647685
Conc: 72.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

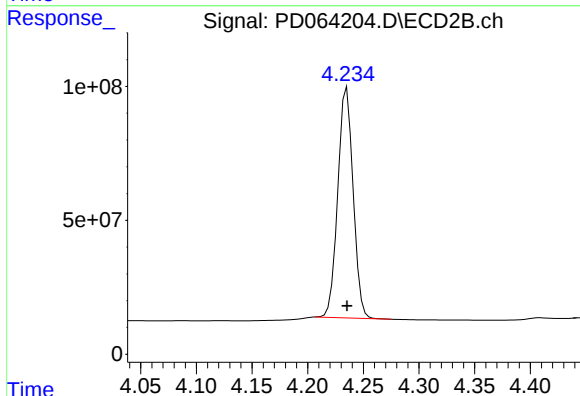


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 824181622
Conc: 70.03 ng/ml

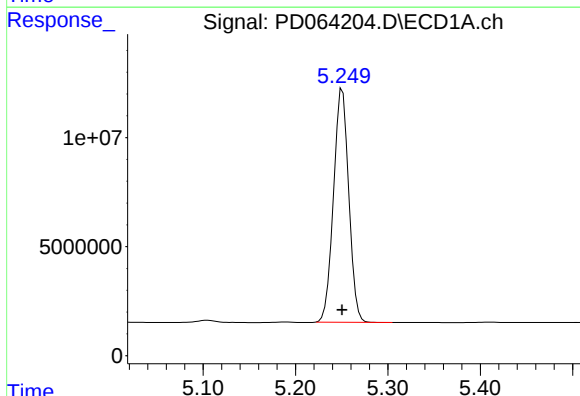


#4 Heptachlor

R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 122655277
Conc: 70.84 ng/ml

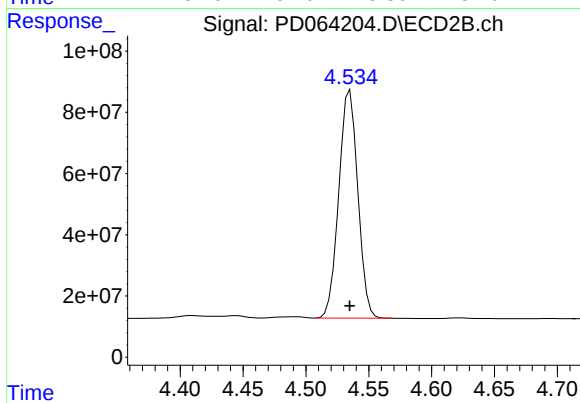

#4 Heptachlor


R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 784579522
Conc: 69.55 ng/ml

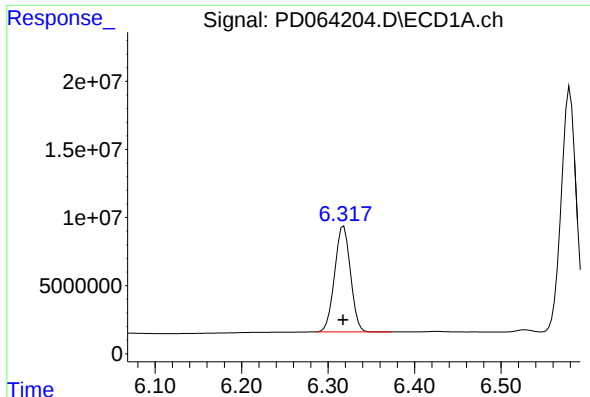

#9 Endosulfan I


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 98138975
Conc: 73.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

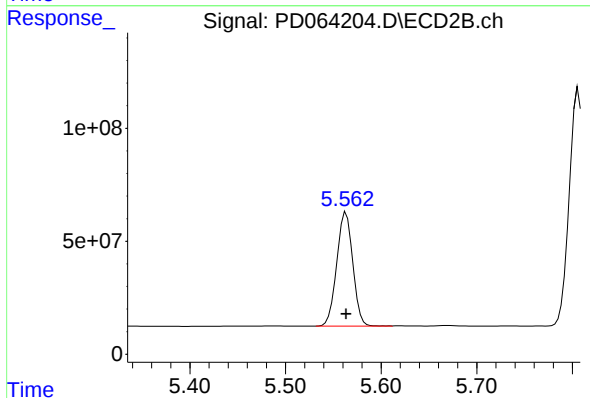


#9 Endosulfan I

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 587912786
Conc: 70.36 ng/ml

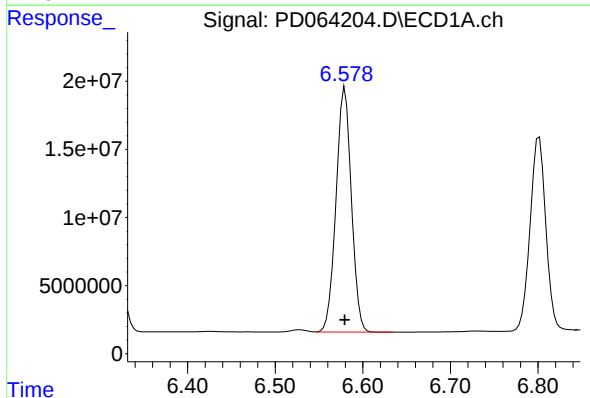


#13 Dieldrin

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 218739637
Conc: 156.85 ng/ml

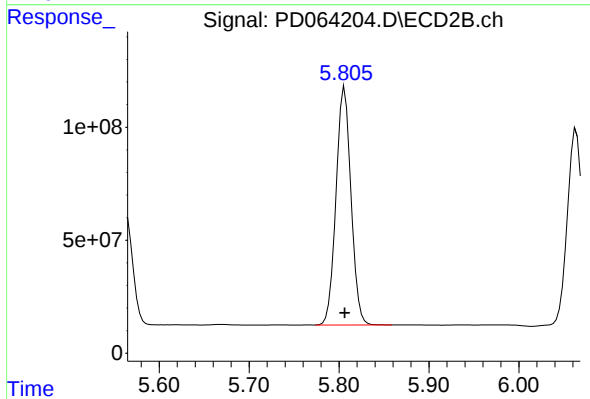

#13 Dieldrin


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 1218312391
Conc: 143.90 ng/ml

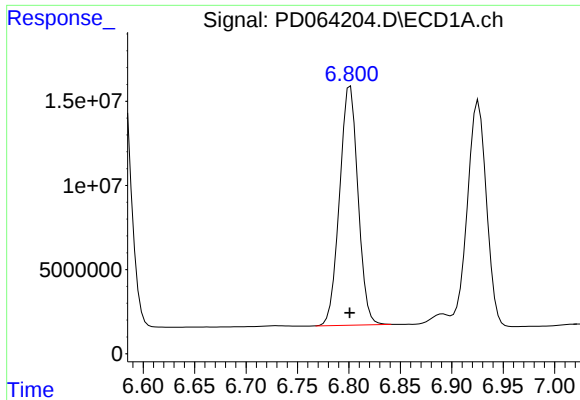

#14 Endrin


R.T.: 6.801 min
Delta R.T.: 0.000 min
Response: 177305270
Conc: 156.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

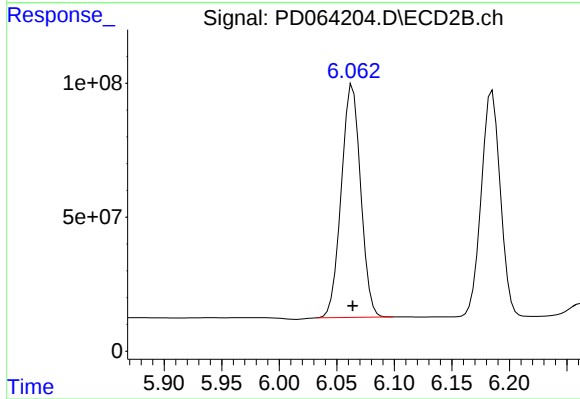


#14 Endrin

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 1021741992
Conc: 141.60 ng/ml

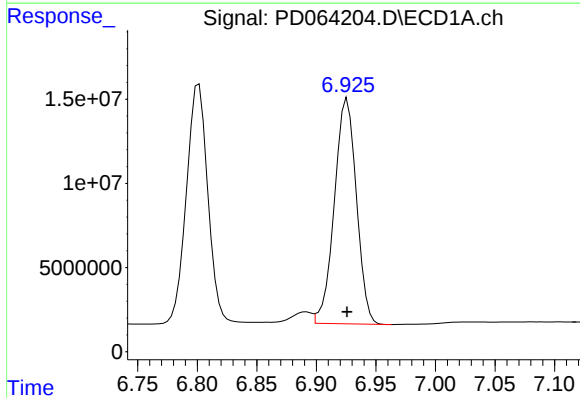


#16 4,4'-DDD

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 172472801
Conc: 157.50 ng/ml

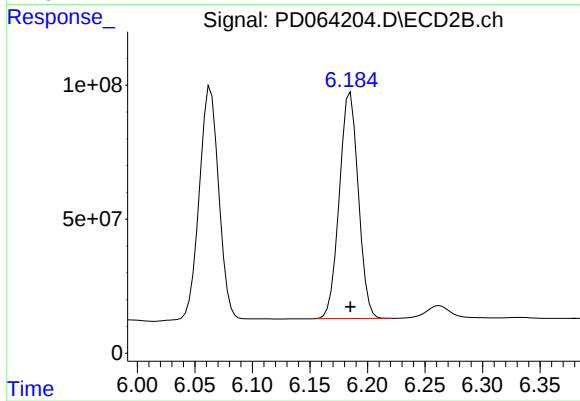

#16 4,4'-DDD


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 971392112
Conc: 145.00 ng/ml

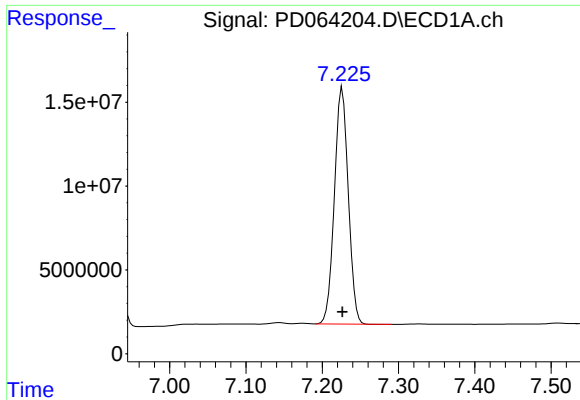

#17 4,4'-DDT


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 177562263
Conc: 160.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

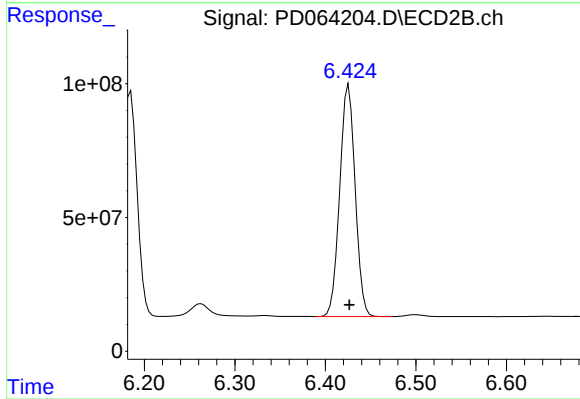


#17 4,4'-DDT

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 1025431556
Conc: 146.92 ng/ml

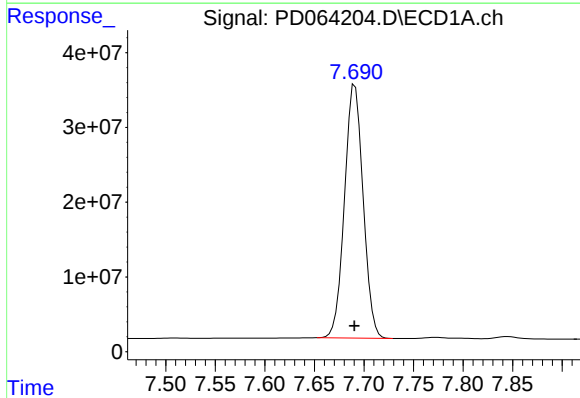


#20 Methoxychlor

R.T.: 7.691 min
Delta R.T.: 0.000 min
Response: 443964422
Conc: 663.30 ng/ml

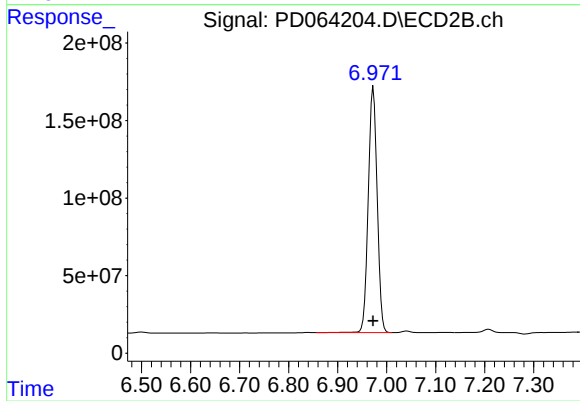

#20 Methoxychlor


R.T.: 6.973 min
Delta R.T.: 0.000 min
Response: 2003771232
Conc: 652.22 ng/ml

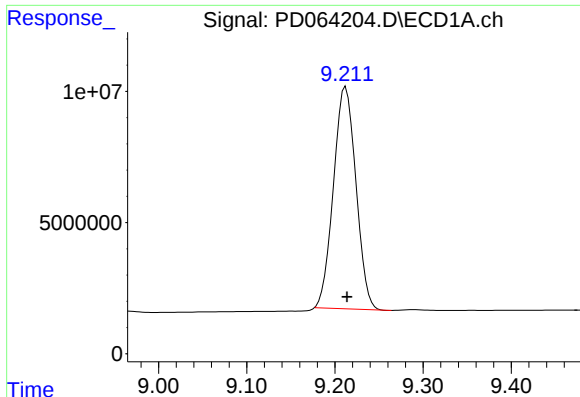

#27 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: -0.001 min
Response: 149811471
Conc: 135.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

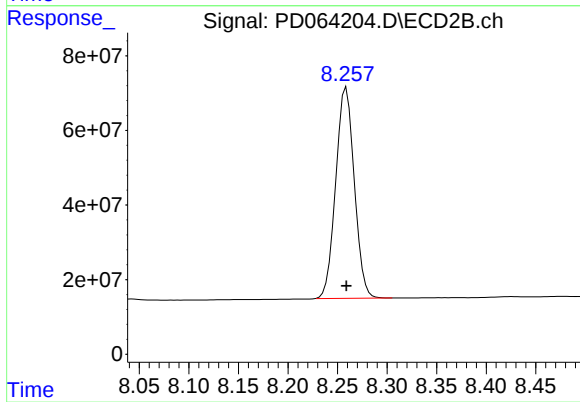

#27 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 737205466
Conc: 140.06 ng/ml