

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 21:17
Operator : AR\AJ
Sample : M2958-04
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
DBK30

Manual Integrations
APPROVED

mohammad
7/19/2021 2:41:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:38:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

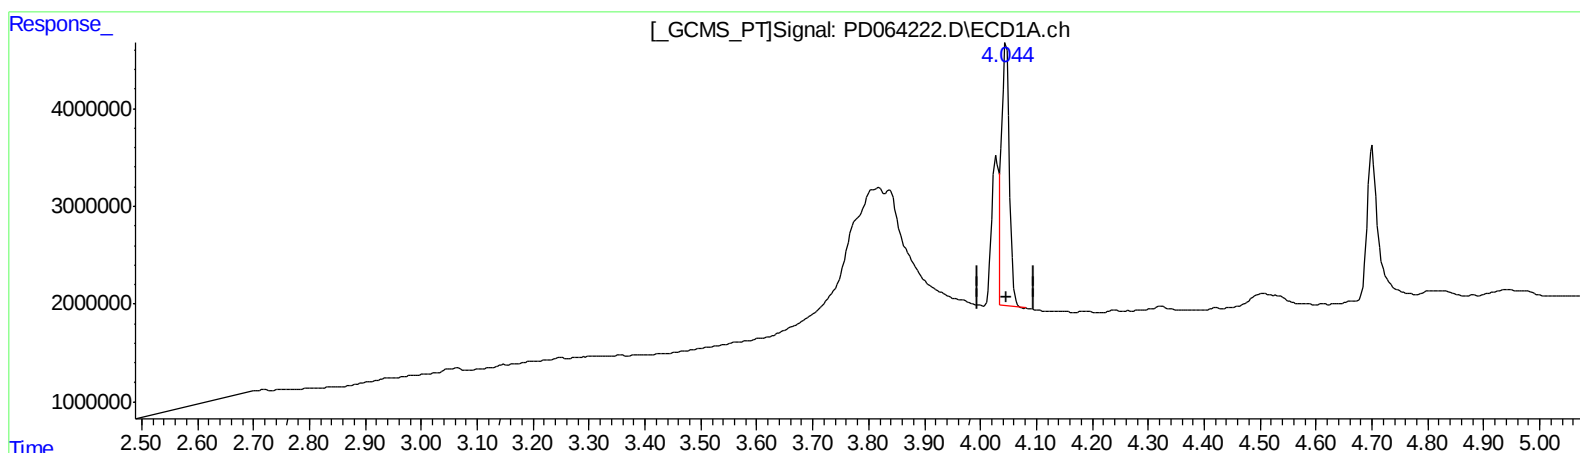

(1) Tetrachloro-m-xylene (SA)

4.046min 21.039 ng/ml

response 28149312

(1) Tetrachloro-m-xylene #2 (SA)

3.512min 21.331 ng/ml m

response 213128207

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 21:17
Operator : AR\AJ
Sample : M2958-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:38:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.046	3.512	28149312	213.1E6	21.039	21.331m
27) SA Decachlor...	9.211	8.258	44322358	184.9E6	41.327	35.403

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_D
ClientSampleId :
DBK30

Manual Integrations
APPROVED

mohammad
7/19/2021 2:41:01 PM

AJ
07/19/21