

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
 Data File : PD064189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2021 12:01
 Operator : AR\AJ
 Sample : RESC05
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC005

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 16:43:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 09 16:20:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.056	3.513	24241290	178.1E6	18.118	17.823
27)	SA Decachlor...	9.229	8.262	40583602	197.0E6	37.841	37.703
Target Compounds							
2)	A alpha-BHC	4.458	3.953	16685663	118.0E6	8.962	8.822
3)	MA gamma-BHC...	4.750	4.236	16129249	103.3E6	9.059	8.487
4)	MA Heptachlor	5.263	4.535	16262809	102.4E6	9.219	8.985
5)	MB Aldrin	5.573	4.784	16216125	103.8E6	10.176	10.029
6)	B beta-BHC	4.929	4.481	7980393	54545722	9.520	10.037
7)	B delta-BHC	5.150	4.687	16239126	107.1E6	9.508	9.742
8)	B Heptachlo...	5.969	5.226	15526241	92743180	10.187	10.150
9)	A Endosulfan I	6.331	5.565	12926875	78649649	9.356	9.301
10)	B trans-Chl...	6.205	5.451	16279254	93687318	10.300	10.072
11)	B cis-Chlor...	6.279	5.510	15975085	90099100	10.187	9.955
12)	B 4,4'-DDE	6.440	5.672	27778305	168.1E6	20.053	20.056
13)	MA Dieldrin	6.593	5.808	26903886	157.1E6	18.574	18.371
14)	MA Endrin	6.815	6.065	21562556	139.8E6	18.263	19.174
15)	B Endosulfa...	7.030	6.337	24733890	135.0E6	20.479	20.746
16)	A 4,4'-DDD	6.940	6.187	20909152	122.8E6	18.363	18.262
17)	MA 4,4'-DDT	7.240	6.428	22353117	129.4E6	19.364	18.480
18)	B Endrin al...	7.156	6.506	20740920	116.7E6	20.160	21.074
19)	B Endosulfa...	7.381	6.718	25233970	127.8E6	20.495	20.749
20)	A Methoxychlor	7.706	6.975	60080728	300.7E6	93.636	97.439
21)	B Endrin ke...	7.860	7.211	28231768	142.8E6	21.243	21.081

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 12:01
Operator : AR\AJ
Sample : RESC05
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 16:43:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 16:20:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

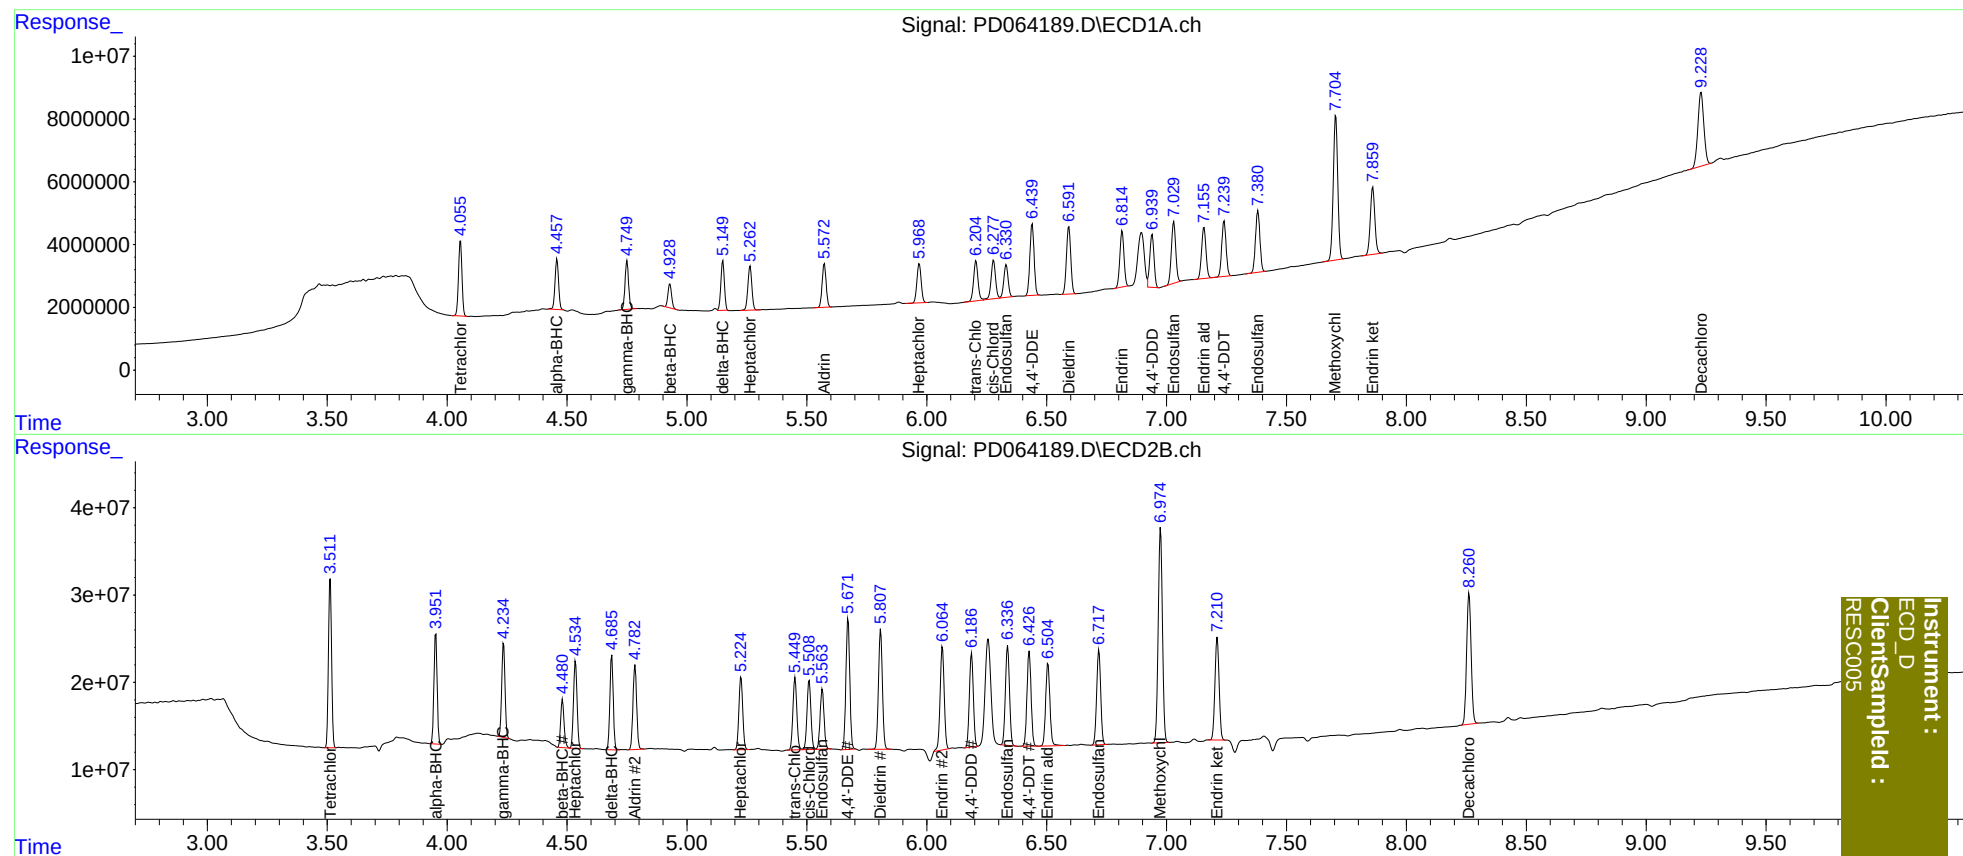

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064189.D
Acq On : 09 Jul 2021 12:01
Operator : AR\AJ
Sample : RESC05
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC005

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Title : GC Extractables
Last Update : Sat Jul 10 02:02:54 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
4.056	4.458	100.00%
4.458	4.750	100.00%
4.750	4.929	100.00%
4.929	5.150	100.00%
5.150	5.264	100.00%
5.264	5.573	100.00%
5.573	5.969	100.00%
5.969	6.205	100.00%
6.205	6.279	100.00%
6.279	6.331	100.00%
6.331	6.440	100.00%
6.440	6.593	100.00%
6.593	6.815	100.00%
6.815	6.940	100.00%
6.940	7.030	100.00%
7.030	7.156	100.00%
7.156	7.240	100.00%
7.240	7.381	100.00%
7.381	7.706	100.00%
7.706	7.860	100.00%
7.860	9.229	100.00%

Signal #2



3.513	3.953	100.00%
3.953	4.236	100.00%
4.236	4.481	100.00%
4.481	4.535	100.00%
4.535	4.687	100.00%
4.687	4.784	100.00%
4.784	5.226	100.00%
5.226	5.451	100.00%
5.451	5.510	99.30%
5.510	5.565	100.00%
5.565	5.672	100.00%
5.672	5.808	100.00%
5.808	6.065	100.00%
6.065	6.187	100.00%
6.187	6.337	100.00%
6.337	6.428	100.00%
6.428	6.506	100.00%
6.506	6.718	100.00%
6.718	6.975	100.00%
6.975	7.211	100.00%
7.211	8.262	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070921\
Data File : PD064189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2021 12:01
Operator : AR\AJ
Sample : RESC05
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC005

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 16:43:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 09 16:20:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

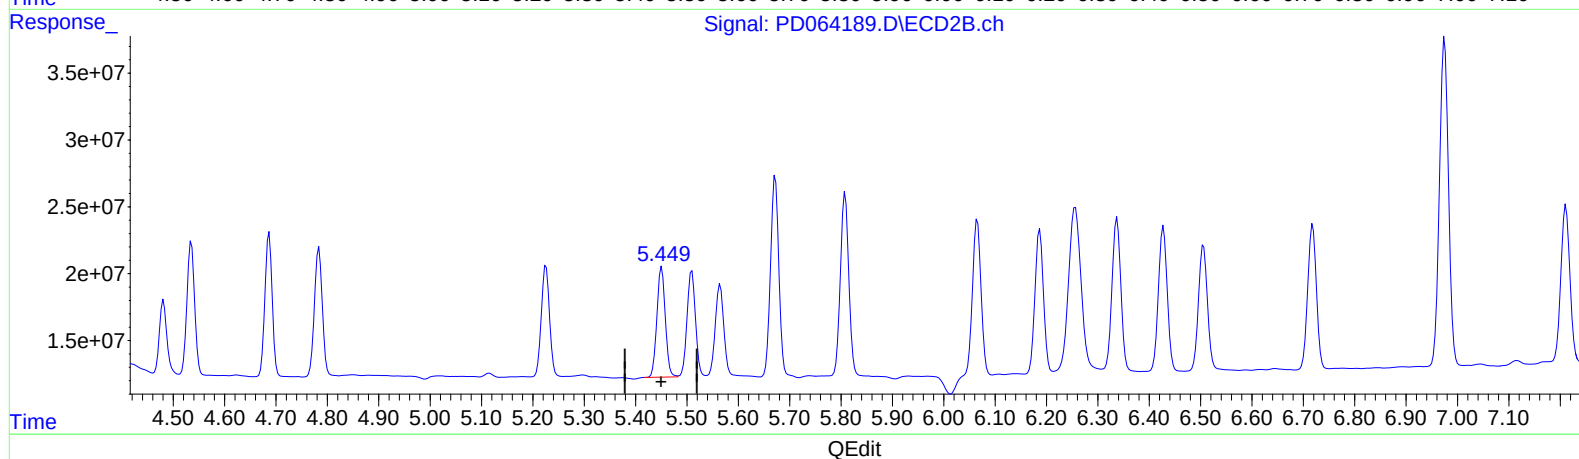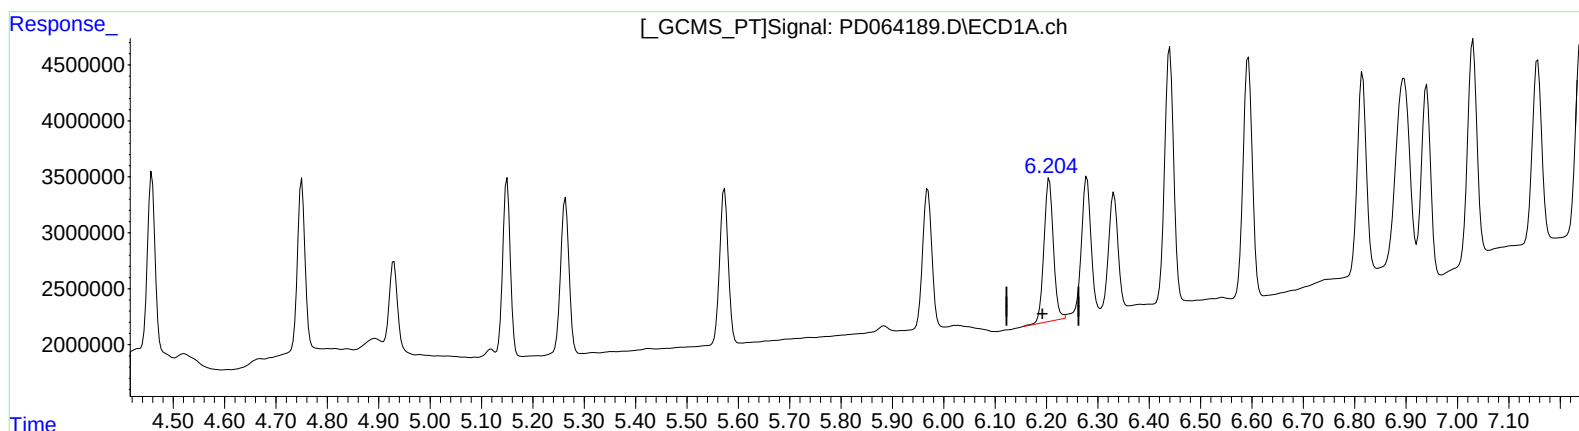

(10) trans-Chlordane (B)

6.205min 10.300 ng/ml

response 16279254

(10) trans-Chlordane #2 (B)

5.451min 10.072 ng/ml

response 93687318