

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
 Data File : PD070784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2022 13:24
 Operator : AR\AJ
 Sample : N3608-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/11/2022
 Supervised By :Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 23:00:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 15:26:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	4.124	55113252	449.2E6	22.575	17.368
28)	SA Decachlor...	8.261	9.312	64502759	159.8E6	26.014	19.422 #
Target Compounds							
12)	B 4,4'-DDE	5.657	6.513	13739991	99277569	4.726m	4.855m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
Data File : PD070784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2022 13:24
Operator : AR\AJ
Sample : N3608-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 23:00:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 15:26:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

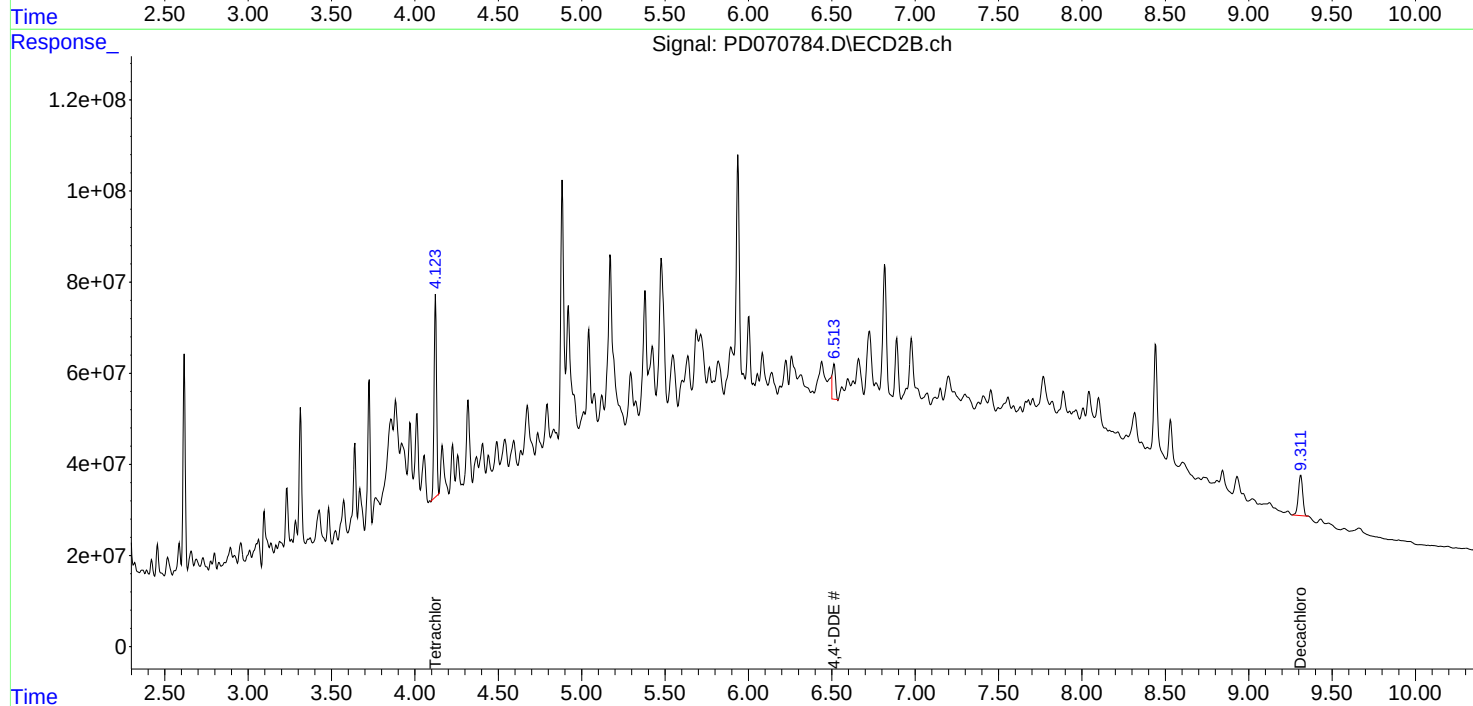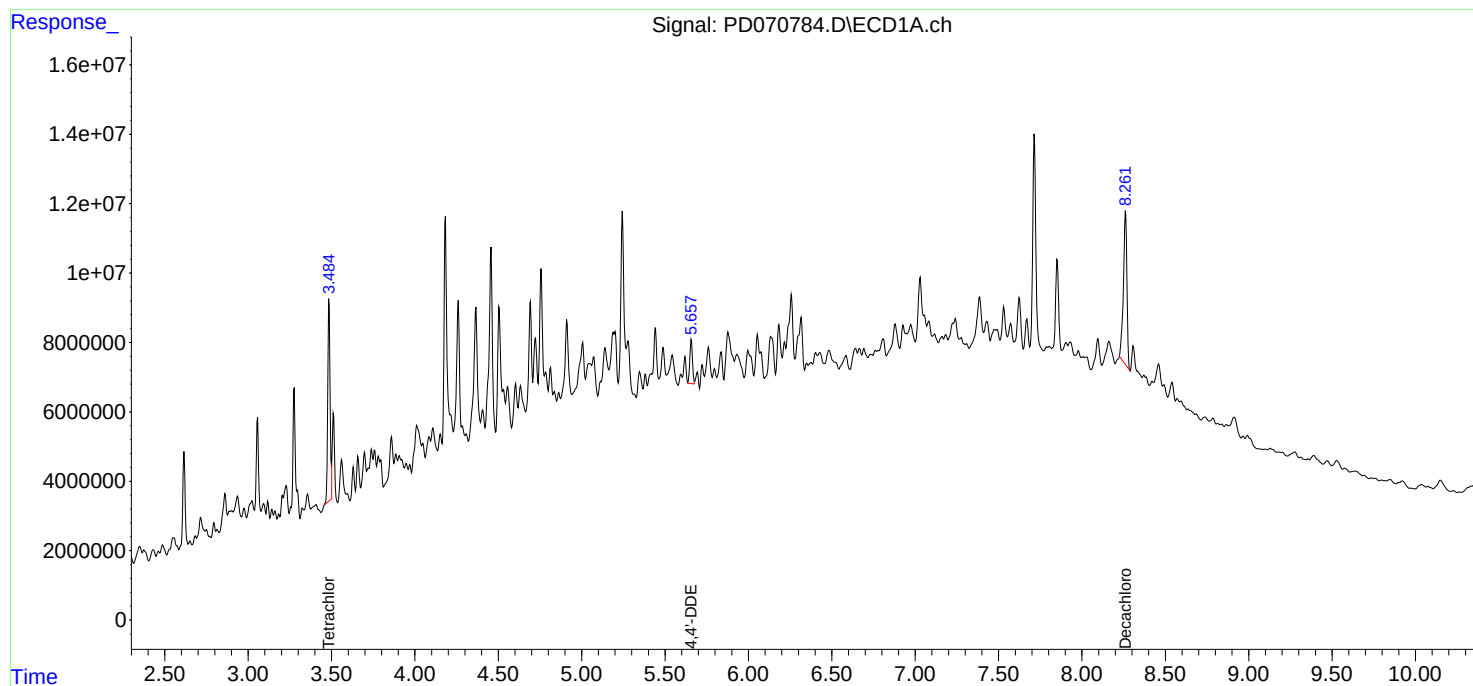

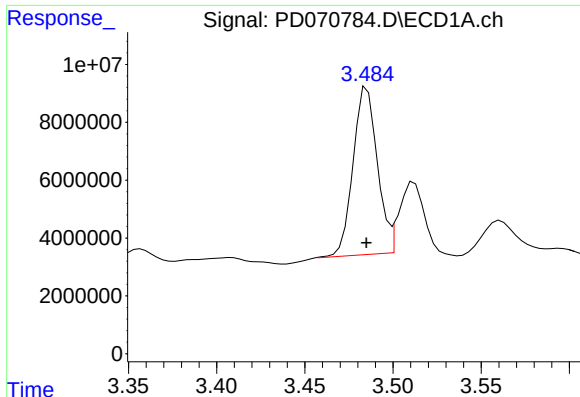


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 55113252
Conc: 22.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

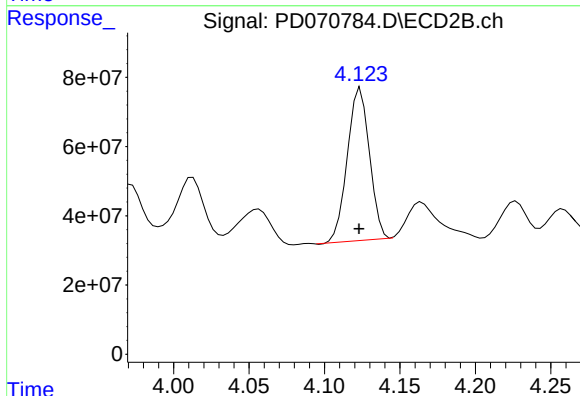


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.001 min
Response: 449151285
Conc: 17.37 ng/ml

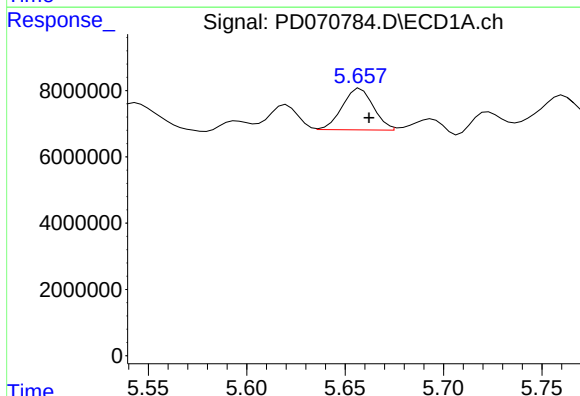


#12 4,4'-DDE

R.T.: 5.657 min
Delta R.T.: -0.006 min
Response: 13739991
Conc: 4.73 ng/ml m

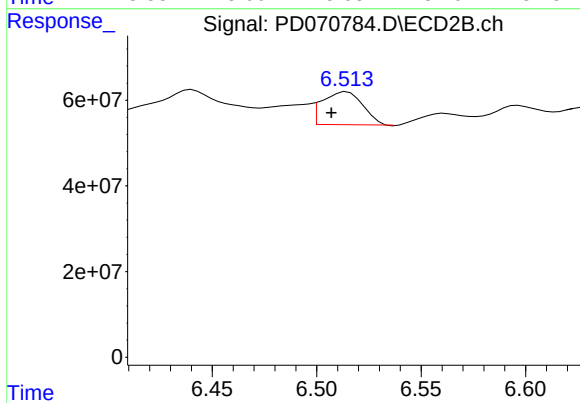

#12 4,4'-DDE

R.T.: 6.513 min
Delta R.T.: 0.006 min
Response: 99277569
Conc: 4.85 ng/ml m

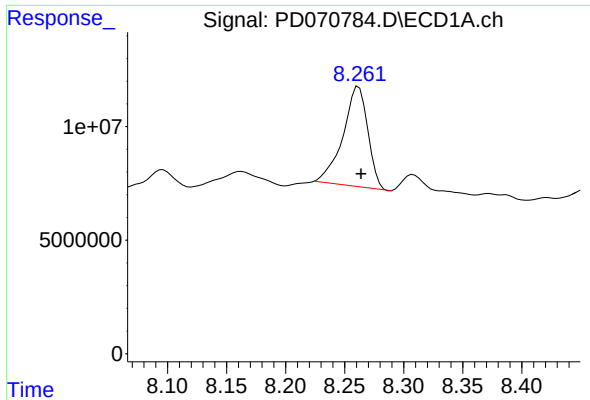


#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: -0.002 min
Response: 64502759
Conc: 26.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

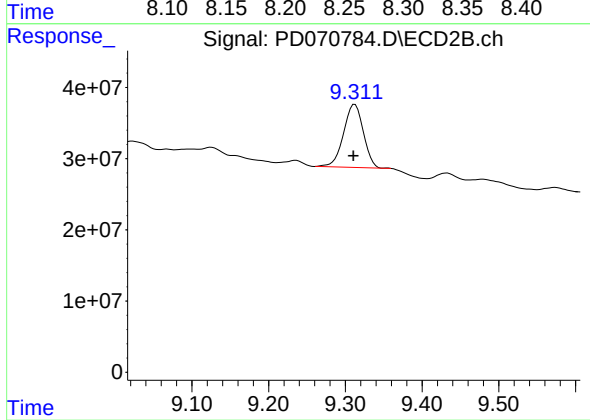

#28 Decachlorobiphenyl

R.T.: 9.312 min
Delta R.T.: 0.002 min
Response: 159785278
Conc: 19.42 ng/ml