

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
 Data File : PD070795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2022 16:16
 Operator : AR\AJ
 Sample : N3622-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20220497A-SIM-C3AA-COMPOSITE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/11/2022
 Supervised By :Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 23:07:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 15:26:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.503f	4.123	21955039	252.1E6	8.993m	9.746
28) SA Decachlor...	8.281f	9.312	18788143	70070386	7.577	8.517

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
Data File : PD070795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2022 16:16
Operator : AR\AJ
Sample : N3622-08
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
20220497A-SIM-C3AA-COMPOSITE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/11/2022
Supervised By : Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 23:07:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 15:26:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

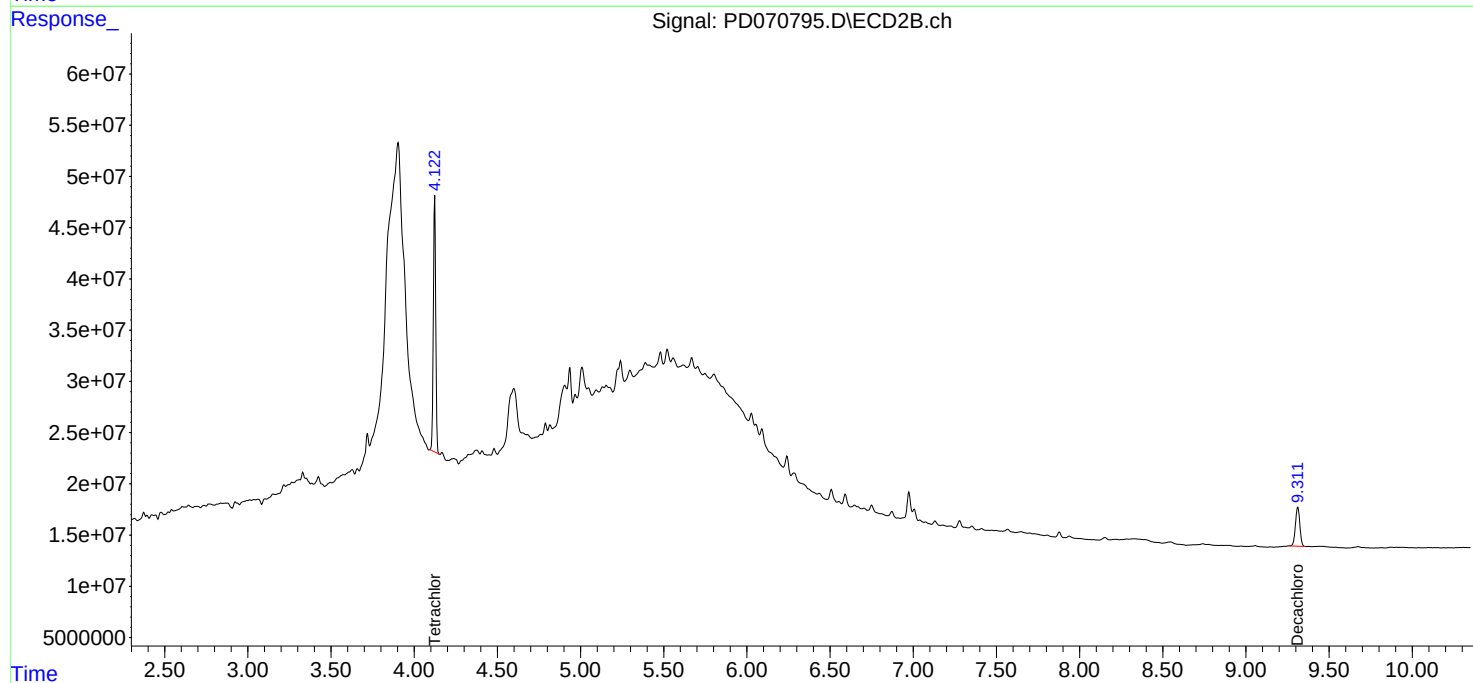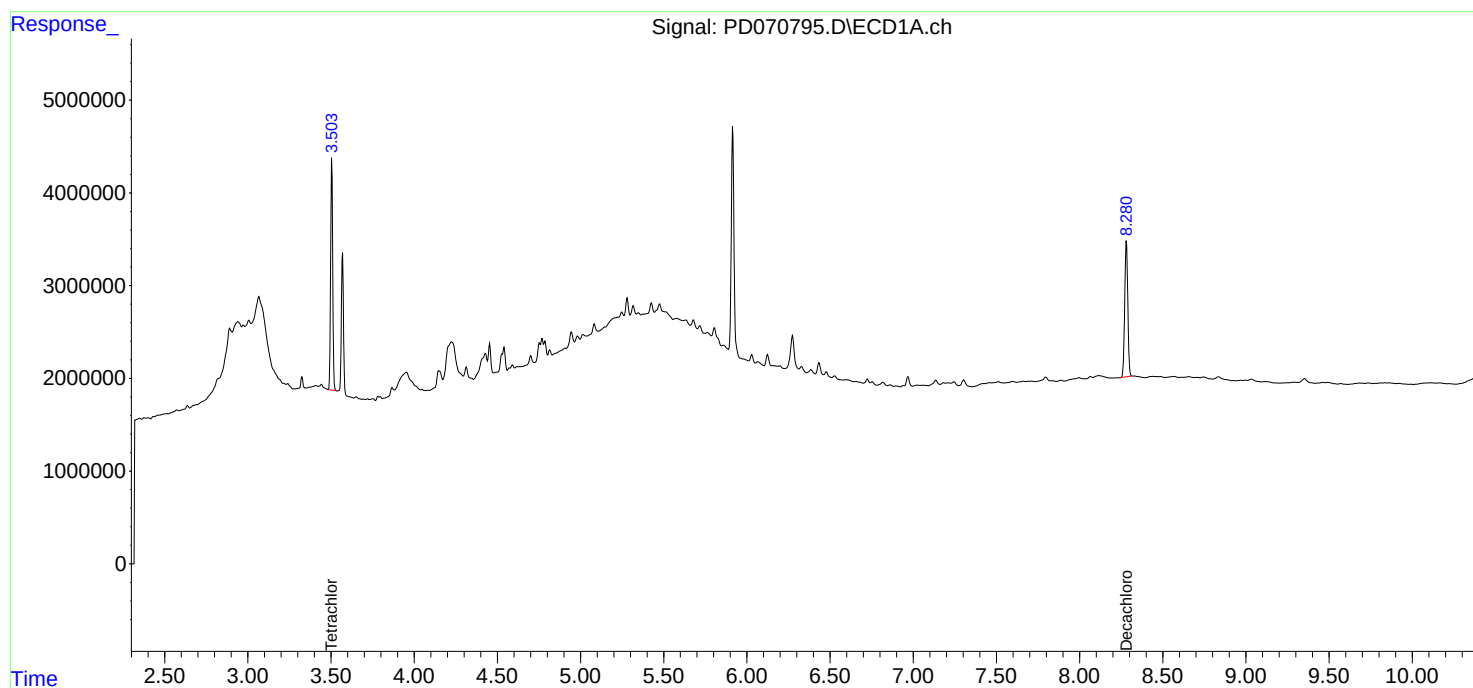

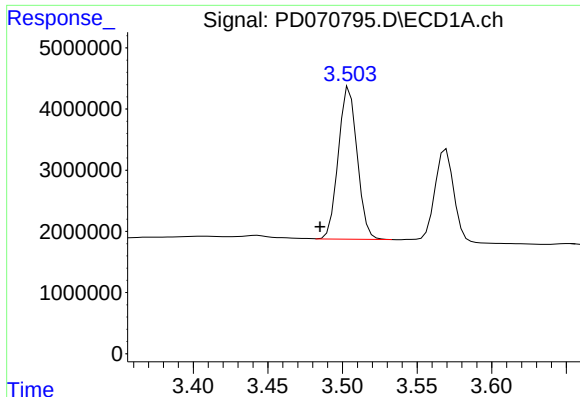


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: 0.018 min
Response: 21955039
Conc: 8.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
20220497A-SIM-C3AA-COMPOSITE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

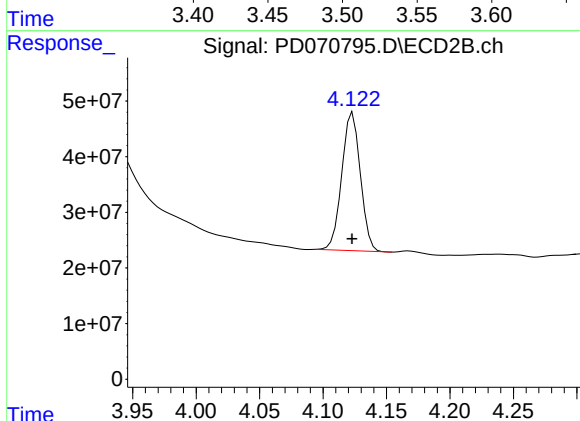


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 252053966
Conc: 9.75 ng/ml

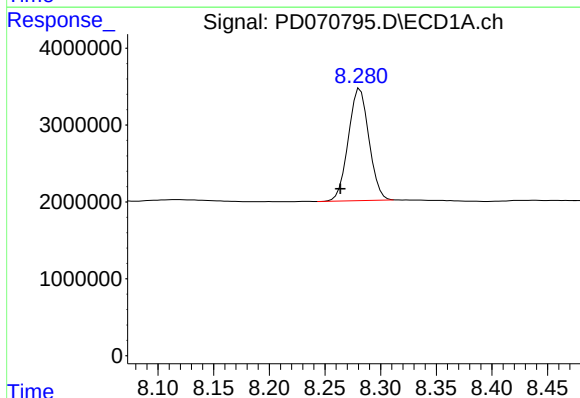

#28 Decachlorobiphenyl

R.T.: 8.281 min
Delta R.T.: 0.018 min
Response: 18788143
Conc: 7.58 ng/ml

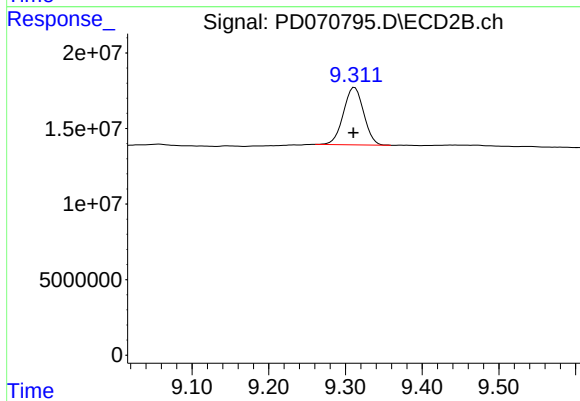

#28 Decachlorobiphenyl

R.T.: 9.312 min
Delta R.T.: 0.001 min
Response: 70070386
Conc: 8.52 ng/ml