

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
 Data File : PD070798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2022 16:58
 Operator : AR\AJ
 Sample : N3631-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-3-070722

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/11/2022
 Supervised By : Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 23:08:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 15:26:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.485	4.124	29574764	337.2E6	12.114	13.039
2) SA Decachlor...	8.261	9.312	30858047	116.7E6	12.445	14.182
Target Compounds						
17) MA 4,4'-DDT	6.419	7.305	2103945	9604073	0.843	0.630m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070922\
Data File : PD070798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2022 16:58
Operator : AR\AJ
Sample : N3631-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SU-3-070722


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/11/2022
Supervised By : Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 23:08:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 15:26:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

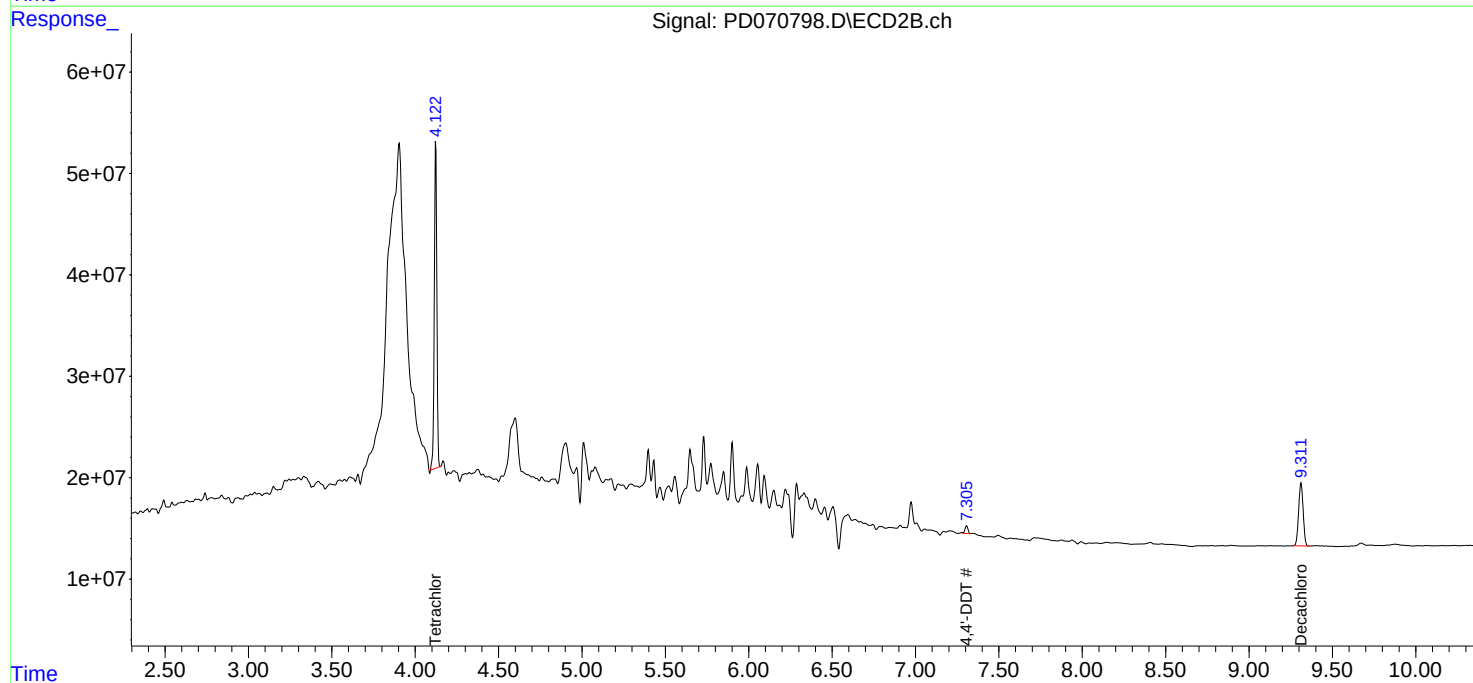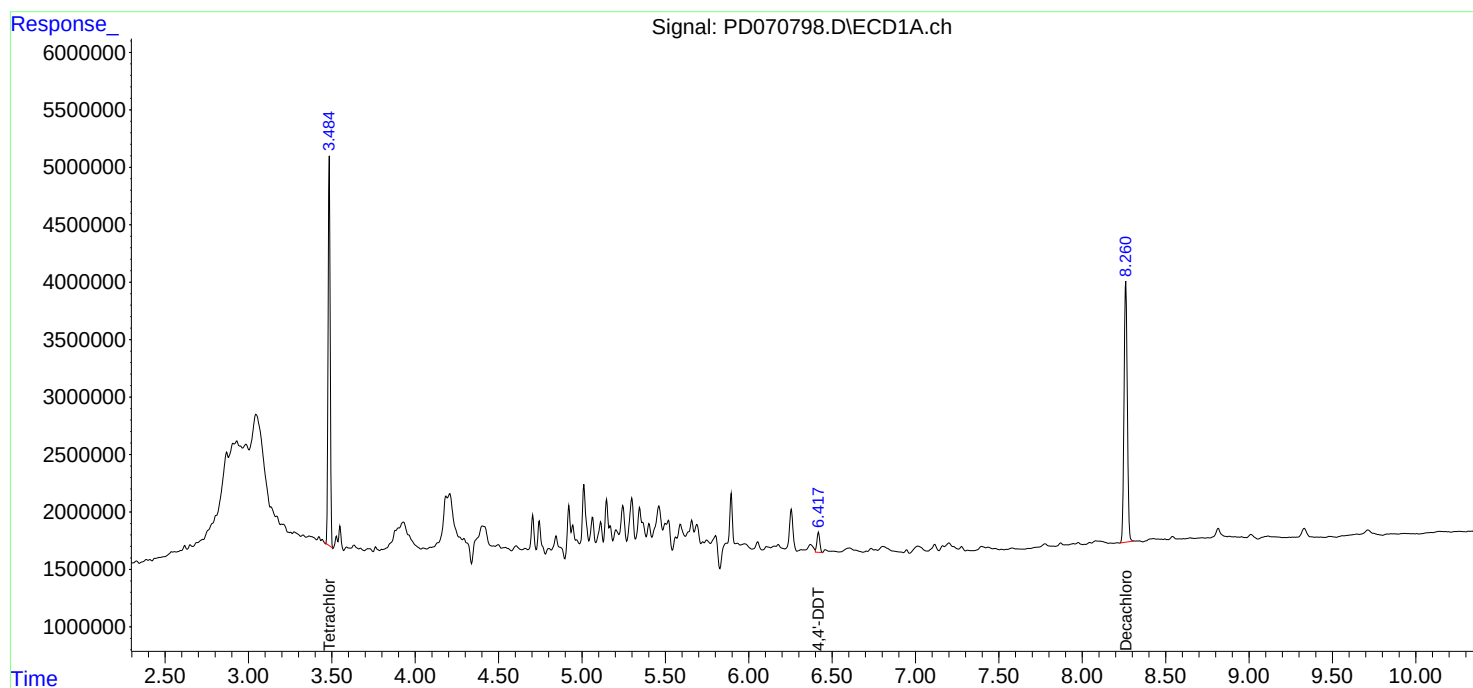

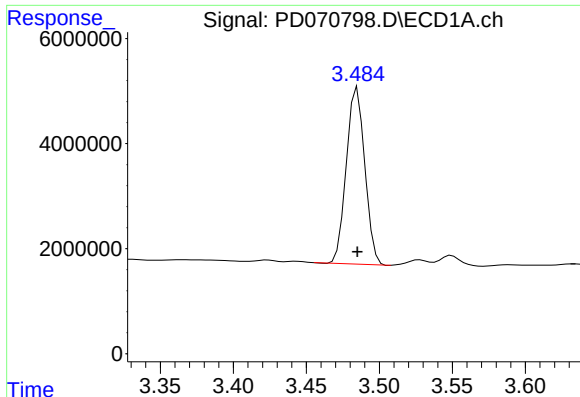


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 29574764
Conc: 12.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-3-070722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

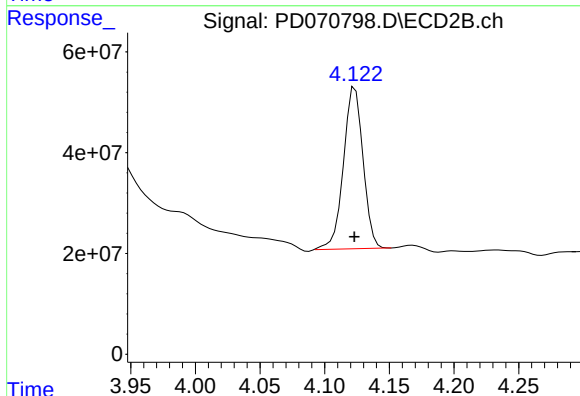


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 337205874
Conc: 13.04 ng/ml

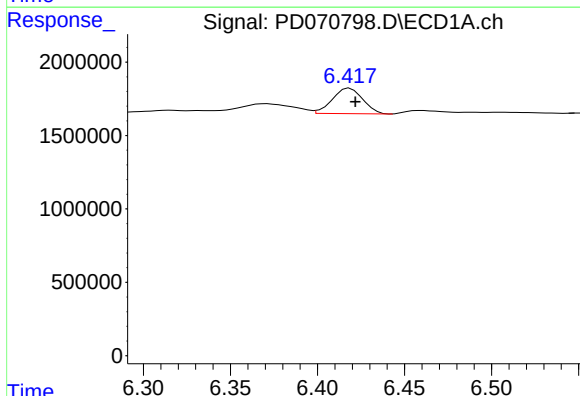


#17 4,4'-DDT

R.T.: 6.419 min
Delta R.T.: -0.003 min
Response: 2103945
Conc: 0.84 ng/ml

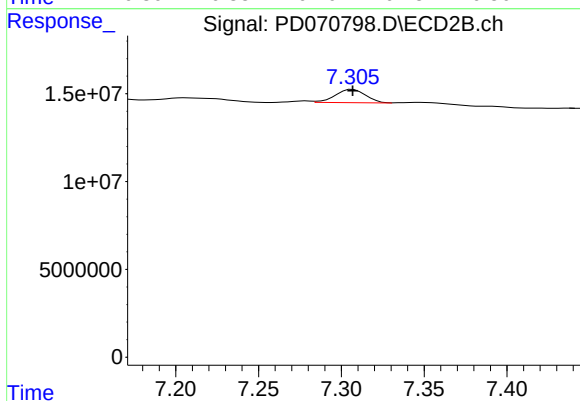

#17 4,4'-DDT

R.T.: 7.305 min
Delta R.T.: -0.001 min
Response: 9604073
Conc: 0.63 ng/ml m

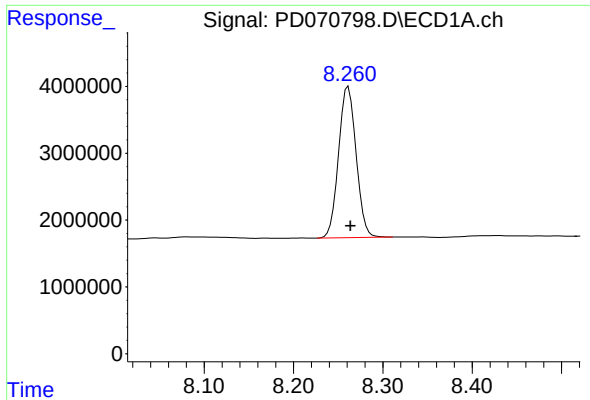


#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: -0.002 min
Response: 30858047
Conc: 12.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-3-070722

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

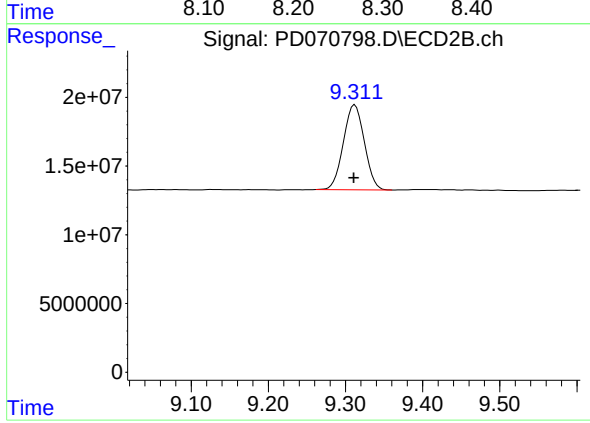

#28 Decachlorobiphenyl

R.T.: 9.312 min
Delta R.T.: 0.001 min
Response: 116677869
Conc: 14.18 ng/ml