

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
Data File : PD076410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 08:59
Operator : AR\AJ
Sample : 03494-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 02:35:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
20) A	Methoxychlor	0.000	6.668f	0	111790	0.245
26)	Toxaphene-5	0.000	6.668f	0	111790	3.177


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
Data File : PD076410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 08:59
Operator : AR\AJ
Sample : 03494-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 02:35:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

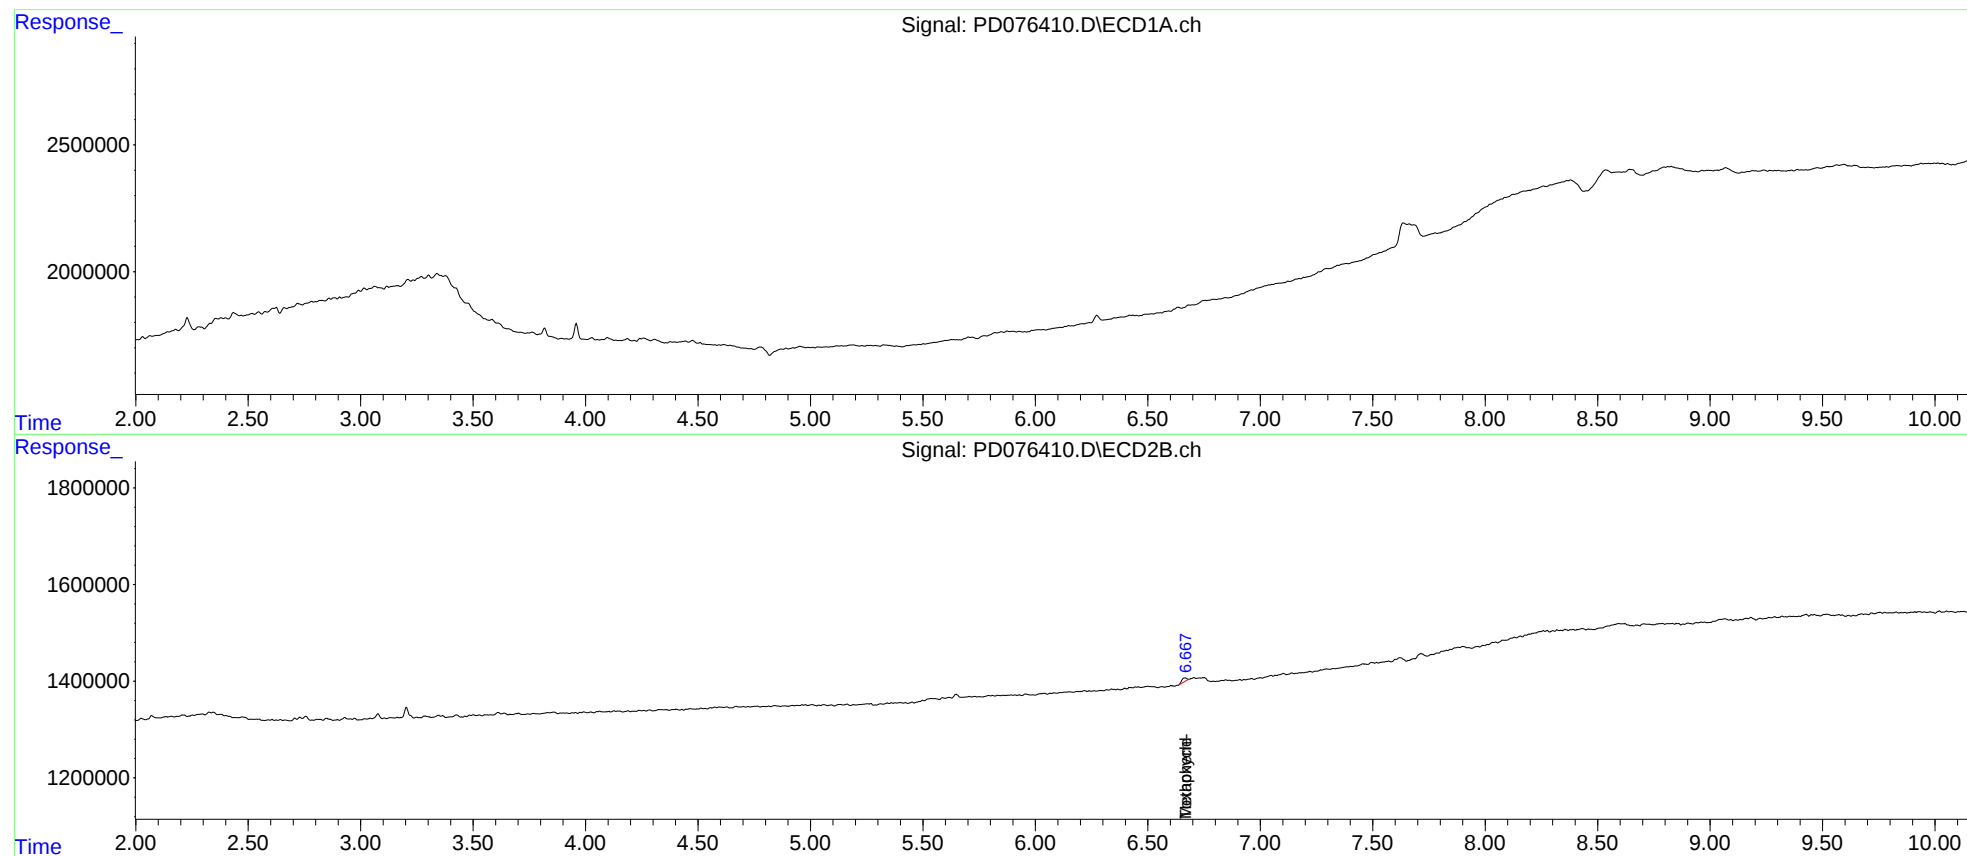

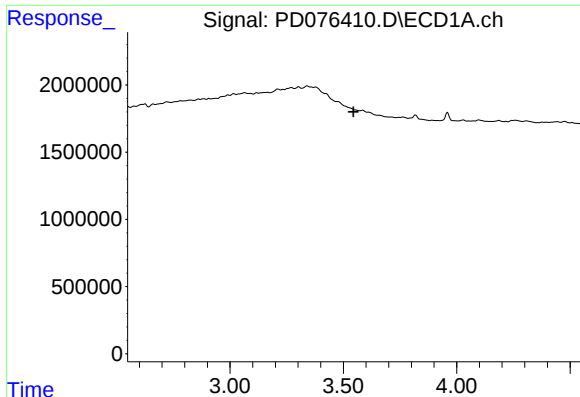


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.545 min
Response: 0
Conc: N.D.

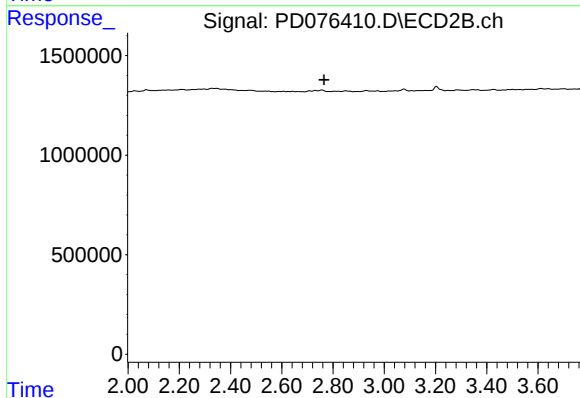


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.765 min
Response: 0
Conc: N.D.

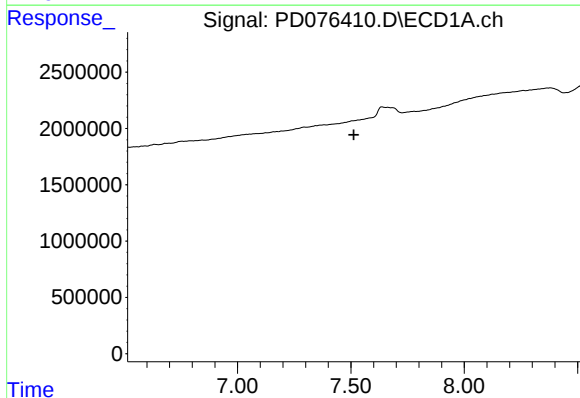


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.513 min
Response: 0
Conc: N.D.

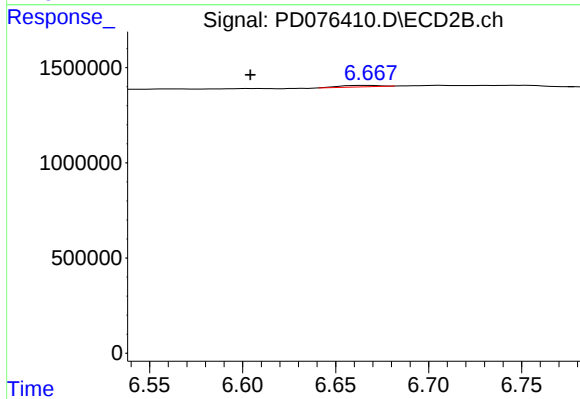


#20 Methoxychlor

R.T.: 6.668 min
Delta R.T.: 0.064 min
Response: 111790
Conc: 0.25 ng/ml

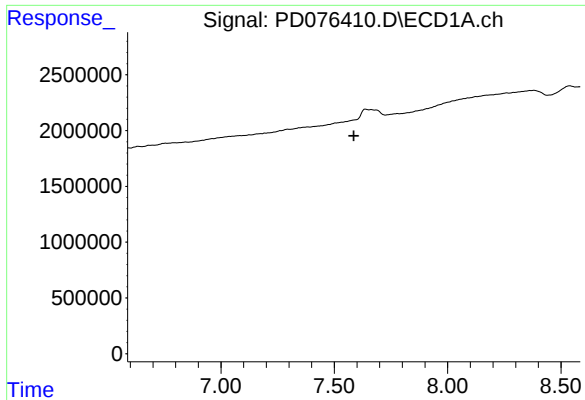


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.586 min
Response: 0
Conc: N.D.

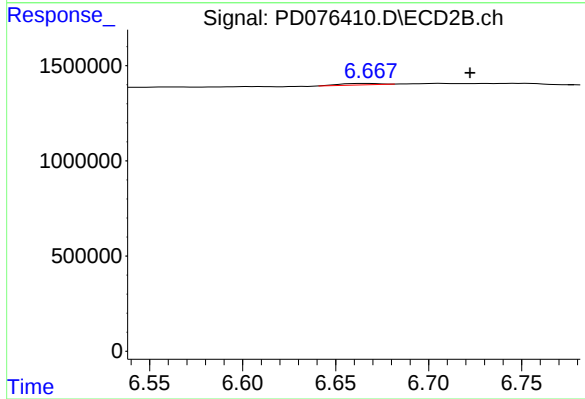


#26 Toxaphene-5

R.T.: 6.668 min
Delta R.T.: -0.054 min
Response: 111790
Conc: 3.18 ng/ml

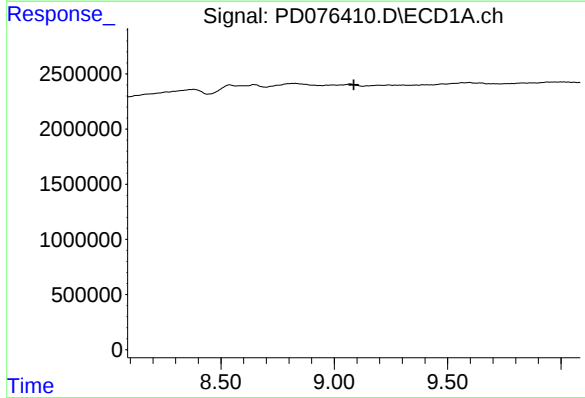

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.085 min
Response: 0
Conc: N.D.

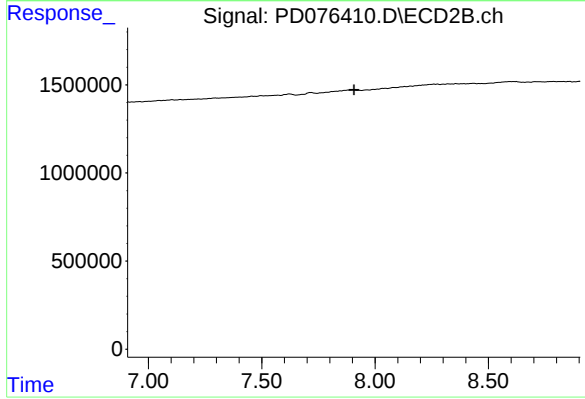

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.908 min
Response: 0
Conc: N.D.