

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
 Data File : PD076440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2023 20:55
 Operator : AR\AJ
 Sample : 03414-21MSD
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4634MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/11/2023
 Supervised By :Ankita Jodhani 07/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:04:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 14:30:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.766	708.2E6	11102336	326.637m	10.788 #
27)	SA Decachlor...	9.085	7.908	49739251	20910676	19.609	22.915
Target Compounds							
2)	A alpha-BHC	4.000	3.266	179.3E6	72537781	49.369m	47.269m
3)	MA gamma-BHC...	4.337	3.589	589.0E6	71137712	173.389m	49.431m#
4)	MA Heptachlor	4.924	3.935	154.9E6	344.9E6	43.411m	238.617 #
5)	MB Aldrin	5.269	4.231	146.4E6	260.8E6	42.579	184.272 #
6)	B beta-BHC	4.523	3.893	81190353	25295577	53.637m	37.724 #
7)	B delta-BHC	4.786	4.125	177.3E6	108.6E6	51.923m	76.357 #
8)	B Heptachlo...	5.693	4.717	246.8E6	80717280	77.419	61.003
9)	A Endosulfan I	6.083	5.090	132.4E6	39051084	45.568	33.753 #
10)	B trans-Chl...	5.952	4.967	165.6E6	48465525	53.691m	38.373m#
11)	B cis-Chlor...	6.032	5.031	156.3E6	49638586	49.021	38.265m
12)	B 4,4'-DDE	6.204	5.222	361.9E6	117.2E6	124.409	109.801
13)	MA Dieldrin	6.359	5.354	333.2E6	205.6E6	103.346	155.860 #
14)	MA Endrin	6.589	5.629	316.8E6	124.0E6	122.762	109.393m
15)	B Endosulfa...	6.807	5.923	233.2E6	115.0E6	86.274m	103.474
16)	A 4,4'-DDD	6.724	5.777	276.6E6	93793919	121.118	116.096
17)	MA 4,4'-DDT	7.037	6.026	237.7E6	136.4E6	104.983m	163.694 #
18)	B Endrin al...	6.939	6.102	172.9E6	62914666	96.068	85.871m
19)	B Endosulfa...	7.174	6.326	238.0E6	107.7E6	94.005	105.083
20)	A Methoxychlor	7.514	6.602	617.6E6	227.4E6	462.817	498.403m
21)	B Endrin ke...	7.660	6.831	320.3E6	101.2E6	112.292m	85.918m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
Data File : PD076440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 20:55
Operator : AR\AJ
Sample : 03414-21MSD
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 03:04:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

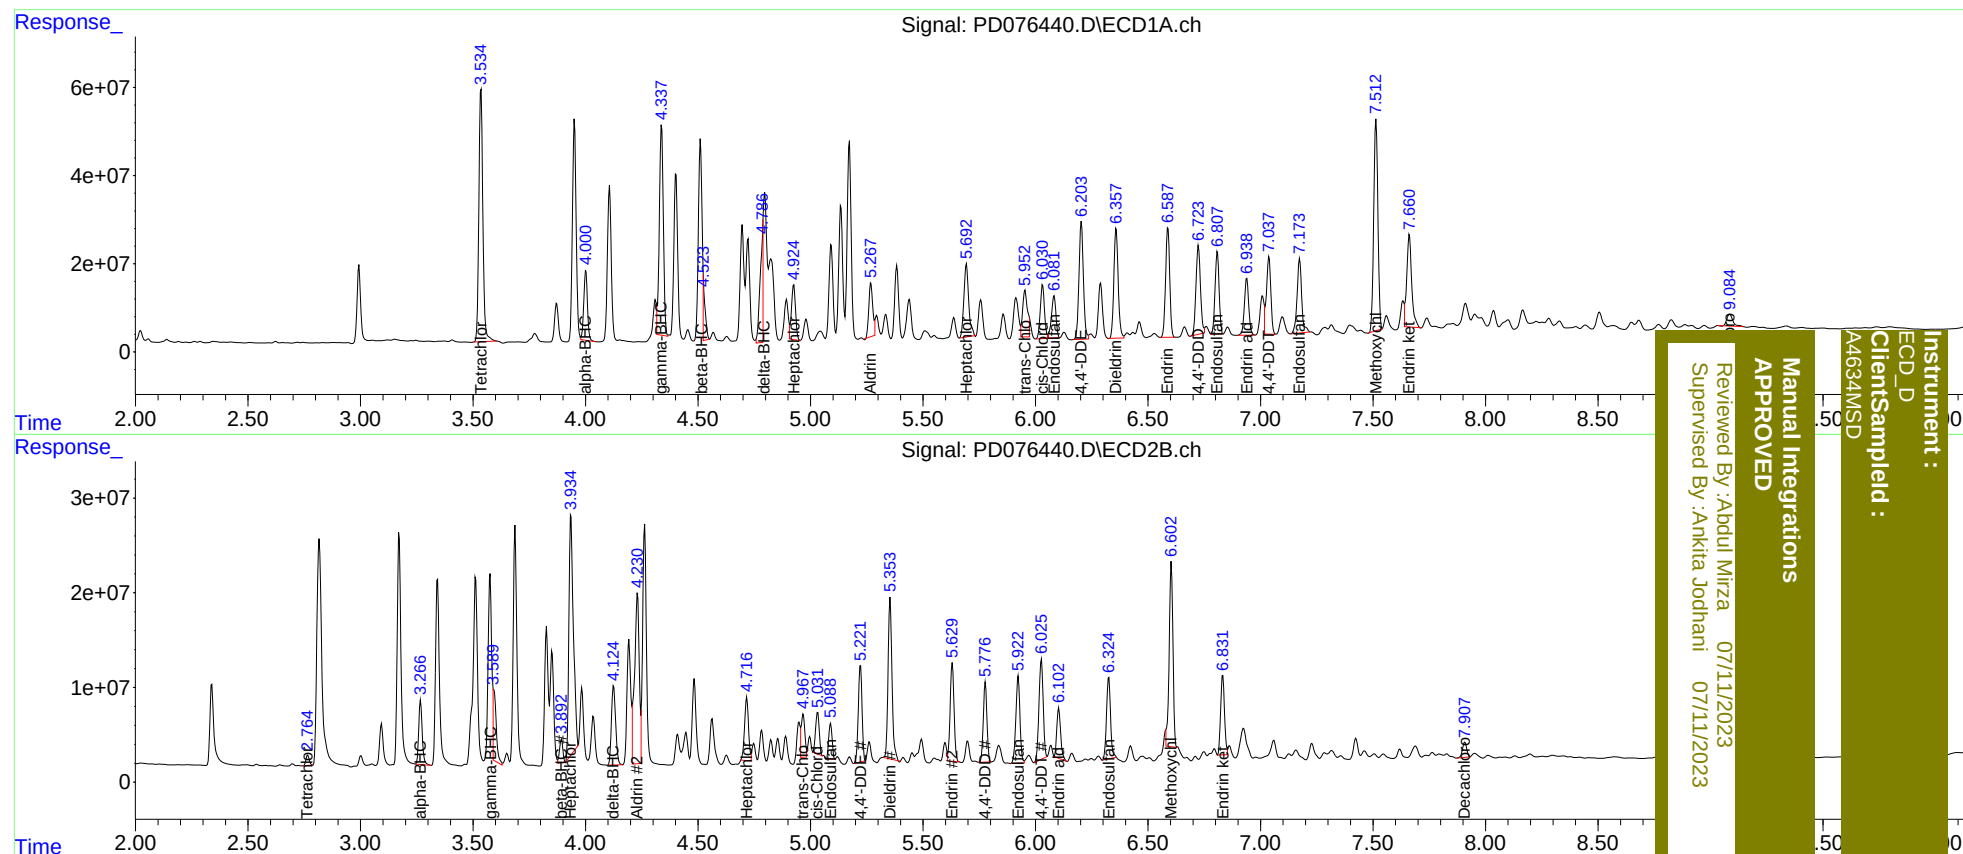

Instrument :
ECD_D
ClientSampled :
A4634MSD
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 07/11/2023
Supervised By :Ankita Jodhani 07/11/2023