

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
 Data File : PD076422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2023 15:27
 Operator : AR\AJ
 Sample : 03414-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46G0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/11/2023
 Supervised By : Ankita Jodhani 07/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:49:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 14:30:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.766	19193907	7689645	8.852	7.472
2) SA Decachlor...	9.084	7.908	40245822	15407190	15.866m	16.884
Target Compounds						
8) B Heptachlo...	5.689	4.697	1150255	1092971	0.361	0.826m#
16) A 4,4'-DDD	6.724	5.774	908928	396976	0.398m	0.491m
17) MA 4,4'-DDT	7.009	6.023	956412	524575	0.422m	0.629 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
Data File : PD076422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 15:27
Operator : AR\AJ
Sample : 03414-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 02:49:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

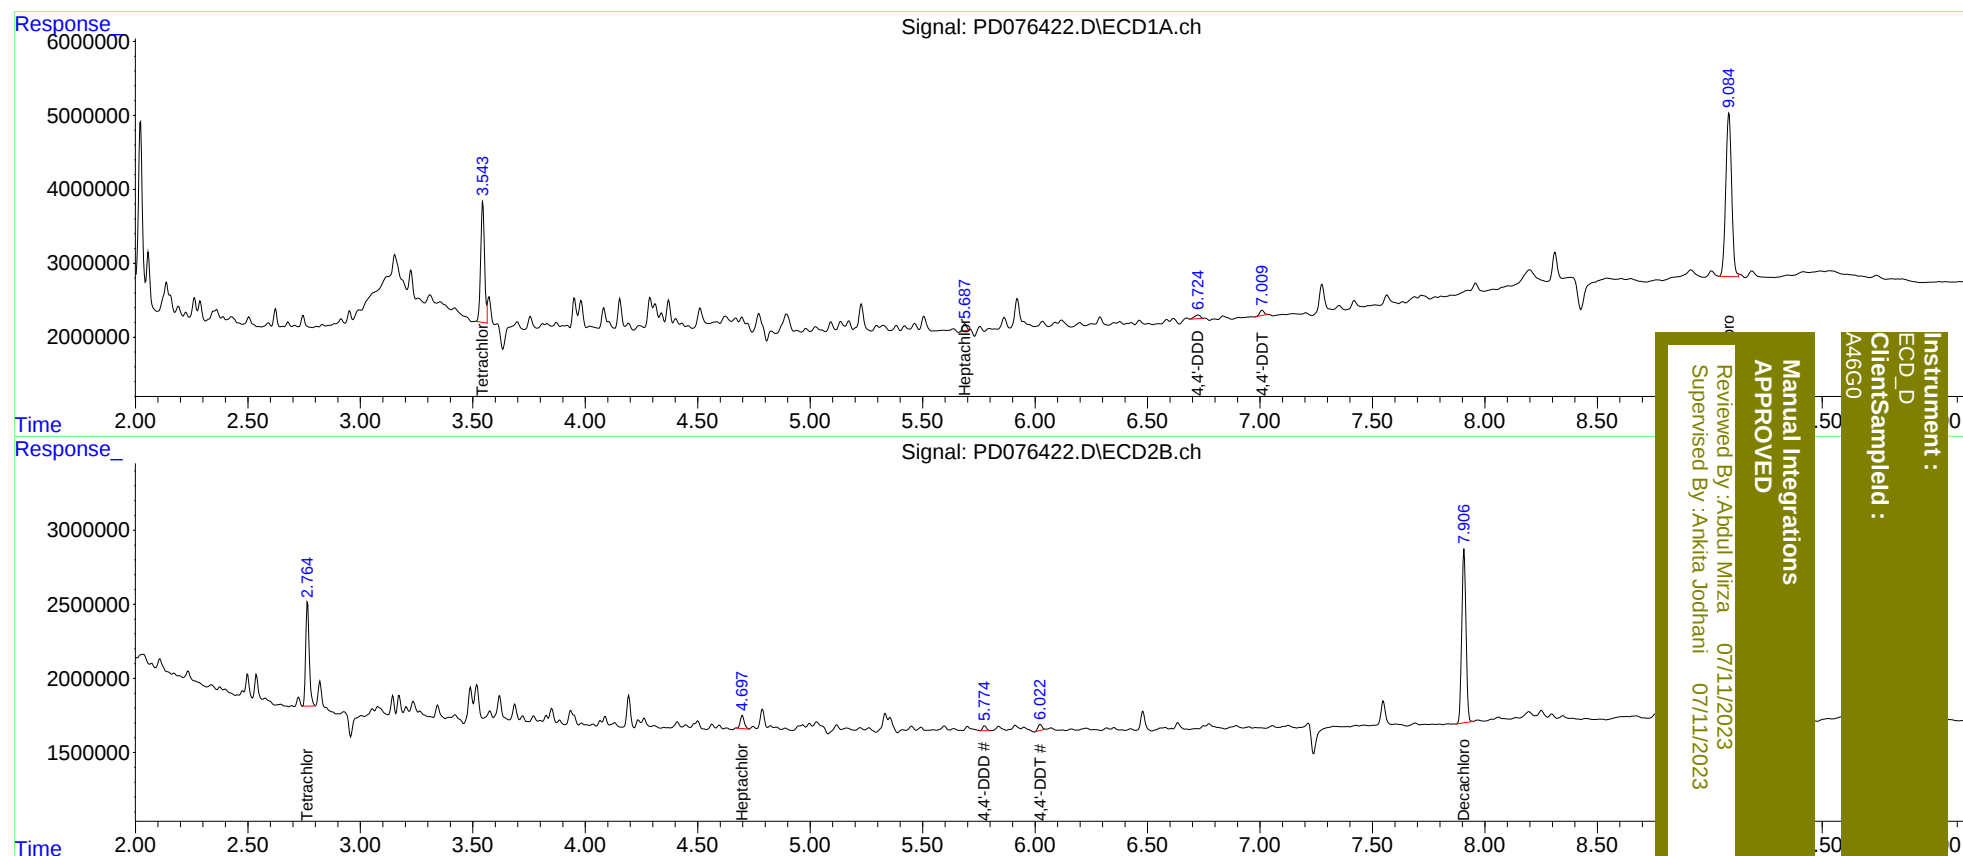

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/11/2023
Supervised By: Ankita Jodhani 07/11/2023

Instrument :
ECD_D
ClientSampled :
A46G0