

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
 Data File : PD076439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2023 20:42
 Operator : AR\AJ
 Sample : 03414-20MS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4634MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/11/2023
 Supervised By : Ankita Jodhani 07/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:03:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 14:30:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.766	699.8E6	11287039	322.736	10.968 #
27)	SA Decachlor...	9.085	7.908	52555201	20517803	20.719	22.485
Target Compounds							
2)	A alpha-BHC	4.000	3.267	185.8E6	72571840	51.170m	47.291
3)	MA gamma-BHC...	4.337	3.589	581.2E6	74419971	171.103m	51.711m#
4)	MA Heptachlor	4.924	3.936	150.1E6	348.3E6	42.064m	240.973 #
5)	MB Aldrin	5.269	4.232	149.9E6	263.2E6	43.596	185.939 #
6)	B beta-BHC	4.510	3.894	613.0E6	25223571	404.993m	37.616 #
7)	B delta-BHC	4.785	4.126	168.3E6	109.6E6	49.296m	77.101 #
8)	B Heptachlo...	5.693	4.718	254.5E6	84686340	79.817	64.002
9)	A Endosulfan I	6.083	5.090	139.3E6	39734676	47.927	34.343 #
10)	B trans-Chl...	5.952	4.967	131.5E6	54008692	42.620m	42.761m
11)	B cis-Chlor...	6.032	5.032	162.1E6	52346038	50.845	40.352
12)	B 4,4'-DDE	6.204	5.222	369.5E6	118.1E6	127.027	110.637
13)	MA Dieldrin	6.358	5.355	340.0E6	211.2E6	105.449	160.083 #
14)	MA Endrin	6.588	5.629	326.1E6	128.3E6	126.375	113.247m
15)	B Endosulfa...	6.807	5.923	236.7E6	116.7E6	87.555m	104.955
16)	A 4,4'-DDD	6.724	5.777	281.1E6	95516938	123.088	118.229
17)	MA 4,4'-DDT	7.036	6.026	219.4E6	138.2E6	96.889m	165.820 #
18)	B Endrin al...	6.939	6.102	176.4E6	62731410	97.999	85.621m
19)	B Endosulfa...	7.173	6.325	243.7E6	109.4E6	96.283	106.758
20)	A Methoxychlor	7.514	6.602	636.4E6	242.7E6	476.924	531.944m
21)	B Endrin ke...	7.659	6.831	347.6E6	101.9E6	121.861m	86.470m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070923\
Data File : PD076439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 20:42
Operator : AR\AJ
Sample : 03414-20MS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 03:03:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

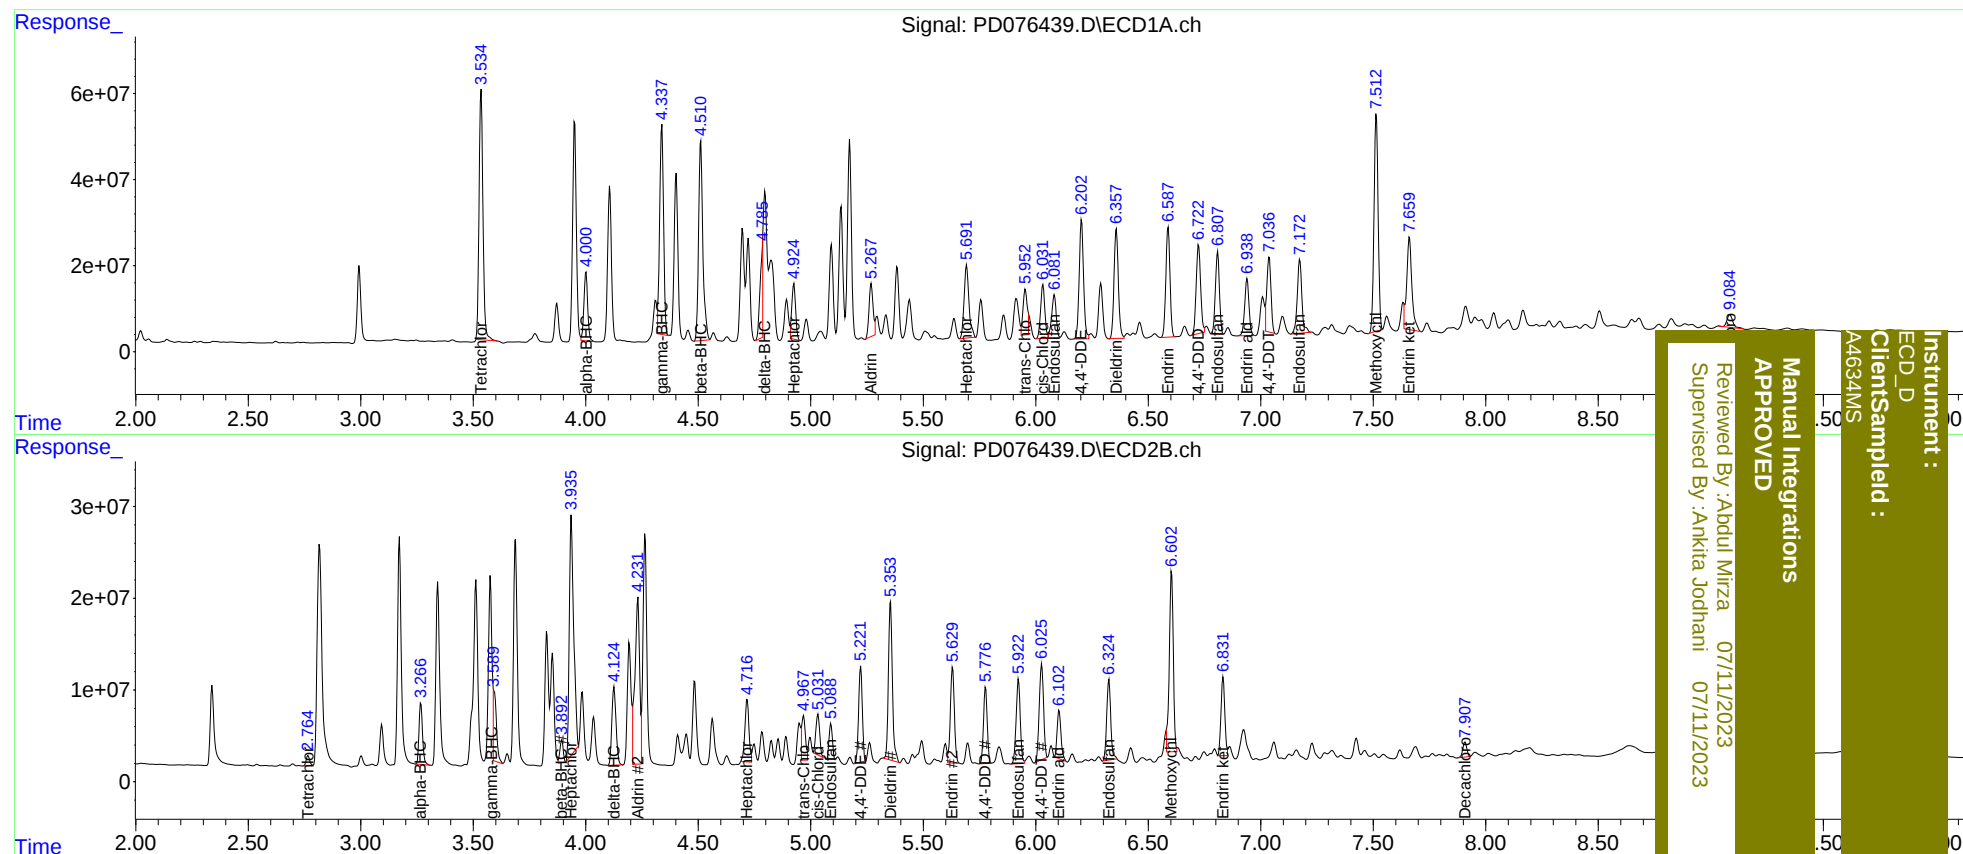

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 07/11/2023
Supervised By: Ankita Jodhani 07/11/2023

Instrument :
ECD_D
Client Sampled :
A4634MS