

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070925\
 Data File : PD089418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 18:33
 Operator : AR\AJ
 Sample : Q2529-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-98

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/10/2025
 Supervised By : mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:47:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.878	51122413	334.1E6	17.918	19.707m
28)	SA Decachlor...	9.071	8.071	56264790	304.4E6	14.325	15.396

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070925\
Data File : PD089418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2025 18:33
Operator : AR\AJ
Sample : Q2529-05
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-98


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/10/2025
Supervised By : mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:47:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 05:39:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

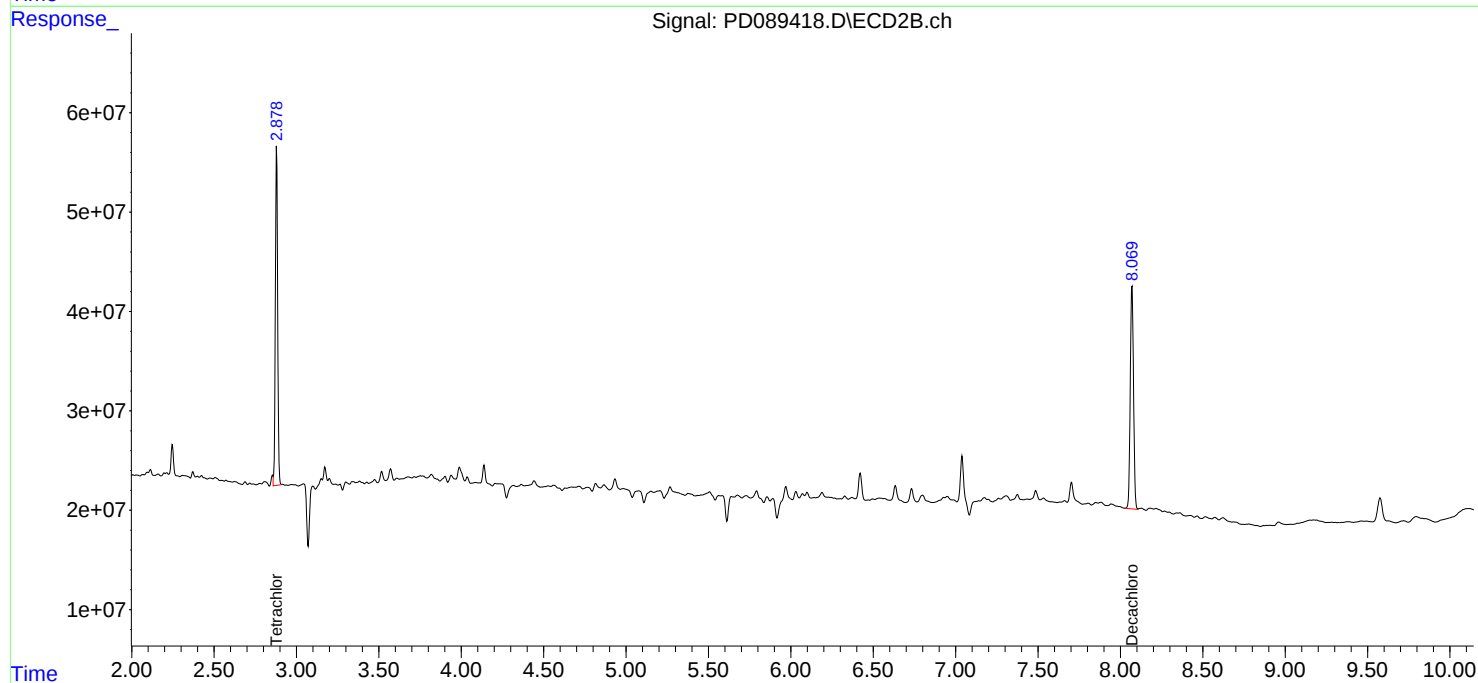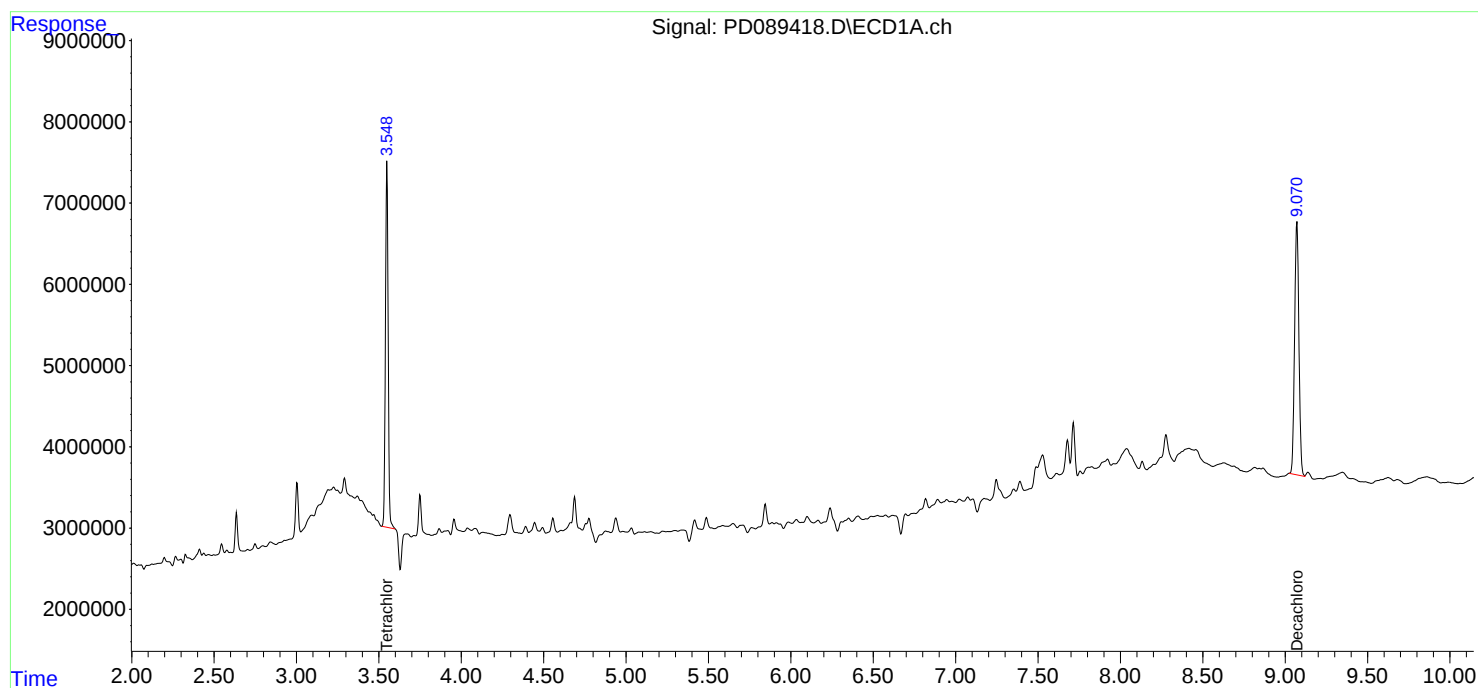

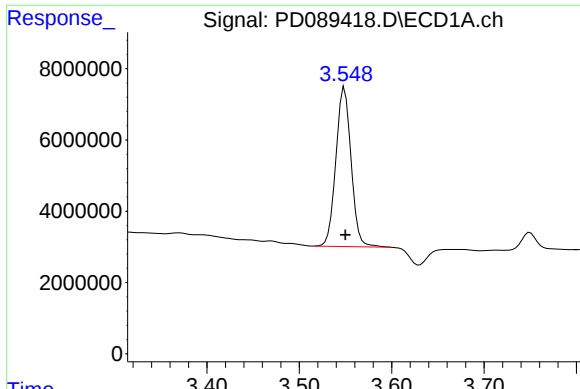


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 51122413
Conc: 17.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-98


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/10/2025
Supervised By :mohammad ahmed 07/11/2025

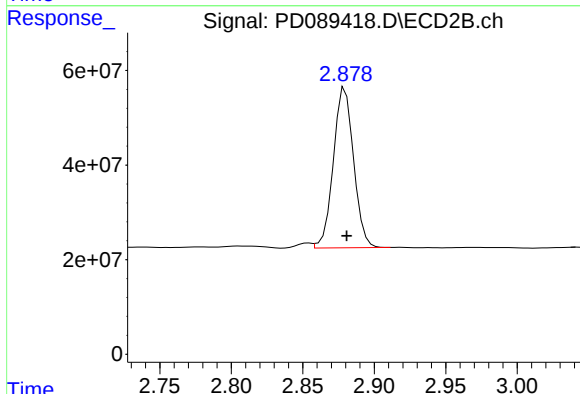


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: -0.003 min
Response: 334102966
Conc: 19.71 ng/ml m

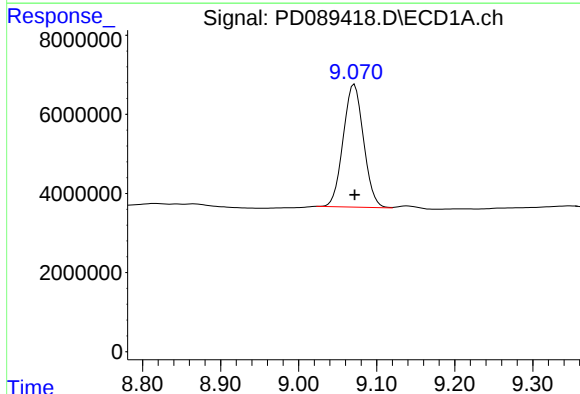

#28 Decachlorobiphenyl

R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 56264790
Conc: 14.33 ng/ml

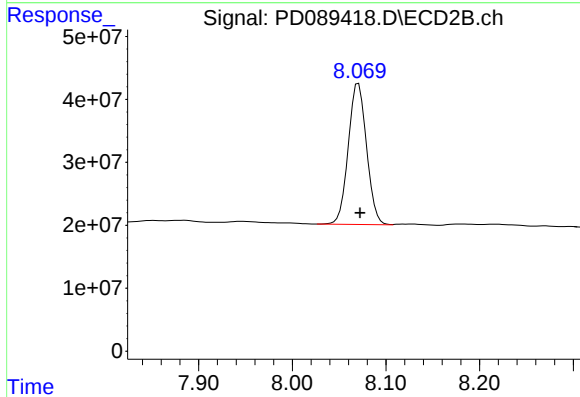

#28 Decachlorobiphenyl

R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 304376987
Conc: 15.40 ng/ml