

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 10:39
 Operator : AJ\MA
 Sample : PB130044BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 14:23:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.213	3.867	34869217	48758412	19.124	19.734
28)	SA Decachlor...	7.852	8.863	34981655	43084362	19.371	19.761
Target Compounds							
2)	A alpha-BHC	0.000	4.245	0	573291	N.D.	0.152 #
3)	MA gamma-BHC...	0.000	4.532	0	1714499	N.D.	0.496 #
6)	B beta-BHC	0.000	4.724f	0	3180802	N.D.	2.246 #
10)	B gamma-Chl...	0.000	5.940	0	1236580	N.D.	0.425 #
11)	B alpha-Chl...	0.000	6.019	0	1204612	N.D.	0.419 #
15)	B Endosulfa...	0.000	6.774f	0	1038069	N.D.	0.421 #
25)	Chlordane-3	0.000	5.940	0	1236580	N.D.	3.325 #
26)	Chlordane-4	0.000	6.019	0	1204612	N.D.	2.769 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 10:39
Operator : AJ\MA
Sample : PB130044BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 14:23:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

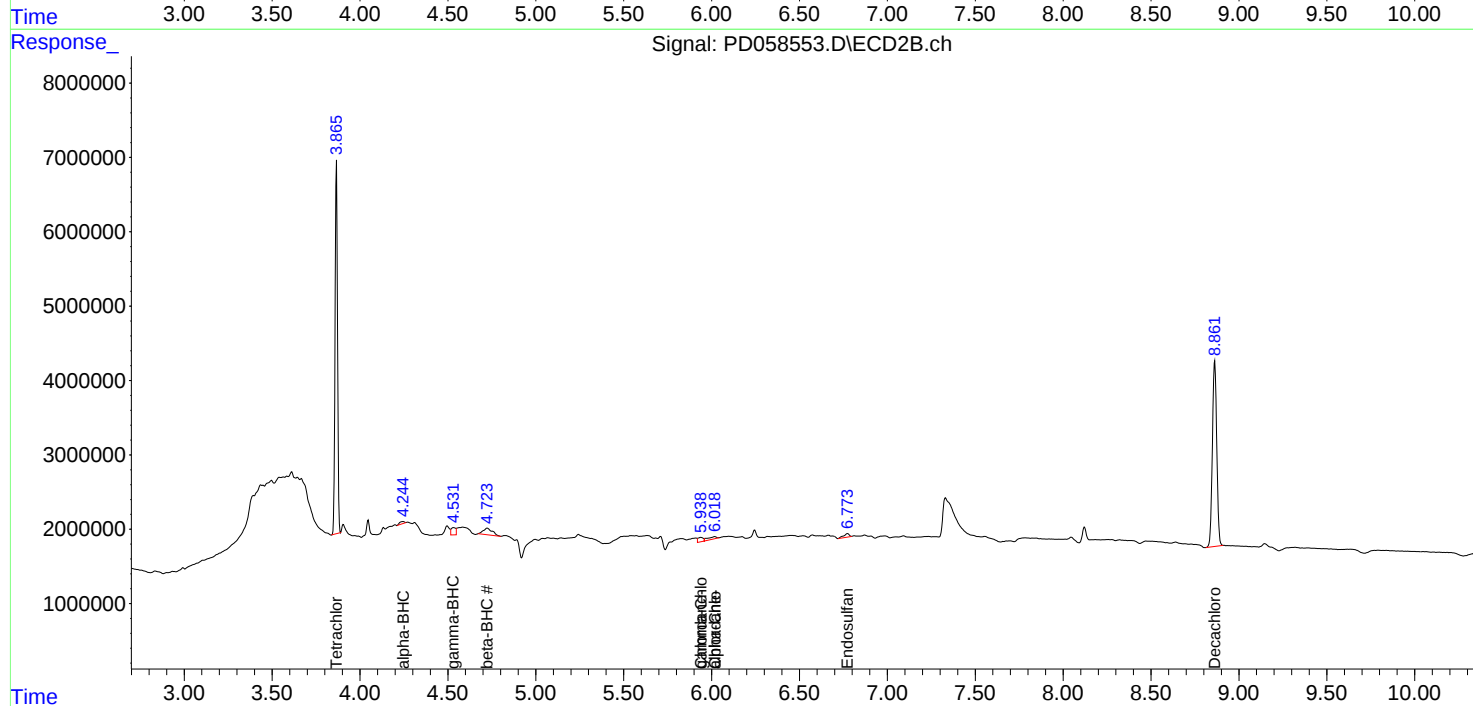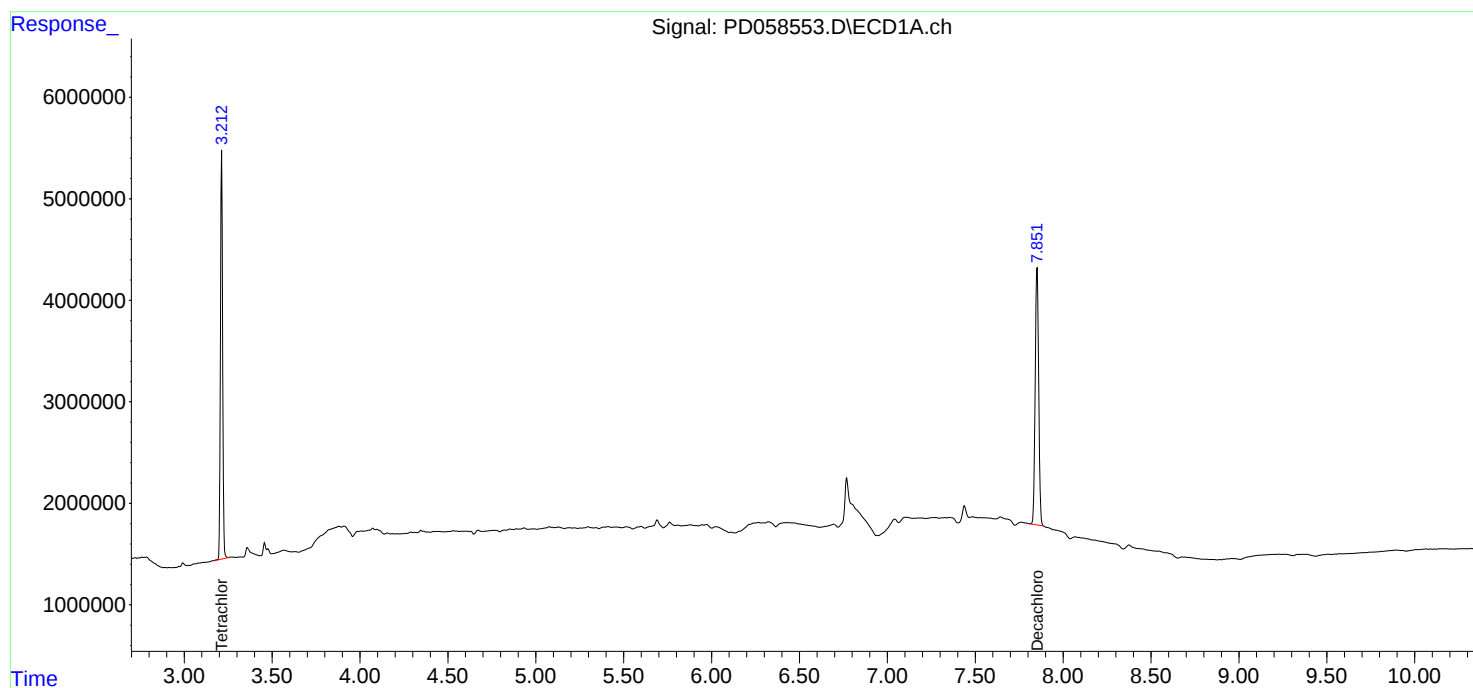


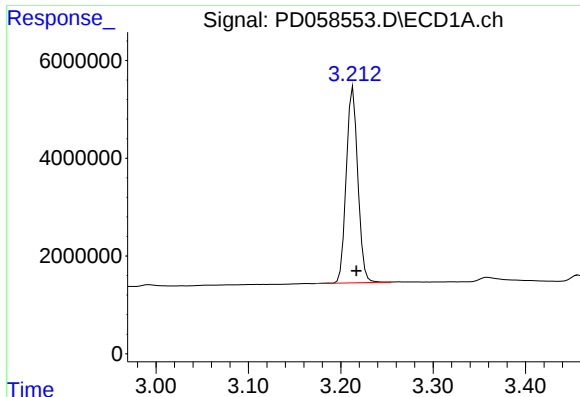

#1 Tetrachloro-m-xylene


R.T.: 3.213 min
Delta R.T.: -0.004 min
Response: 34869217
Conc: 19.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

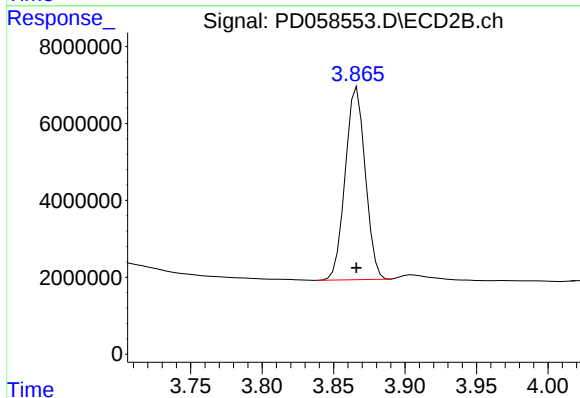


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 48758412
Conc: 19.73 ng/ml

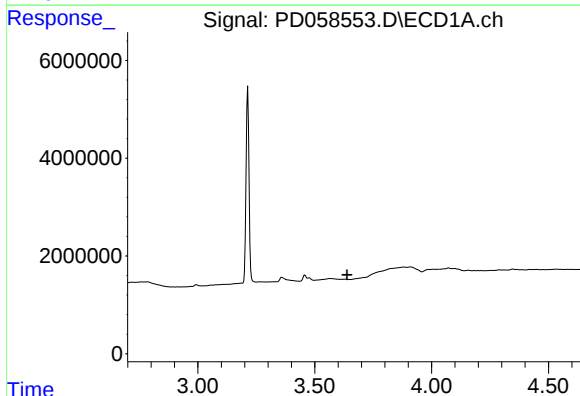


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.639 min
Response: 0
Conc: N.D.

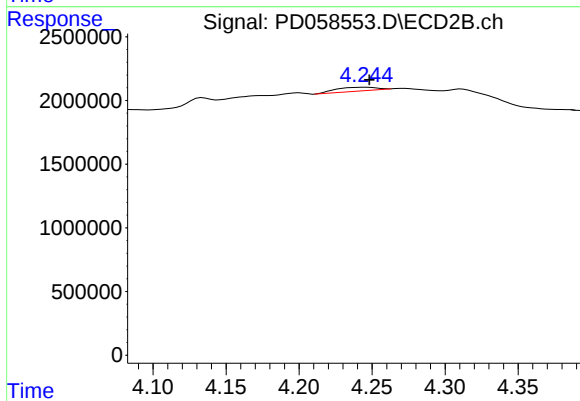

#2 alpha-BHC


R.T.: 4.245 min
Delta R.T.: -0.003 min
Response: 573291
Conc: 0.15 ng/ml

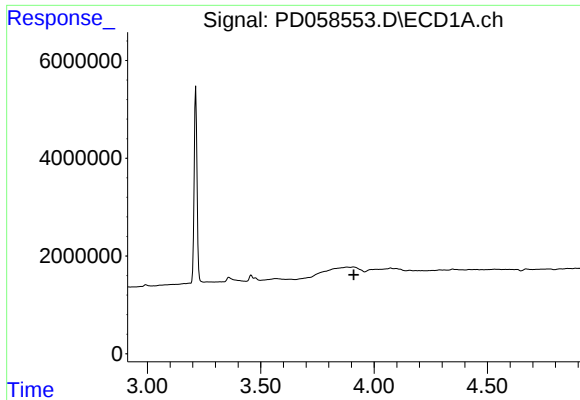

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

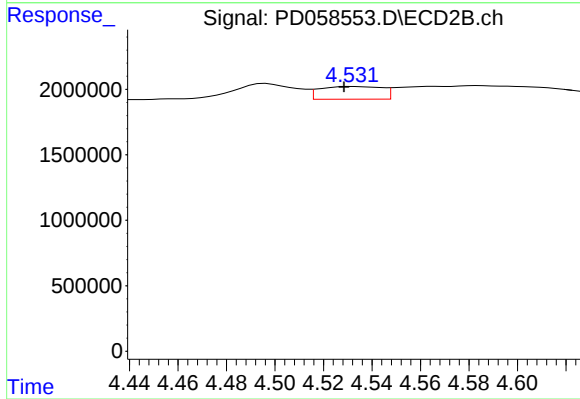


#3 gamma-BHC (Lindane)

R.T.: 4.532 min
Delta R.T.: 0.004 min
Response: 1714499
Conc: 0.50 ng/ml

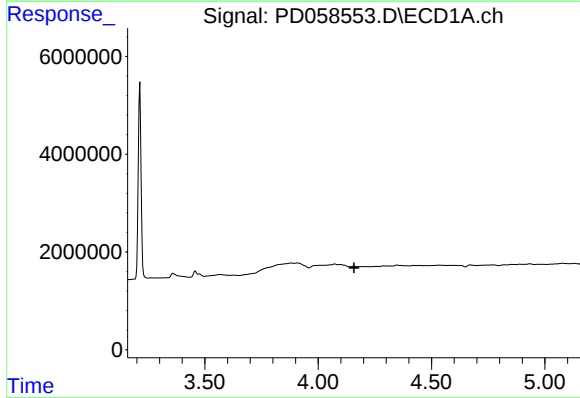


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

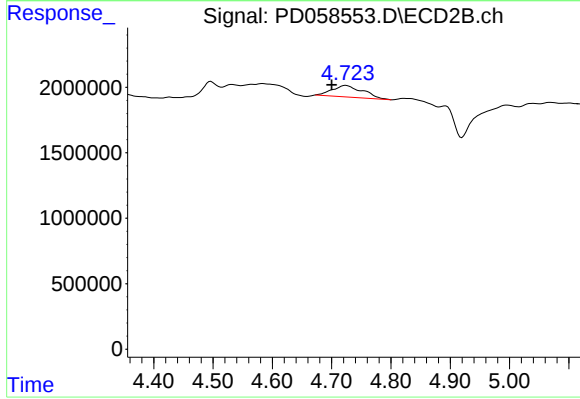

#6 beta-BHC


R.T.: 4.724 min
Delta R.T.: 0.024 min
Response: 3180802
Conc: 2.25 ng/ml

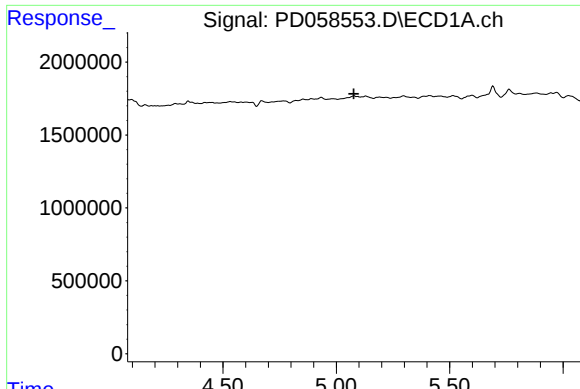

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

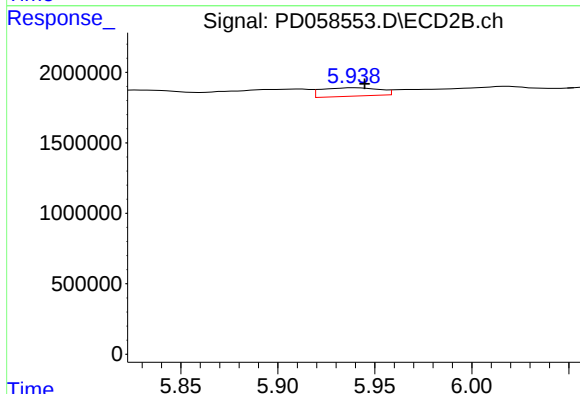


#10 gamma-Chlordane

R.T.: 5.940 min
Delta R.T.: -0.005 min
Response: 1236580
Conc: 0.42 ng/ml

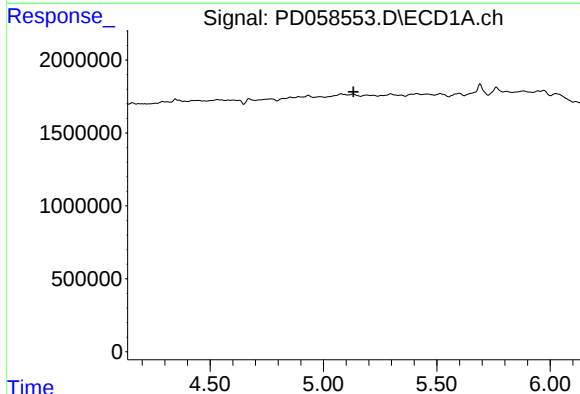


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

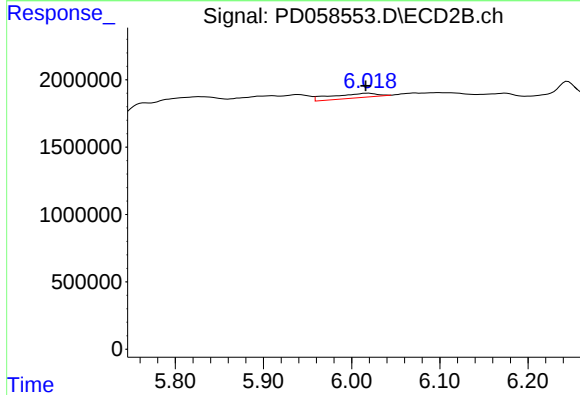

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.003 min
Response: 1204612
Conc: 0.42 ng/ml

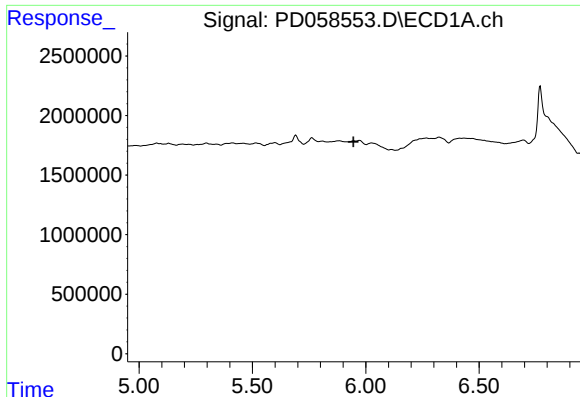

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

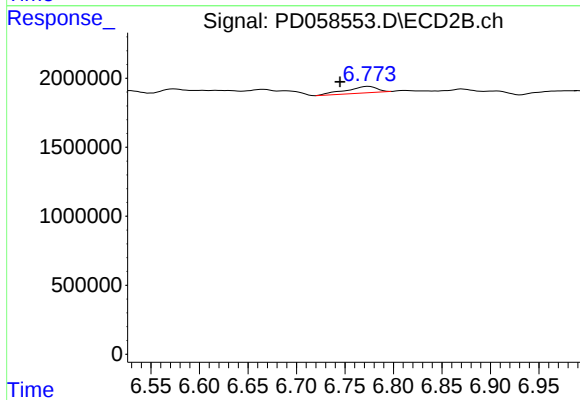


#15 Endosulfan II

R.T.: 6.774 min
Delta R.T.: 0.030 min
Response: 1038069
Conc: 0.42 ng/ml

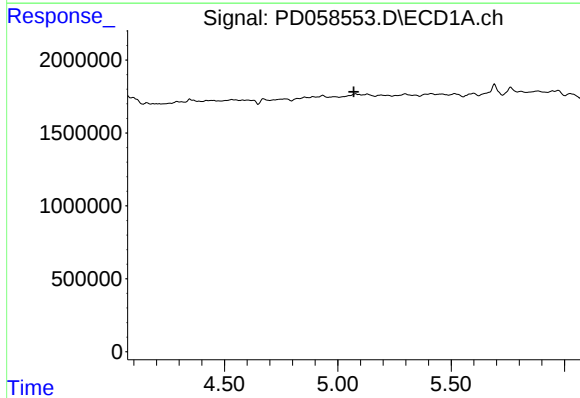


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

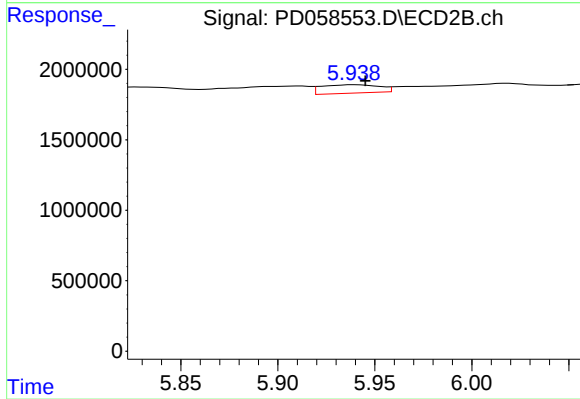

#25 Chlordane-3


R.T.: 5.940 min
Delta R.T.: -0.006 min
Response: 1236580
Conc: 3.32 ng/ml

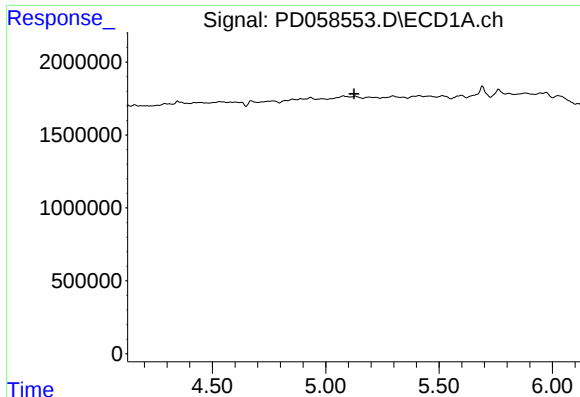

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

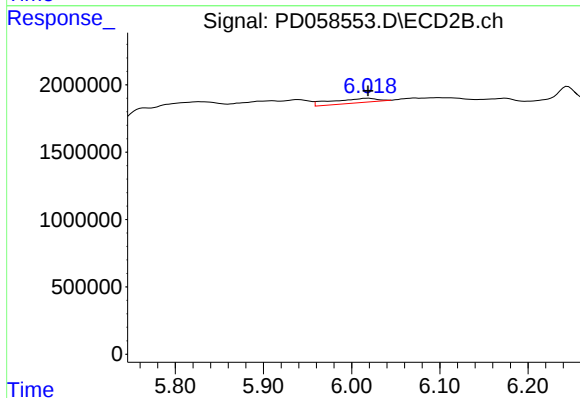


#26 Chlorodane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 1204612
Conc: 2.77 ng/ml

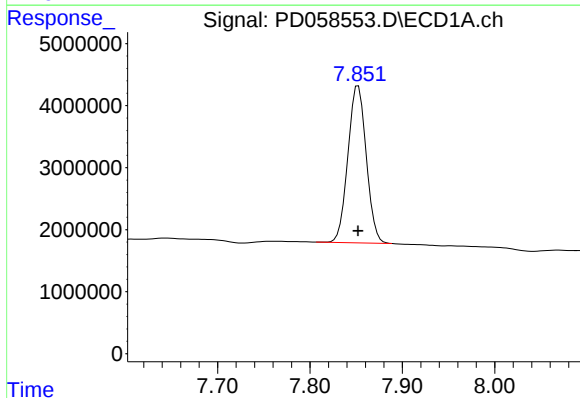

#28 Decachlorobiphenyl

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 34981655
Conc: 19.37 ng/ml

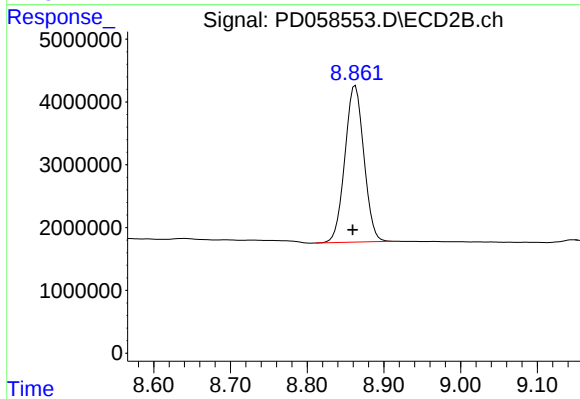

#28 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.004 min
Response: 43084362
Conc: 19.76 ng/ml