

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 15:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 16:15:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.867	31054097	42578386	17.032	17.233
28)	SA Decachlor...	7.848	8.863	27101737	31642405	15.008	14.513
Target Compounds							
8)	B Heptachlo...	0.000	5.712	0	10061661	N.D.	3.456 #
9)	A Endosulfan I	0.000	6.090f	0	1073960	N.D.	0.407 #
10)	B gamma-Chl...	0.000	5.938	0	5187682	N.D.	1.783 #
11)	B alpha-Chl...	0.000	6.031	0	2301949	N.D.	0.800 #
25)	Chlordane-3	0.000	5.938	0	5187682	N.D.	13.947 #
26)	Chlordane-4	0.000	6.031	0	2301949	N.D.	5.292 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 15:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 16:15:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

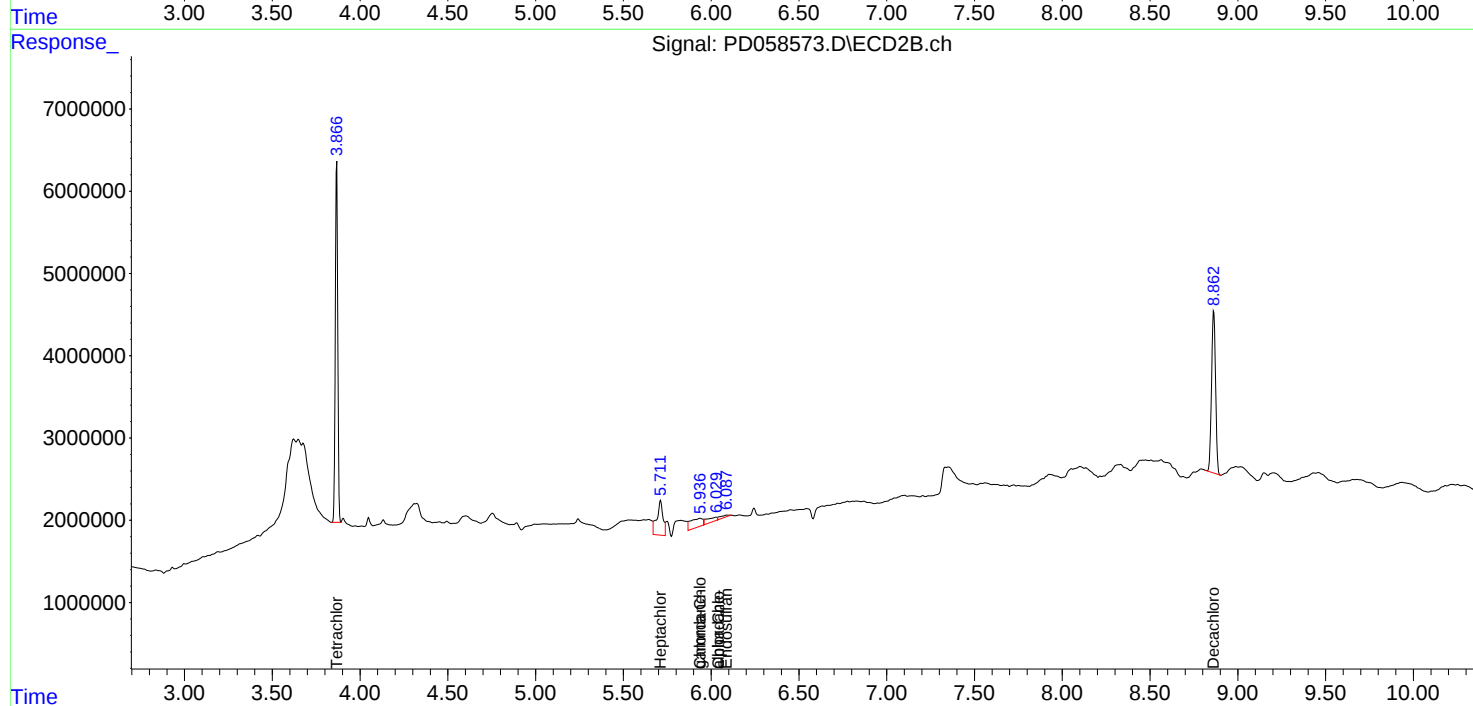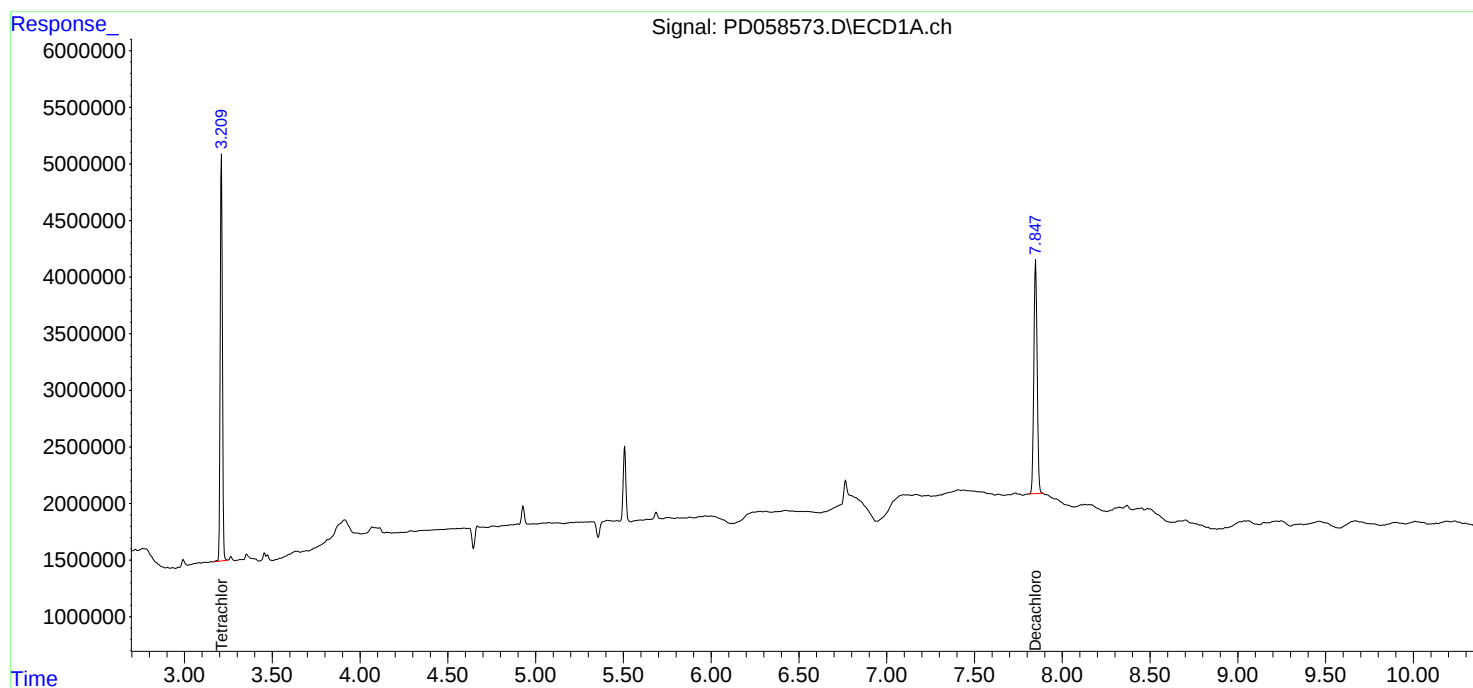


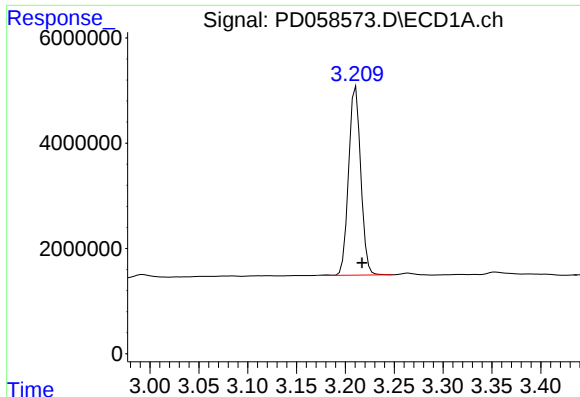

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: -0.006 min
Response: 31054097
Conc: 17.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

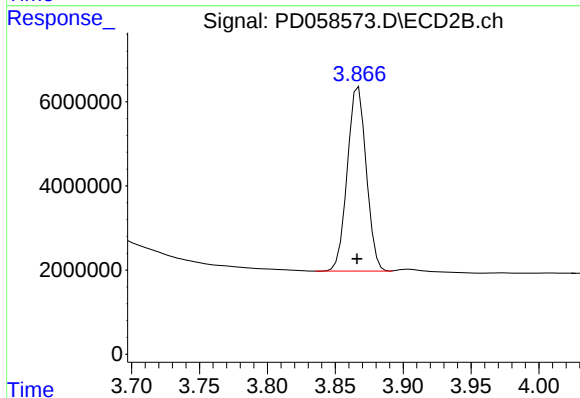


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.001 min
Response: 42578386
Conc: 17.23 ng/ml

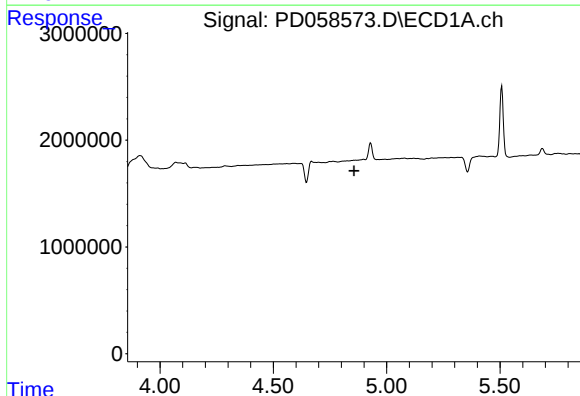


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

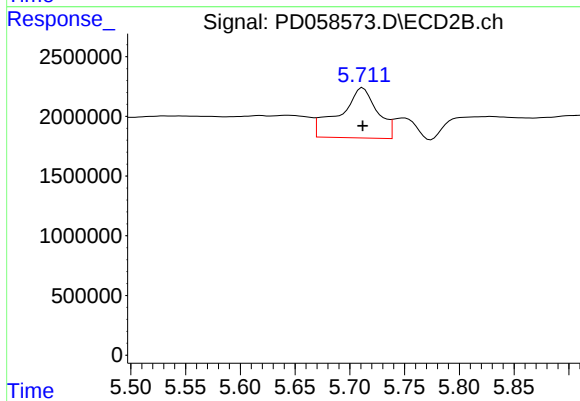

#8 Heptachlor epoxide


R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 10061661
Conc: 3.46 ng/ml

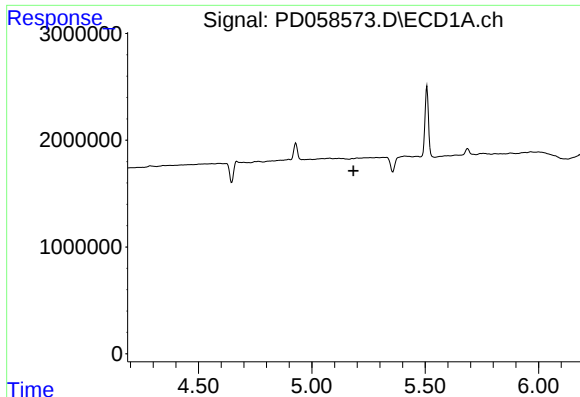

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

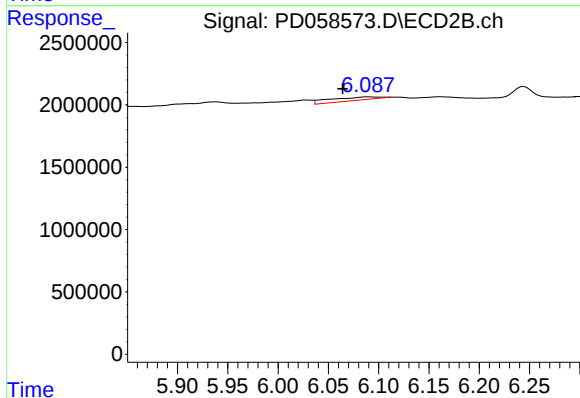


#9 Endosulfan I

R.T.: 6.090 min
Delta R.T.: 0.026 min
Response: 1073960
Conc: 0.41 ng/ml

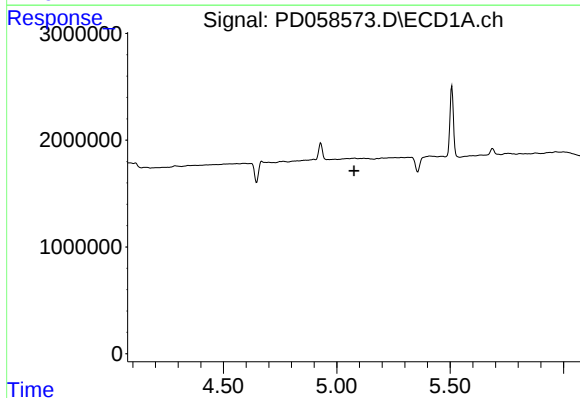


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

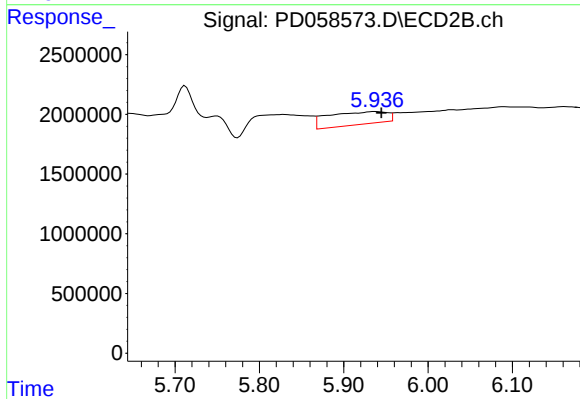

#10 gamma-Chlordane


R.T.: 5.938 min
Delta R.T.: -0.007 min
Response: 5187682
Conc: 1.78 ng/ml

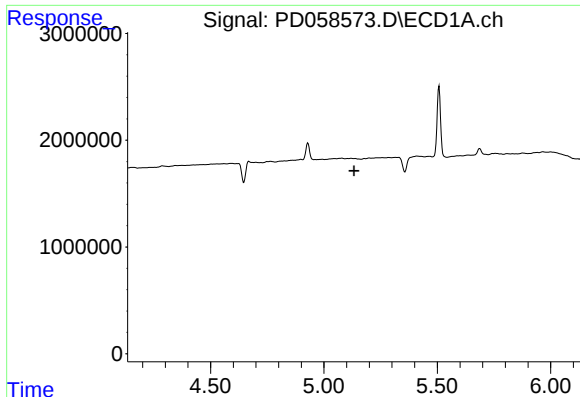

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

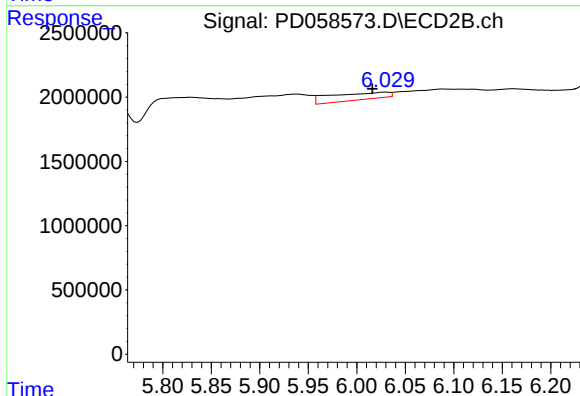


#11 alpha-Chlordane

R.T.: 6.031 min
Delta R.T.: 0.014 min
Response: 2301949
Conc: 0.80 ng/ml

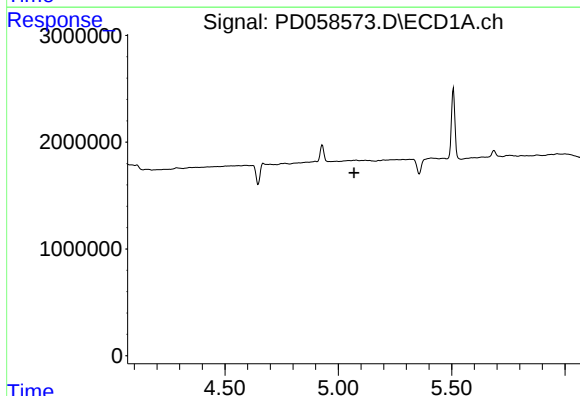


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

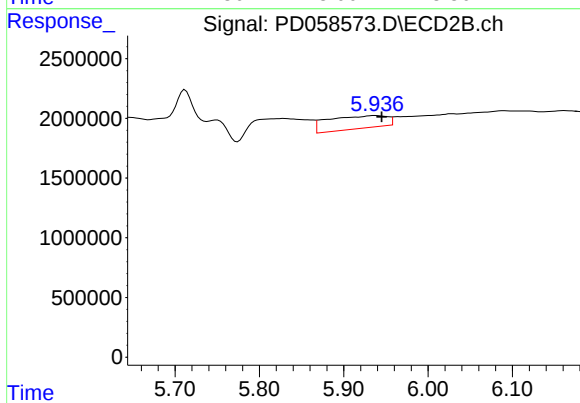

#25 Chlordane-3


R.T.: 5.938 min
Delta R.T.: -0.007 min
Response: 5187682
Conc: 13.95 ng/ml

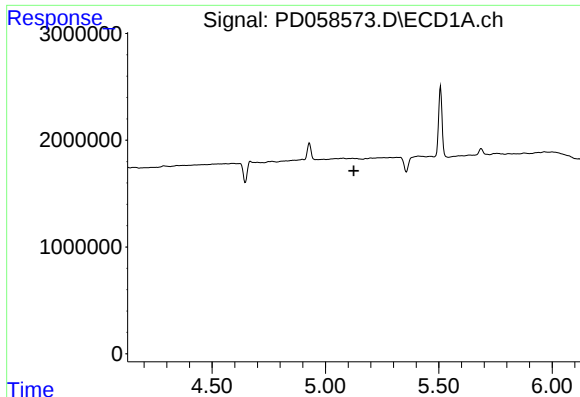

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

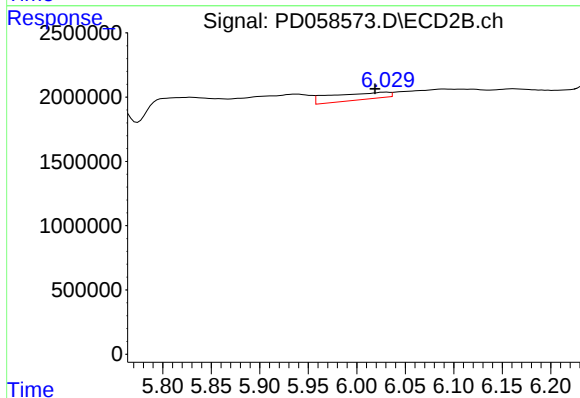


#26 Chlordane-4

R.T.: 6.031 min
Delta R.T.: 0.012 min
Response: 2301949
Conc: 5.29 ng/ml

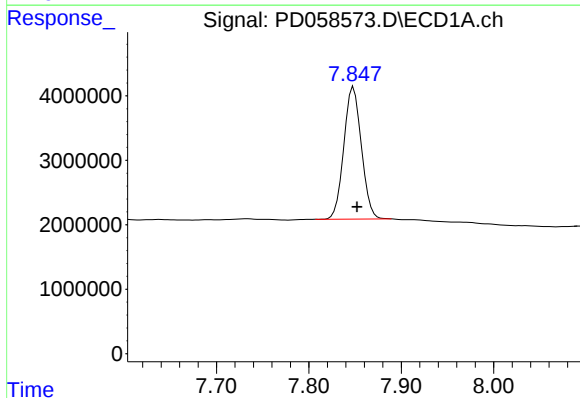

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: -0.004 min
Response: 27101737
Conc: 15.01 ng/ml

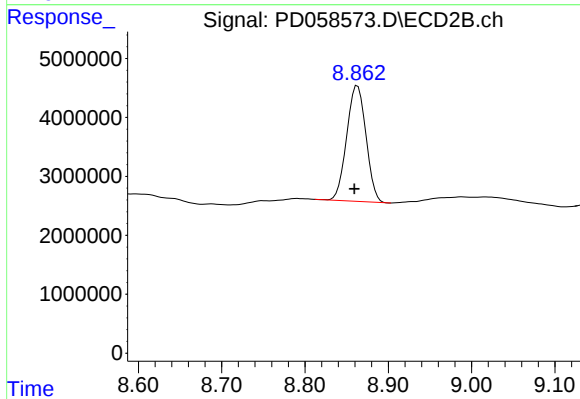

#28 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.004 min
Response: 31642405
Conc: 14.51 ng/ml