

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 19:30
 Operator : AJ\MA
 Sample : L3258-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 06:27:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	31804588	43262663	17.443	17.510
28)	SA Decachlor...	7.849	8.865	28768615	33124896	15.931	15.193
Target Compounds							
7)	B delta-BHC	0.000	4.889f	0	2281772	N.D.	0.742 #
8)	B Heptachlo...	0.000	5.710	0	5678399	N.D.	1.951 #
9)	A Endosulfan I	0.000	6.086f	0	1363305	N.D.	0.517 #
10)	B gamma-Chl...	0.000	5.930	0	2007834	N.D.	0.690 #
15)	B Endosulfa...	0.000	6.771f	0	1664610	N.D.	0.675 #
18)	B Endrin al...	0.000	6.873	0	624199	N.D.	0.292 #
19)	B Endosulfa...	0.000	7.092	0	1335075	N.D.	0.582 #
21)	B Endrin ke...	0.000	7.574f	0	3451454	N.D.	1.268 #
25)	Chlordane-3	0.000	5.930f	0	2007834	N.D.	5.398 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 19:30
Operator : AJ\MA
Sample : L3258-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 06:27:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

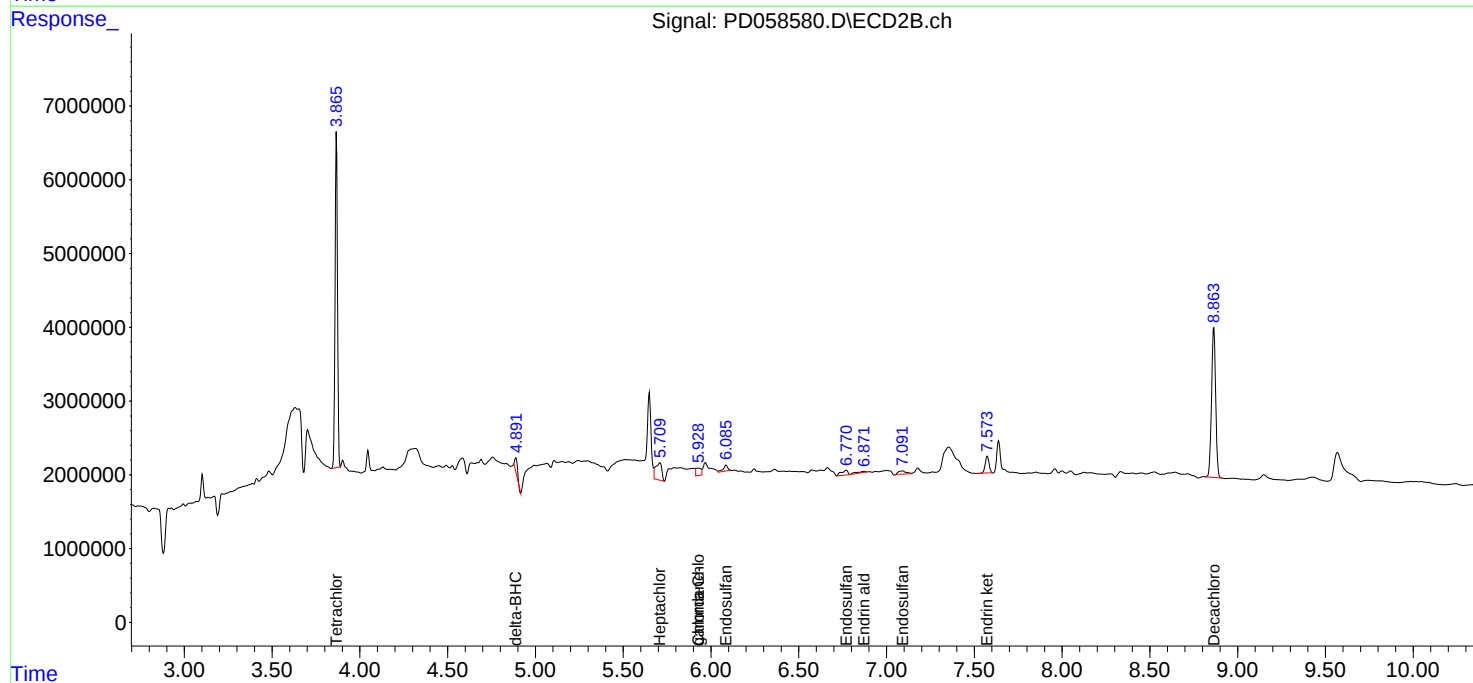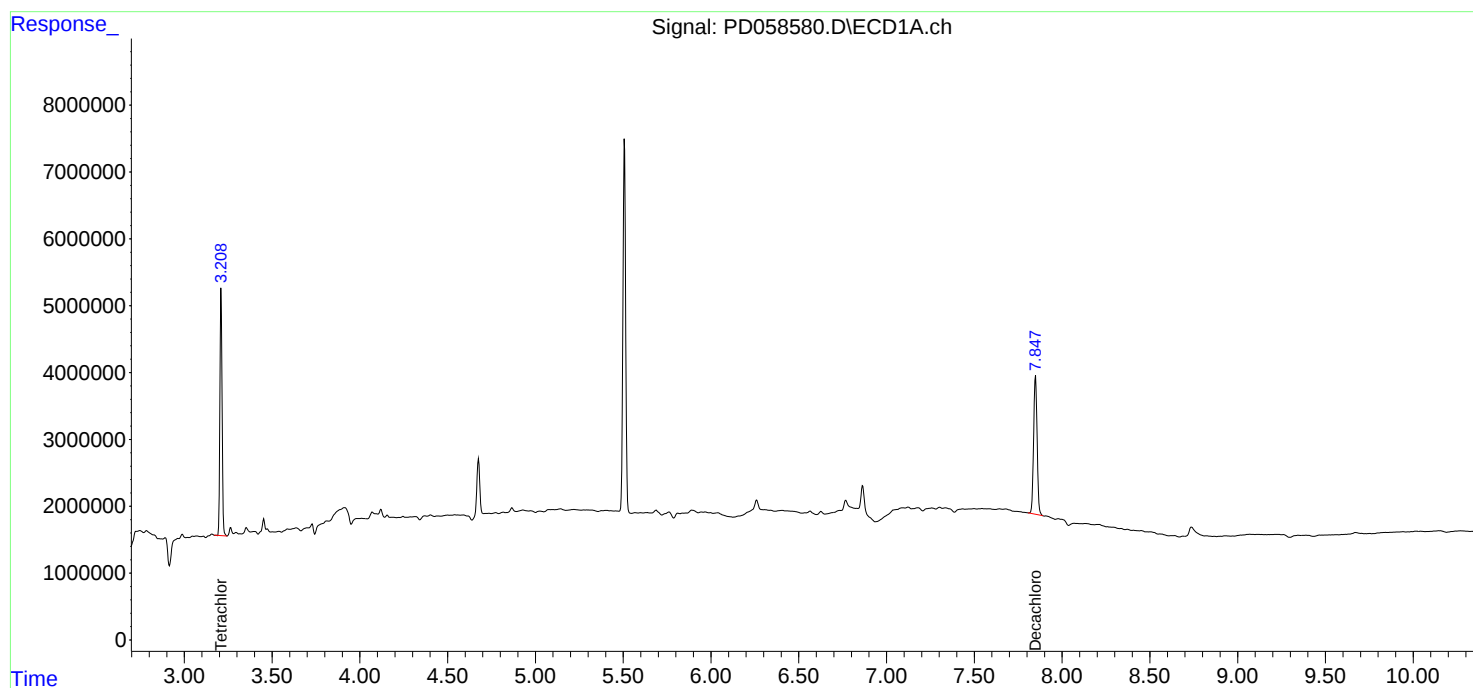


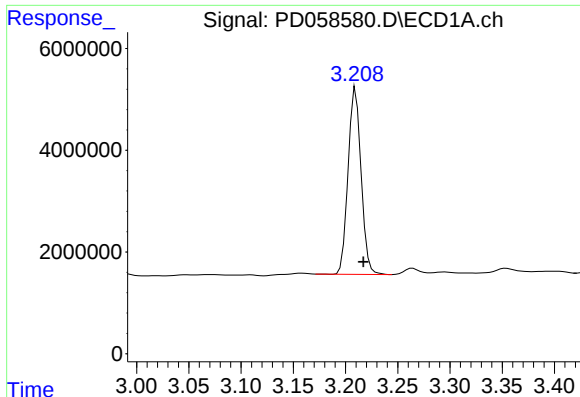

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: -0.007 min
Response: 31804588
Conc: 17.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

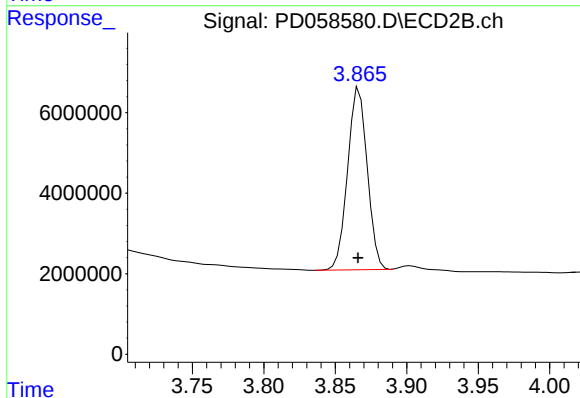


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 43262663
Conc: 17.51 ng/ml

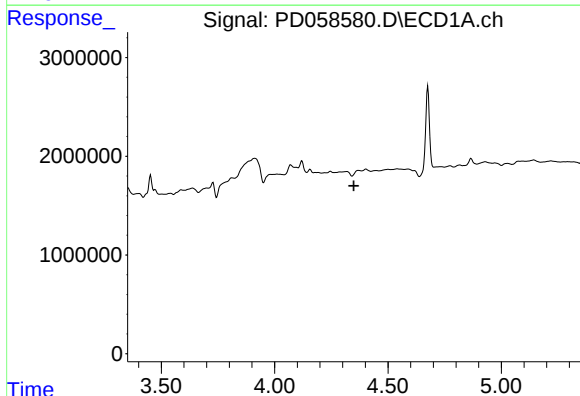


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

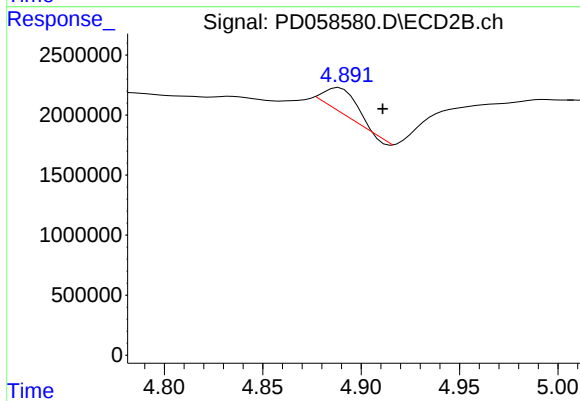

#7 delta-BHC


R.T.: 4.889 min
Delta R.T.: -0.022 min
Response: 2281772
Conc: 0.74 ng/ml

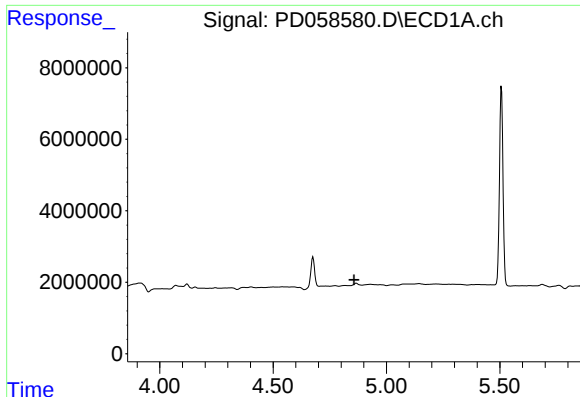

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

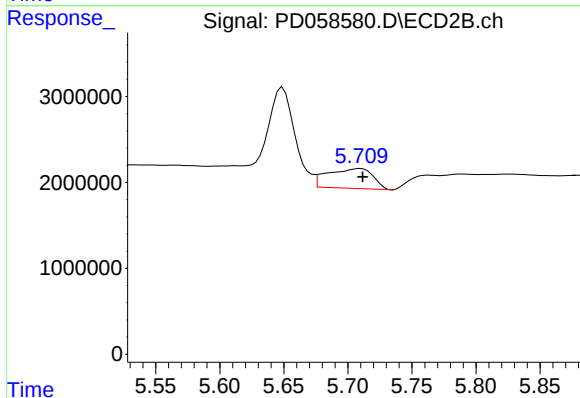


#8 Heptachlor epoxide

R.T.: 5.710 min
Delta R.T.: -0.002 min
Response: 5678399
Conc: 1.95 ng/ml

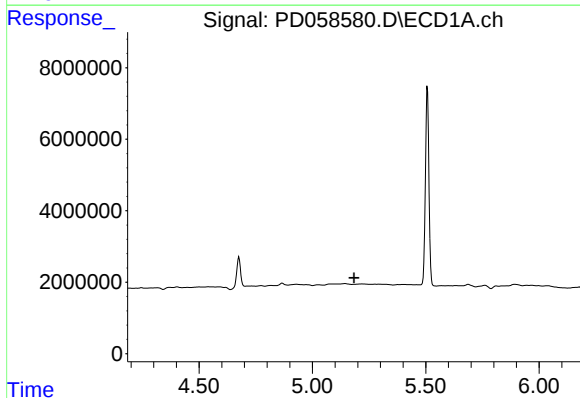


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

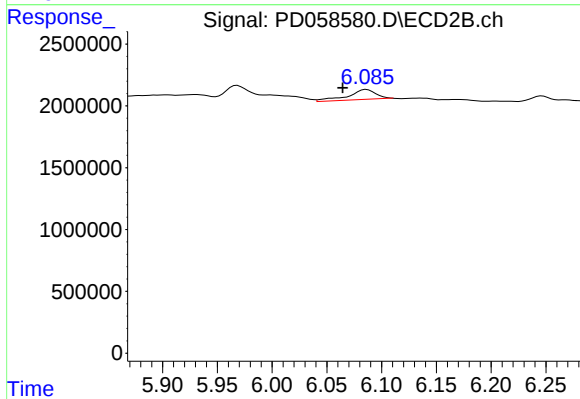

#9 Endosulfan I


R.T.: 6.086 min
Delta R.T.: 0.022 min
Response: 1363305
Conc: 0.52 ng/ml

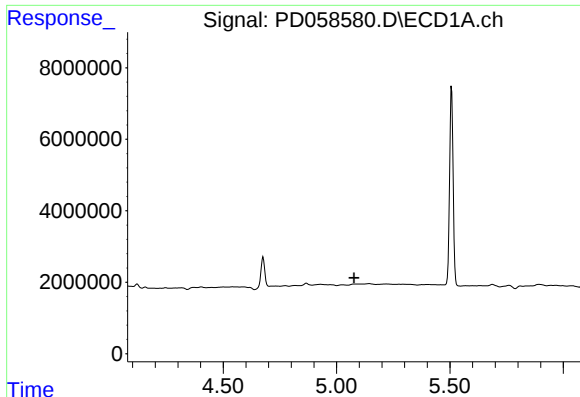

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

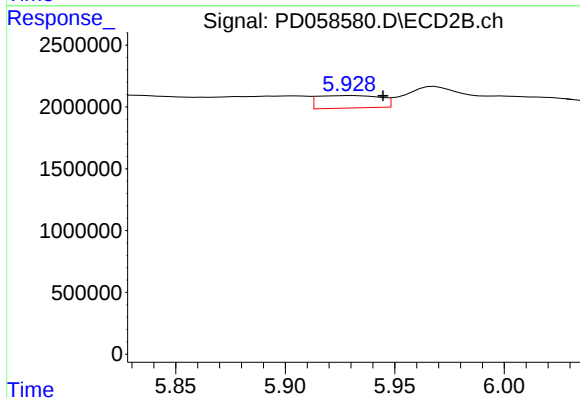


#10 gamma-Chlordane

R.T.: 5.930 min
Delta R.T.: -0.014 min
Response: 2007834
Conc: 0.69 ng/ml

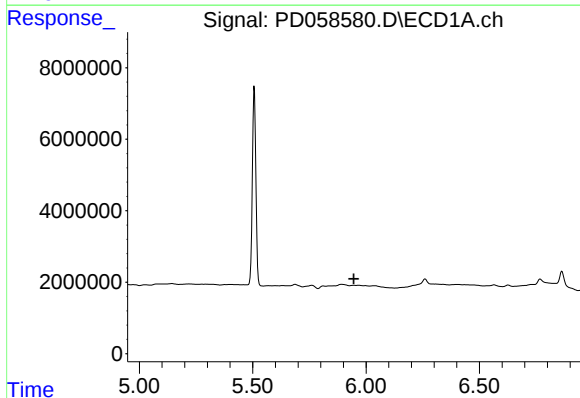


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.946 min
Response: 0
Conc: N.D.

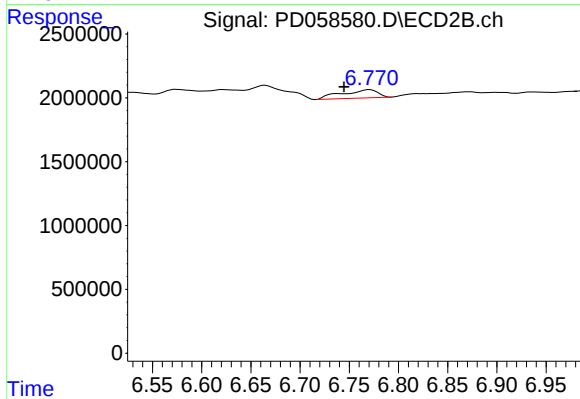

#15 Endosulfan II


R.T.: 6.771 min
Delta R.T.: 0.026 min
Response: 1664610
Conc: 0.67 ng/ml

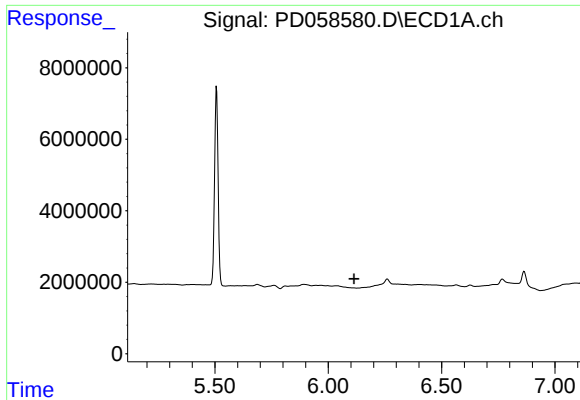

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

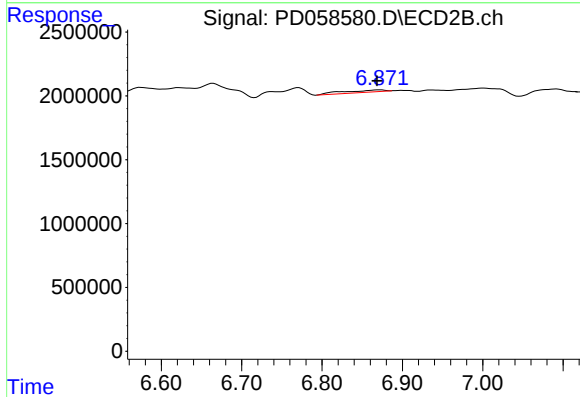


#18 Endrin aldehyde

R.T.: 6.873 min
Delta R.T.: 0.004 min
Response: 624199
Conc: 0.29 ng/ml

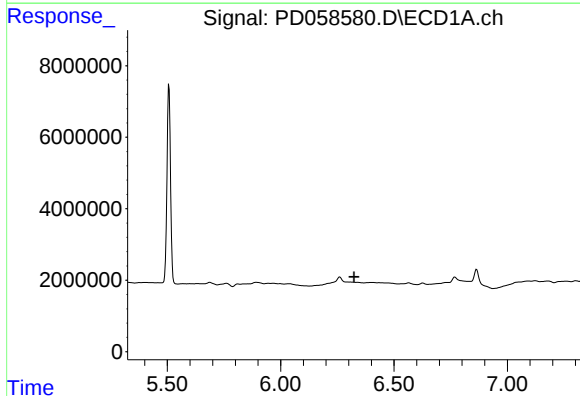


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.324 min
Response: 0
Conc: N.D.

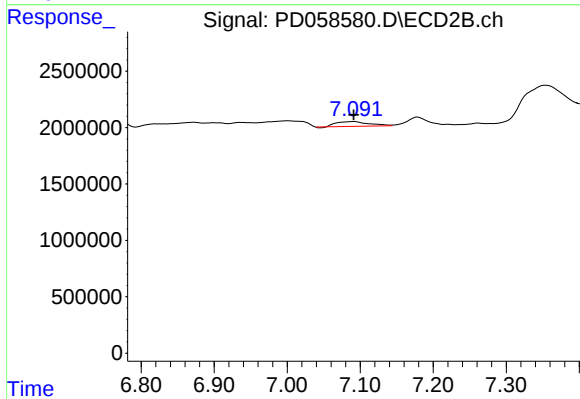

#19 Endosulfan Sulfate


R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 1335075
Conc: 0.58 ng/ml

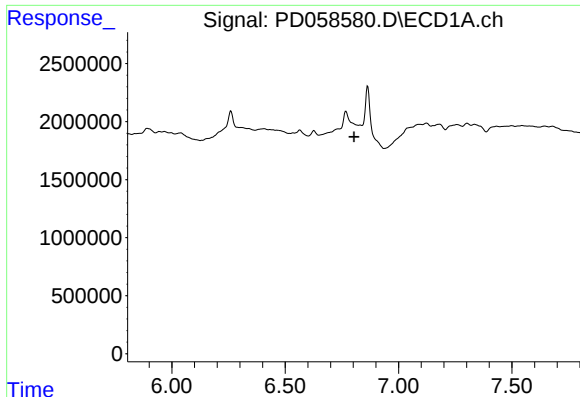

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.804 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

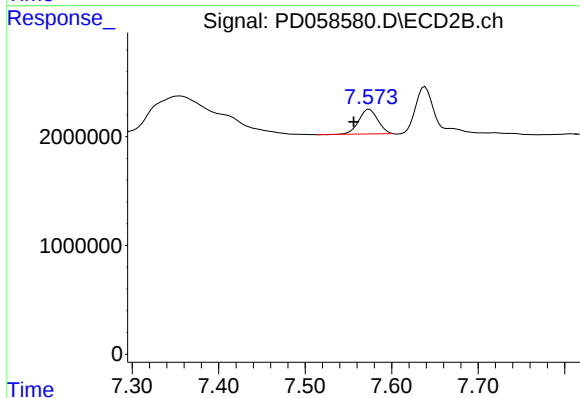


#21 Endrin ketone

R.T.: 7.574 min
Delta R.T.: 0.018 min
Response: 3451454
Conc: 1.27 ng/ml

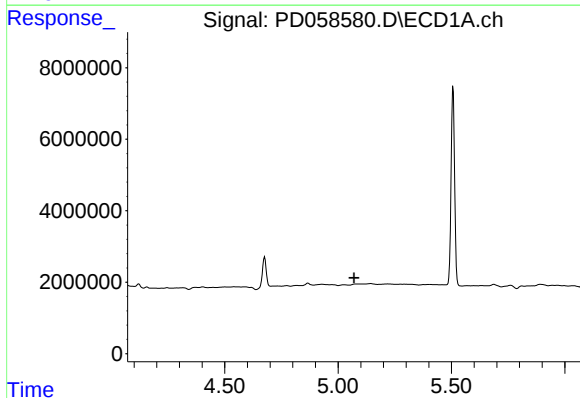


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

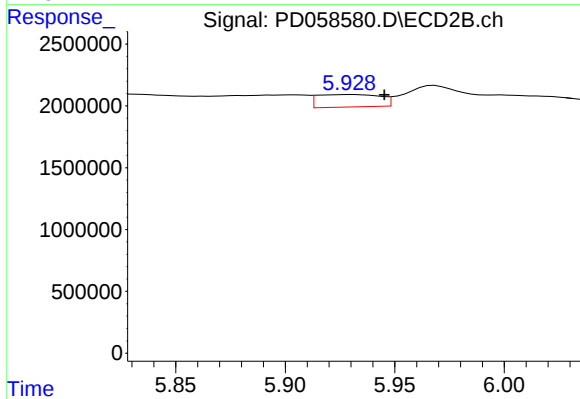

#25 Chlordane-3


R.T.: 5.930 min
Delta R.T.: -0.015 min
Response: 2007834
Conc: 5.40 ng/ml

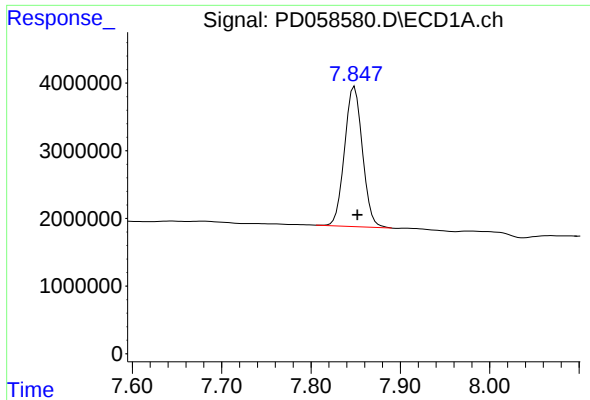

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: -0.003 min
Response: 28768615
Conc: 15.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

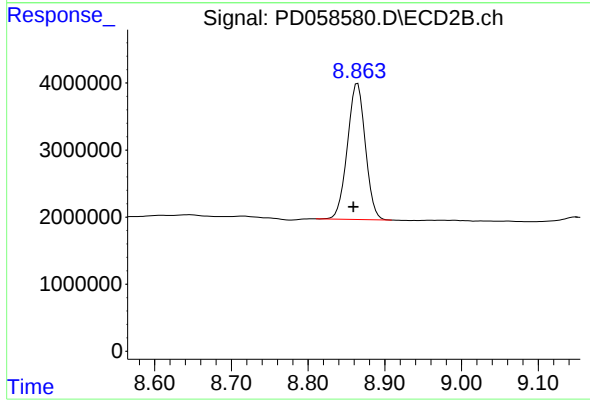

#28 Decachlorobiphenyl

R.T.: 8.865 min
Delta R.T.: 0.005 min
Response: 33124896
Conc: 15.19 ng/ml