

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 19:45
 Operator : AJ\MA
 Sample : L3259-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 06:28:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.233f	3.882f	15276321	17118166	8.378	6.928
28)	SA Decachlor...	7.854	8.869	16519279	21623972	9.148	9.918
Target Compounds							
8)	B Heptachlo...	0.000	5.728f	0	1776159	N.D.	0.610 #
10)	B gamma-Chl...	0.000	5.938	0	2815679	N.D.	0.968 #
12)	B 4,4'-DDE	0.000	6.194f	0	1153333	N.D.	0.420 #
14)	MA Endrin	0.000	6.552f	0	1891744	N.D.	0.889 #
16)	A 4,4'-DDD	0.000	6.688f	0	1642495	N.D.	0.712 #
17)	MA 4,4'-DDT	0.000	6.949	0	2368330	N.D.	1.032 #
23)	Chlordane-1	0.000	4.832	0	2398804	N.D.	26.953 #
25)	Chlordane-3	0.000	5.938	0	2815679	N.D.	7.570 #
27)	Chlordane-5	0.000	6.803	0	1711070	N.D.	21.475 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 19:45
Operator : AJ\MA
Sample : L3259-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 06:28:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

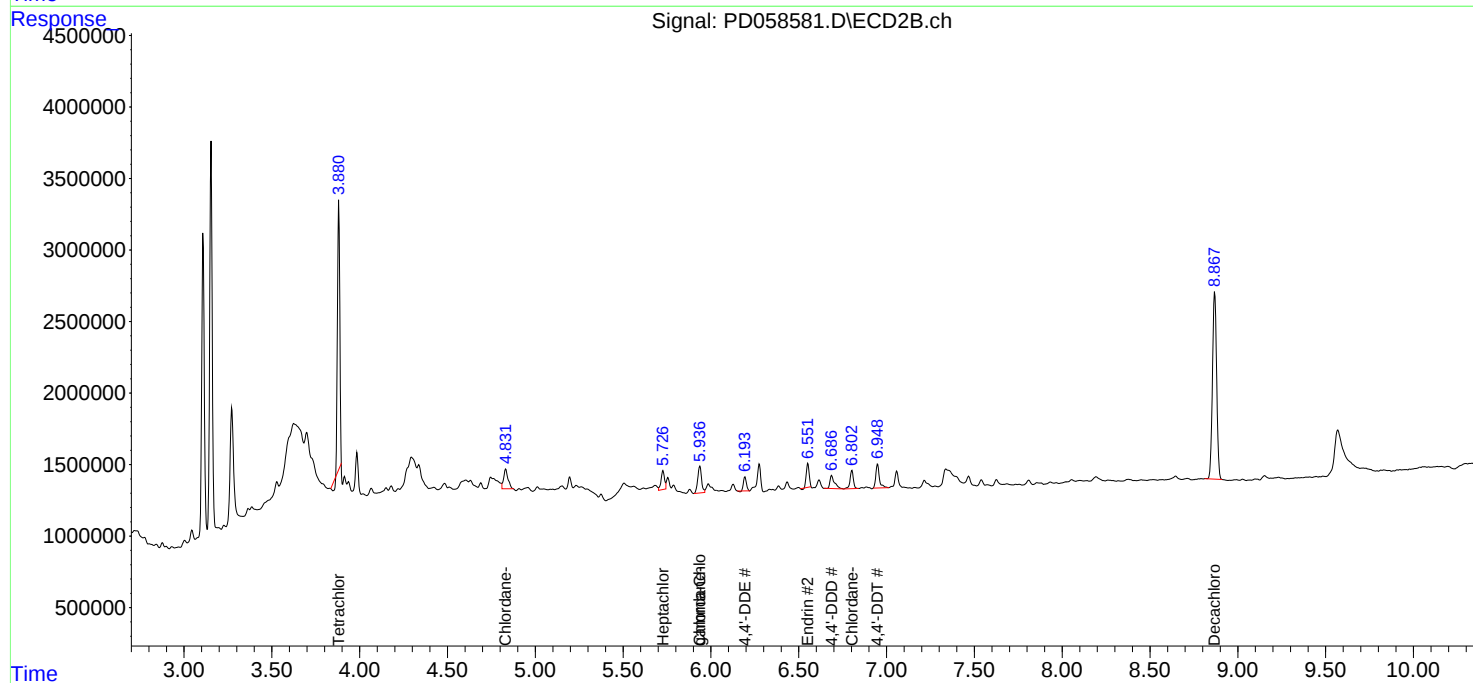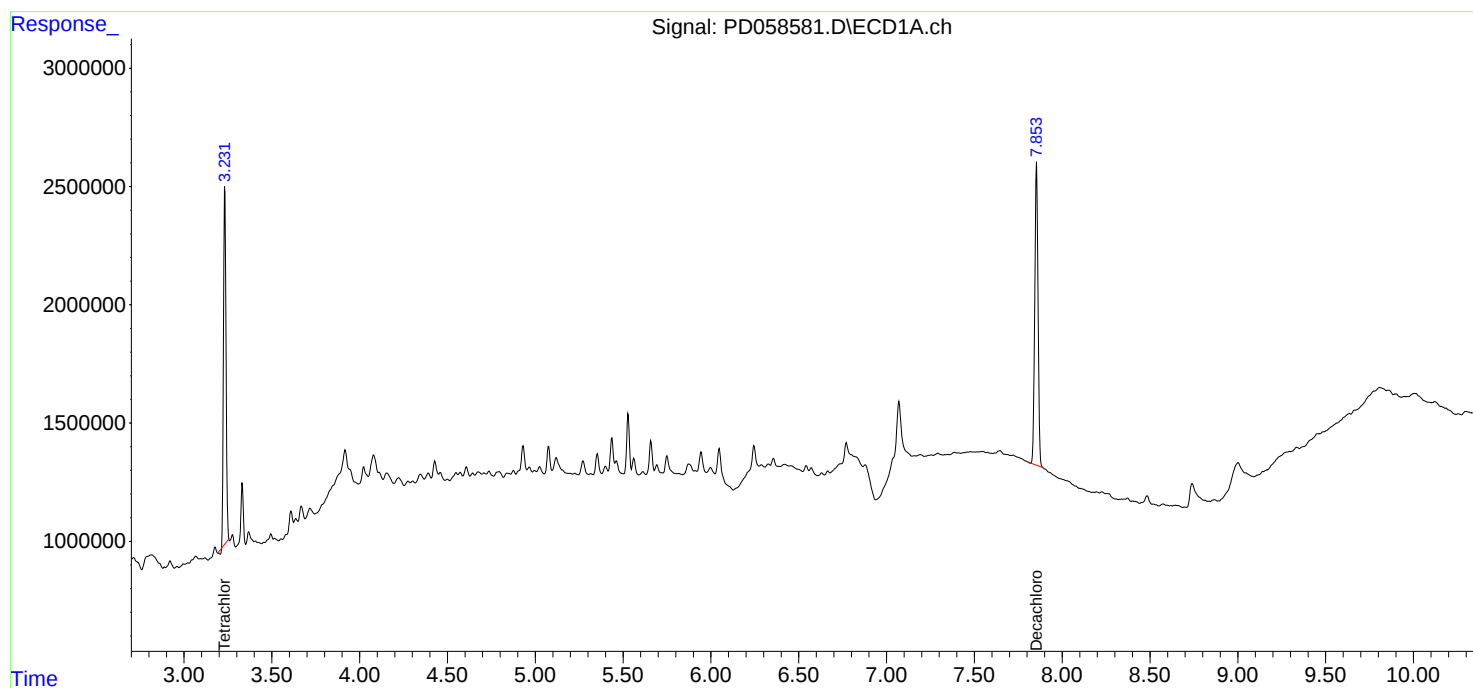


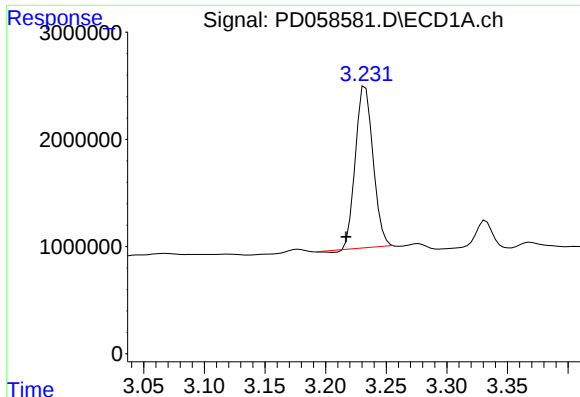

#1 Tetrachloro-m-xylene


R.T.: 3.233 min
Delta R.T.: 0.016 min
Response: 15276321
Conc: 8.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

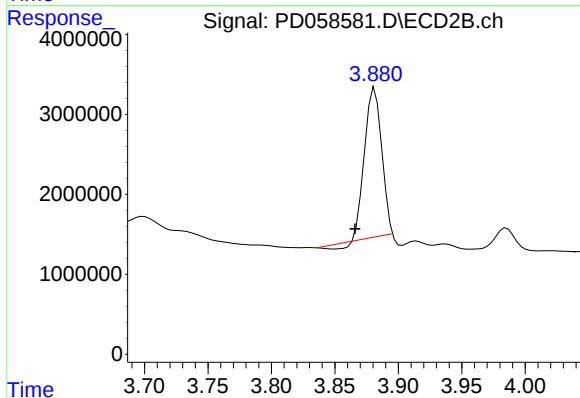


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.016 min
Response: 17118166
Conc: 6.93 ng/ml

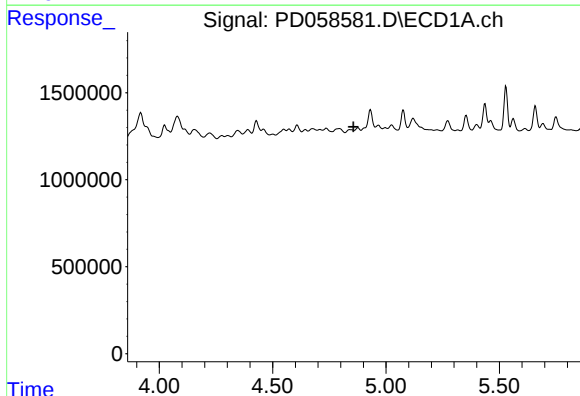


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

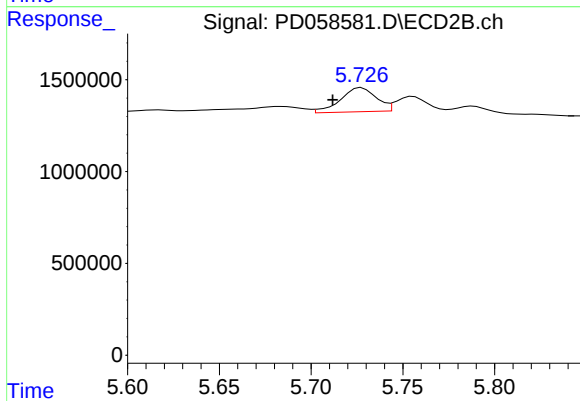

#8 Heptachlor epoxide


R.T.: 5.728 min
Delta R.T.: 0.016 min
Response: 1776159
Conc: 0.61 ng/ml

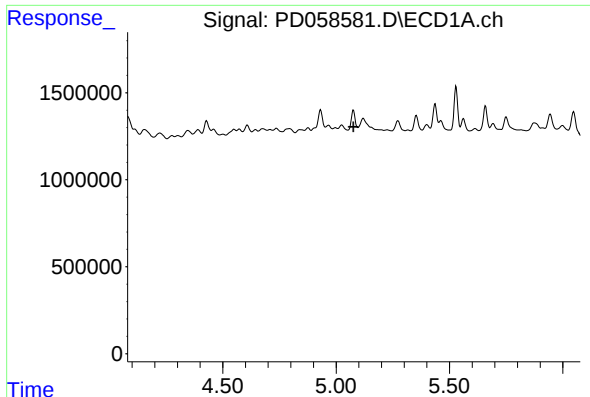

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

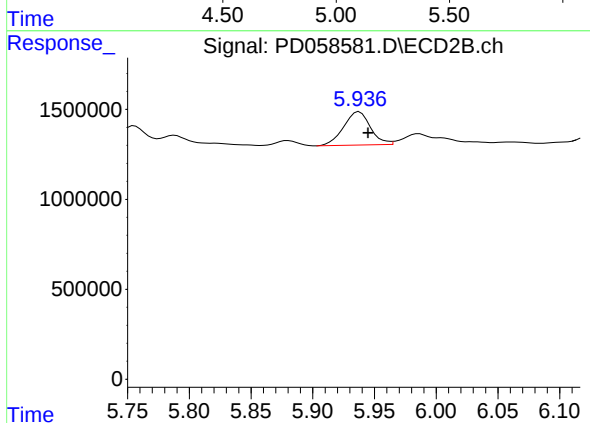


#10 gamma-Chlordane

R.T.: 5.938 min
Delta R.T.: -0.007 min
Response: 2815679
Conc: 0.97 ng/ml

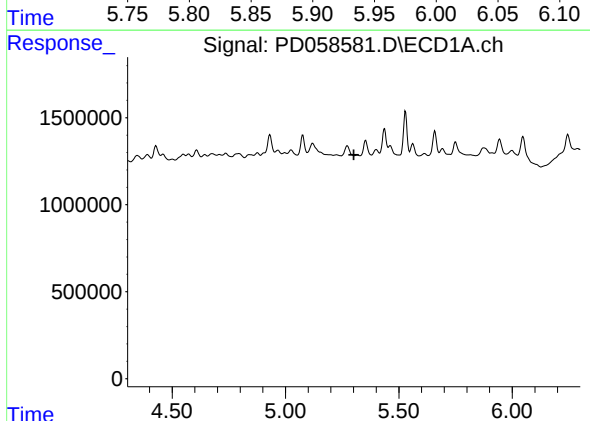


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

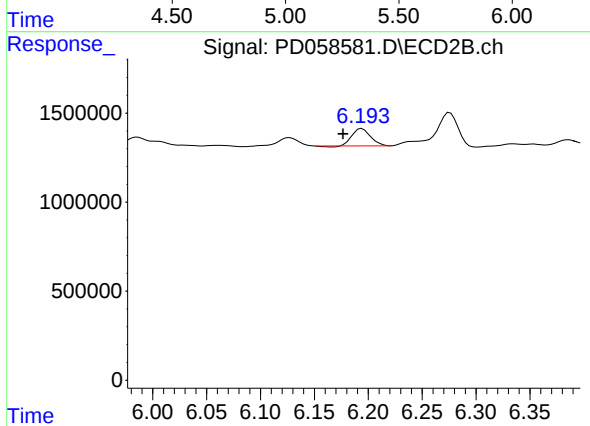

#12 4,4'-DDE


R.T.: 6.194 min
Delta R.T.: 0.018 min
Response: 1153333
Conc: 0.42 ng/ml

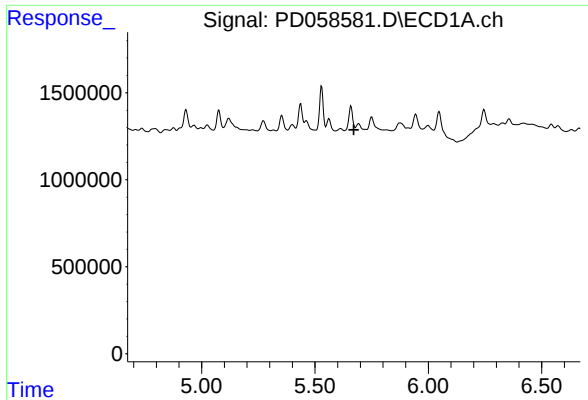

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

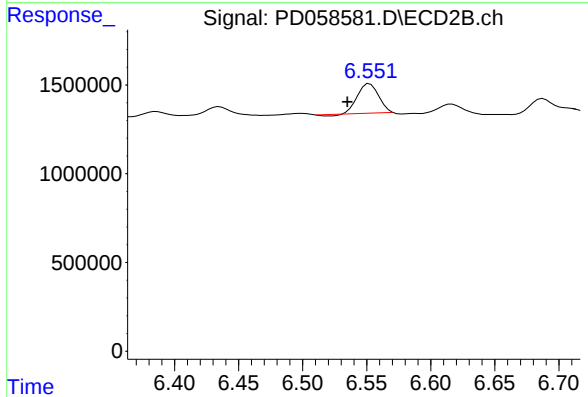


#14 Endrin

R.T.: 6.552 min
Delta R.T.: 0.017 min
Response: 1891744
Conc: 0.89 ng/ml

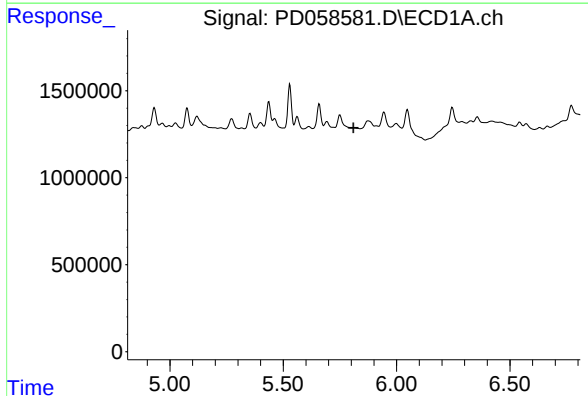


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

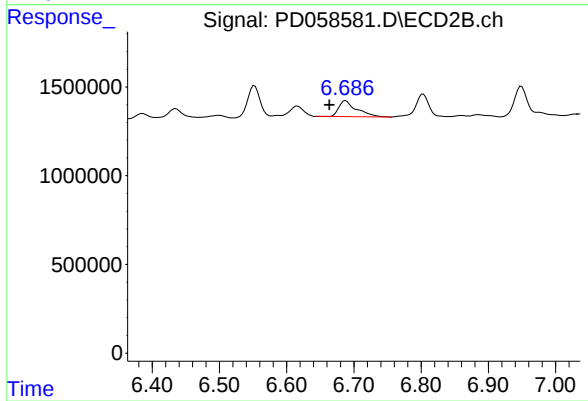

#16 4,4'-DDD


R.T.: 6.688 min
Delta R.T.: 0.024 min
Response: 1642495
Conc: 0.71 ng/ml

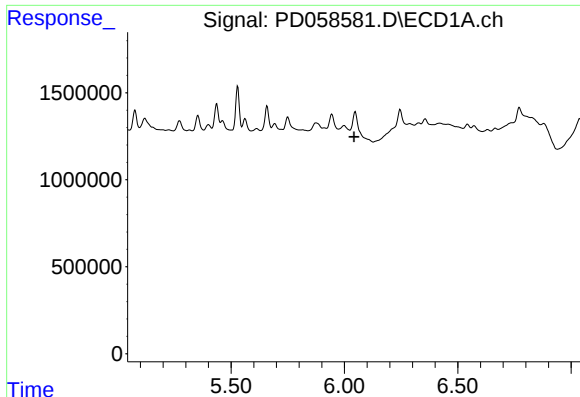

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

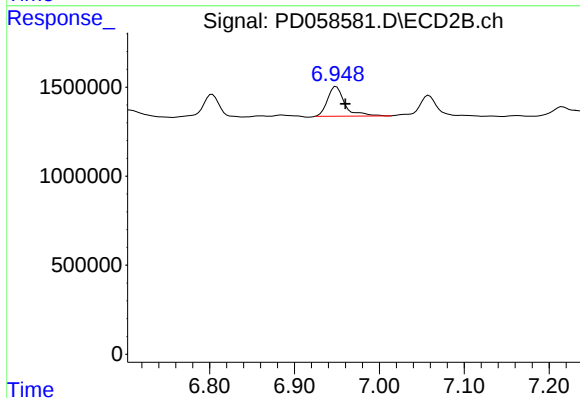


#17 4,4'-DDT

R.T.: 6.949 min
Delta R.T.: -0.011 min
Response: 2368330
Conc: 1.03 ng/ml

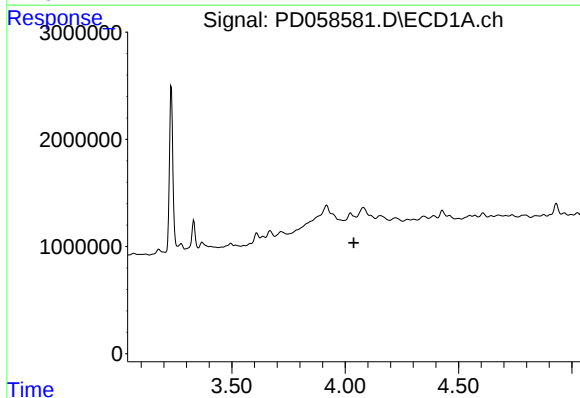


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.038 min
Response: 0
Conc: N.D.

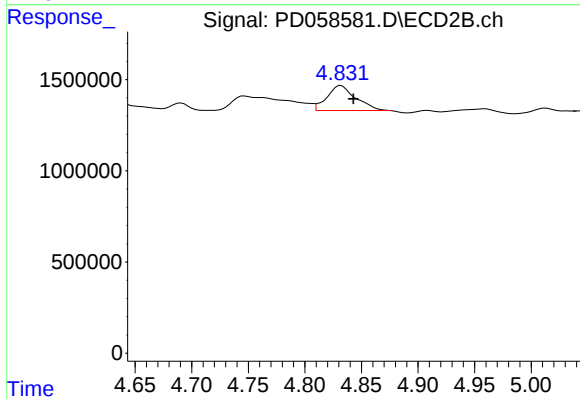

#23 Chlordane-1


R.T.: 4.832 min
Delta R.T.: -0.011 min
Response: 2398804
Conc: 26.95 ng/ml

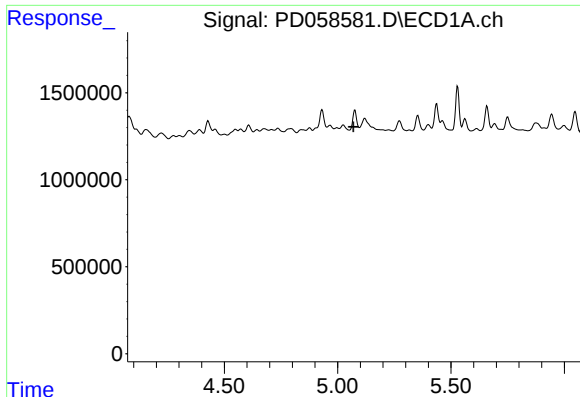

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

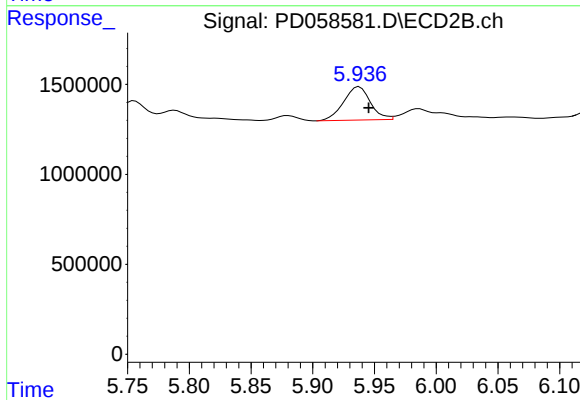


#25 Chlordane-3

R.T.: 5.938 min
Delta R.T.: -0.008 min
Response: 2815679
Conc: 7.57 ng/ml

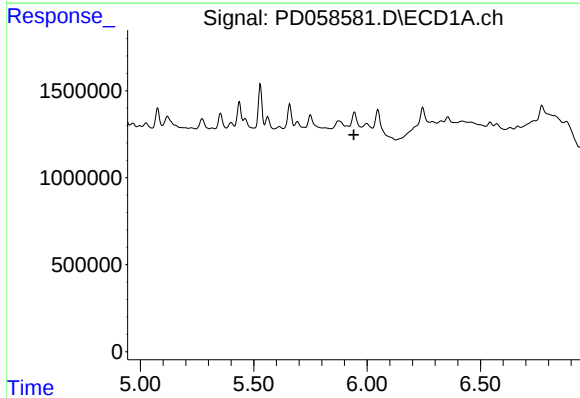


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

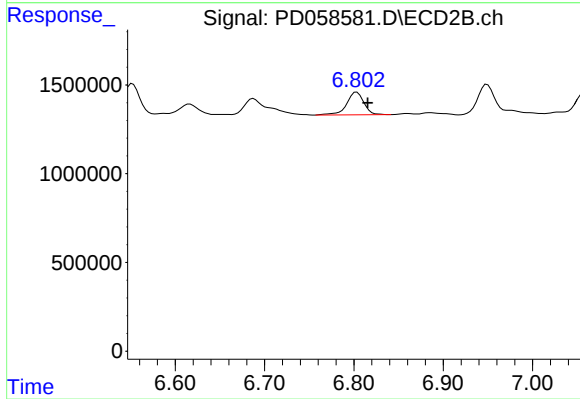

#27 Chlordane-5


R.T.: 6.803 min
Delta R.T.: -0.012 min
Response: 1711070
Conc: 21.47 ng/ml

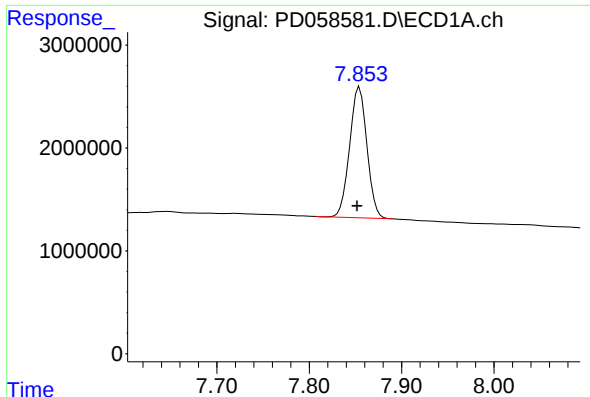

#28 Decachlorobiphenyl

R.T.: 7.854 min
Delta R.T.: 0.002 min
Response: 16519279
Conc: 9.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

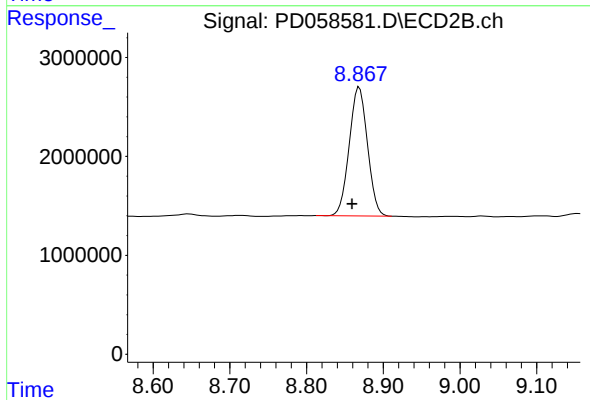

#28 Decachlorobiphenyl

R.T.: 8.869 min
Delta R.T.: 0.010 min
Response: 21623972
Conc: 9.92 ng/ml