

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 20:44
 Operator : AJ\MA
 Sample : L3258-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 06:29:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.867	30702424	42686882	16.839	17.277
28)	SA Decachlor...	7.850	8.865	23914891	28256460	13.243	12.960
Target Compounds							
9)	A Endosulfan I	0.000	6.067	0	608787	N.D.	0.231 #
10)	B gamma-Chl...	0.000	5.937	0	4852559	N.D.	1.668 #
11)	B alpha-Chl...	0.000	6.019	0	2187940	N.D.	0.761 #
25)	Chlordane-3	0.000	5.937	0	4852559	N.D.	13.046 #
26)	Chlordane-4	0.000	6.019	0	2187940	N.D.	5.030 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 20:44
Operator : AJ\MA
Sample : L3258-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 06:29:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

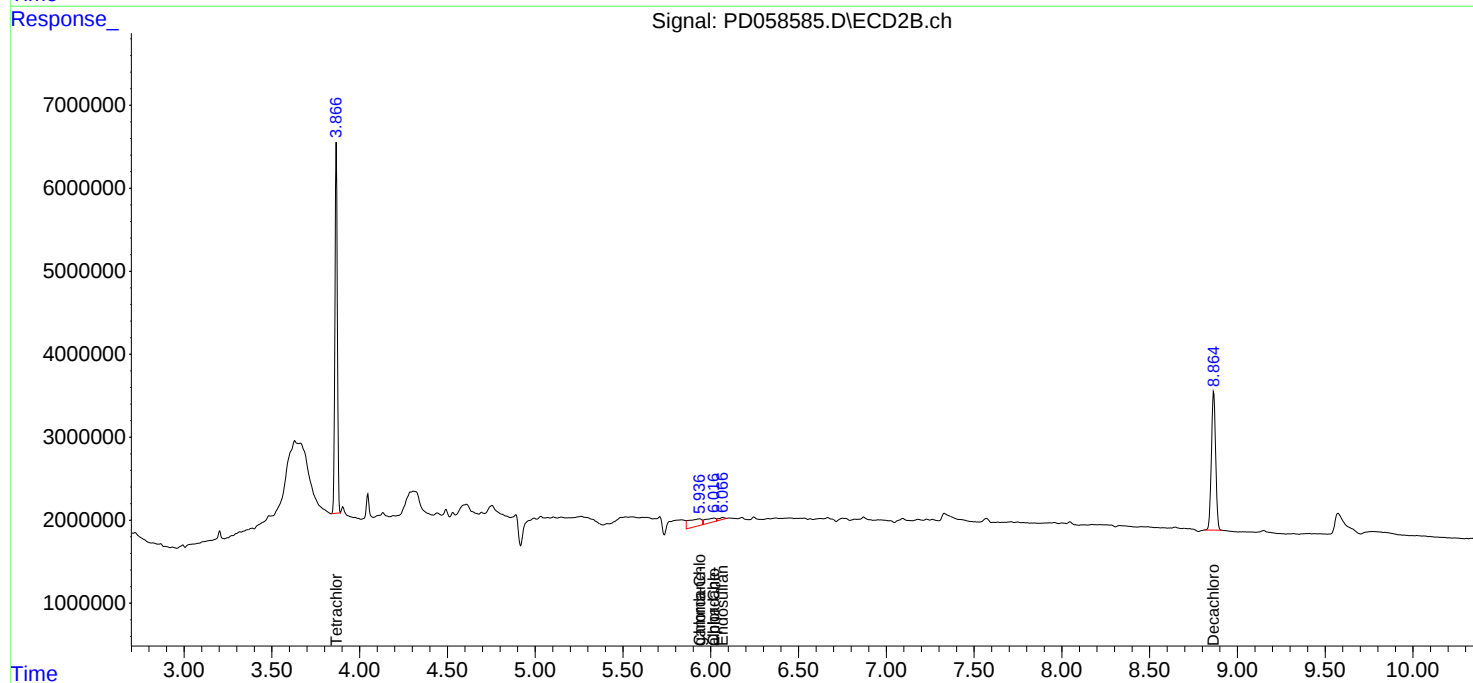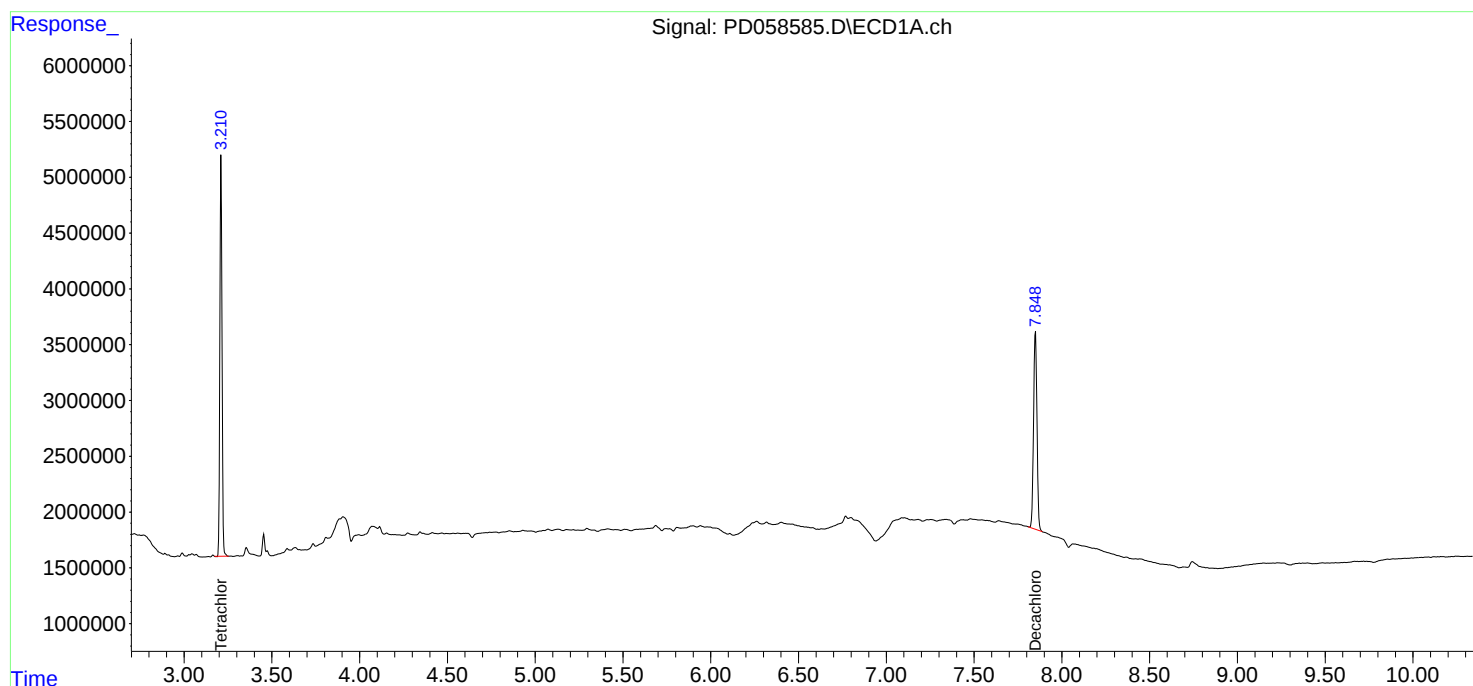


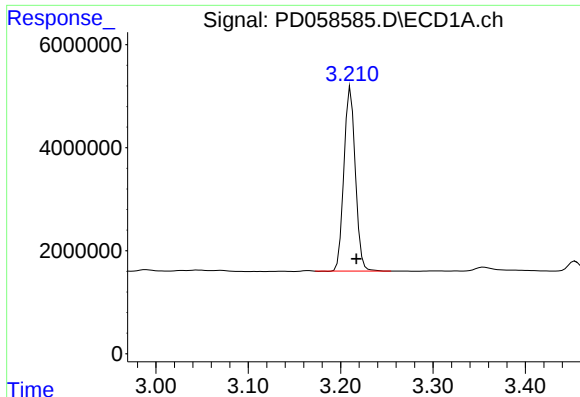

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: -0.006 min
Response: 30702424
Conc: 16.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

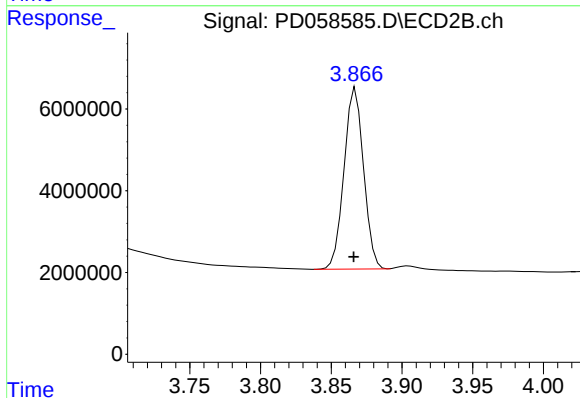


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.001 min
Response: 42686882
Conc: 17.28 ng/ml

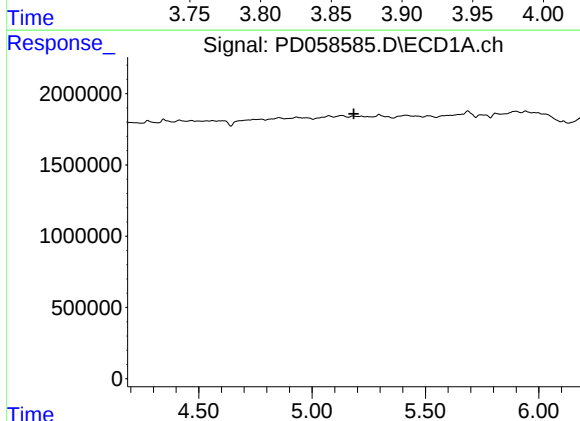


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

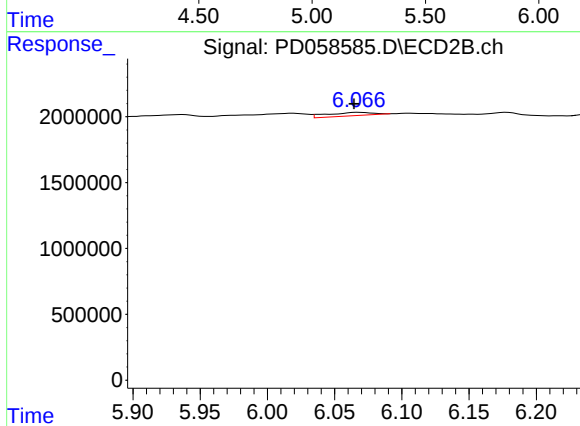

#9 Endosulfan I


R.T.: 6.067 min
Delta R.T.: 0.003 min
Response: 608787
Conc: 0.23 ng/ml

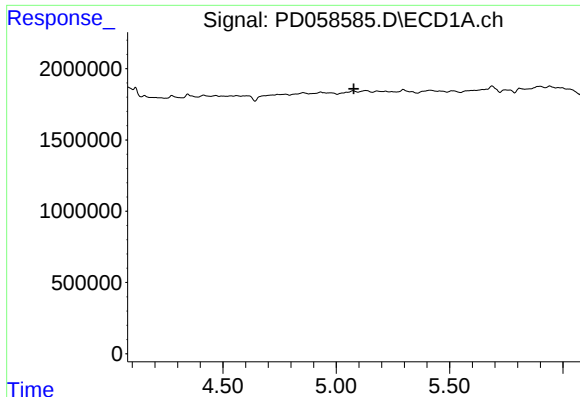

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

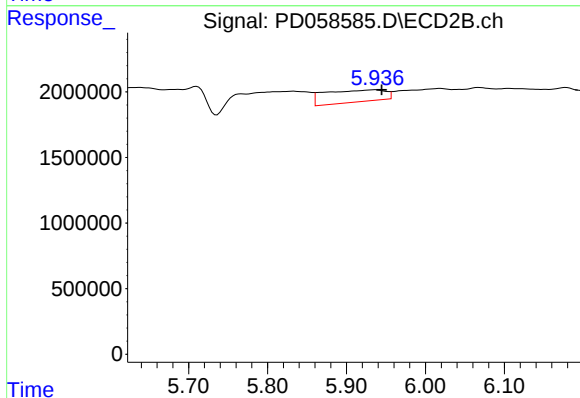


#10 gamma-Chlordane

R.T.: 5.937 min
Delta R.T.: -0.008 min
Response: 4852559
Conc: 1.67 ng/ml

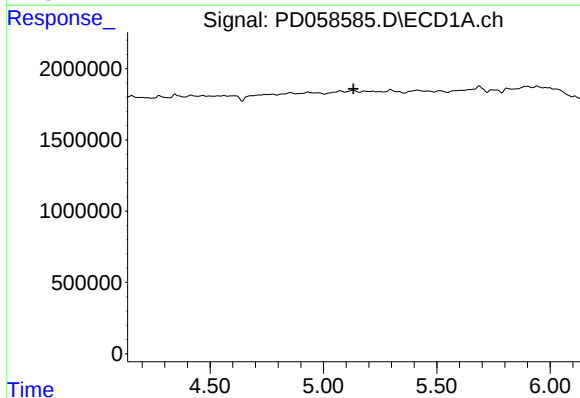


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

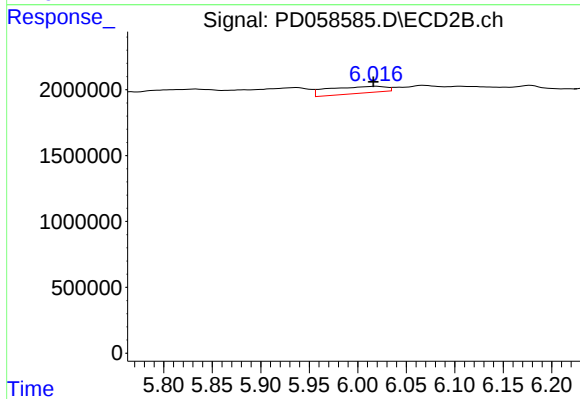

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.003 min
Response: 2187940
Conc: 0.76 ng/ml

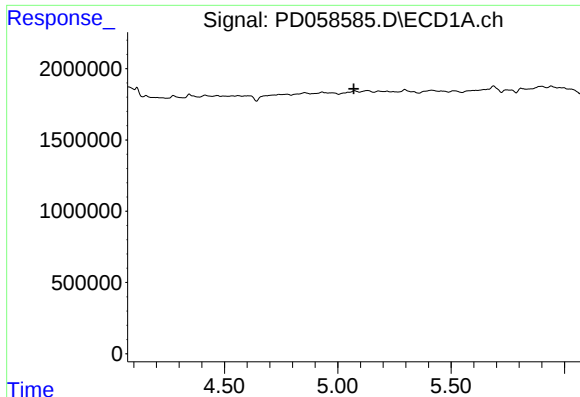

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

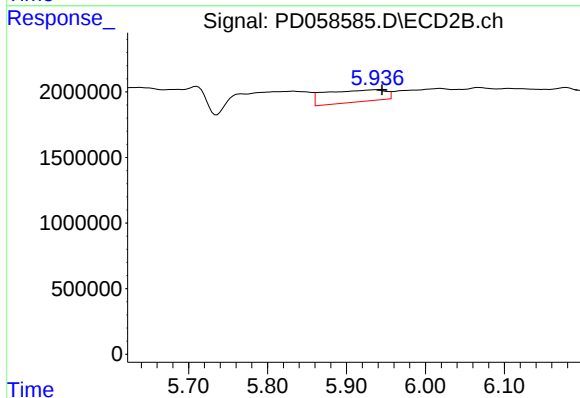


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: -0.009 min
Response: 4852559
Conc: 13.05 ng/ml

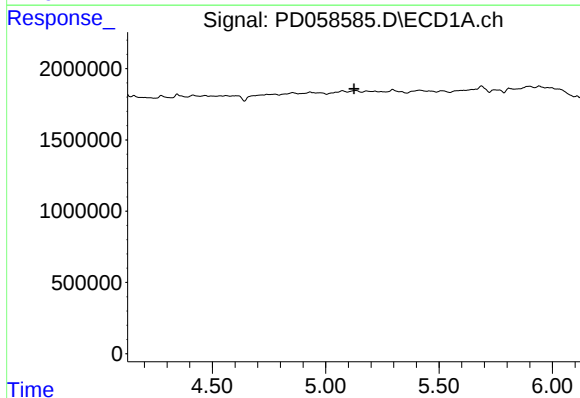


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

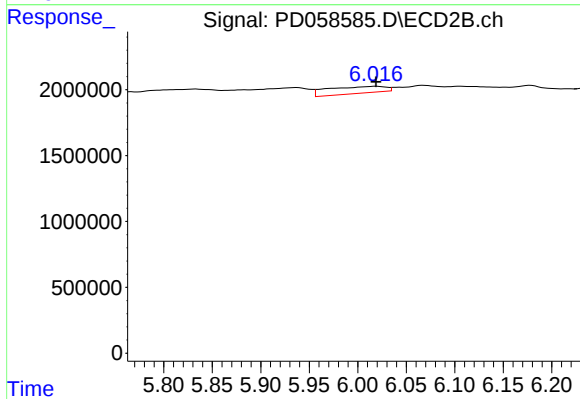

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 2187940
Conc: 5.03 ng/ml

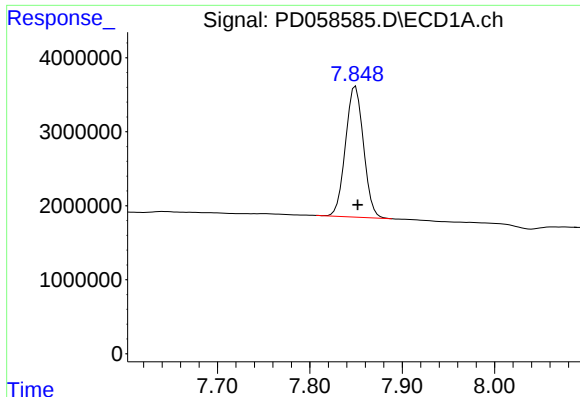

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: -0.002 min
Response: 23914891
Conc: 13.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

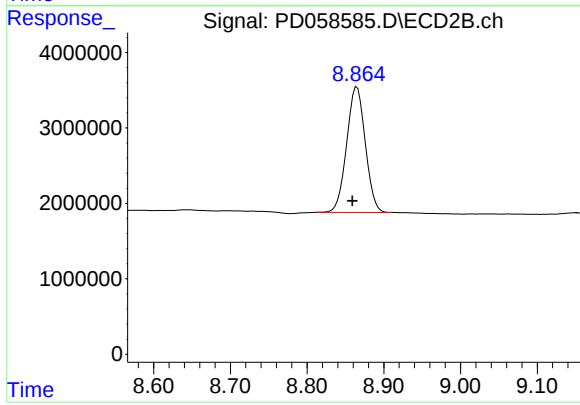

#28 Decachlorobiphenyl

R.T.: 8.865 min
Delta R.T.: 0.006 min
Response: 28256460
Conc: 12.96 ng/ml