

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 20:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 06:29:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	33172821	45875879	18.194	18.567
28)	SA Decachlor...	7.850	8.864	33942853	39844115	18.796	18.275
Target Compounds							
8)	B Heptachlo...	0.000	5.712	0	15278687	N.D.	5.249 #
9)	A Endosulfan I	0.000	6.086f	0	1390083	N.D.	0.527 #
10)	B gamma-Chl...	0.000	5.935	0	9973599	N.D.	3.427 #
11)	B alpha-Chl...	0.000	6.010	0	5075202	N.D.	1.765 #
25)	Chlordane-3	0.000	5.935	0	9973599	N.D.	26.815 #
26)	Chlordane-4	0.000	6.010	0	5075202	N.D.	11.667 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 20:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 06:29:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

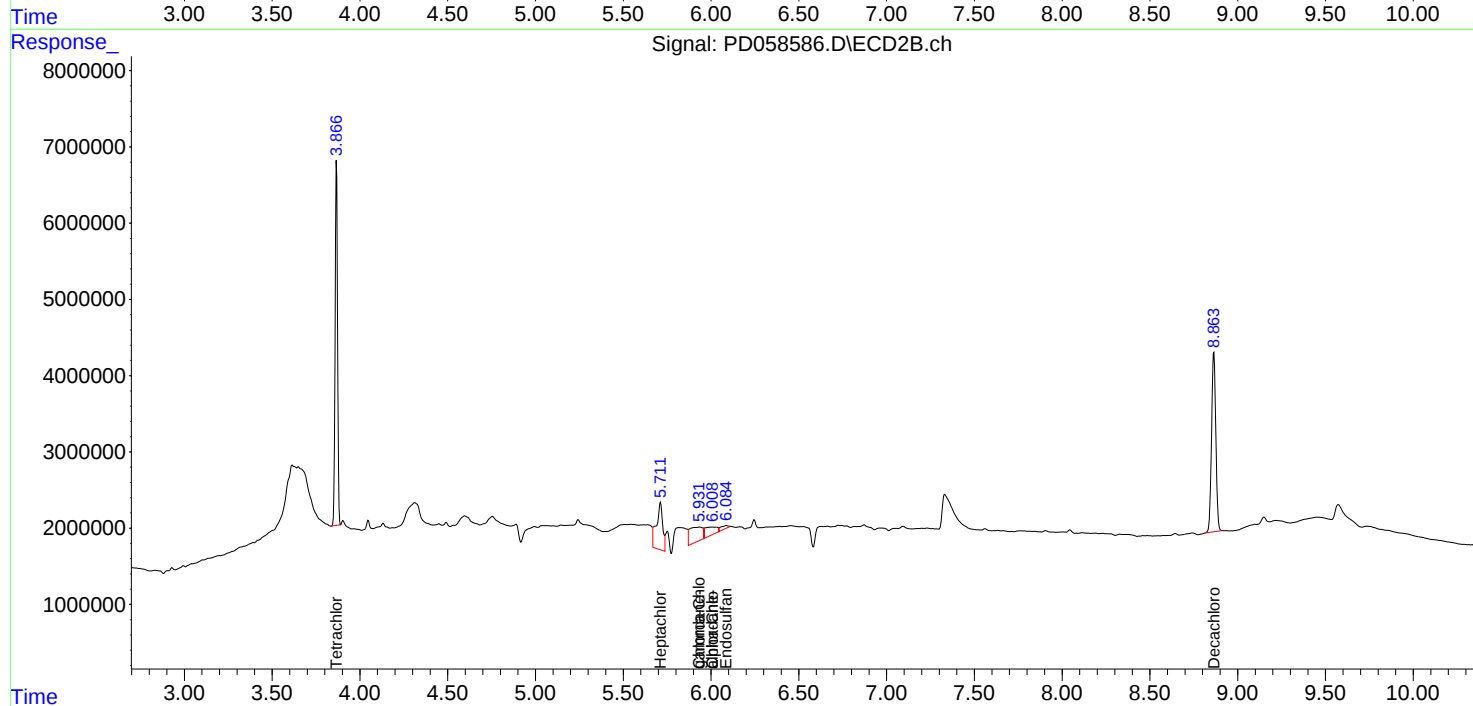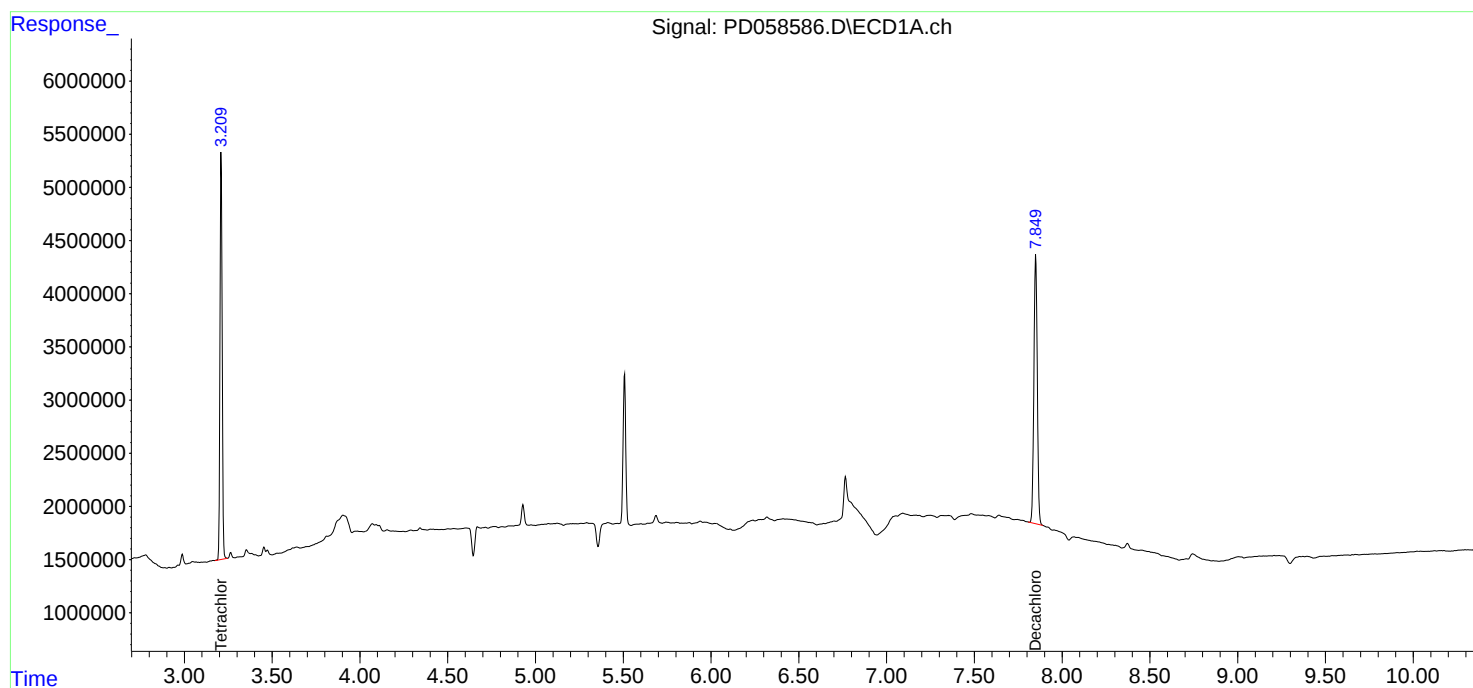


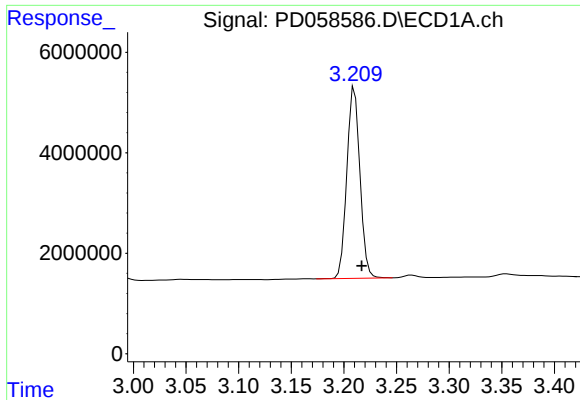

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: -0.007 min
Response: 33172821
Conc: 18.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

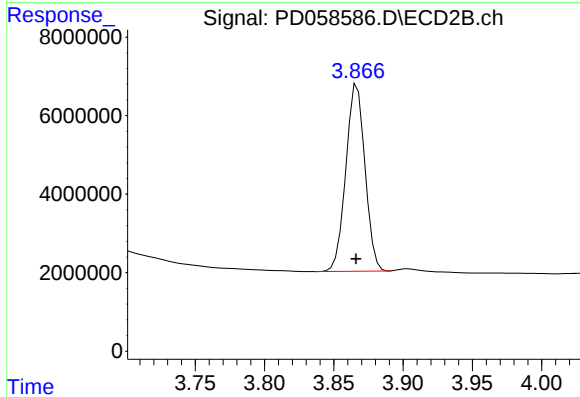


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.001 min
Response: 45875879
Conc: 18.57 ng/ml

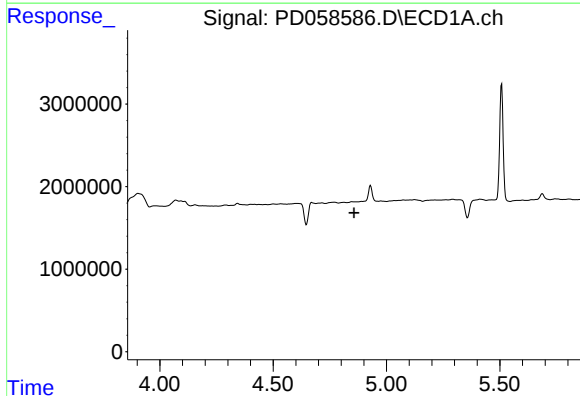


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

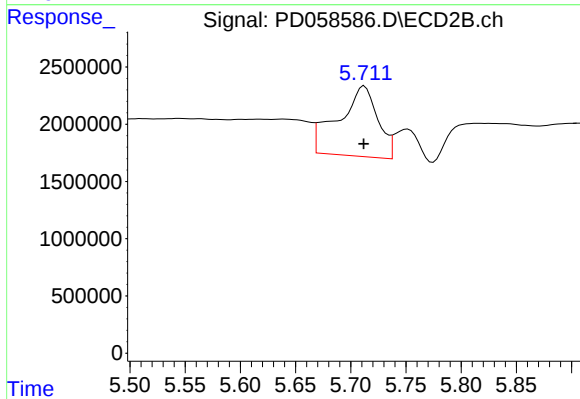

#8 Heptachlor epoxide


R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 15278687
Conc: 5.25 ng/ml

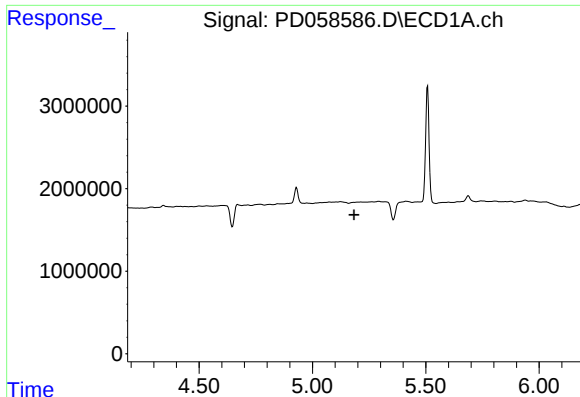

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

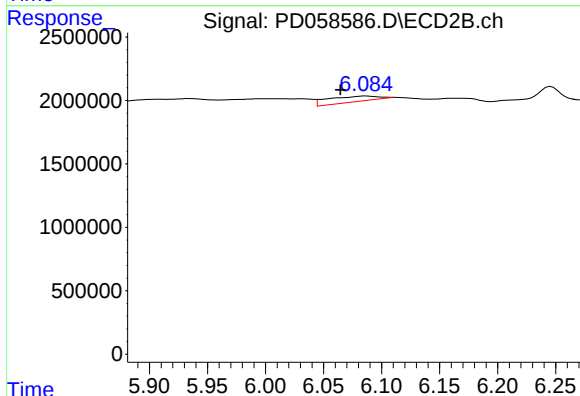


#9 Endosulfan I

R.T.: 6.086 min
Delta R.T.: 0.022 min
Response: 1390083
Conc: 0.53 ng/ml

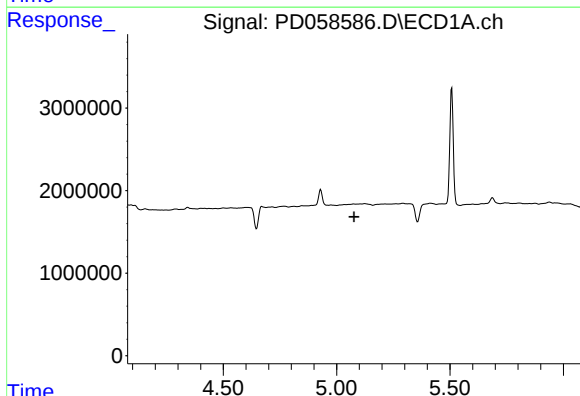


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

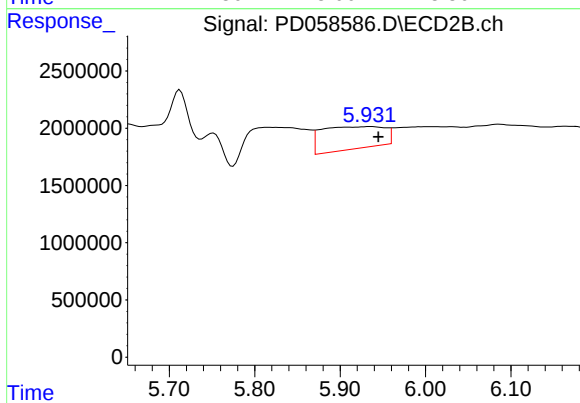

#10 gamma-Chlordane


R.T.: 5.935 min
Delta R.T.: -0.009 min
Response: 9973599
Conc: 3.43 ng/ml

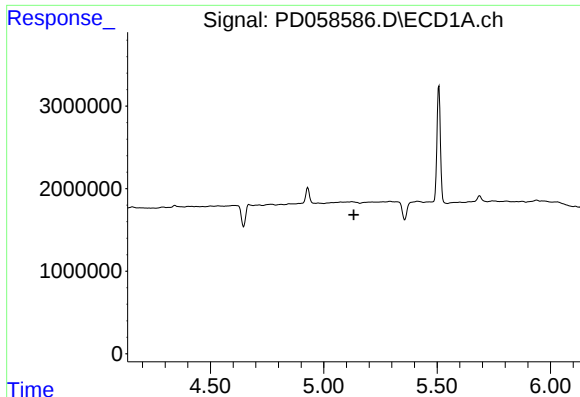

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

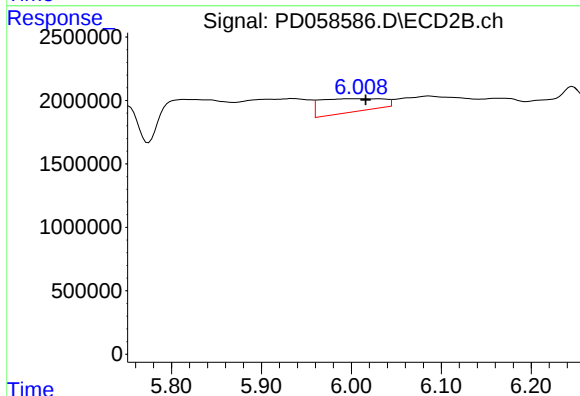


#11 alpha-Chlordane

R.T.: 6.010 min
Delta R.T.: -0.006 min
Response: 5075202
Conc: 1.76 ng/ml

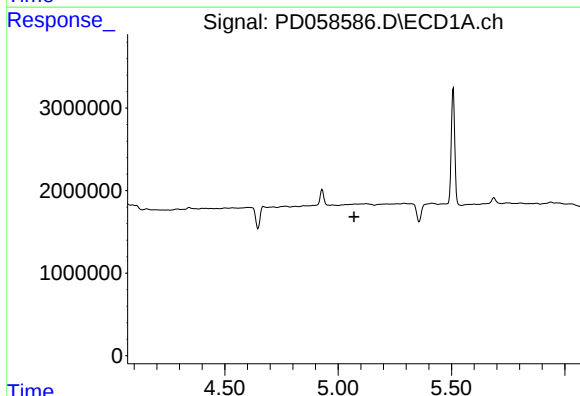


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

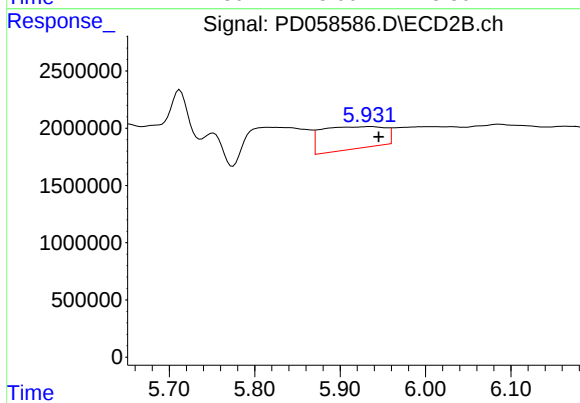

#25 Chlordane-3


R.T.: 5.935 min
Delta R.T.: -0.010 min
Response: 9973599
Conc: 26.81 ng/ml

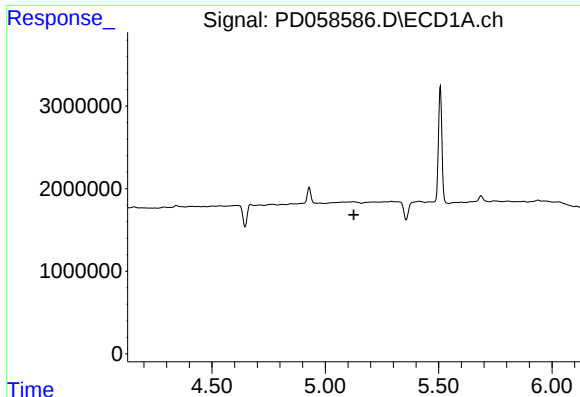

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

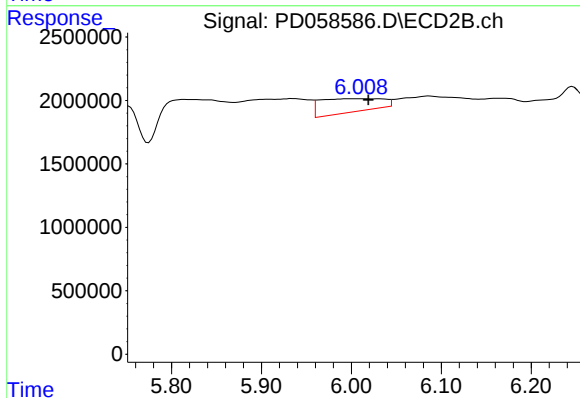


#26 Chlordane-4

R.T.: 6.010 min
Delta R.T.: -0.009 min
Response: 5075202
Conc: 11.67 ng/ml

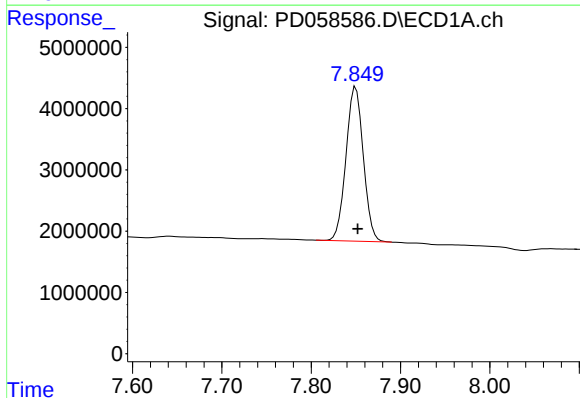

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: -0.002 min
Response: 33942853
Conc: 18.80 ng/ml

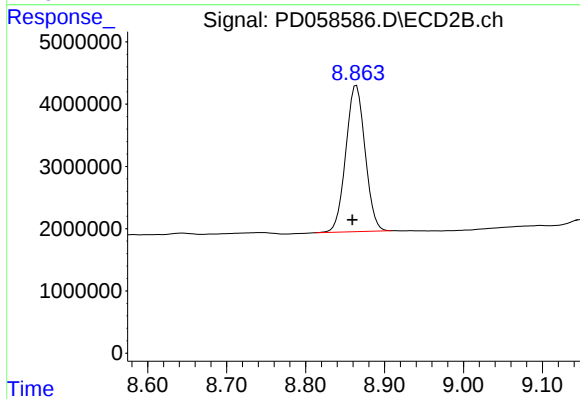

#28 Decachlorobiphenyl

R.T.: 8.864 min
Delta R.T.: 0.005 min
Response: 39844115
Conc: 18.27 ng/ml