

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 13:20
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 15:46:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 13:55:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.210	3.867	85277146	119.0E6	46.620	48.098
7) SA Decachlor...	7.847	8.861	82008920	97750258	47.072	47.169
Target Compounds						
2) Toxaphene-1	5.596	6.413	9796263	12308428	537.850	485.399
3) Toxaphene-2	5.971	6.706	14509243	14205404	501.559	505.883
4) Toxaphene-3	6.213	6.993	14508826	30257240	524.019	487.834
5) Toxaphene-4	6.349	7.077	6627686	18373753	560.979	491.688
6) Toxaphene-5	6.631	7.488	5907109	13681768	563.285	500.274

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 13:20
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 15:46:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 13:55:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

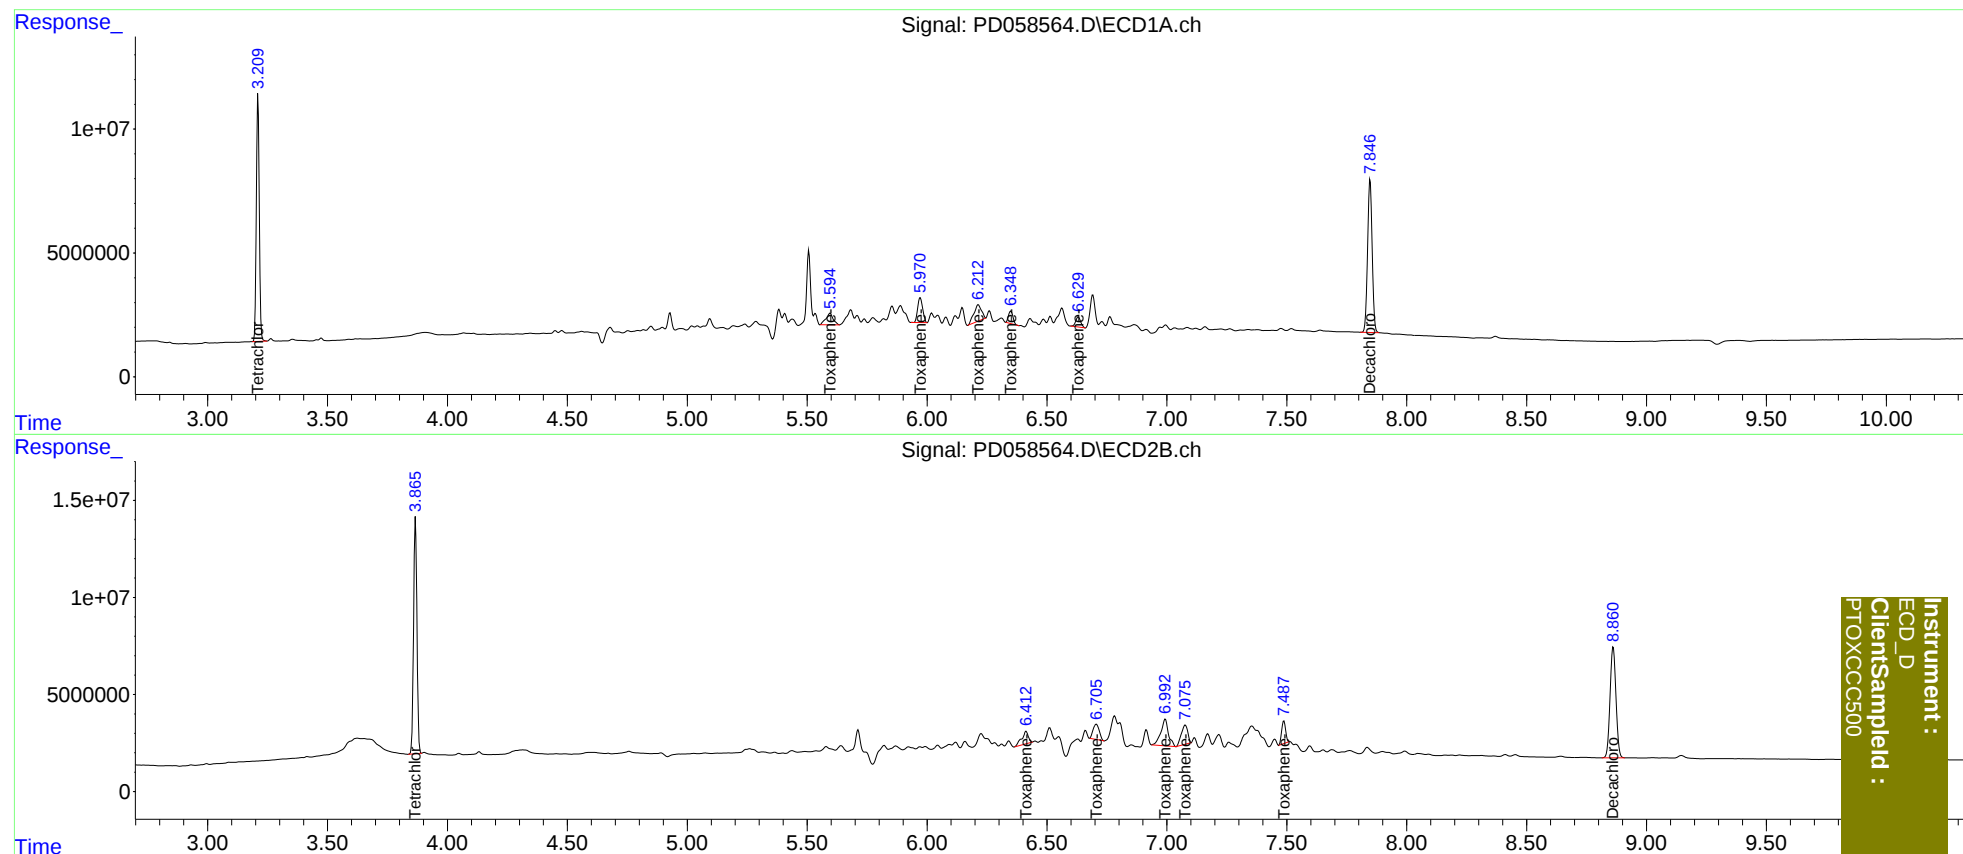

Instrument :
ECD_D
ClientSampled :
PTOXCCC500