

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 10:03
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 14:23:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	94758791	119.9E6	51.971	48.540
28)	SA Decachlor...	7.847	8.861	81592112	95137912	45.182	43.636
Target Compounds							
23)	Chlordane-1	4.038	4.843	27785519	43757538	476.164	491.652
24)	Chlordane-2	4.522	5.306	32137889	46599016	497.177	471.716
25)	Chlordane-3	5.070	5.946	98863936	186.4E6	482.986	501.057
26)	Chlordane-4	5.126	6.019	91304982	216.1E6	478.466	496.755
27)	Chlordane-5	5.941	6.816	32352470	38140092	526.466	478.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 10:03
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 14:23:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

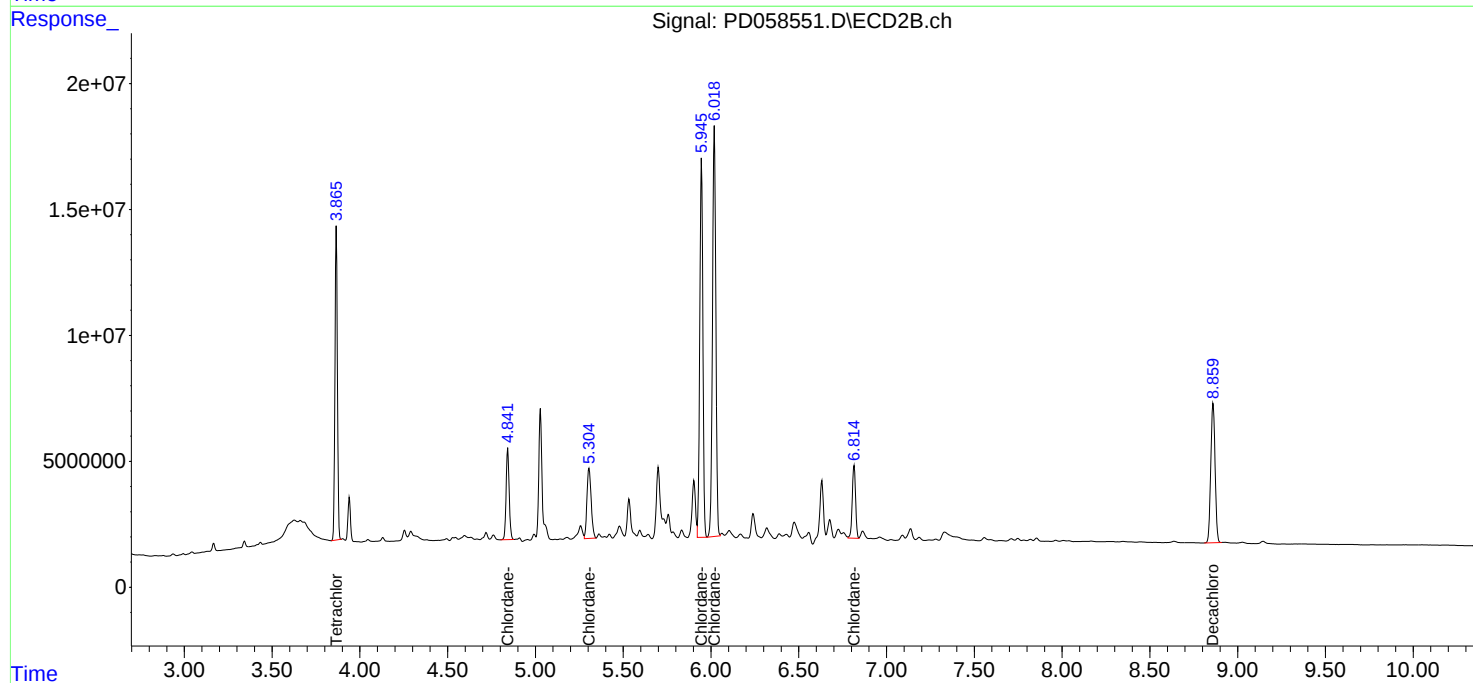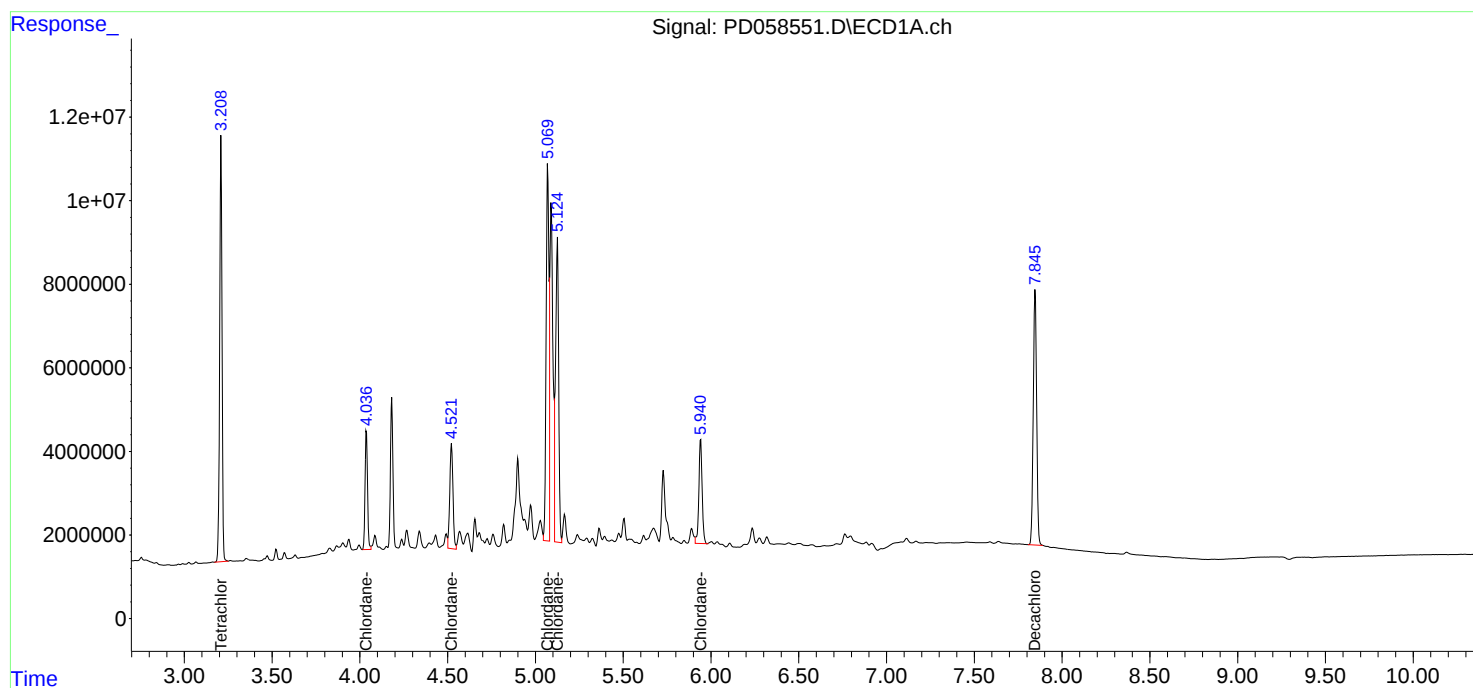


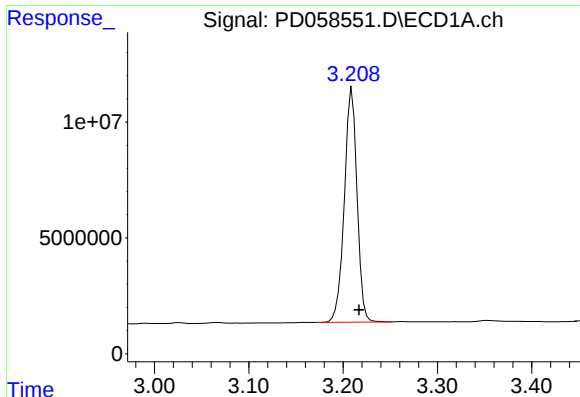

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: -0.007 min
Response: 94758791
Conc: 51.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

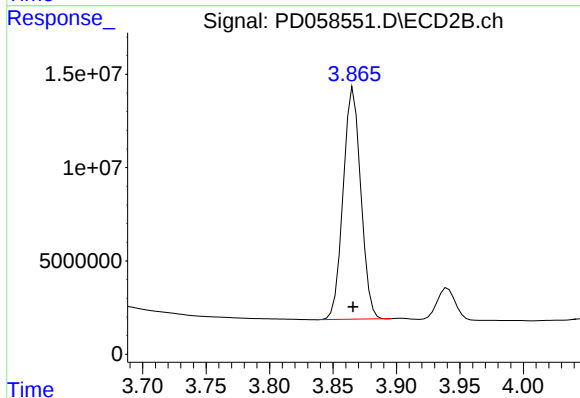


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 119930559
Conc: 48.54 ng/ml

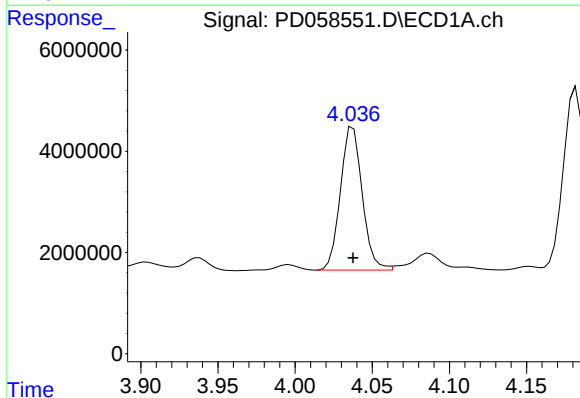


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 27785519
Conc: 476.16 ng/ml

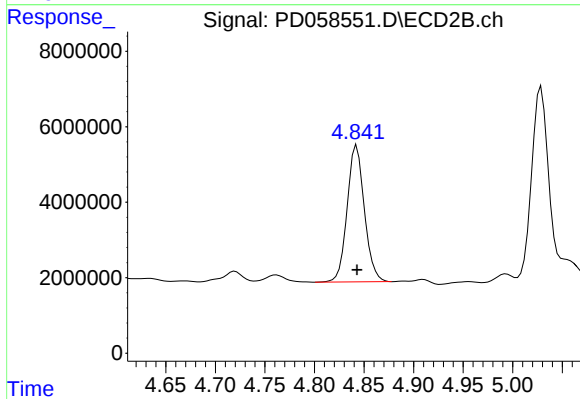

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 43757538
Conc: 491.65 ng/ml

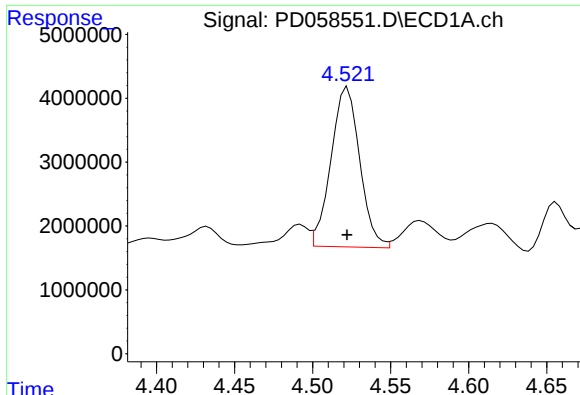

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 32137889
Conc: 497.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

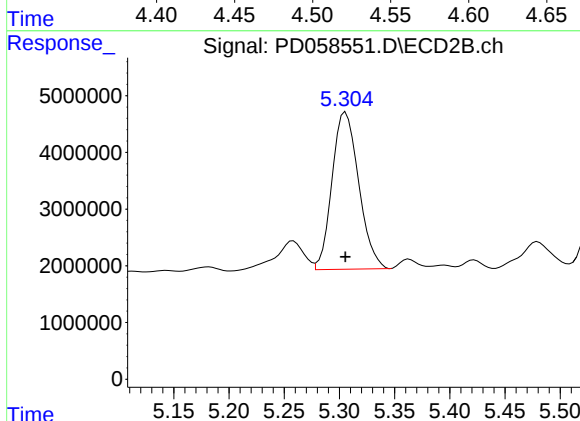


#24 Chlordane-2

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 46599016
Conc: 471.72 ng/ml

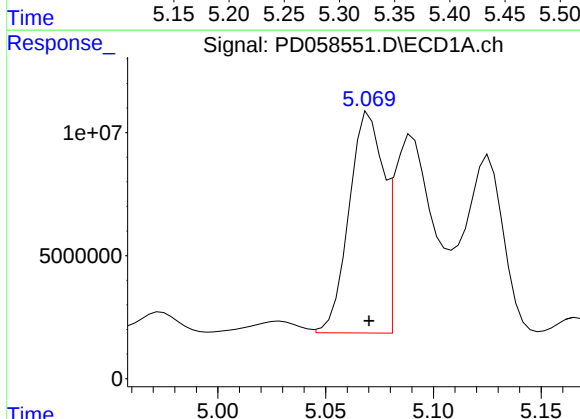


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 98863936
Conc: 482.99 ng/ml

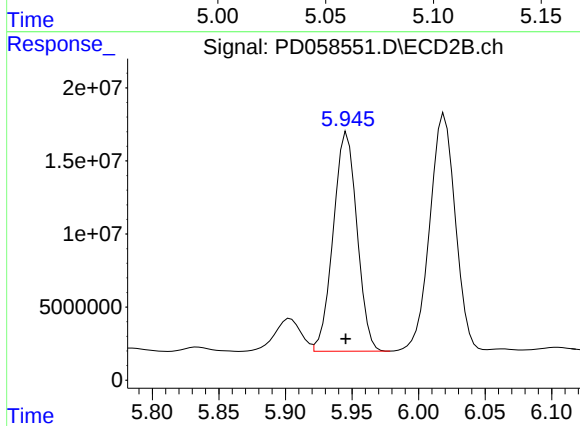

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.001 min
Response: 186365838
Conc: 501.06 ng/ml

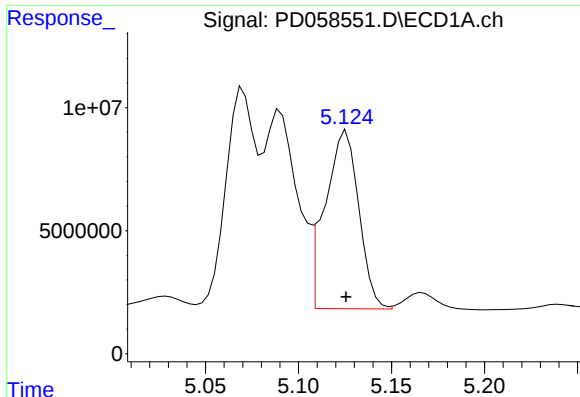

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 91304982
Conc: 478.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

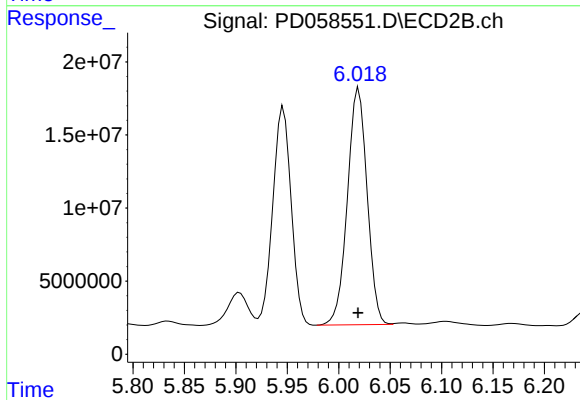


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 216088506
Conc: 496.75 ng/ml

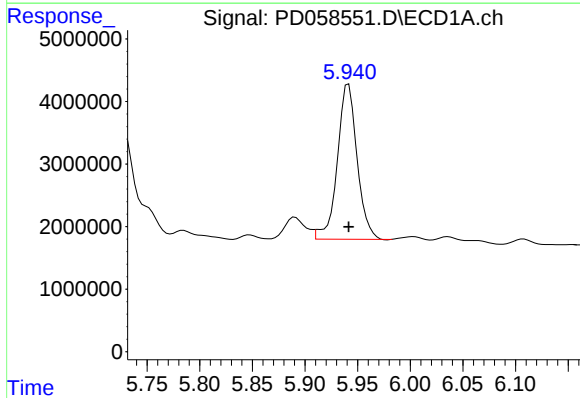


#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 32352470
Conc: 526.47 ng/ml

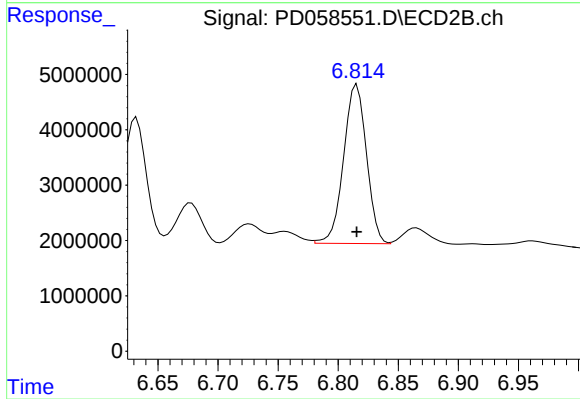

#27 Chlordane-5


R.T.: 6.816 min
Delta R.T.: 0.000 min
Response: 38140092
Conc: 478.67 ng/ml

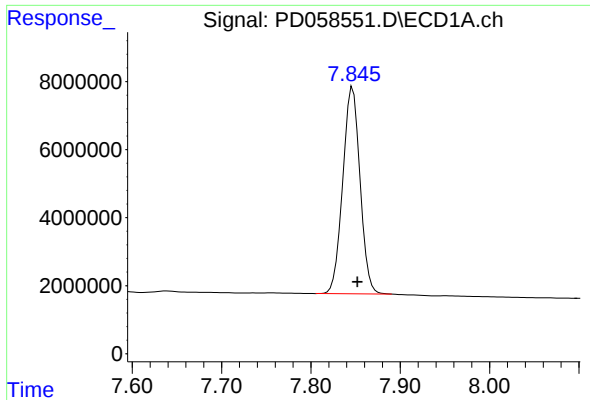

#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.005 min
Response: 81592112
Conc: 45.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

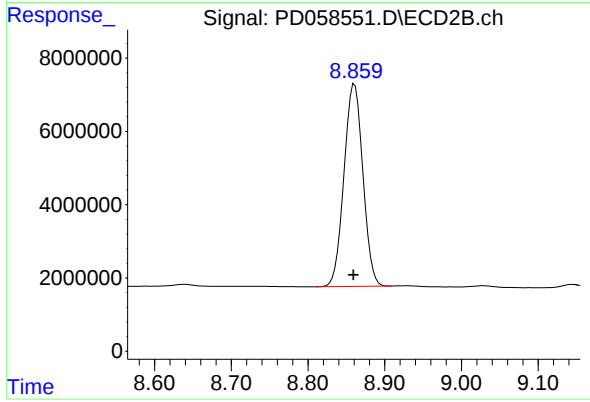

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.001 min
Response: 95137912
Conc: 43.64 ng/ml