

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 13:05
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 14:26:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	94889432	118.4E6	52.042	47.909
28)	SA Decachlor...	7.848	8.861	82166172	94843377	45.500	43.500
Target Compounds							
23)	Chlordane-1	4.038	4.843	27677107	43329104	474.306	486.838
24)	Chlordane-2	4.523	5.306	32240175	45562721	498.760	461.226
25)	Chlordane-3	5.071	5.946	99267104	187.1E6	484.955	503.127
26)	Chlordane-4	5.126	6.019	91781714	218.7E6	480.965	502.711
27)	Chlordane-5	5.942	6.817	31758113	38906365	516.795	488.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 13:05
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 14:26:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

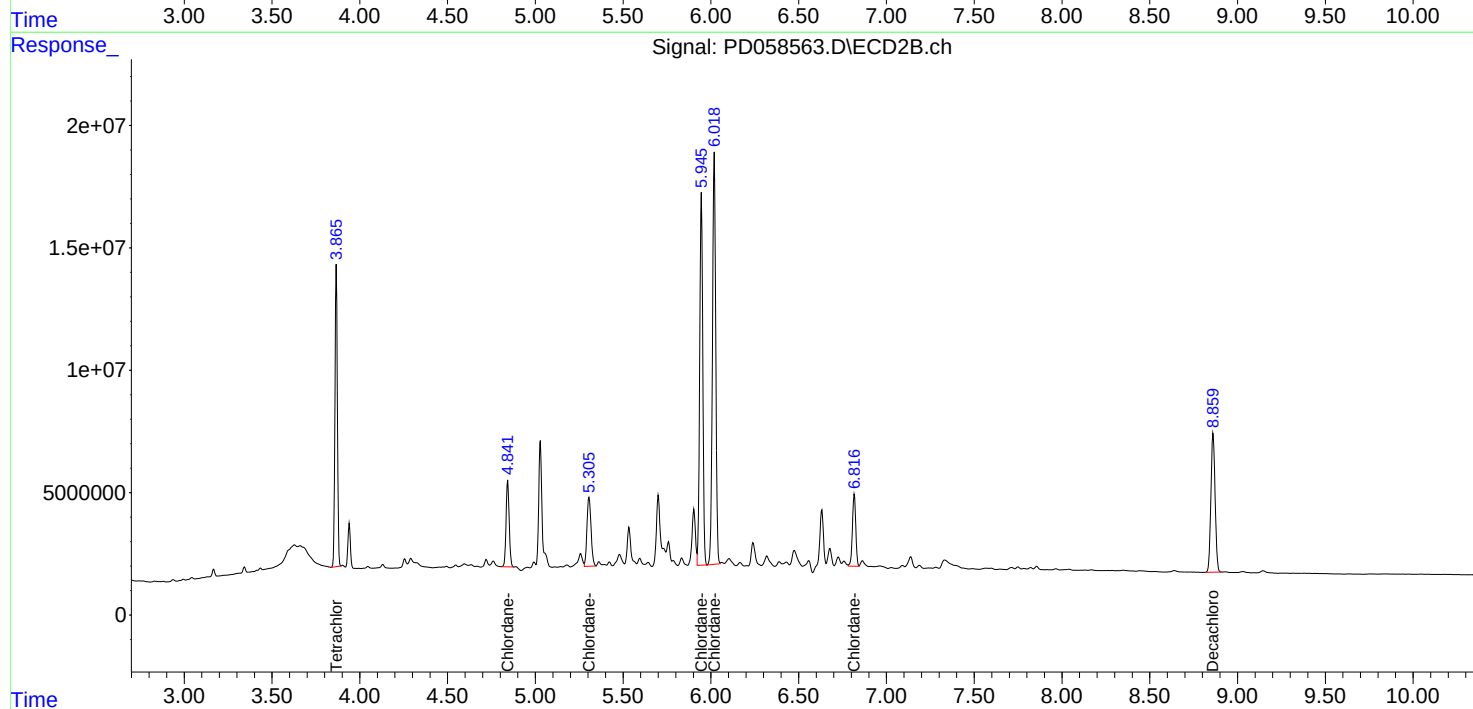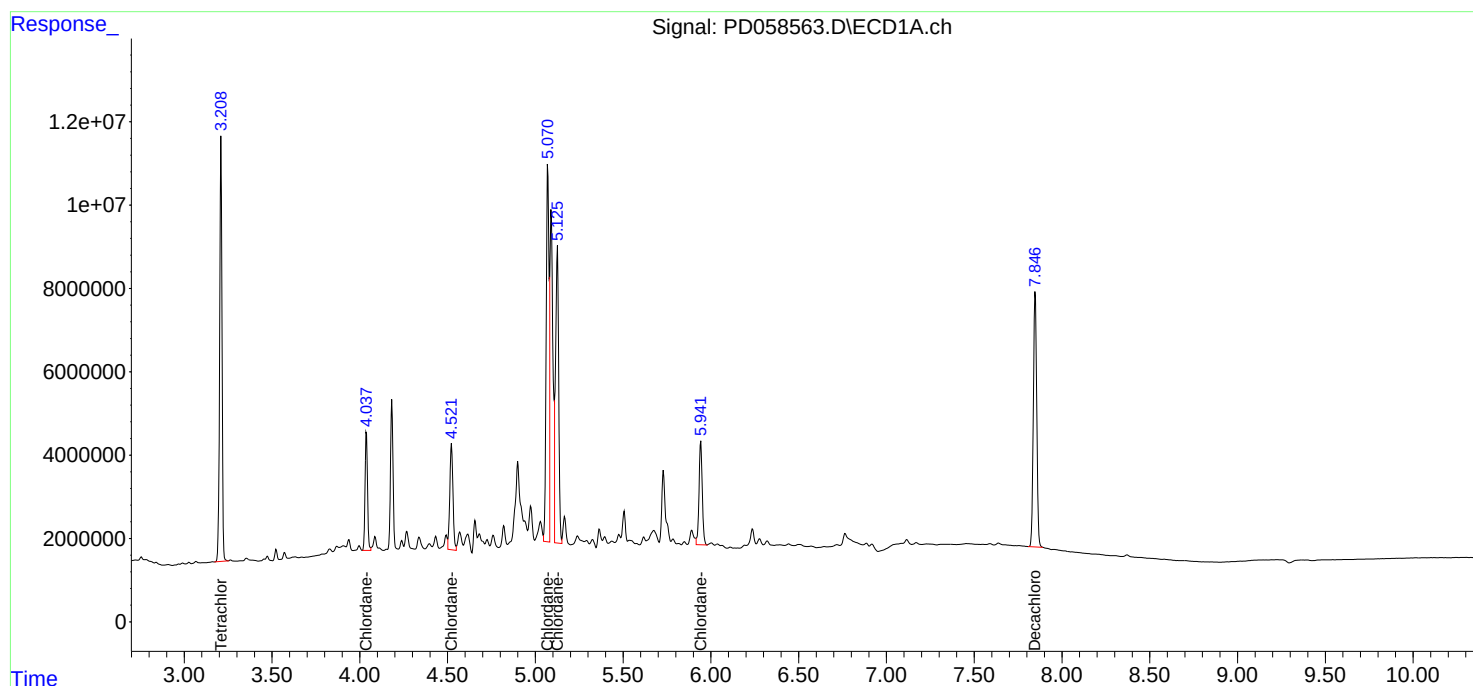


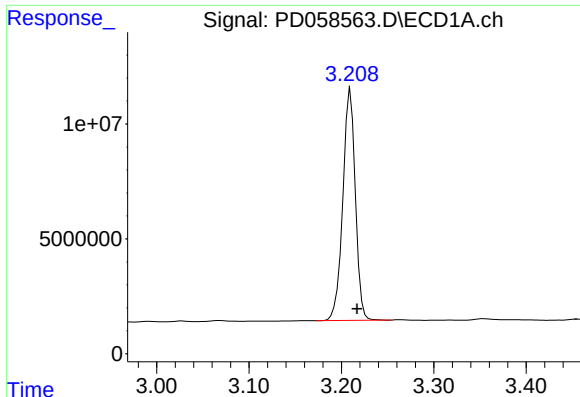

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: -0.007 min
Response: 94889432
Conc: 52.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

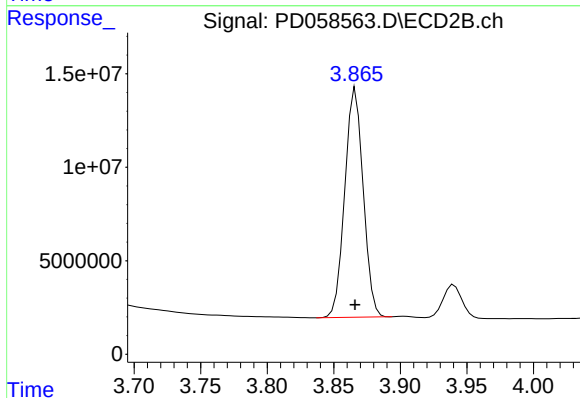


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 118371668
Conc: 47.91 ng/ml

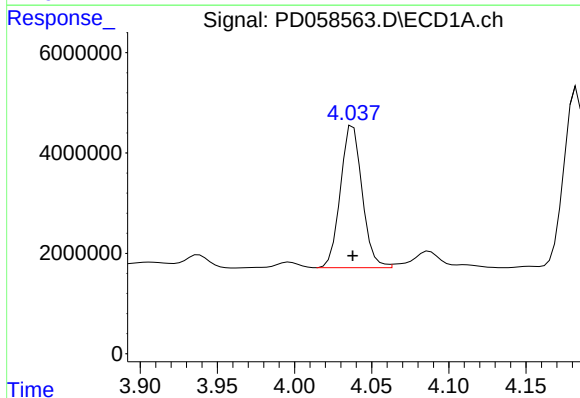


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 27677107
Conc: 474.31 ng/ml

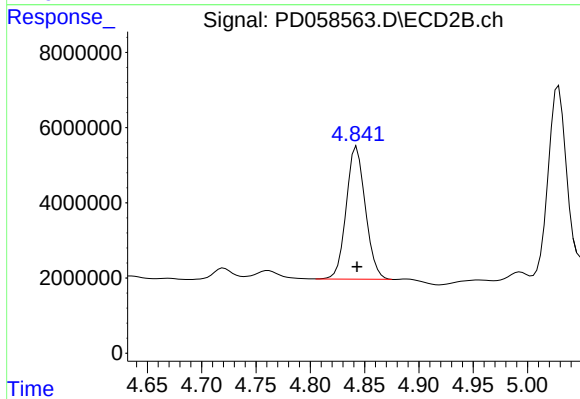

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 43329104
Conc: 486.84 ng/ml

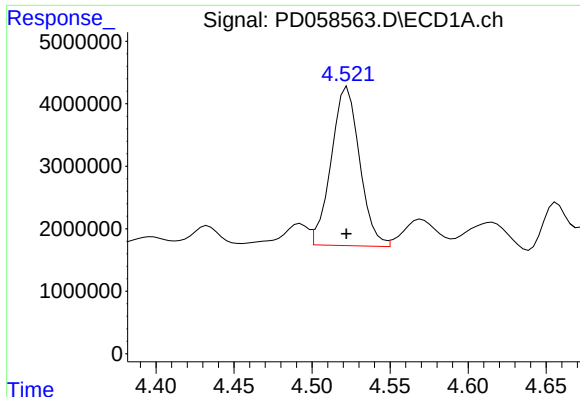

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 32240175
Conc: 498.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

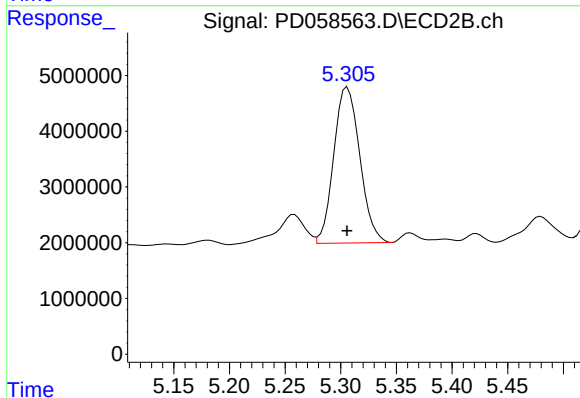


#24 Chlordane-2

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 45562721
Conc: 461.23 ng/ml

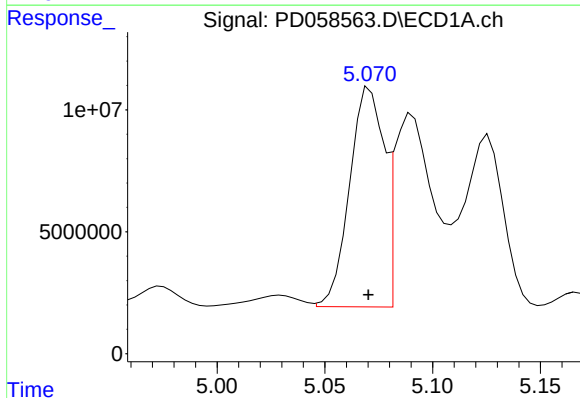


#25 Chlordane-3

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 99267104
Conc: 484.96 ng/ml

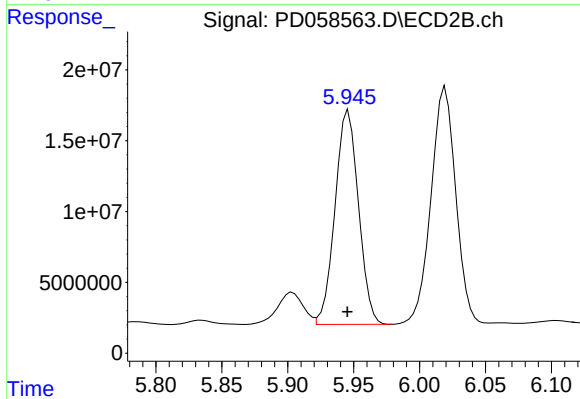

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 187135743
Conc: 503.13 ng/ml

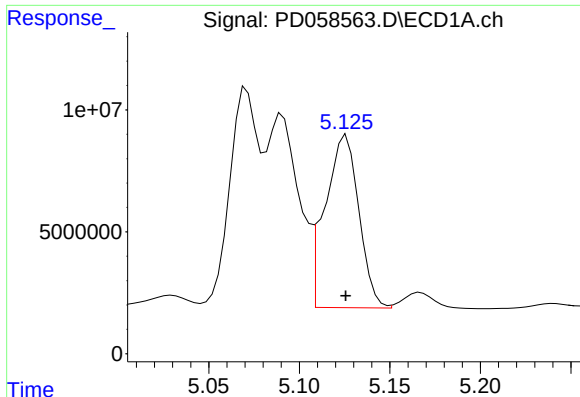

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 91781714
Conc: 480.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

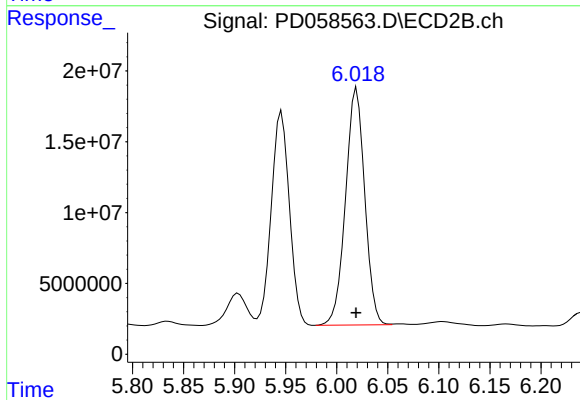


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 218679589
Conc: 502.71 ng/ml

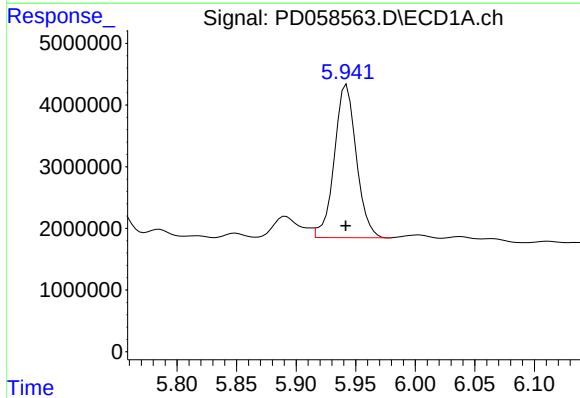


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 31758113
Conc: 516.79 ng/ml

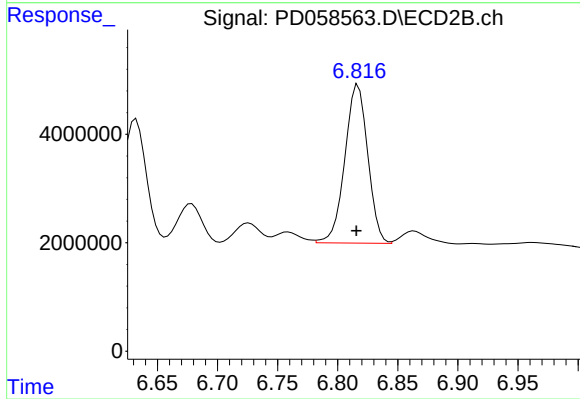

#27 Chlordane-5


R.T.: 6.817 min
Delta R.T.: 0.002 min
Response: 38906365
Conc: 488.29 ng/ml

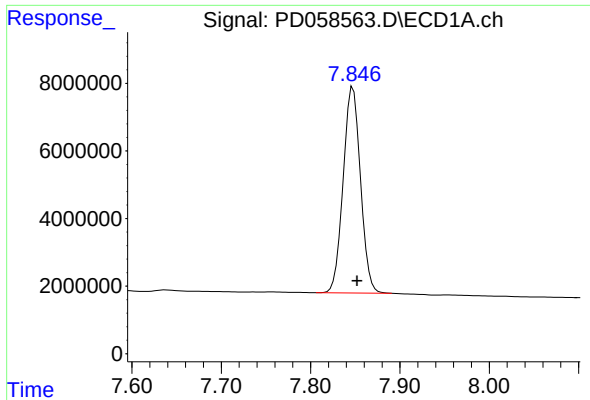

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: -0.004 min
Response: 82166172
Conc: 45.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

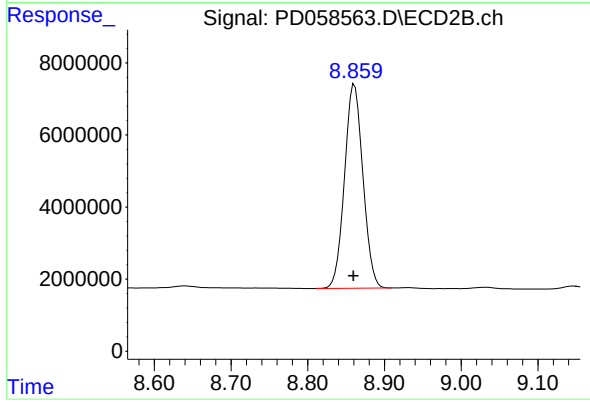

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.002 min
Response: 94843377
Conc: 43.50 ng/ml