

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 14:34
 Operator : AJ\MA
 Sample : L3255-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CHRT-58

Manual Integrations
 APPROVED

Ankita
 7/13/2020 3:26:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 04:40:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.214	3.868	24954633	28015719	13.686	11.339m
28) SA Decachlor...	7.847	8.861	21305717	27277224	11.798m	12.511m
Target Compounds						
16) A 4,4'-DDD	5.810	6.660	10572400	28499426	8.082m	12.361m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 14:34
Operator : AJ\MA
Sample : L3255-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
CHRT-58


Manual Integrations
APPROVED

Ankita
7/13/2020 3:26:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 04:40:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

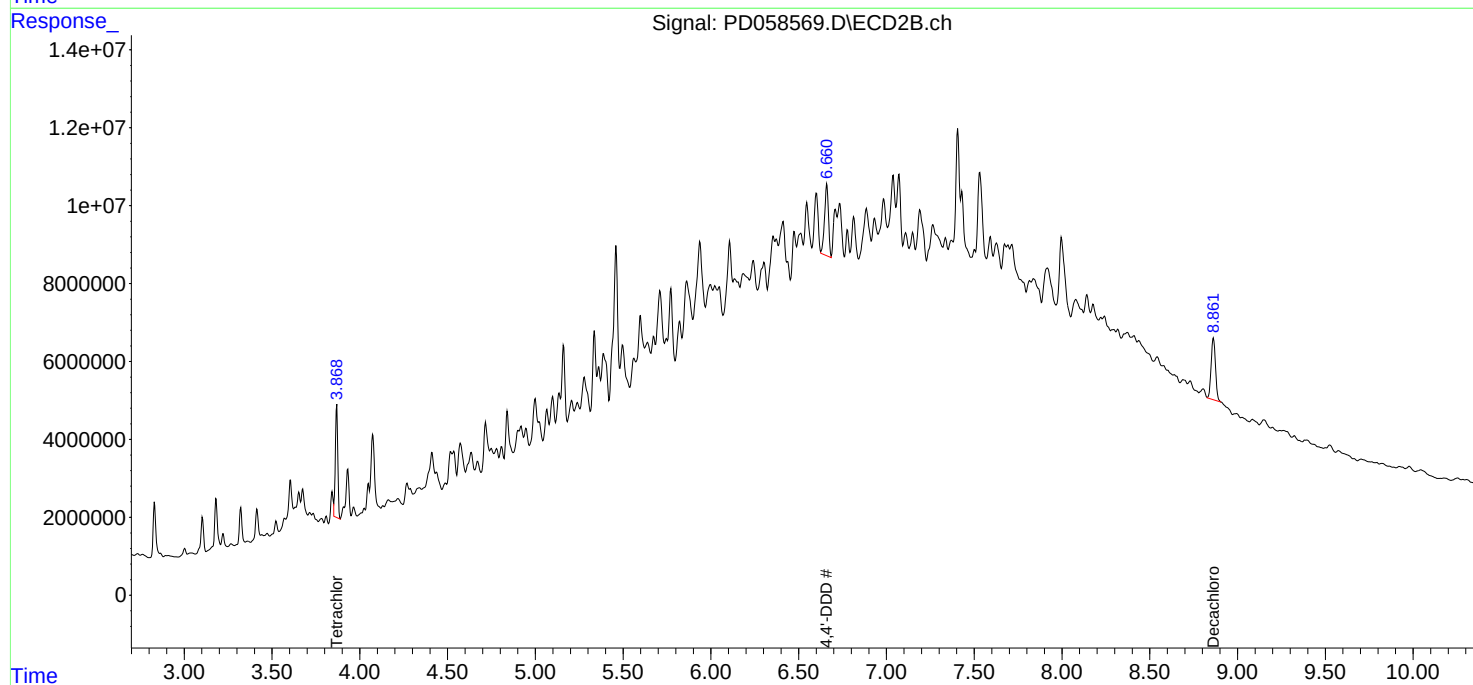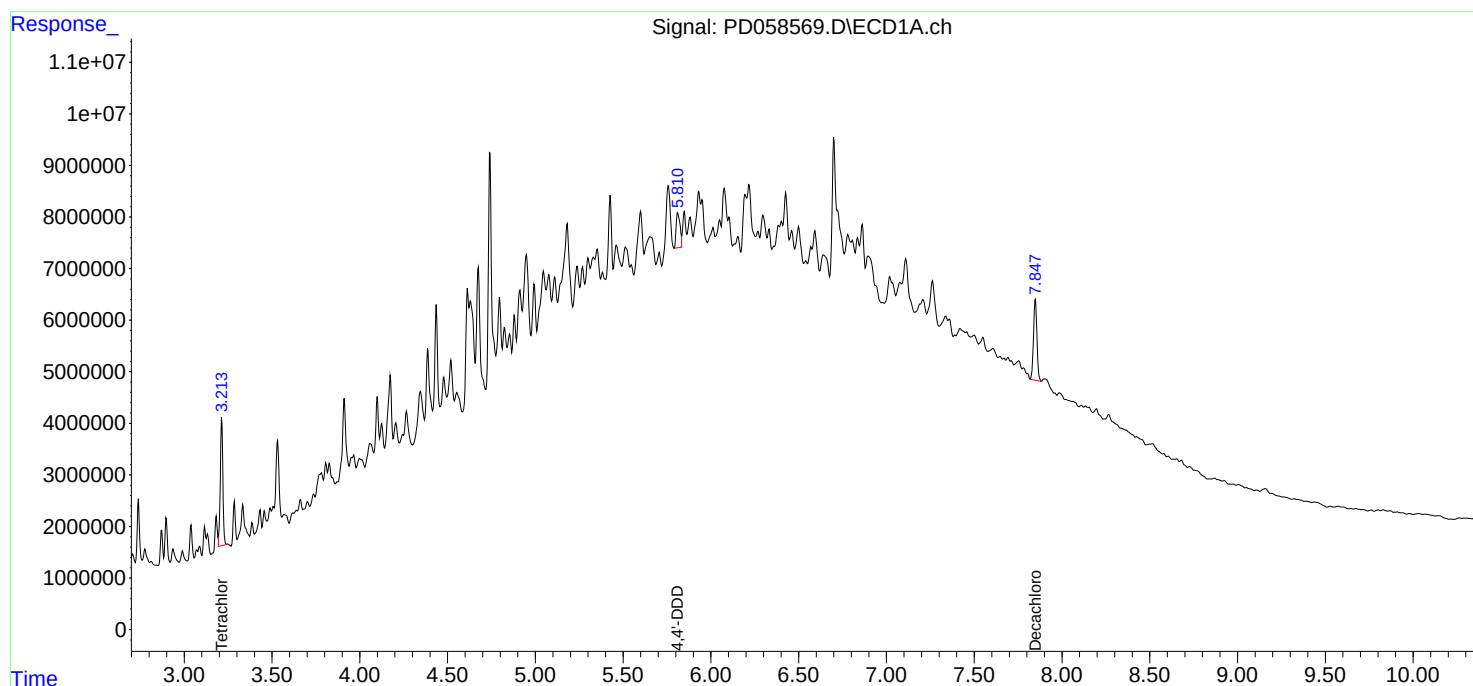

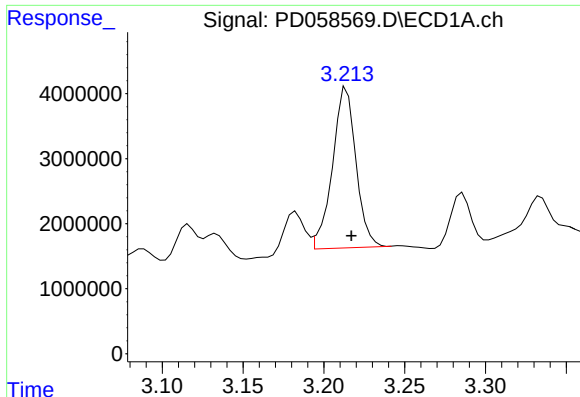


#1 Tetrachloro-m-xylene

R.T.: 3.214 min
Delta R.T.: -0.003 min
Response: 24954633
Conc: 13.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHRT-58


Manual Integrations
APPROVED

Ankita
7/13/2020 3:26:40 PM

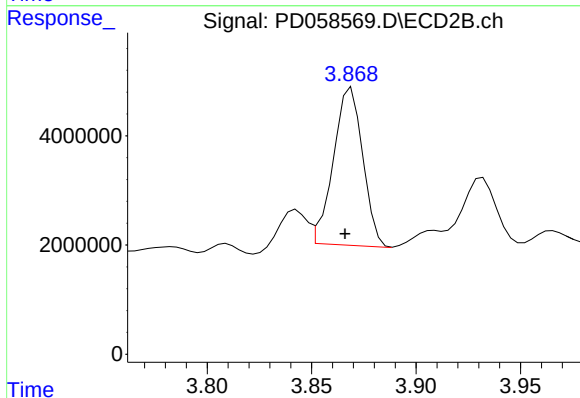


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: 0.002 min
Response: 28015719
Conc: 11.34 ng/ml m

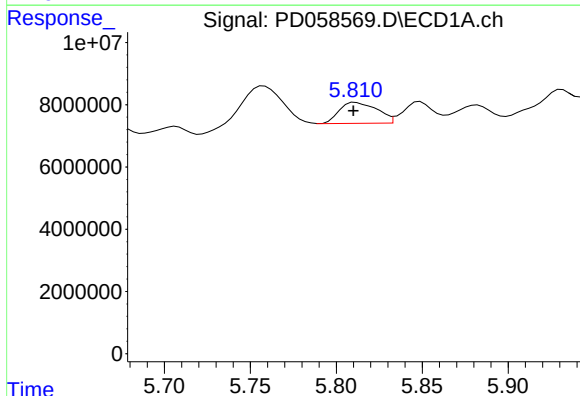


#16 4,4'-DDD

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 10572400
Conc: 8.08 ng/ml m

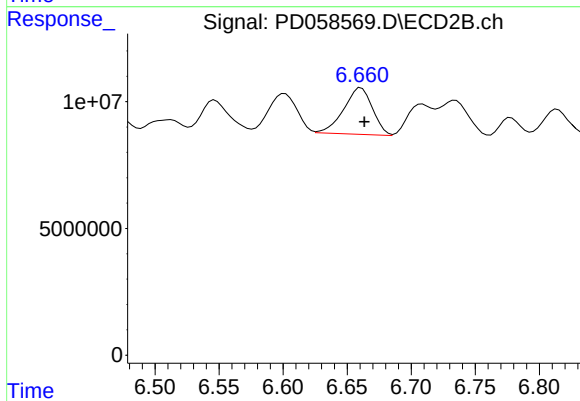

#16 4,4'-DDD

R.T.: 6.660 min
Delta R.T.: -0.004 min
Response: 28499426
Conc: 12.36 ng/ml m

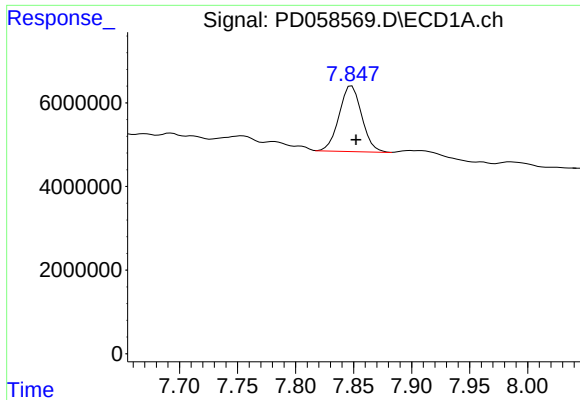


#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.005 min
Response: 21305717
Conc: 11.80 ng/ml m

Instrument :
ECD_D
ClientSampleId :
CHRT-58

Manual Integrations
APPROVED

Ankita
7/13/2020 3:26:40 PM

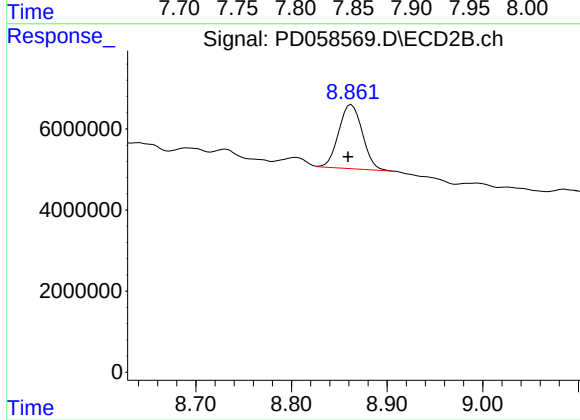

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.002 min
Response: 27277224
Conc: 12.51 ng/ml m