

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
 Data File : PD058582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 20:00
 Operator : AJ\MA
 Sample : PB130051BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB130051BL

Manual Integrations
 APPROVED

Ankita
 7/13/2020 3:28:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 06:28:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	29202656	38537908	16.016	15.597
28)	SA Decachlor...	7.849	8.864	38710301	35226080	21.436m	16.157

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071020\
Data File : PD058582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 20:00
Operator : AJ\MA
Sample : PB130051BL
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PB130051BL


Manual Integrations
APPROVED

Ankita
7/13/2020 3:28:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 06:28:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

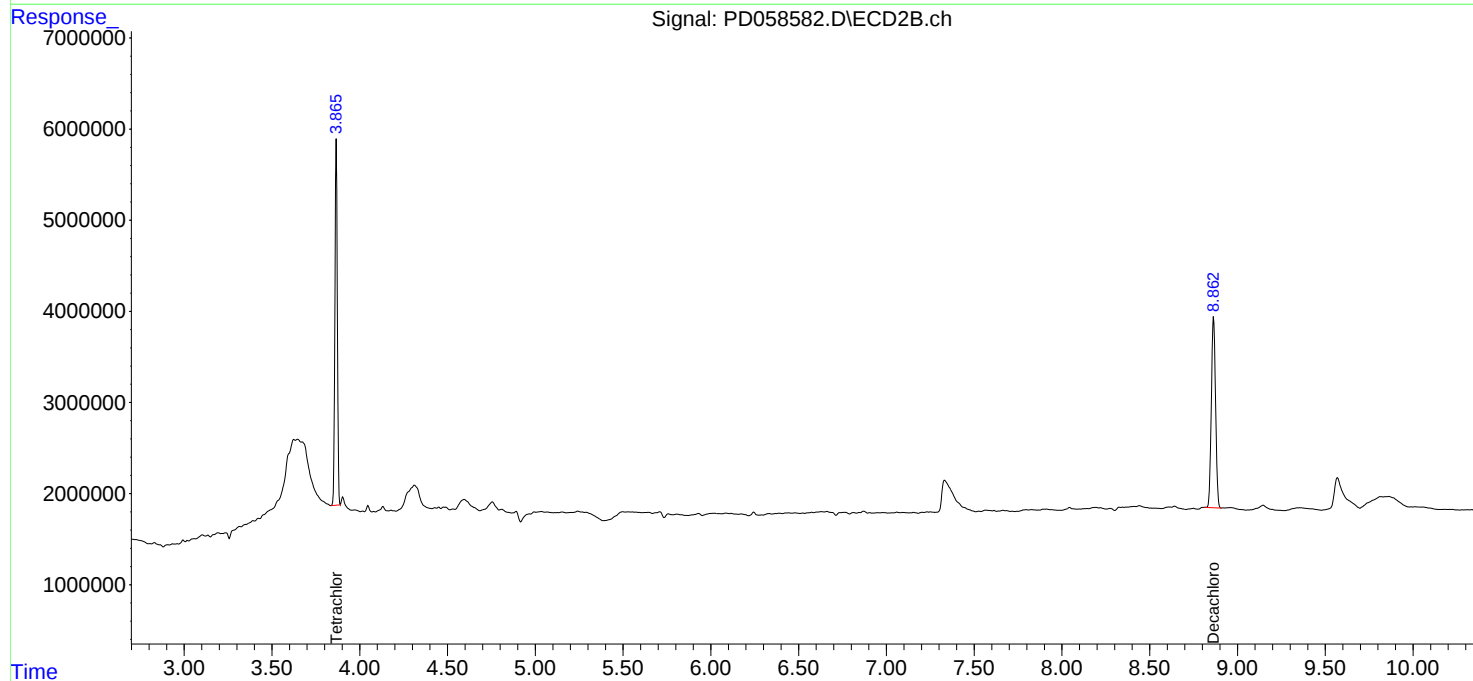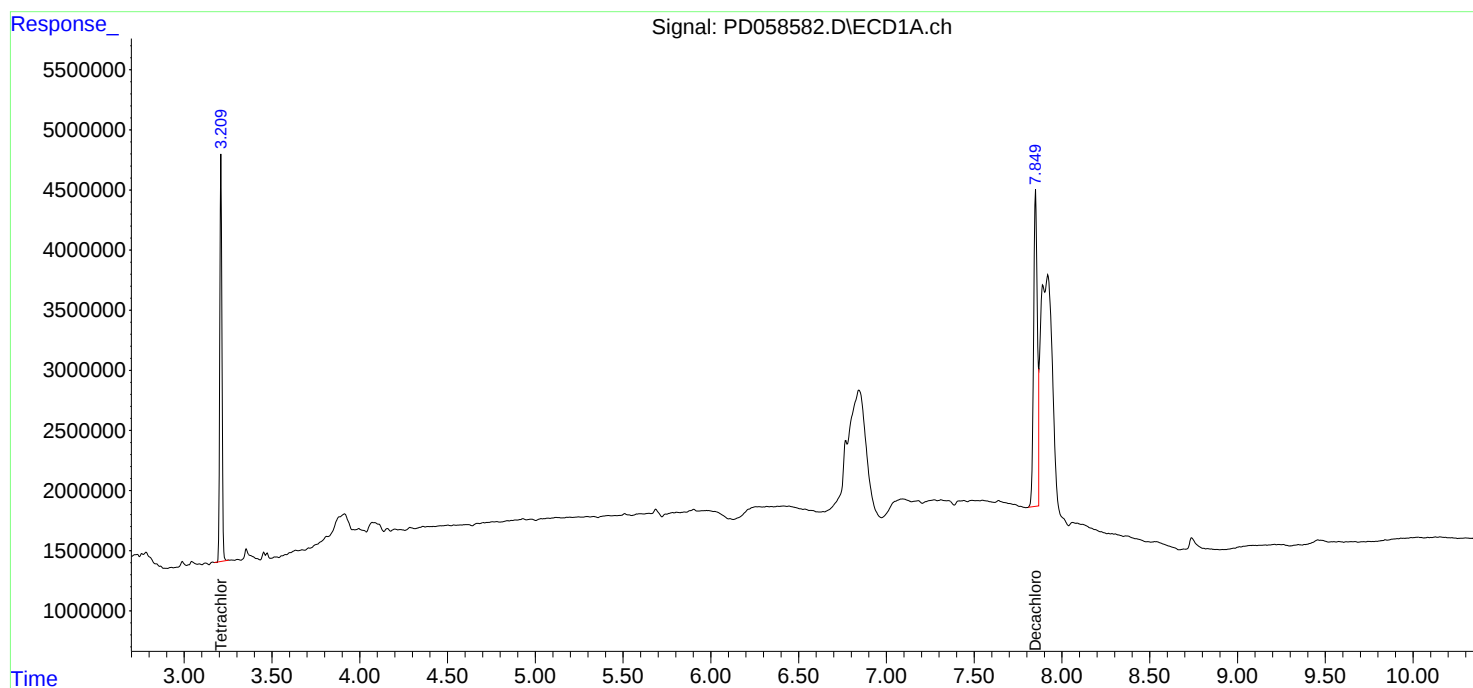

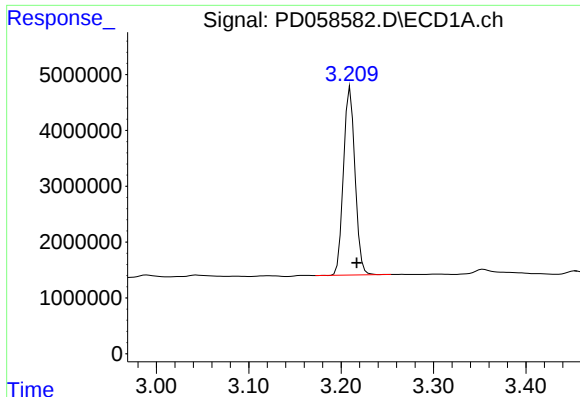


#1 Tetrachloro-m-xylene

R.T.: 3.210 min
Delta R.T.: -0.007 min
Response: 29202656
Conc: 16.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB130051BL


Manual Integrations
APPROVED

Ankita
7/13/2020 3:28:05 PM

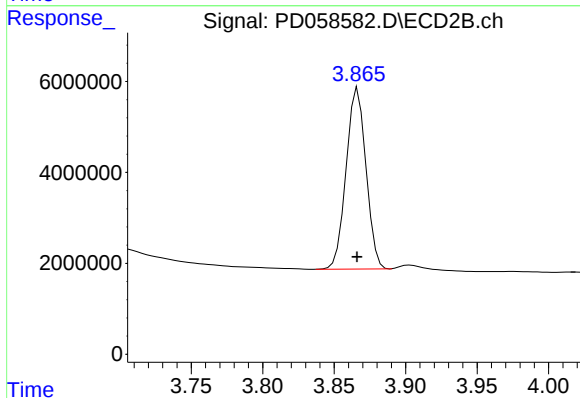


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 38537908
Conc: 15.60 ng/ml

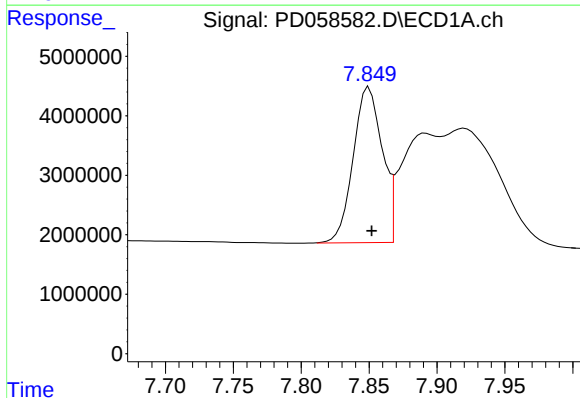

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: -0.003 min
Response: 38710301
Conc: 21.44 ng/ml m

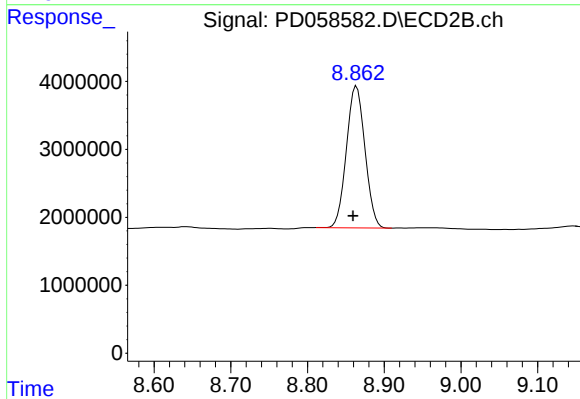

#28 Decachlorobiphenyl

R.T.: 8.864 min
Delta R.T.: 0.005 min
Response: 35226080
Conc: 16.16 ng/ml