

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071023\
 Data File : PD076465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2023 22:01
 Operator : AR\AJ
 Sample : 03509-17RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-WWS-04RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/11/2023
 Supervised By :Ankita Jodhani 07/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 05:05:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:21:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.763	35349262	17503465	10.789	11.019m
28) SA Decachlor...	9.086	7.907	34196235	15602415	9.618	12.397 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071023\
Data File : PD076465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2023 22:01
Operator : AR\AJ
Sample : 03509-17RE
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-WWS-04RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/11/2023
Supervised By : Ankita Jodhani 07/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 05:05:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:21:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

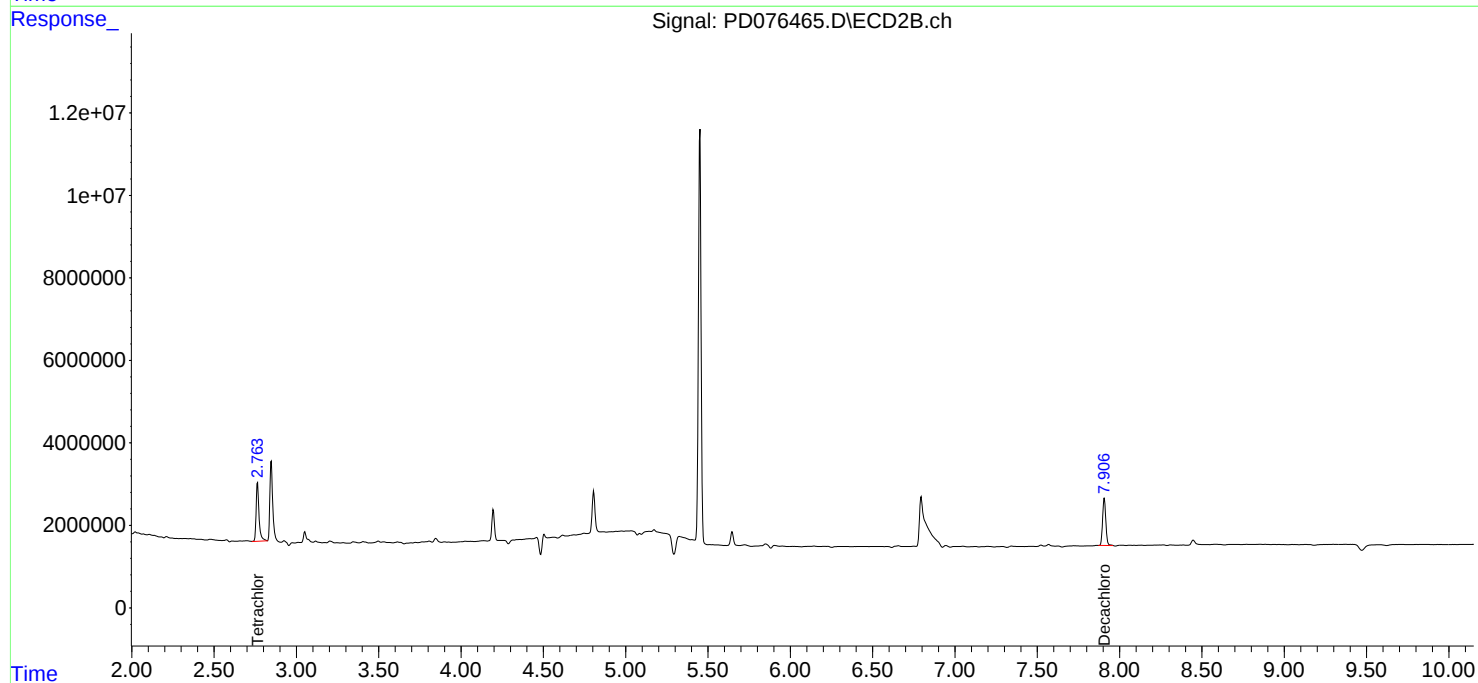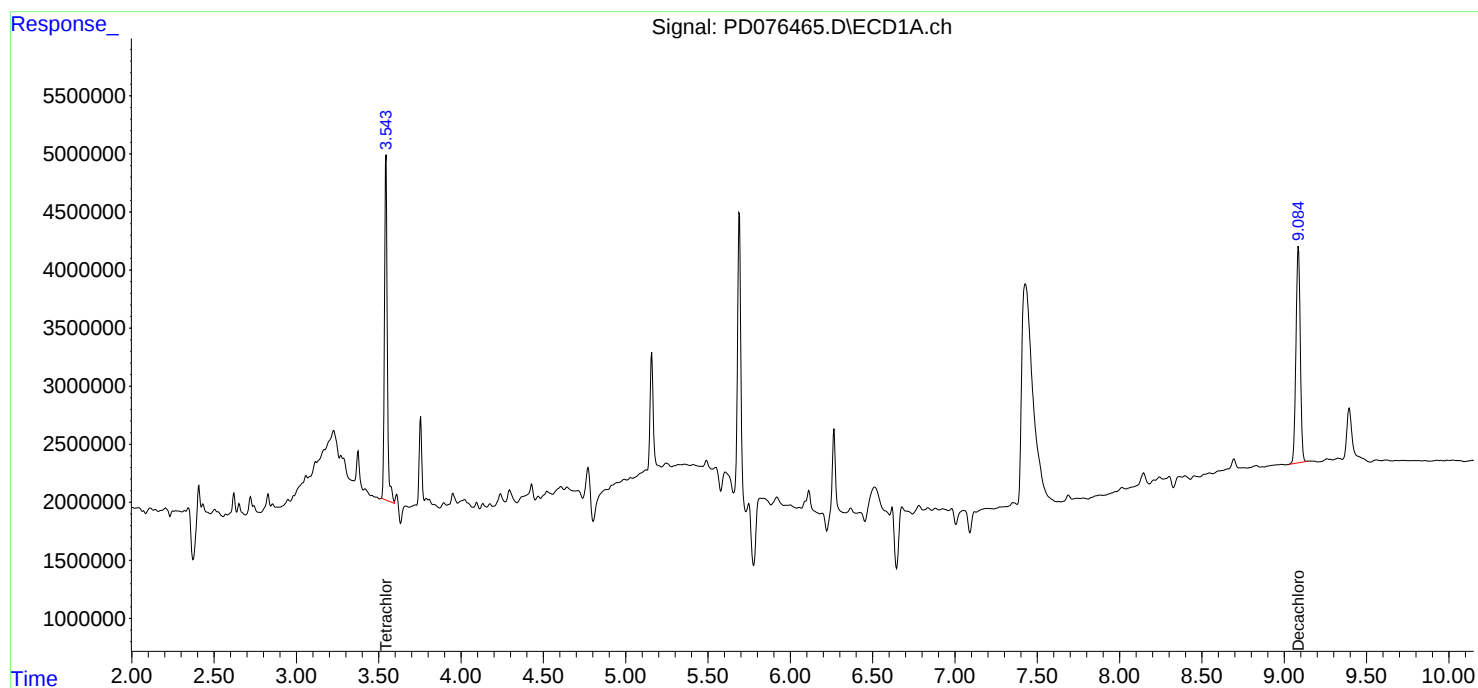

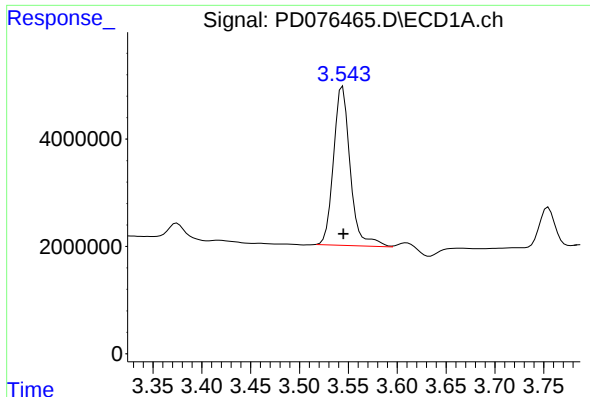


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 35349262
Conc: 10.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-WWS-04RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/11/2023
Supervised By :Ankita Jodhani 07/11/2023

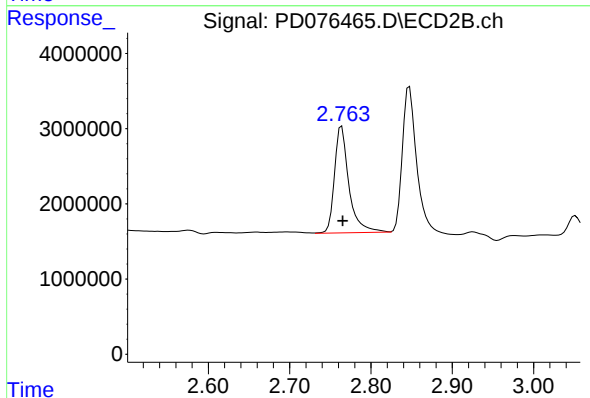


#1 Tetrachloro-m-xylene

R.T.: 2.763 min
Delta R.T.: -0.003 min
Response: 17503465
Conc: 11.02 ng/ml m

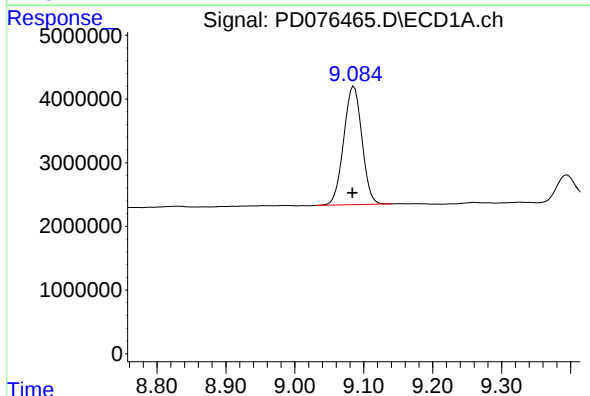

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.002 min
Response: 34196235
Conc: 9.62 ng/ml

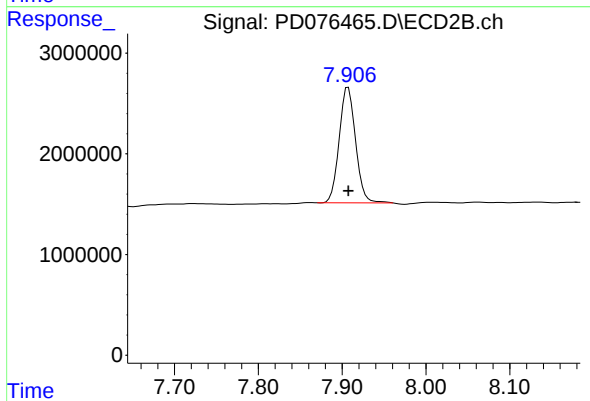

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 15602415
Conc: 12.40 ng/ml