

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 18:18
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:59:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 00:56:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.762	218.3E6	343.5E6	100.187	103.447
28)	SA Decachlor...	9.086	7.907	226.5E6	106.7E6	94.482	93.323
Target Compounds							
23)	Chlordane-1	4.711	3.762	1108.6E6	400.7E6	1020.709	1011.004
24)	Chlordane-2	5.242	4.338	989.9E6	370.4E6	989.746	978.922
25)	Chlordane-3	5.954	4.970	4795.7E6	1325.8E6	1006.289	973.594
26)	Chlordane-4	6.036	5.033	5588.6E6	1284.5E6	1000.957	992.903
27)	Chlordane-5	6.888	5.929	975.5E6	485.4E6	1026.596	1010.106



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 18:18
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:59:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 00:56:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

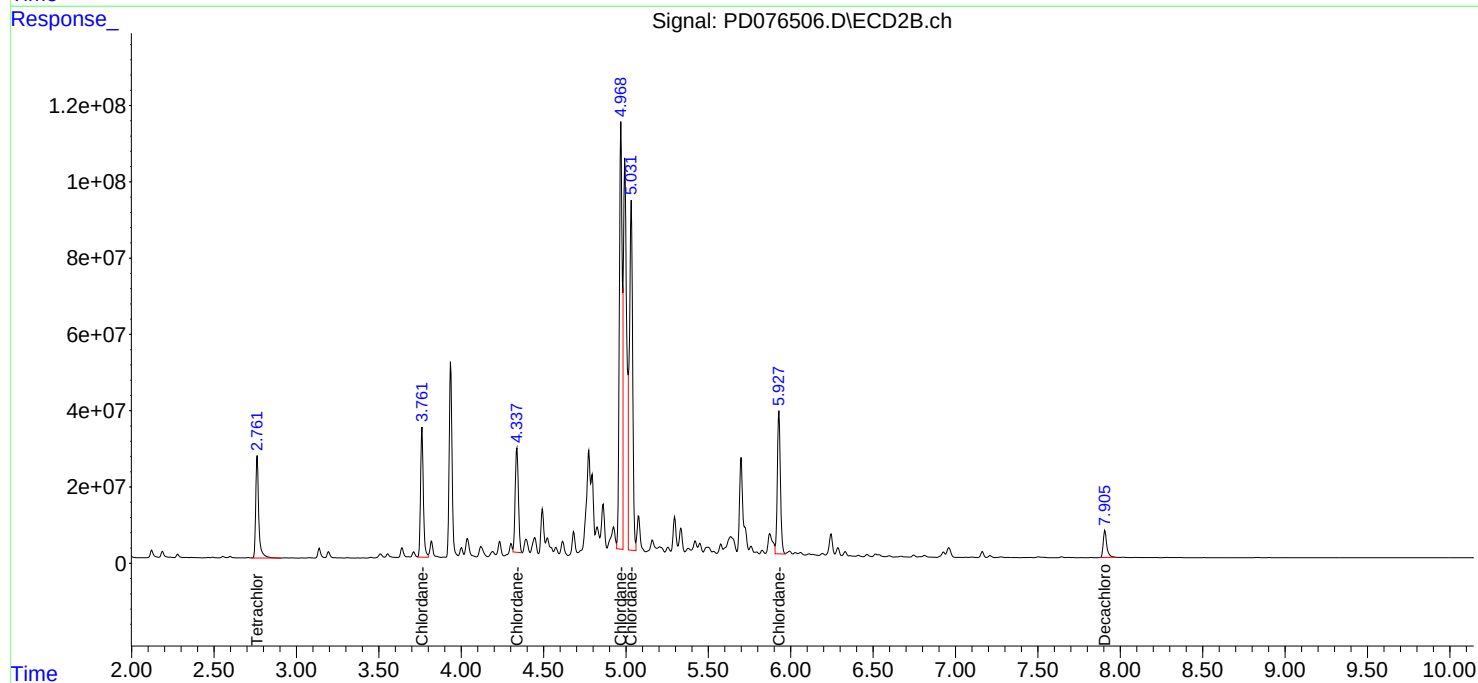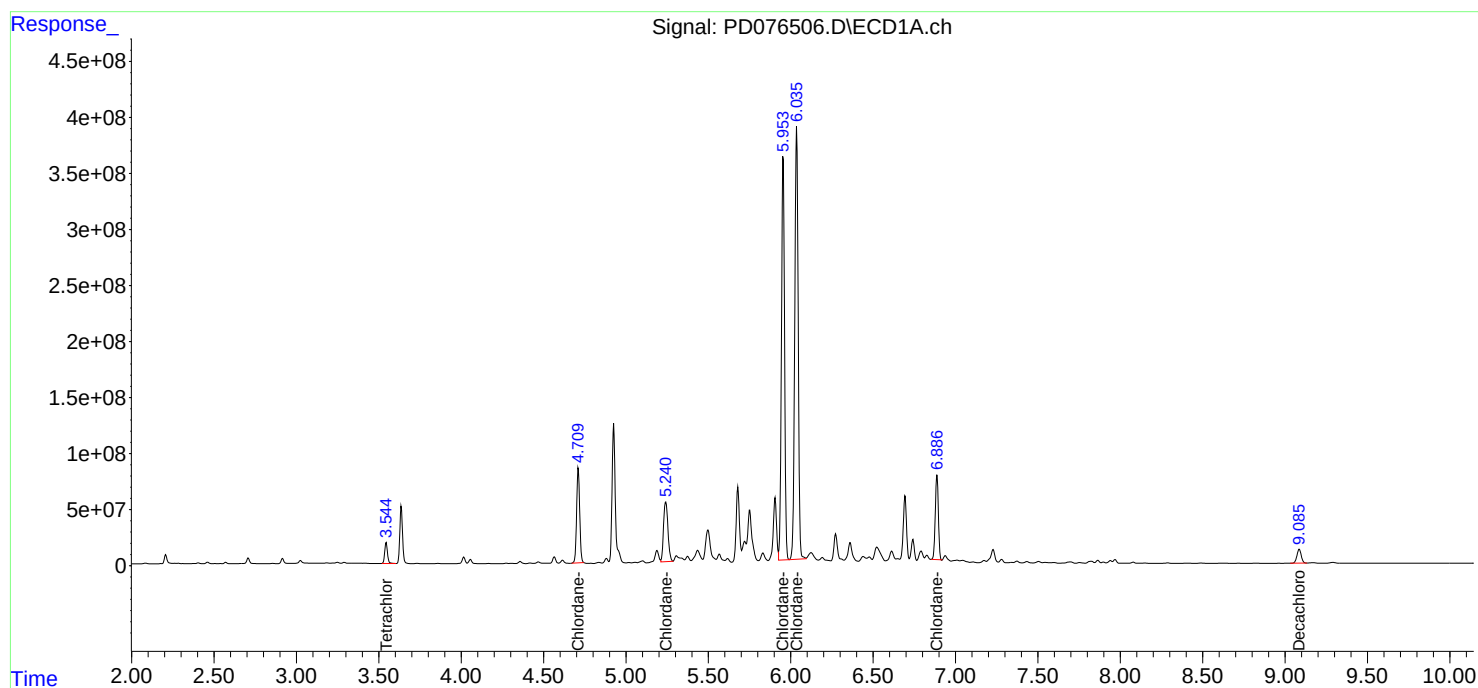


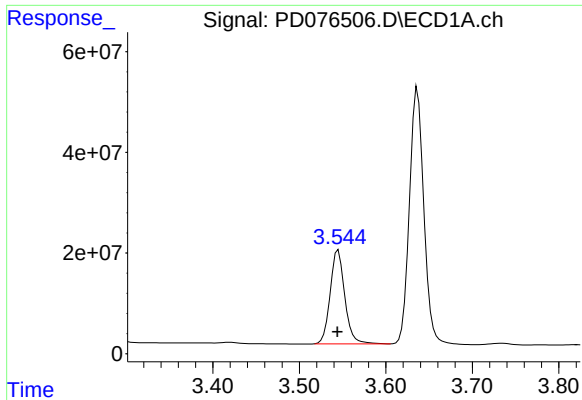

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.001 min
Response: 218300334
Conc: 100.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

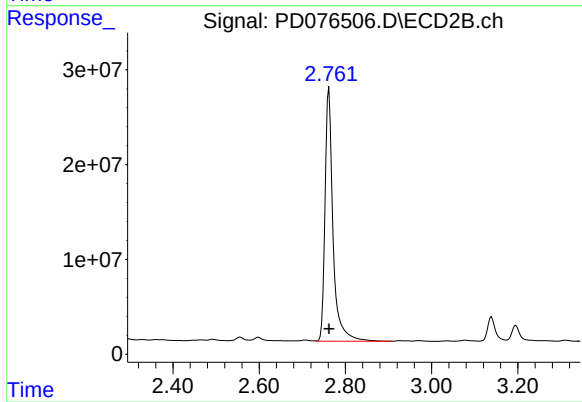


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 343530185
Conc: 103.45 ng/ml

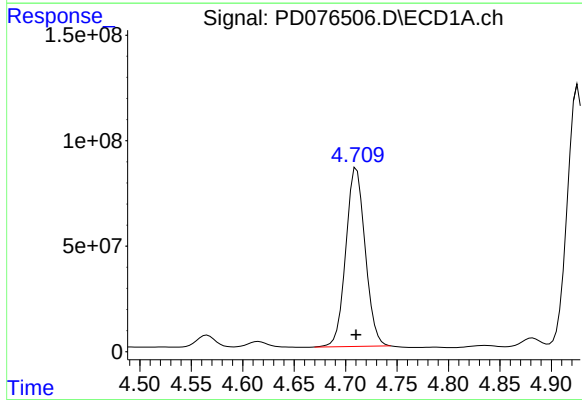


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 1108619399
Conc: 1020.71 ng/ml

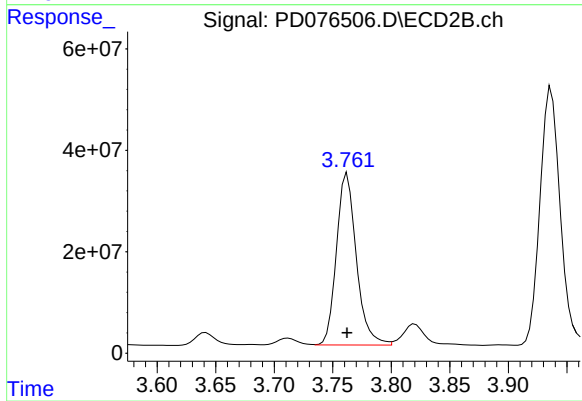

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 400660444
Conc: 1011.00 ng/ml

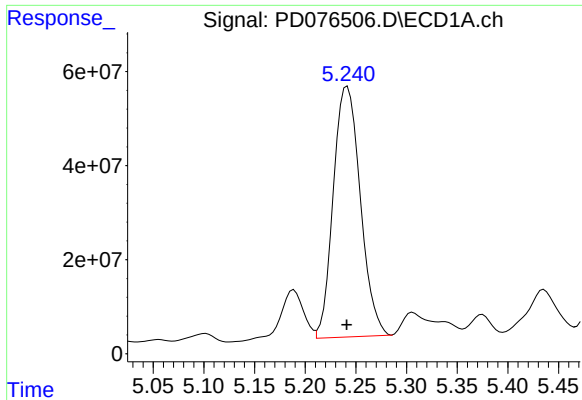

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 989857704
Conc: 989.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

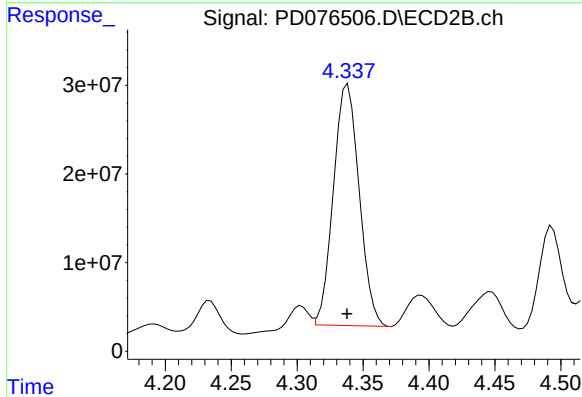


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 370377368
Conc: 978.92 ng/ml

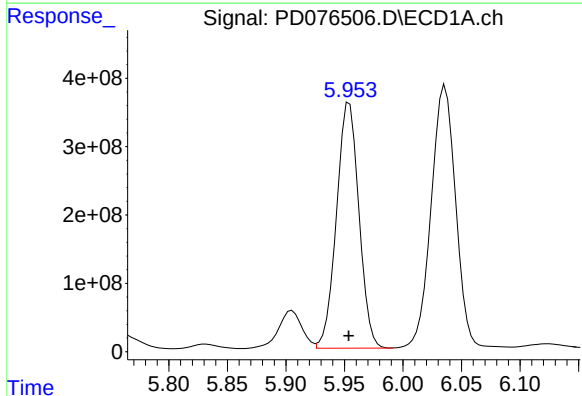


#25 Chlordane-3

R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 4795719098
Conc: 1006.29 ng/ml

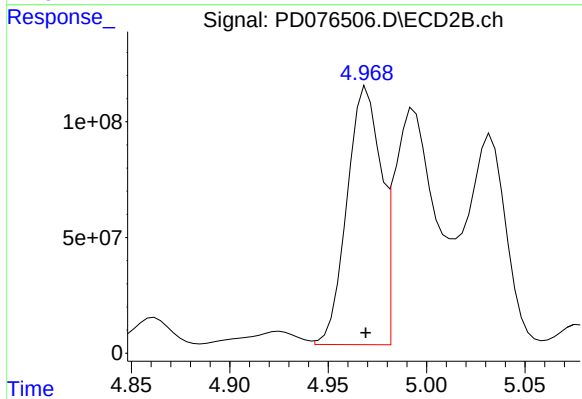

#25 Chlordane-3


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 1325816557
Conc: 973.59 ng/ml

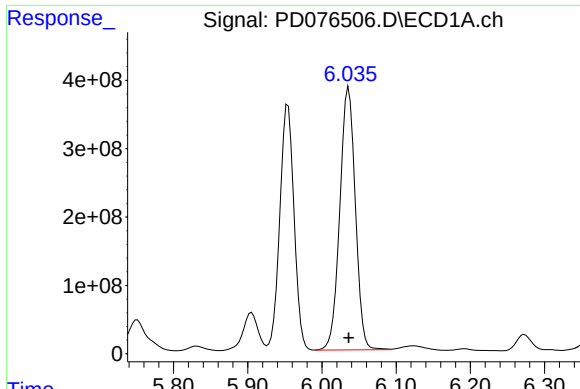

#26 Chlordane-4


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 5588603968
Conc: 1000.96 ng/m

Instrument :
ECD_D
ClientSampleId :

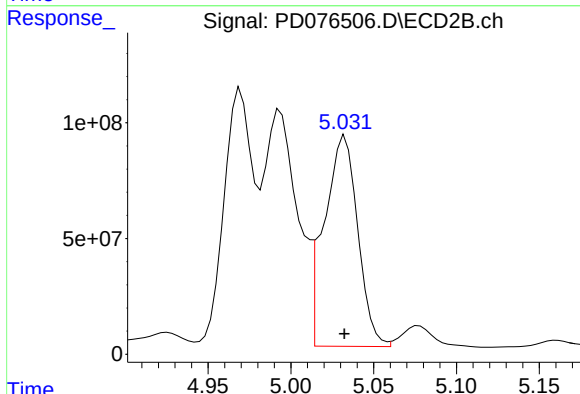


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 1284497059
Conc: 992.90 ng/ml

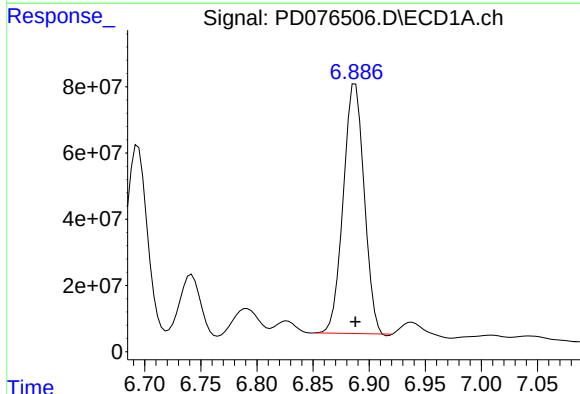


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 975480886
Conc: 1026.60 ng/ml

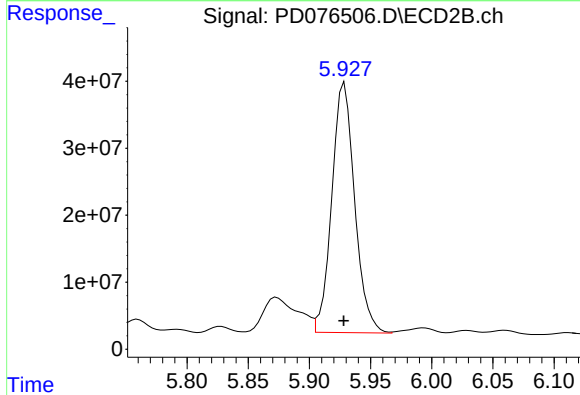

#27 Chlordane-5

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 485424891
Conc: 1010.11 ng/ml

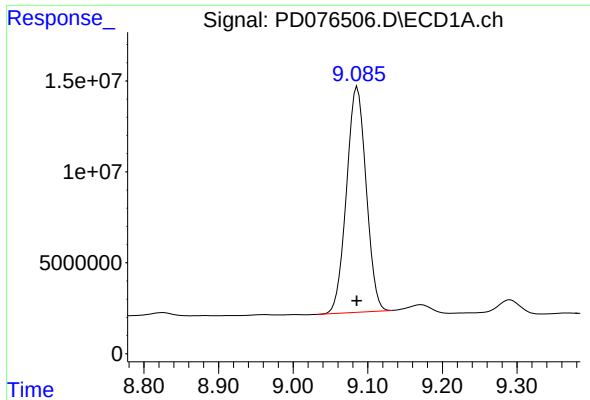

#28 Decachlorobiphenyl


R.T.: 9.086 min

Delta R.T.: 0.000 min

Response: 226484923

Conc: 94.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

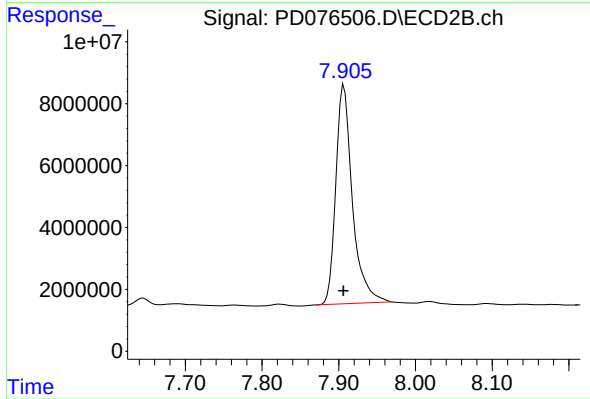

#28 Decachlorobiphenyl

R.T.: 7.907 min

Delta R.T.: 0.000 min

Response: 106745816

Conc: 93.32 ng/ml