

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071123\
 Data File : PS023699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 19:29
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 02:01:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.384	6.806	3139193	724992	2.485	1.728 #
Target Compounds							
1) T	Dalapon	2.468	2.583	597979	4209479	<MDL	6.014 #
2) T	3,5-DICHL...	5.771	5.987	1240395	779549	<MDL	1.204 #
3) T	4-Nitroph...	6.212	6.378f	1336607	344296	1.494	1.194
5) T	DICAMBA	6.519	6.985	347603	452175	<MDL	<MDL #
8) T	DICHLORPROP	7.110	7.606	-1579637	533493	N.D.	1.147
9) T	2,4-D	0.000	7.820f	0	367396	N.D.	<MDL
10) T	Pentachlo...	7.539	0.000	498639	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.070	0.000	584417	0	<MDL	N.D. #
12) T	2,4,5-T	8.323	9.079	1662323	2543673	<MDL	1.042 #
13) T	2,4-DB	8.854	0.000	1963544	0	1.994	N.D. #
14) T	DINOSEB	9.889	0.000	514913	0	<MDL	N.D. #
15) T	Picloram	9.710	10.829	37744703	9149858	3.219	2.163 #
16) T	DCPA	10.145	10.829	1594232	9149858	<MDL	3.298 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071123\
Data File : PS023699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 19:29
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 02:01:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

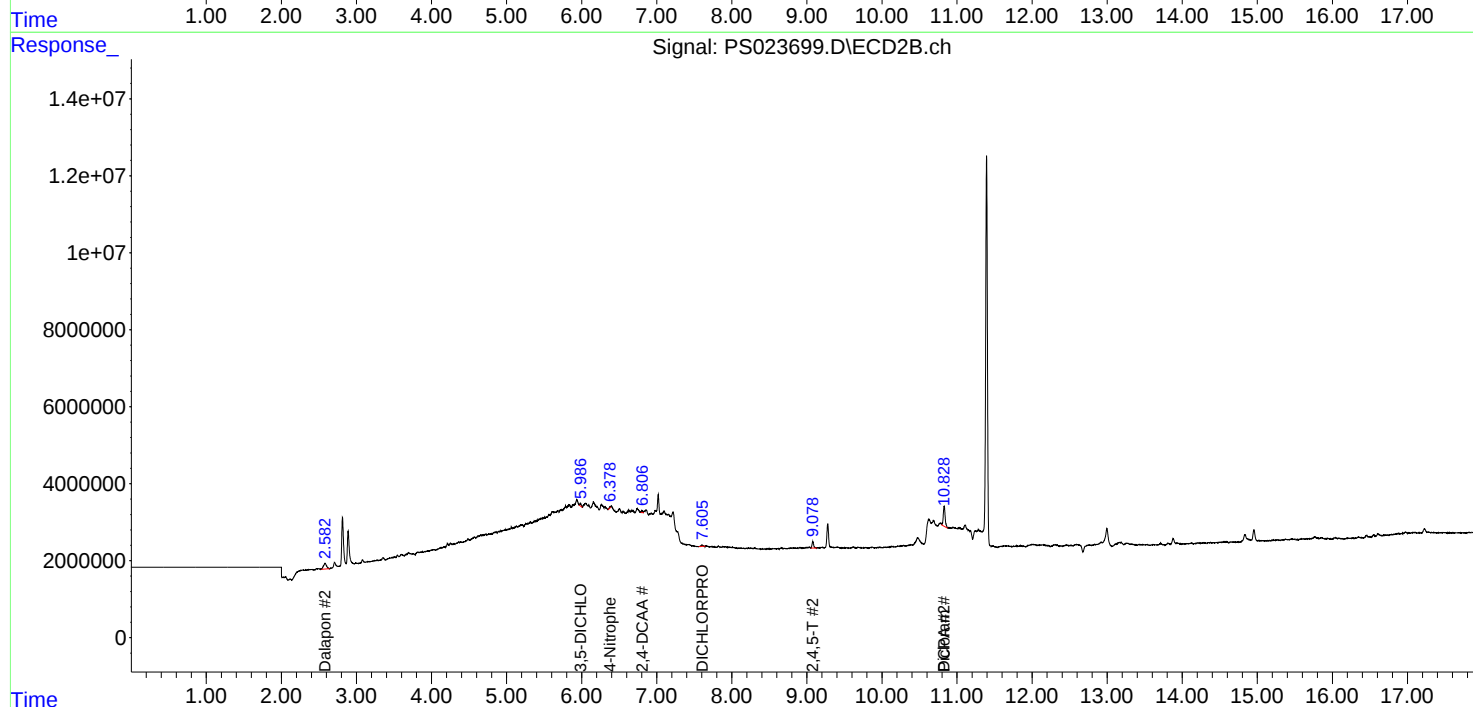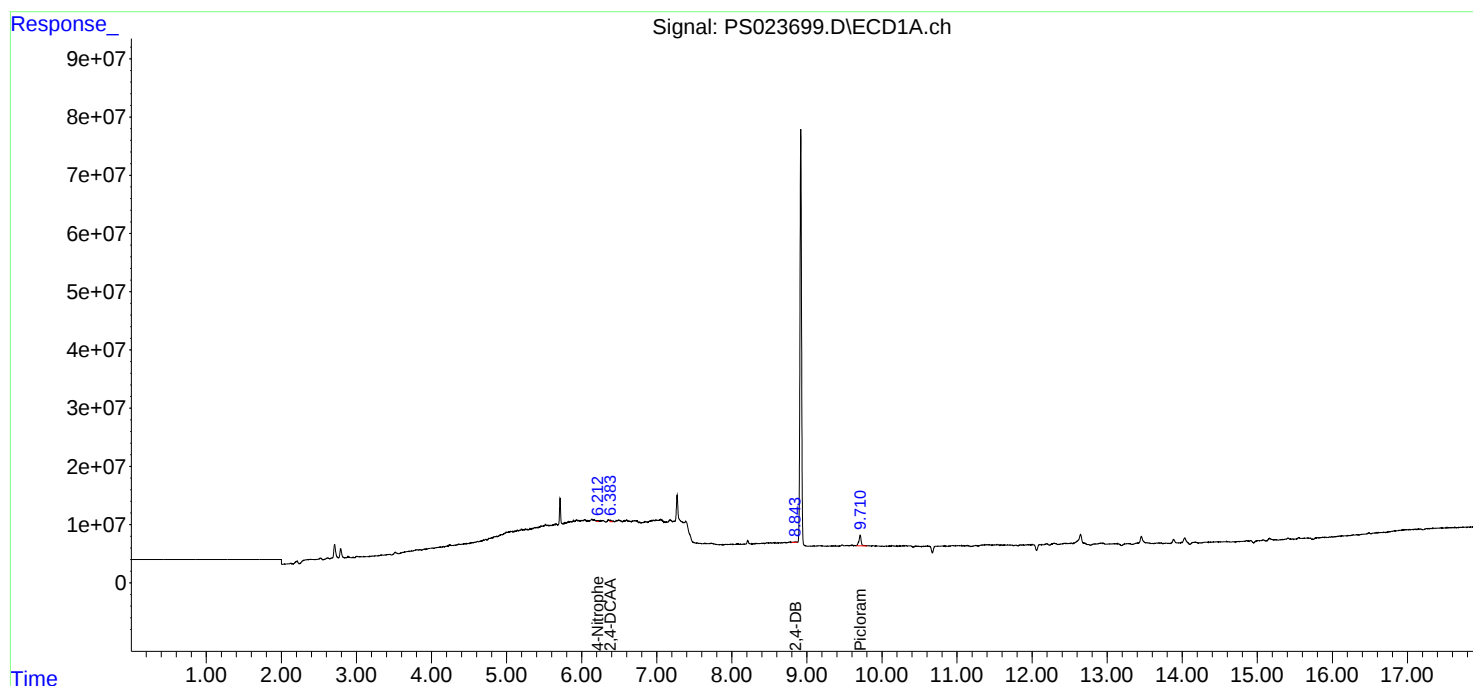


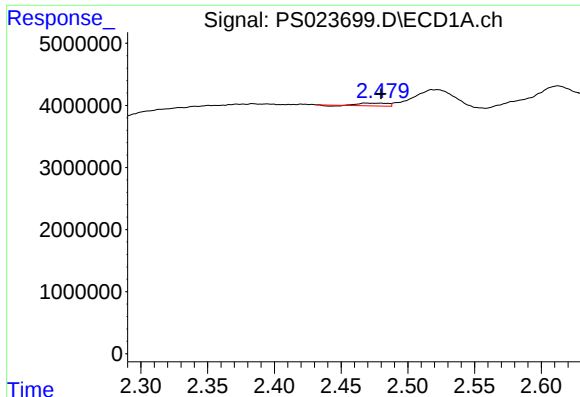

#1 Dalapon


R.T.: 2.468 min
Delta R.T.: -0.012 min
Response: 597979
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

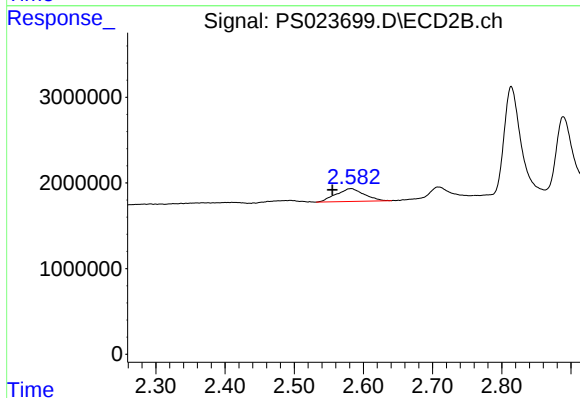


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: 0.028 min
Response: 4209479
Conc: 6.01 ng/ml

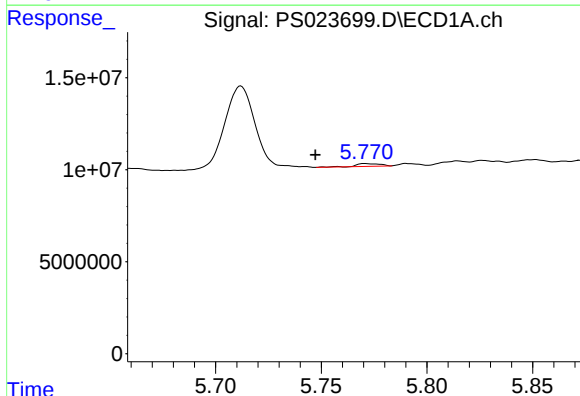


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.771 min
Delta R.T.: 0.024 min
Response: 1240395
Conc: N.D.

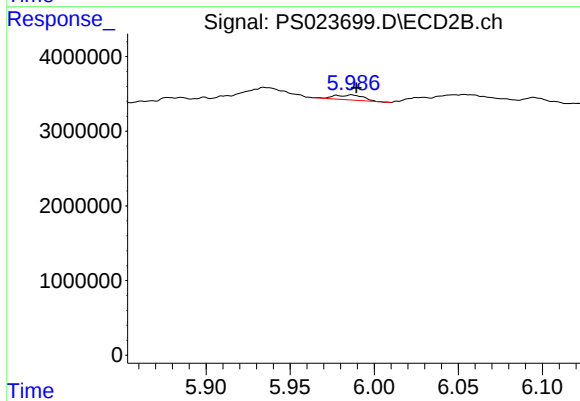

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.987 min
Delta R.T.: -0.003 min
Response: 779549
Conc: 1.20 ng/ml

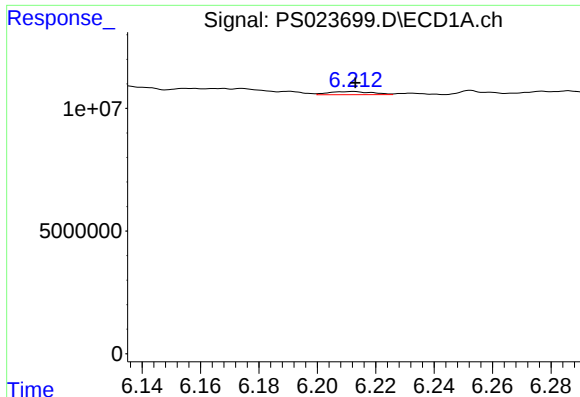

#3 4-Nitrophenol


R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 1336607
Conc: 1.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

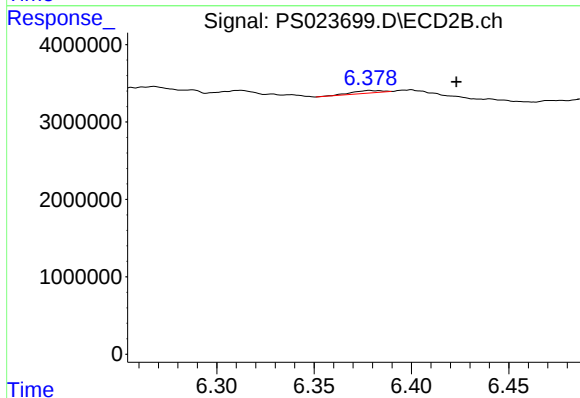


#3 4-Nitrophenol

R.T.: 6.378 min
Delta R.T.: -0.045 min
Response: 344296
Conc: 1.19 ng/ml

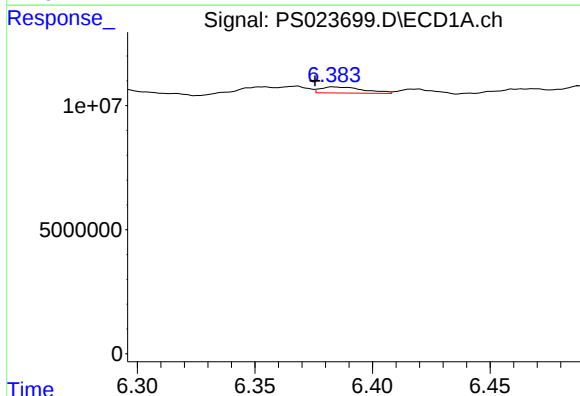


#4 2,4-DCAA

R.T.: 6.384 min
Delta R.T.: 0.008 min
Response: 3139193
Conc: 2.49 ng/ml

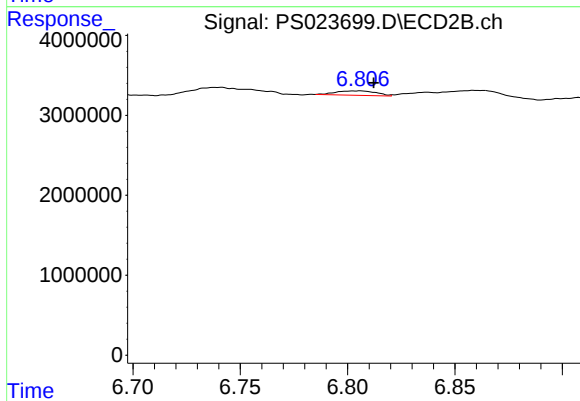

#4 2,4-DCAA


R.T.: 6.806 min
Delta R.T.: -0.006 min
Response: 724992
Conc: 1.73 ng/ml

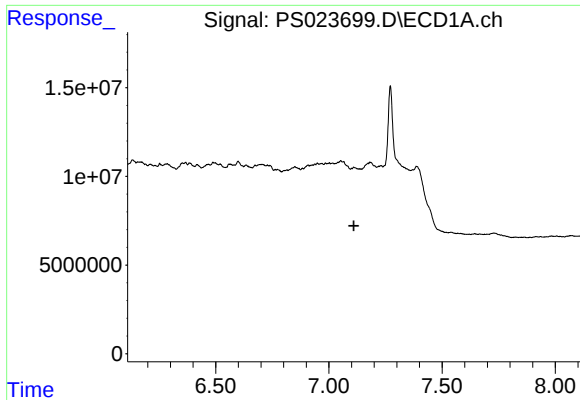

#8 DICHLORPROP


R.T.: 7.110 min
Delta R.T.: 0.000 min
Response: -1579637
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

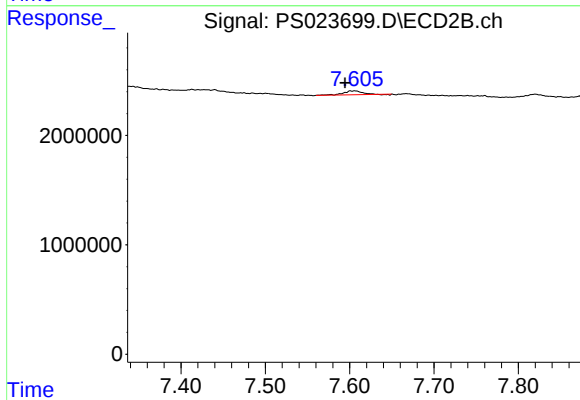


#8 DICHLORPROP

R.T.: 7.606 min
Delta R.T.: 0.012 min
Response: 533493
Conc: 1.15 ng/ml

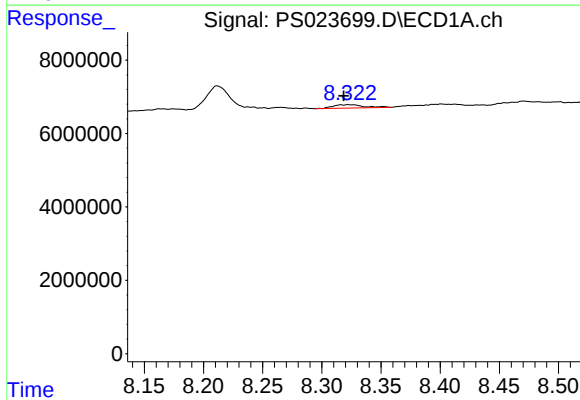


#12 2,4,5-T

R.T.: 8.323 min
Delta R.T.: 0.005 min
Response: 1662323
Conc: N.D.

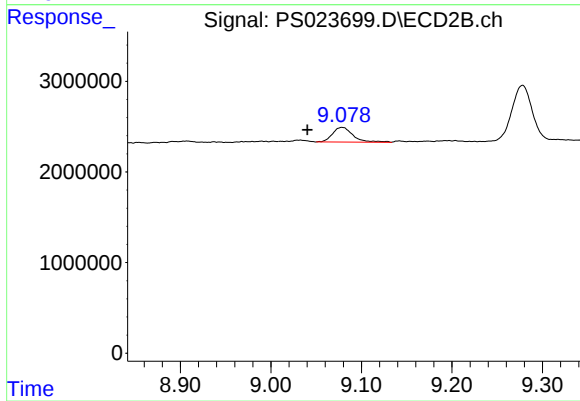

#12 2,4,5-T


R.T.: 9.079 min
Delta R.T.: 0.038 min
Response: 2543673
Conc: 1.04 ng/ml

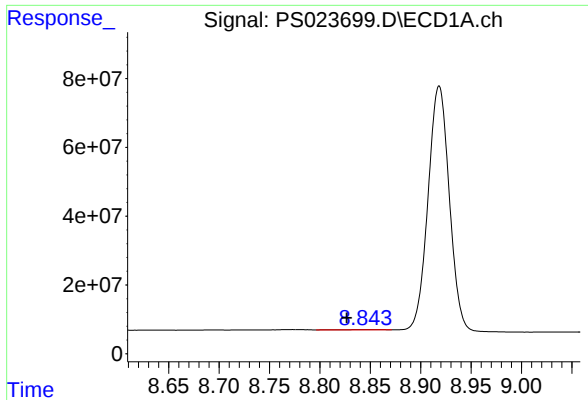

#13 2,4-DB


R.T.: 8.854 min
Delta R.T.: 0.028 min
Response: 1963544
Conc: 1.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

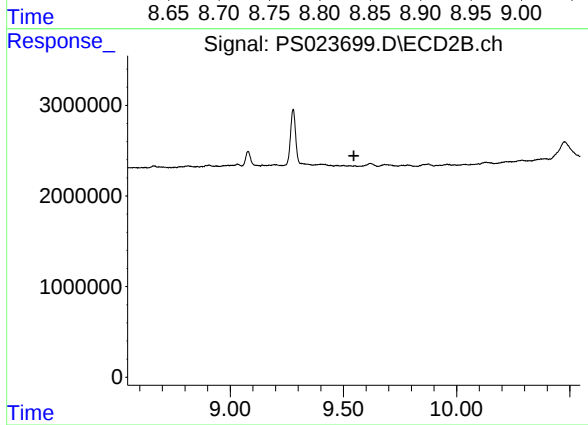


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.546 min
Response: 0
Conc: N.D.

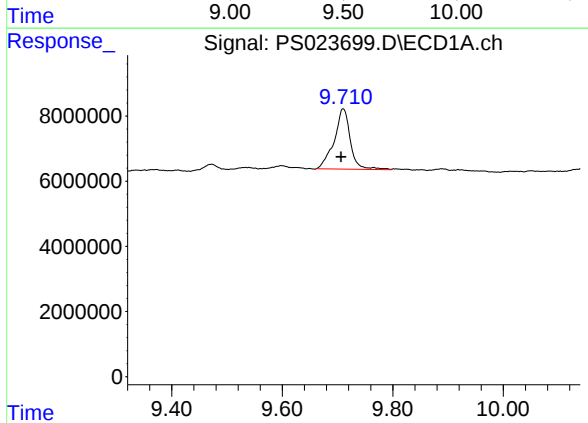


#15 Picloram

R.T.: 9.710 min
Delta R.T.: 0.004 min
Response: 37744703
Conc: 3.22 ng/ml

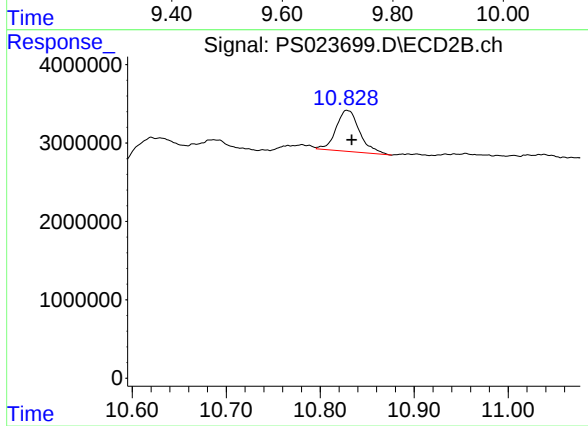

#15 Picloram


R.T.: 10.829 min
Delta R.T.: -0.005 min
Response: 9149858
Conc: 2.16 ng/ml

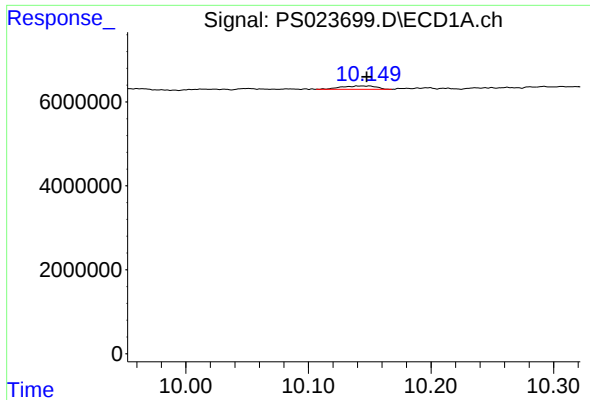

#16 DCPA

R.T.: 10.145 min
Delta R.T.: -0.003 min
Response: 1594232
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

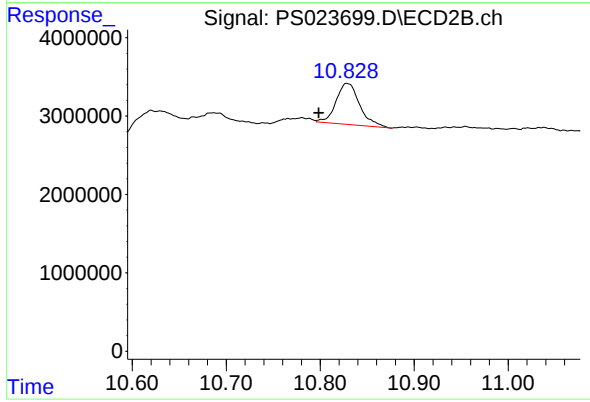

#16 DCPA

R.T.: 10.829 min
Delta R.T.: 0.030 min
Response: 9149858
Conc: 3.30 ng/ml