

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 18:31
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:12:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:12:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.762	160.2E6	250.5E6	73.960	74.434
28)	SA Decachlor...	9.086	7.908	170.6E6	80257921	73.774	73.707
Target Compounds							
23)	Chlordane-1	4.710	3.762	812.7E6	293.8E6	743.688	741.444
24)	Chlordane-2	5.242	4.338	735.1E6	279.6E6	742.477	747.937
25)	Chlordane-3	5.954	4.969	3553.9E6	989.4E6	745.576	740.805
26)	Chlordane-4	6.036	5.033	4156.9E6	969.7E6	746.103	751.470
27)	Chlordane-5	6.888	5.929	715.3E6	355.5E6	745.253	740.610



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 18:31
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:12:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:12:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

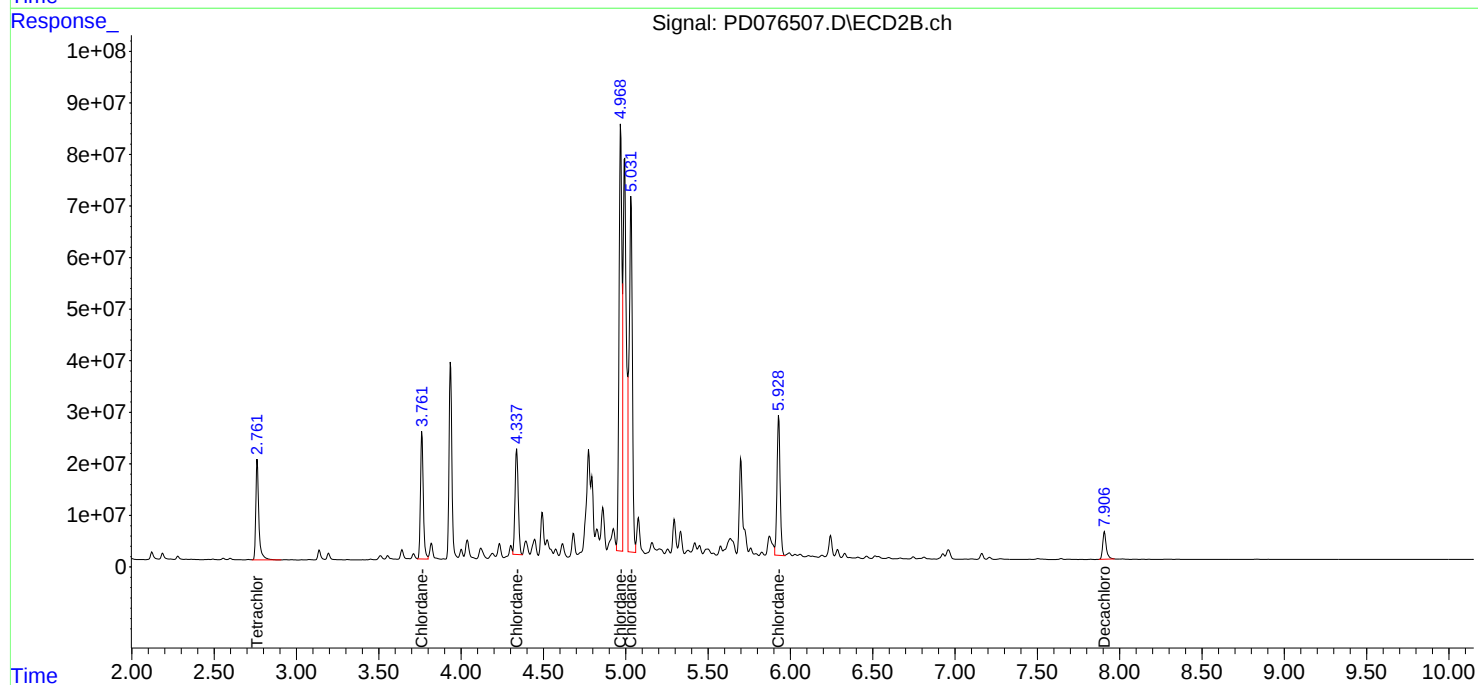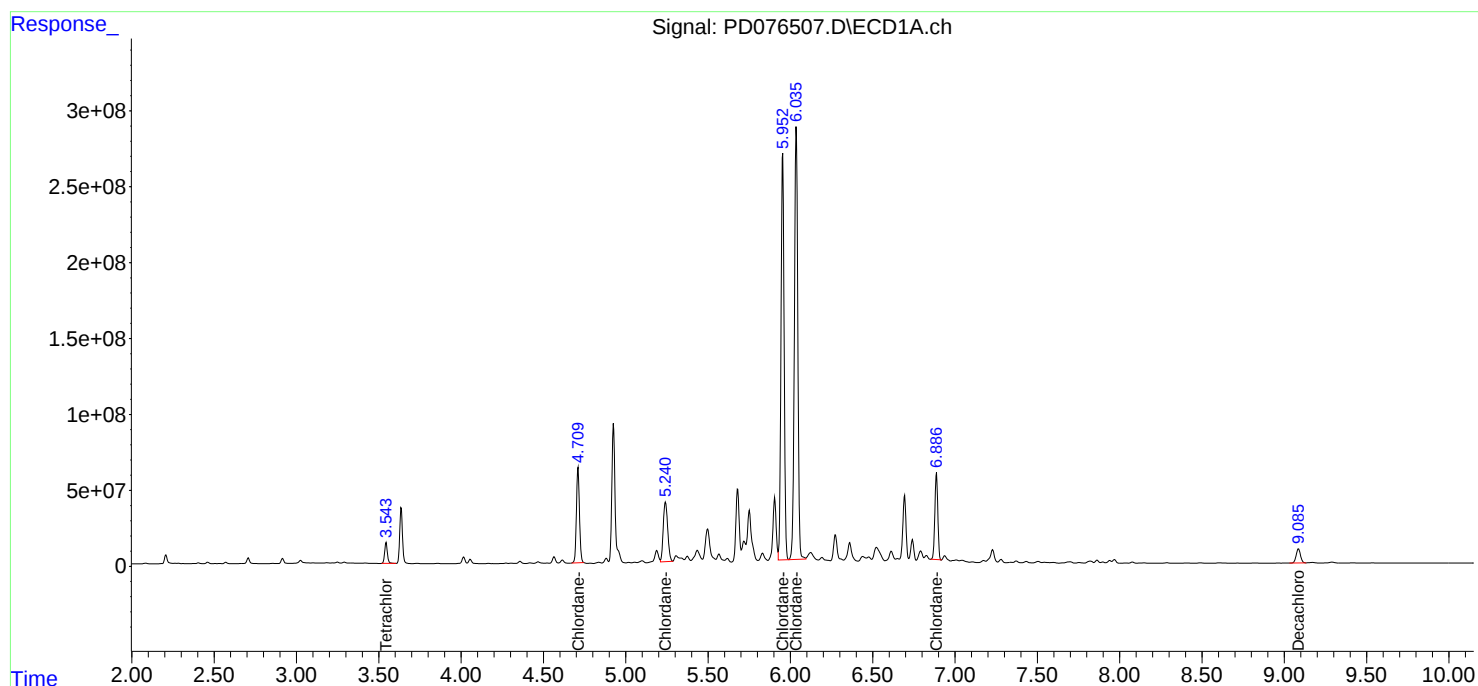


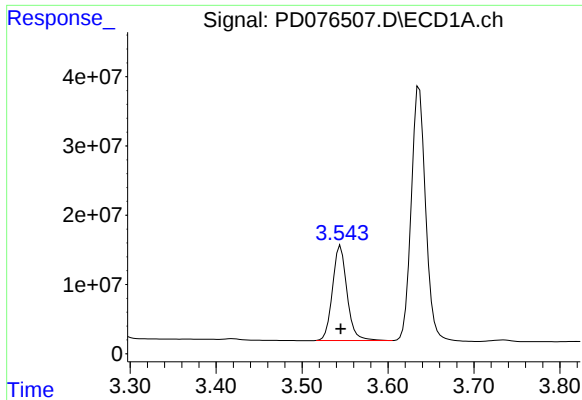

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 160193344
Conc: 73.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

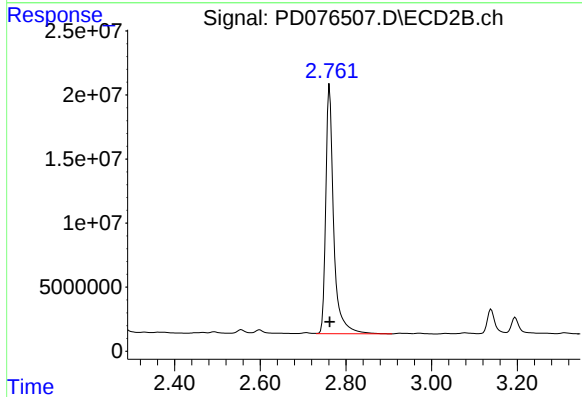


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 250495655
Conc: 74.43 ng/ml

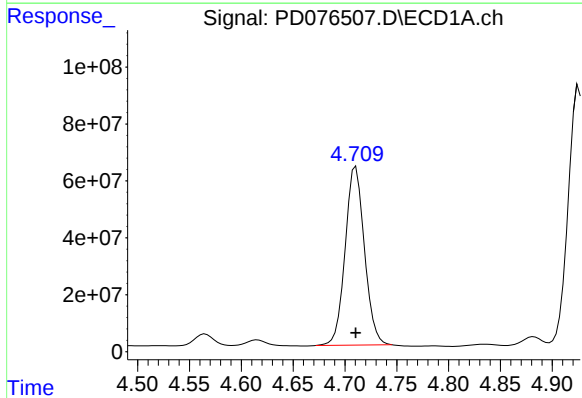


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 812683862
Conc: 743.69 ng/ml

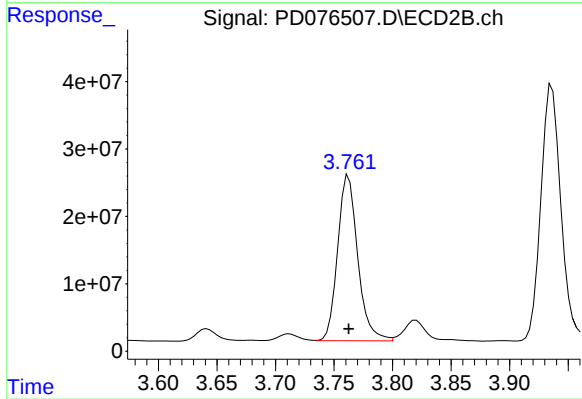

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 293775044
Conc: 741.44 ng/ml

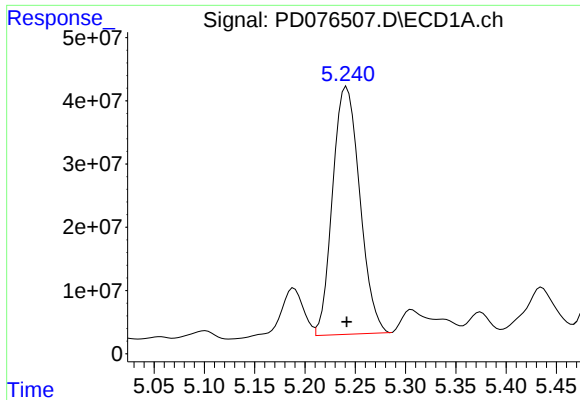

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 735066678
Conc: 742.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

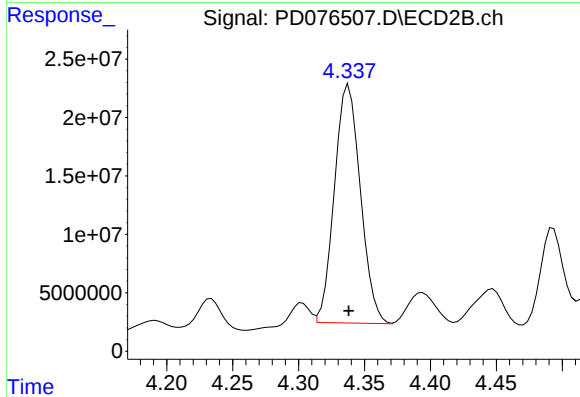


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 279616797
Conc: 747.94 ng/ml

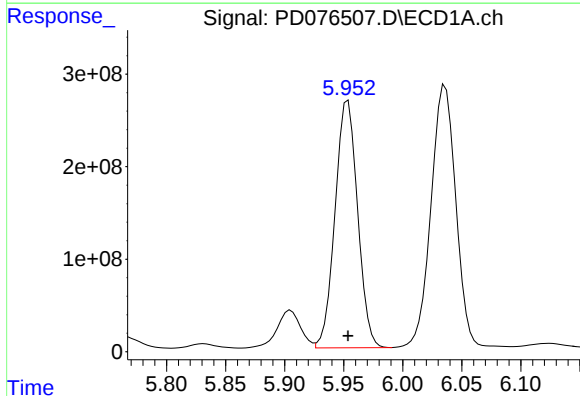


#25 Chlordane-3

R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 3553916374
Conc: 745.58 ng/ml

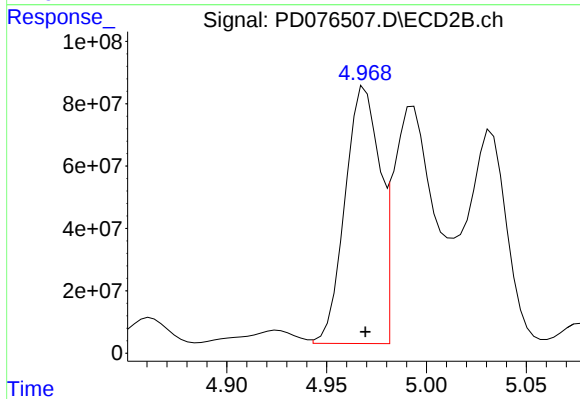

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 989426834
Conc: 740.81 ng/ml

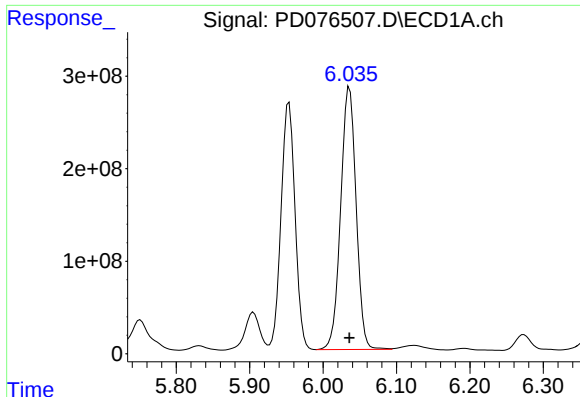

#26 Chlordane-4


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 4156884607
Conc: 746.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

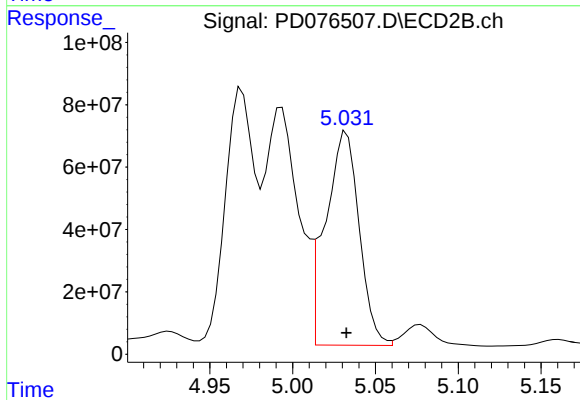


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 969660403
Conc: 751.47 ng/ml

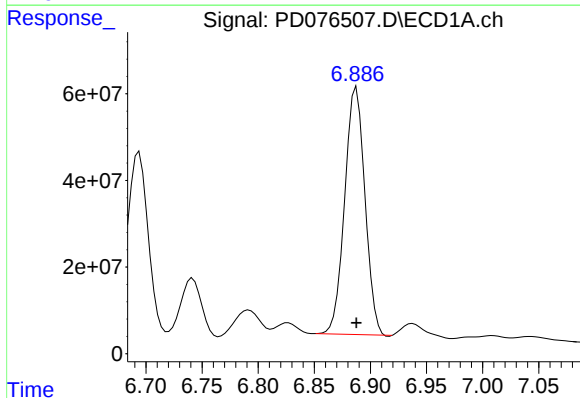


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 715299530
Conc: 745.25 ng/ml

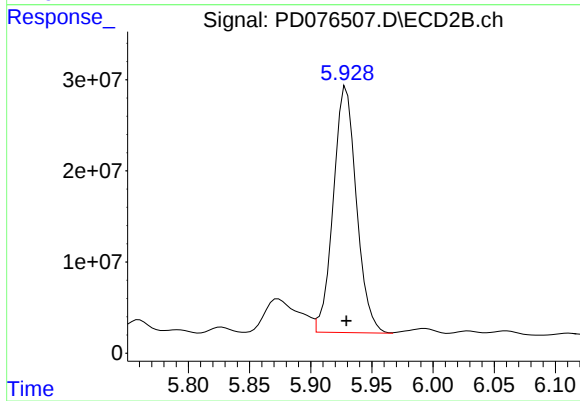

#27 Chlordane-5

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 355486856
Conc: 740.61 ng/ml

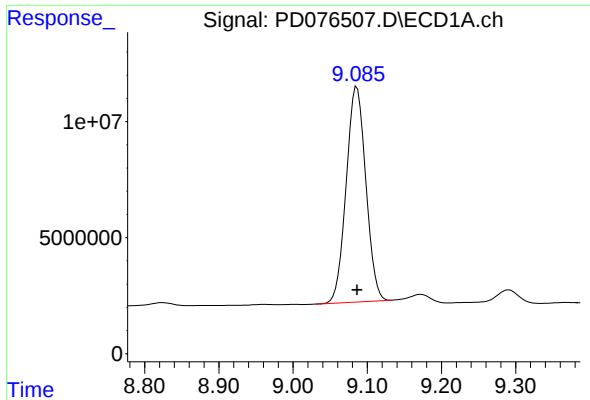

#28 Decachlorobiphenyl


R.T.: 9.086 min

Delta R.T.: 0.000 min

Response: 170573097

Conc: 73.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

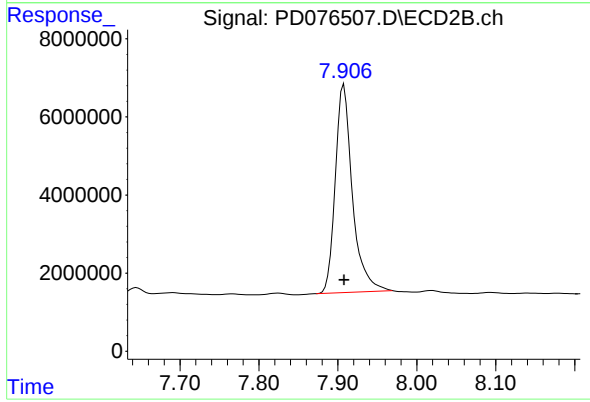

#28 Decachlorobiphenyl

R.T.: 7.908 min

Delta R.T.: 0.000 min

Response: 80257921

Conc: 73.71 ng/ml