

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 18:45
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:06:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:06:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.762	108.9E6	166.0E6	50.000	50.000
28)	SA Decachlor...	9.085	7.907	119.9E6	56452765	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.710	3.762	543.1E6	198.1E6	500.000	500.000
24)	Chlordane-2	5.241	4.338	500.1E6	189.2E6	500.000	500.000
25)	Chlordane-3	5.954	4.969	2382.9E6	680.9E6	500.000	500.000
26)	Chlordane-4	6.036	5.032	2791.6E6	646.8E6	500.000	500.000
27)	Chlordane-5	6.888	5.928	475.1E6	240.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 18:45
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:06:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:06:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

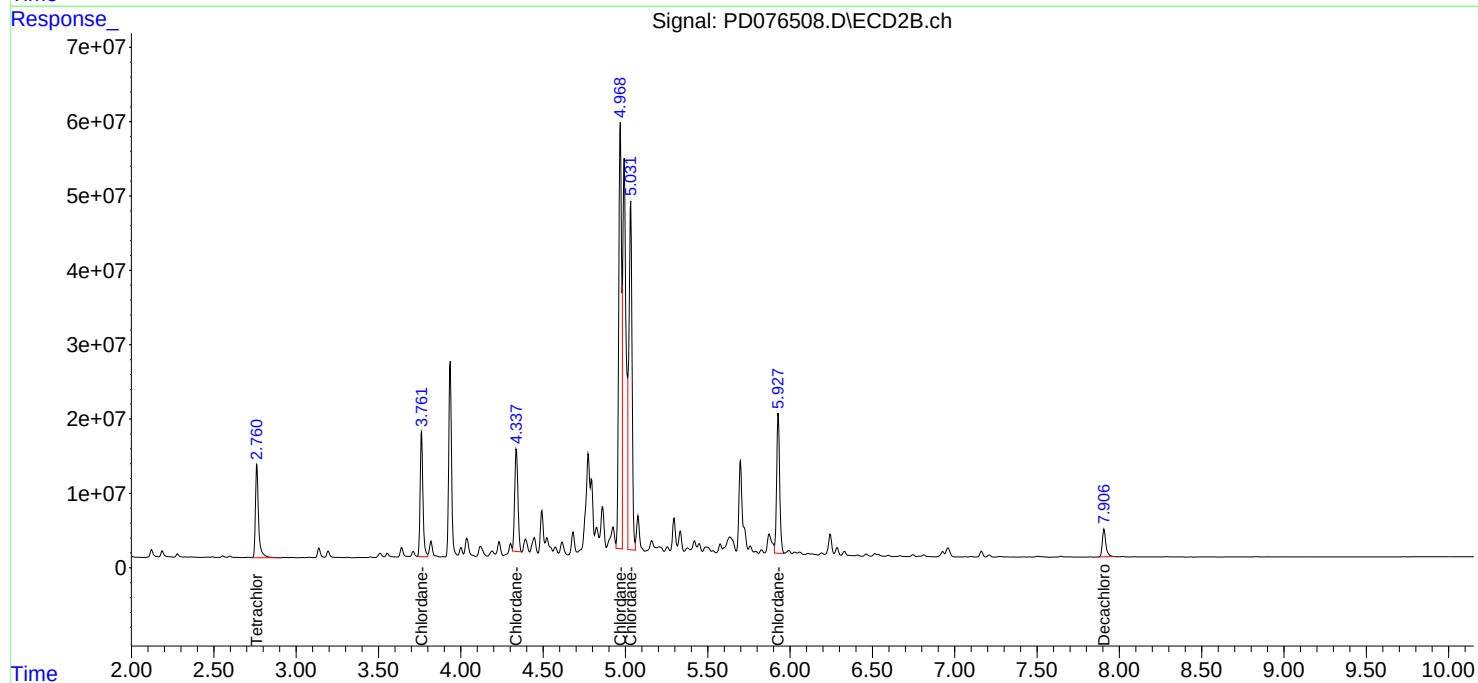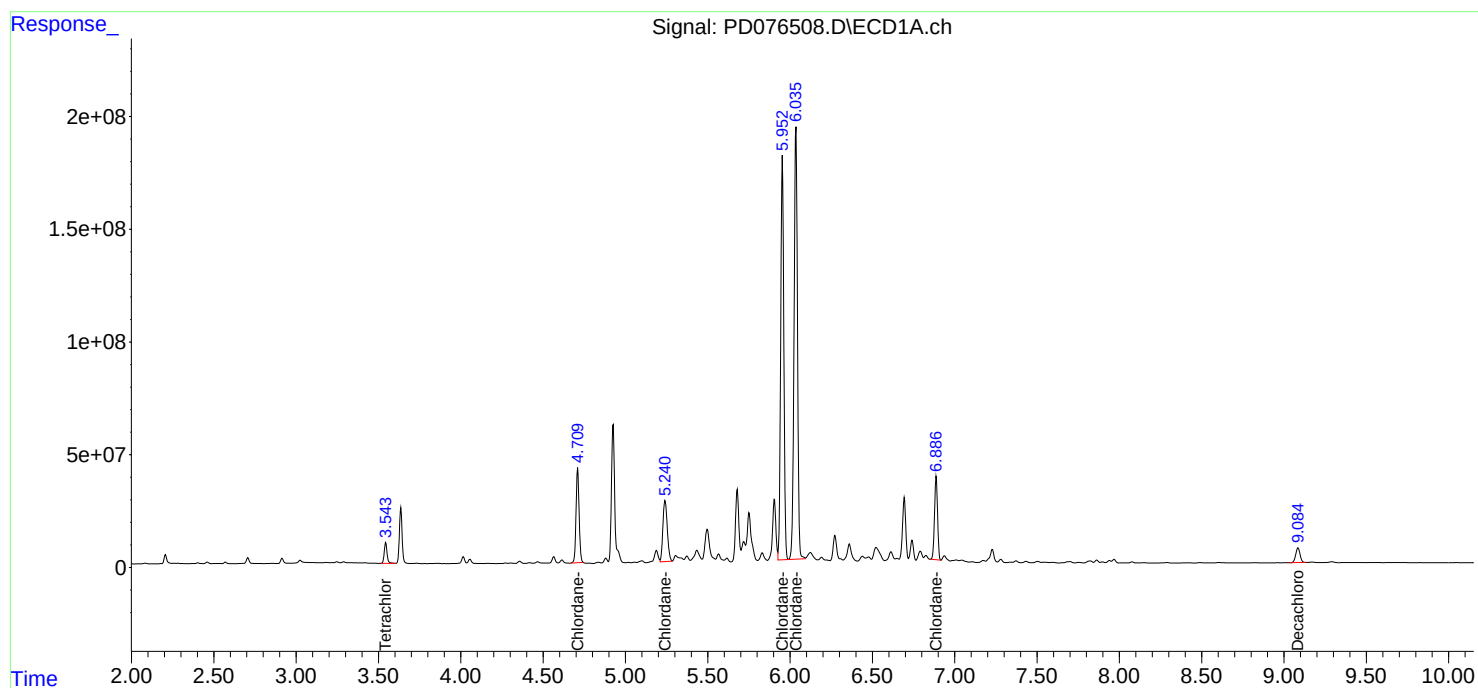


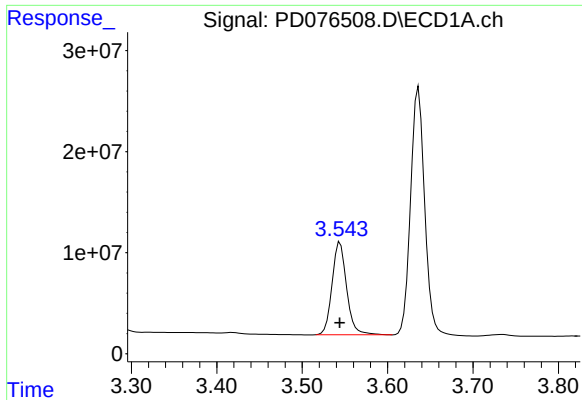

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 108946174
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

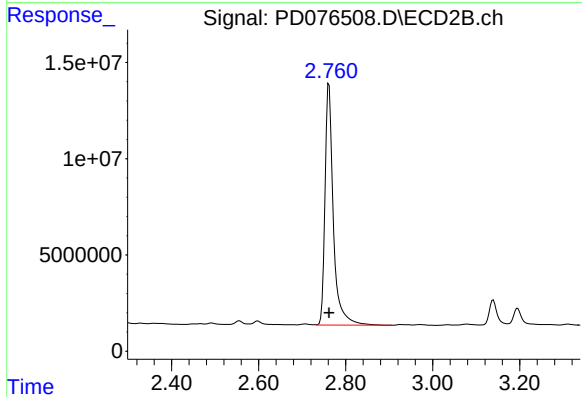


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 166042005
Conc: 50.00 ng/ml

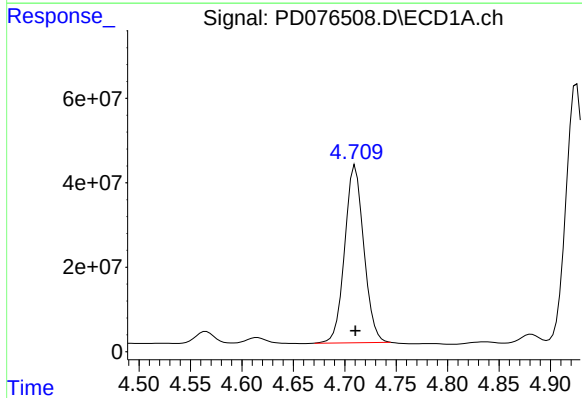


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 543063231
Conc: 500.00 ng/ml

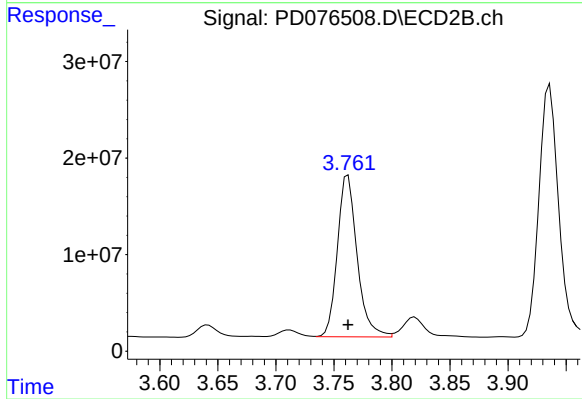

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 198149692
Conc: 500.00 ng/ml

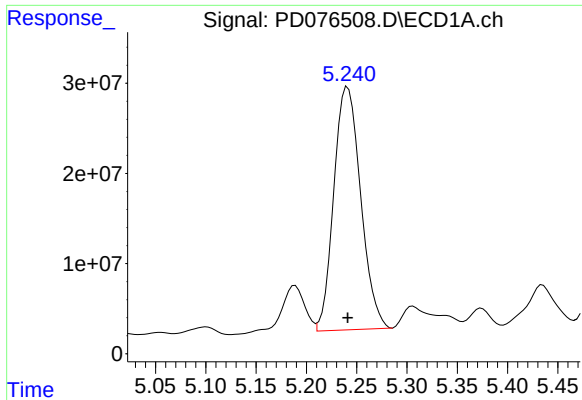

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 500056587
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

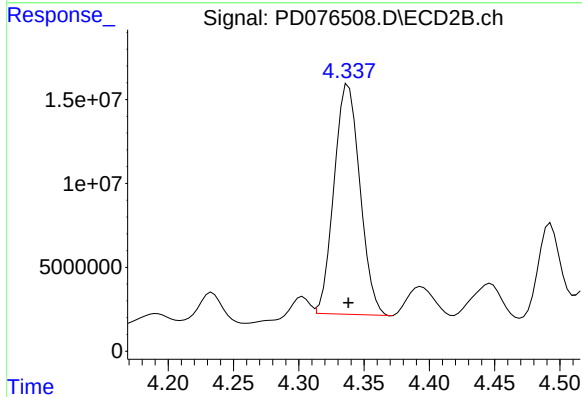


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 189176177
Conc: 500.00 ng/ml

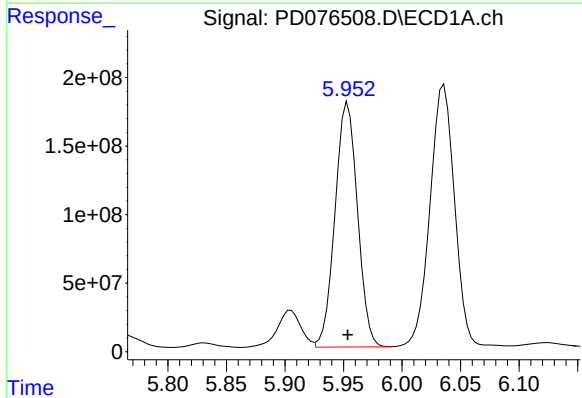


#25 Chlordane-3

R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 2382873878
Conc: 500.00 ng/ml

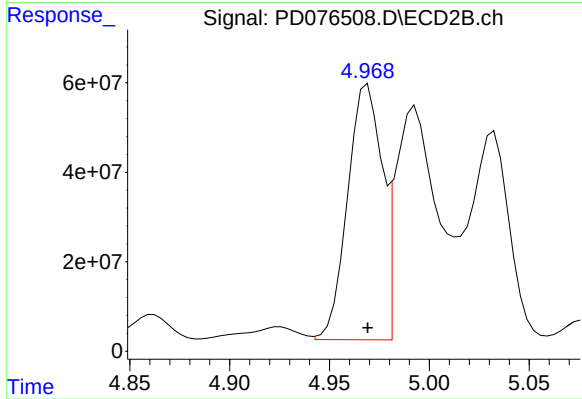

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 680888066
Conc: 500.00 ng/ml

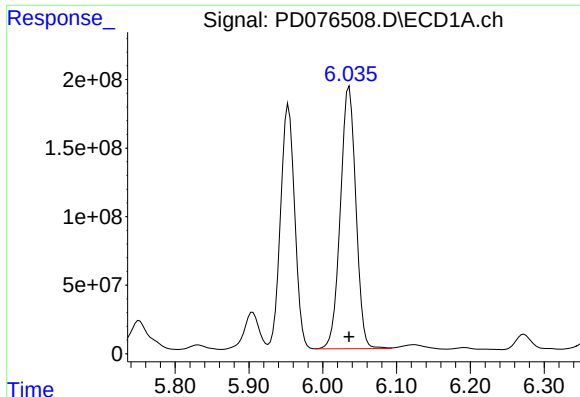

#26 Chlordane-4


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 2791629932
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

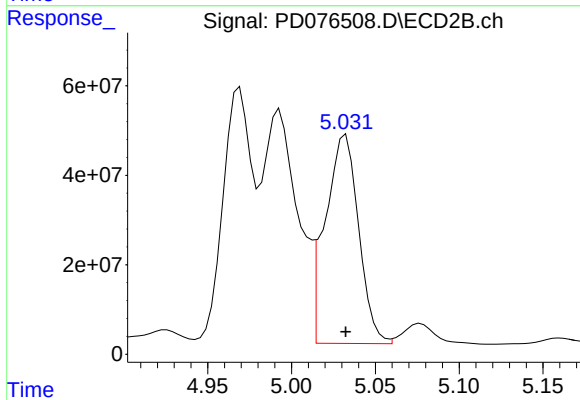


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 646839112
Conc: 500.00 ng/ml

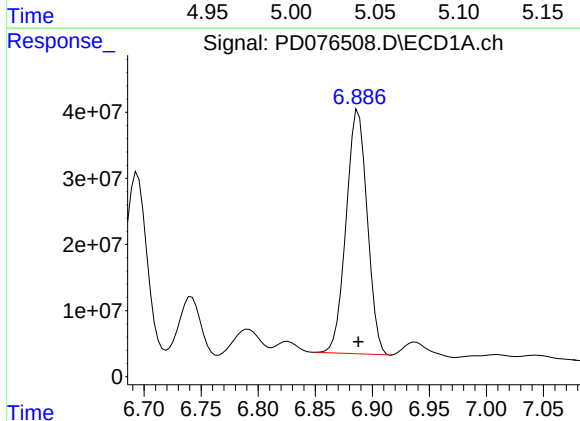


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 475104439
Conc: 500.00 ng/ml

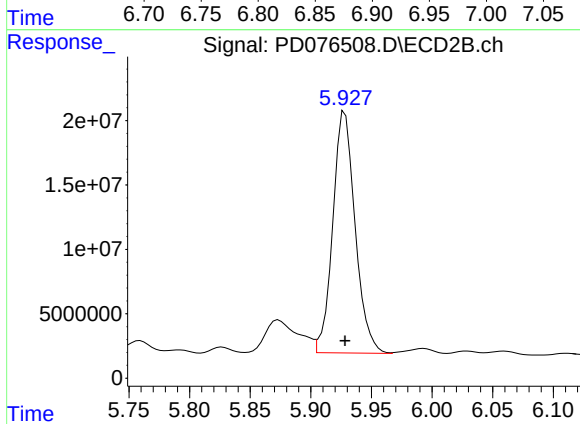

#27 Chlordane-5


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 240284251
Conc: 500.00 ng/ml

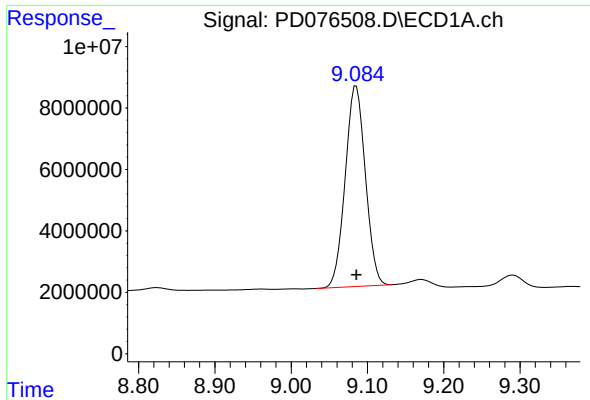

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 119856326
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

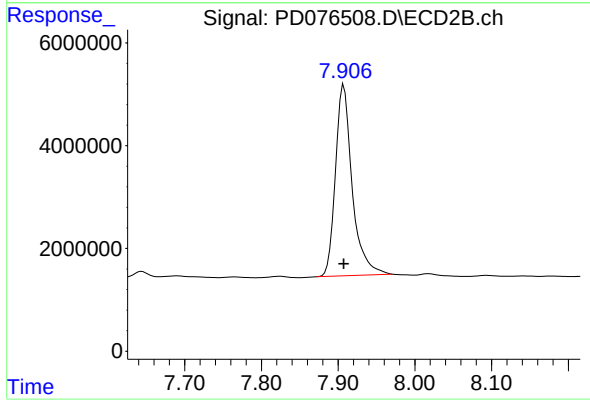

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 56452765
Conc: 50.00 ng/ml