

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 18:58
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:15:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:15:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.762	55884324	80688148	25.596	24.224
28)	SA Decachlor...	9.085	7.907	64501786	29820500	27.112	26.748
Target Compounds							
23)	Chlordane-1	4.710	3.762	269.3E6	99264624	247.289	250.397
24)	Chlordane-2	5.241	4.338	258.9E6	100.6E6	258.529	263.995
25)	Chlordane-3	5.953	4.969	1210.4E6	342.7E6	252.935	254.892
26)	Chlordane-4	6.035	5.032	1429.0E6	334.7E6	254.832	256.957
27)	Chlordane-5	6.888	5.928	235.4E6	118.4E6	246.395	247.493


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 18:58
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:15:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:15:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

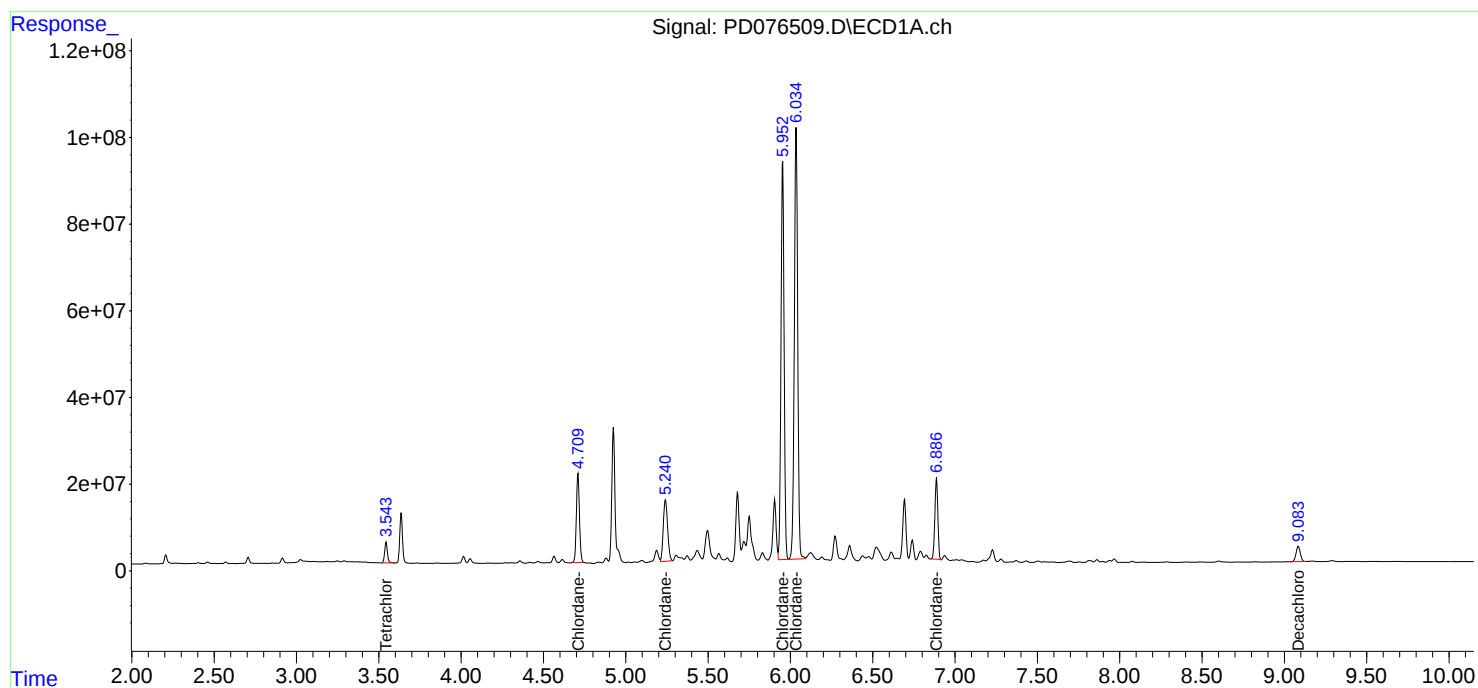


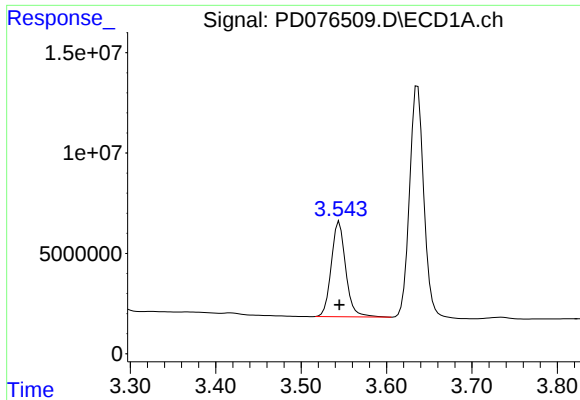

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 55884324
Conc: 25.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

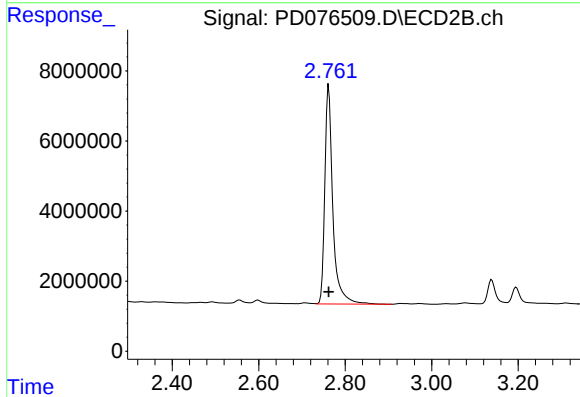


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 80688148
Conc: 24.22 ng/ml

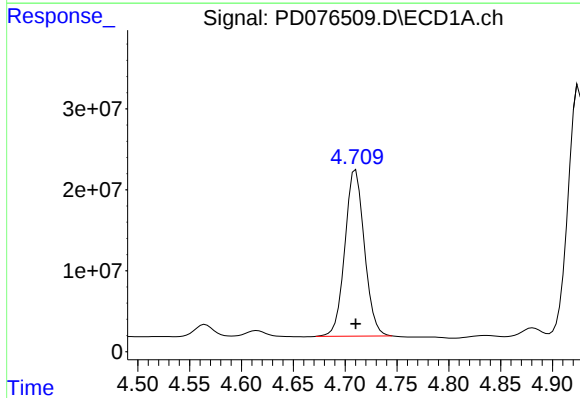


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 269257618
Conc: 247.29 ng/ml

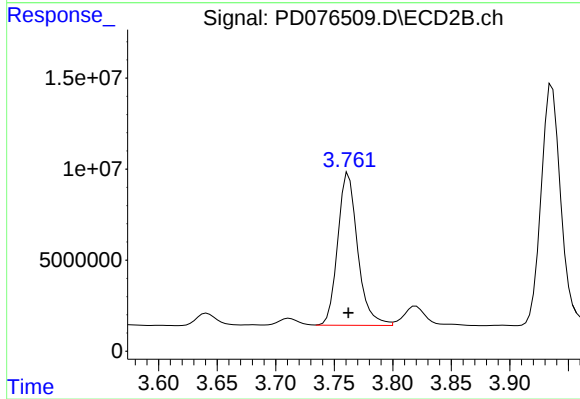

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 99264624
Conc: 250.40 ng/ml

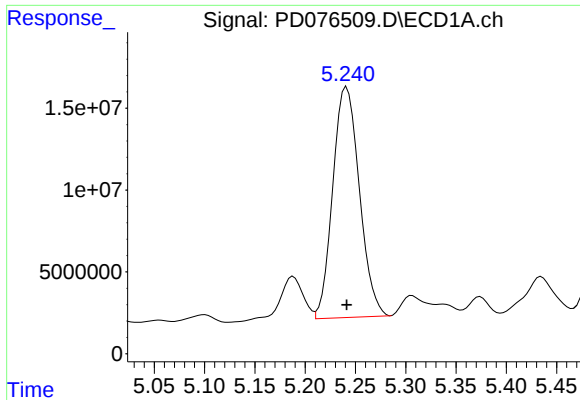

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 258893613
Conc: 258.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

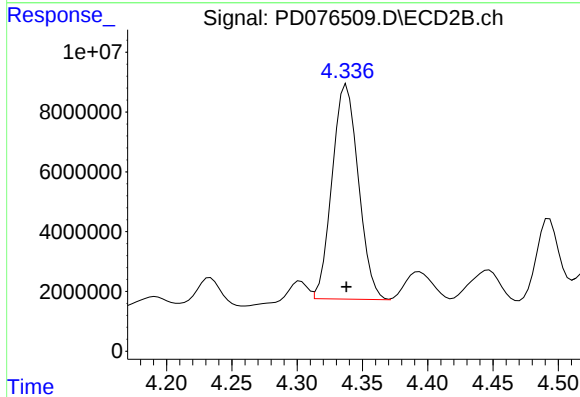


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 100571440
Conc: 264.00 ng/ml

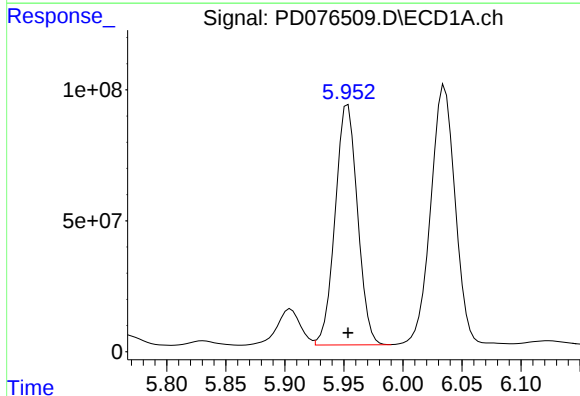


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 1210397113
Conc: 252.94 ng/ml

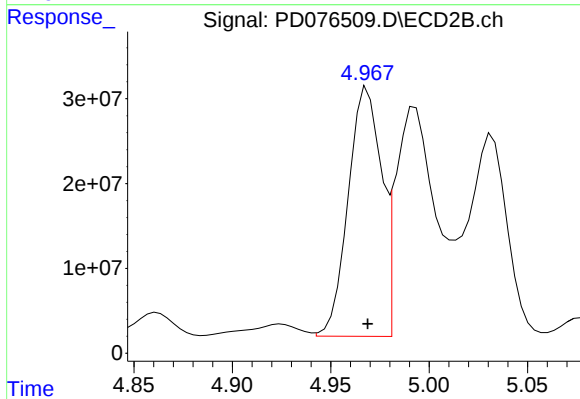

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 342671311
Conc: 254.89 ng/ml

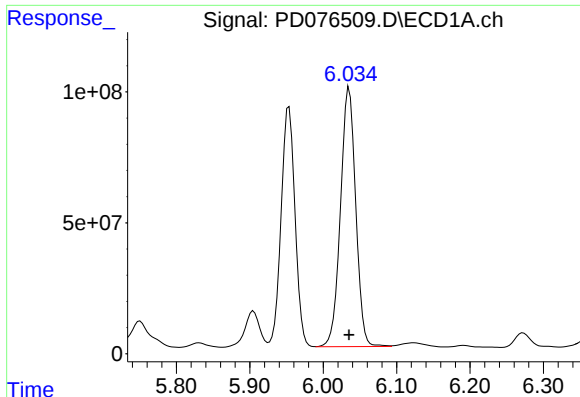

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 1428996096
Conc: 254.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

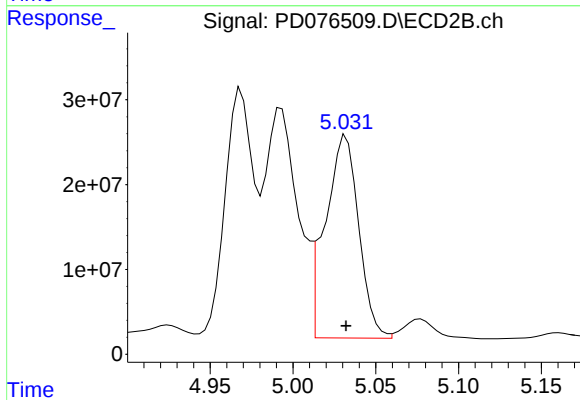


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 334670191
Conc: 256.96 ng/ml

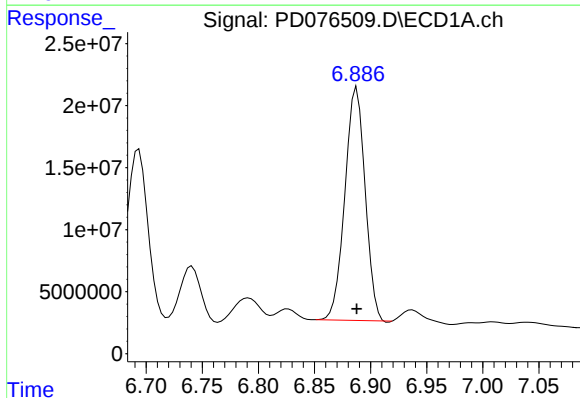


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 235360629
Conc: 246.40 ng/ml

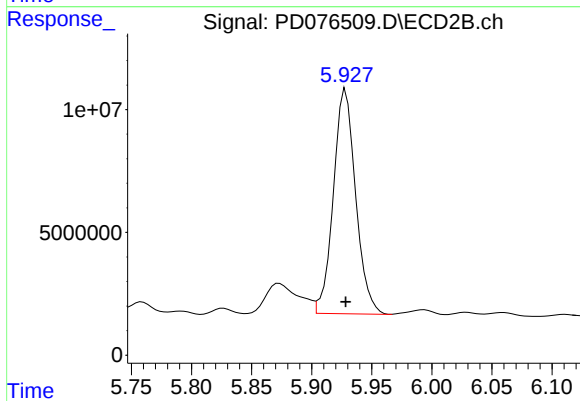

#27 Chlordane-5


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 118398596
Conc: 247.49 ng/ml

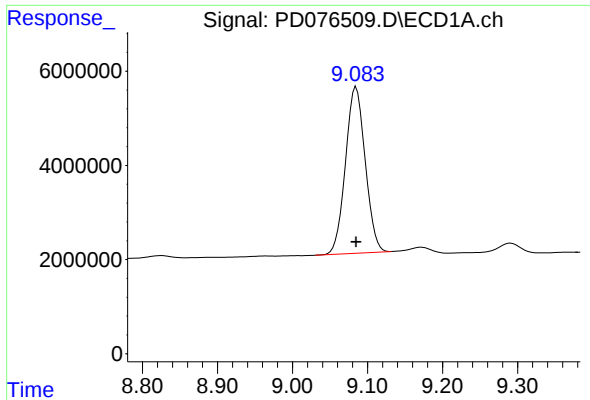

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 64501786
Conc: 27.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

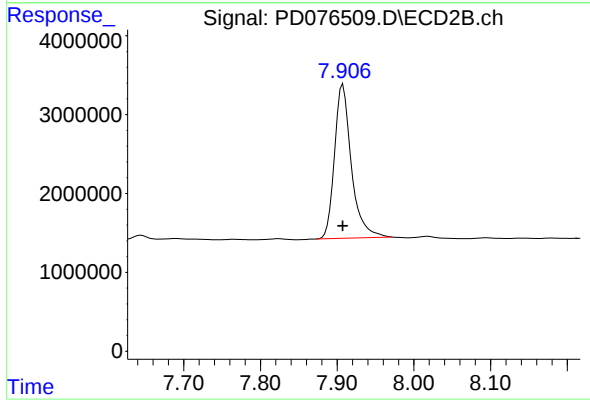

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 29820500
Conc: 26.75 ng/ml