

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 19:11
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:16:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:16:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.763	12010314	14555995	5.393	4.483
28)	SA Decachlor...	9.086	7.908	15078559	6840732	6.016	5.869
Target Compounds							
23)	Chlordane-1	4.710	3.763	53180797	20225051	49.069	50.811
24)	Chlordane-2	5.241	4.338	58302824	22706961	56.367	57.399
25)	Chlordane-3	5.953	4.969	234.4E6	67746607	49.184	50.314
26)	Chlordane-4	6.035	5.032	282.9E6	65901199	50.364	50.478
27)	Chlordane-5	6.887	5.929	45676749	23470383	48.239	49.246



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 19:11
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:16:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:16:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

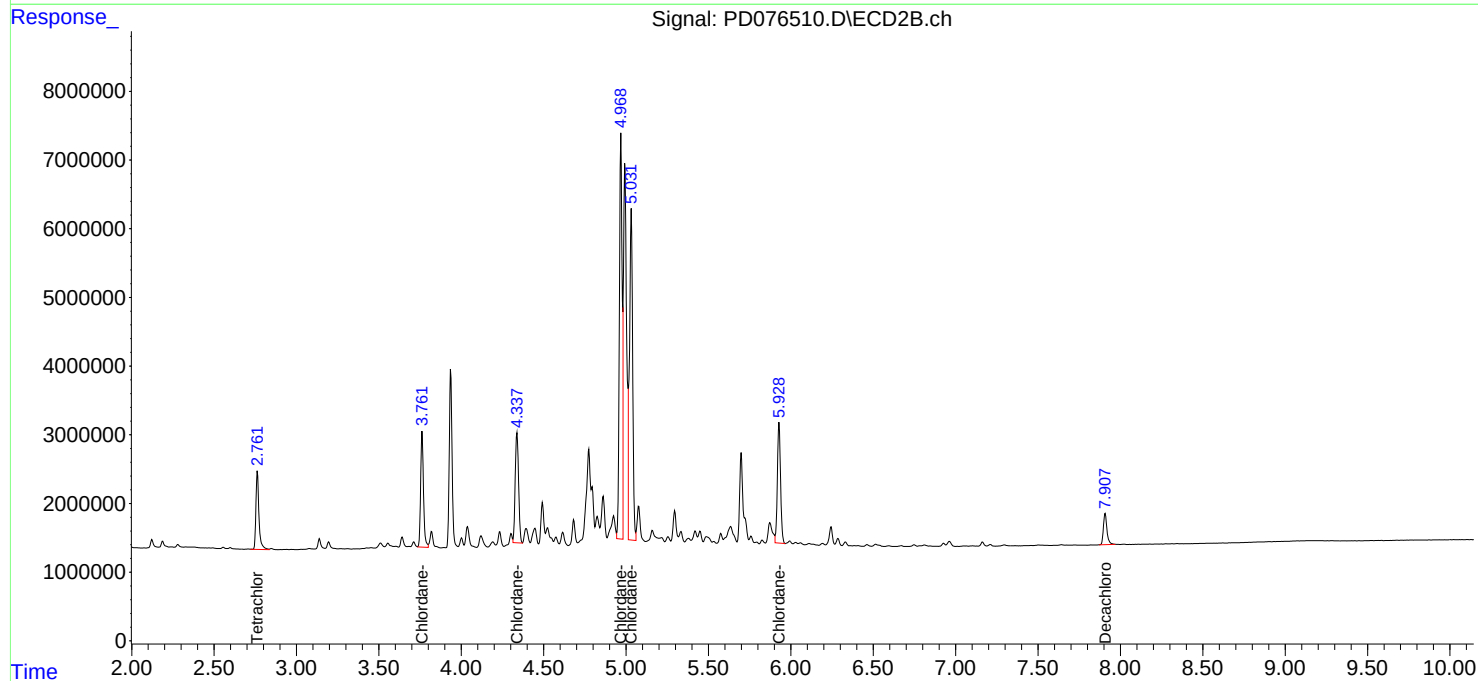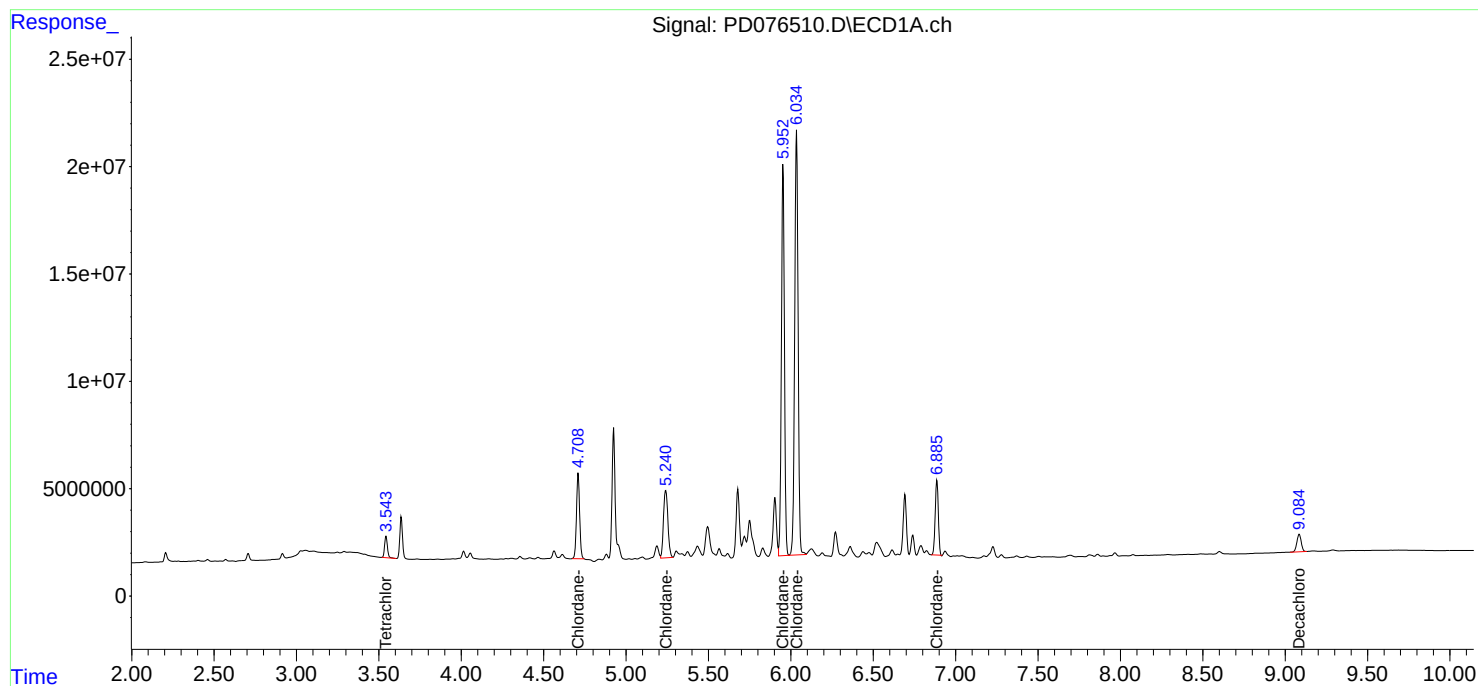


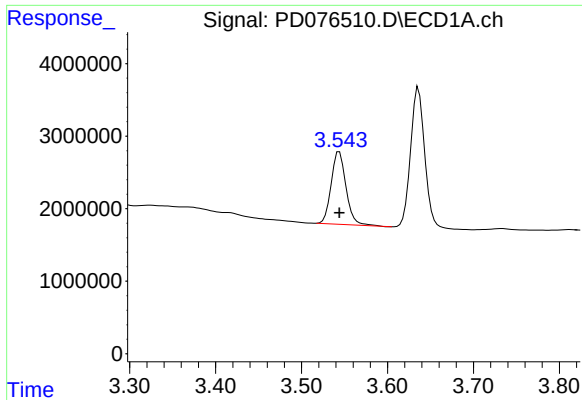

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 12010314
Conc: 5.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

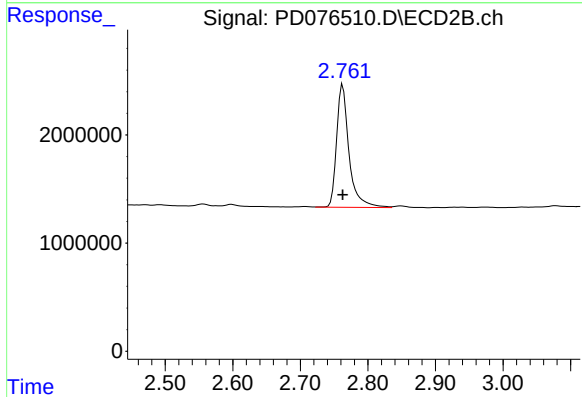


#1 Tetrachloro-m-xylene

R.T.: 2.763 min
Delta R.T.: 0.000 min
Response: 14555995
Conc: 4.48 ng/ml

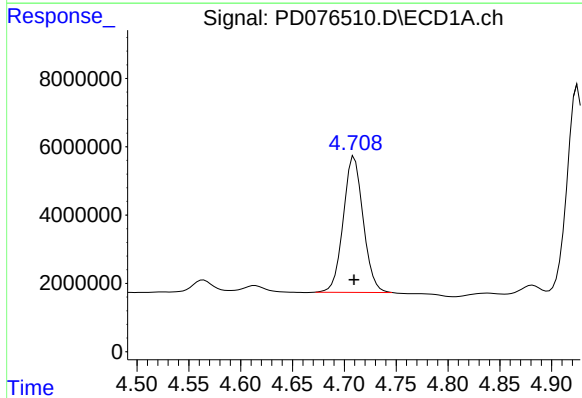


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 53180797
Conc: 49.07 ng/ml

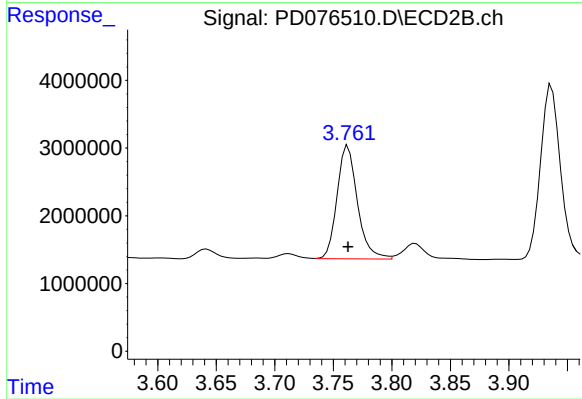

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 20225051
Conc: 50.81 ng/ml

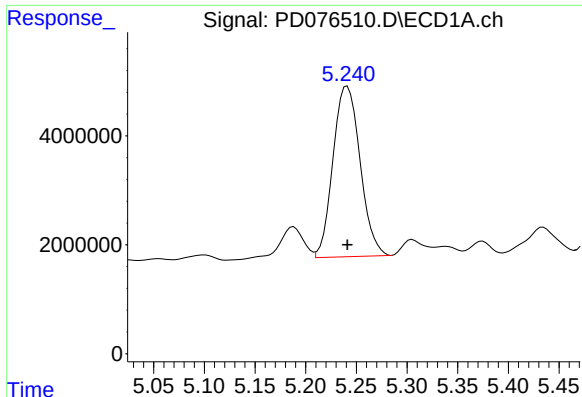

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 58302824
Conc: 56.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

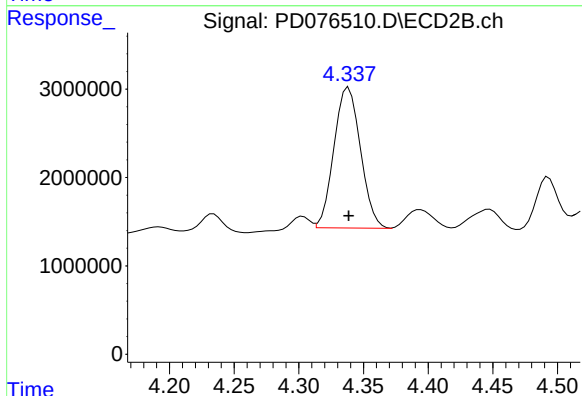


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 22706961
Conc: 57.40 ng/ml

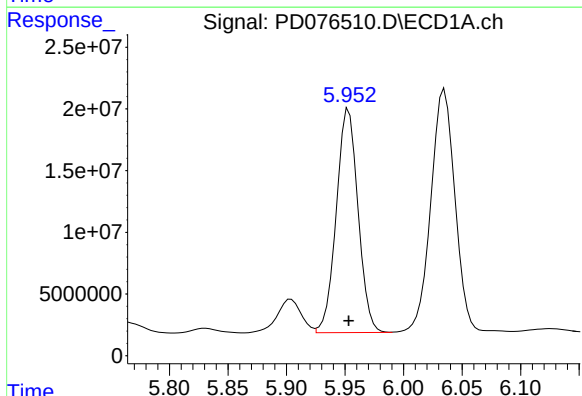


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 234411812
Conc: 49.18 ng/ml

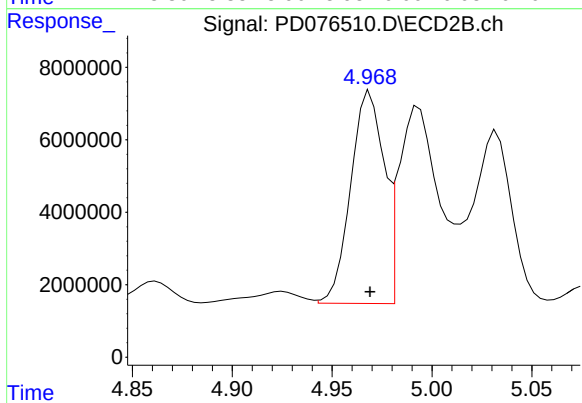

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 67746607
Conc: 50.31 ng/ml

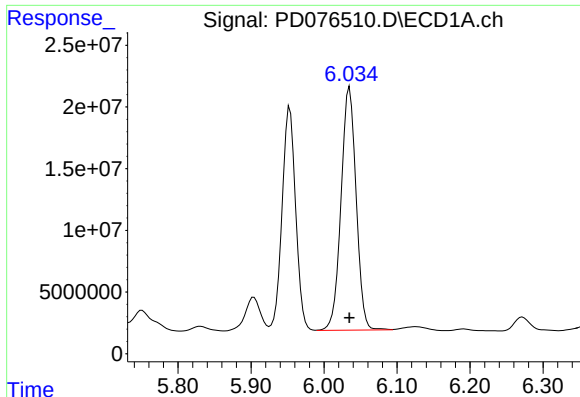

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 282932530
Conc: 50.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

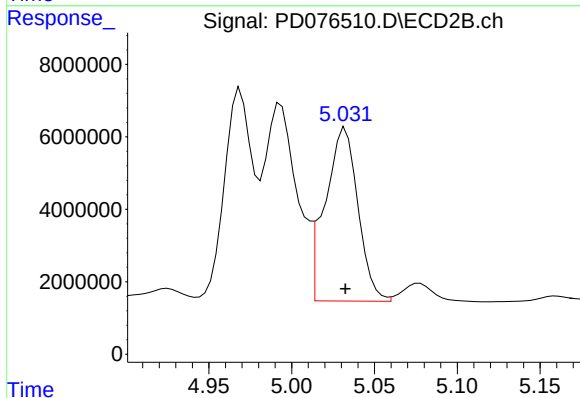


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 65901199
Conc: 50.48 ng/ml

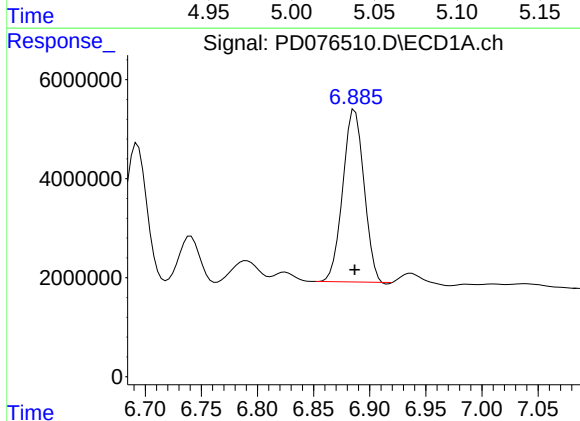


#27 Chlordane-5

R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 45676749
Conc: 48.24 ng/ml

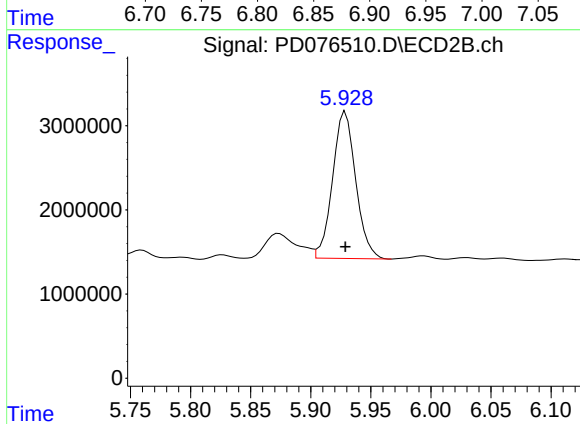

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 23470383
Conc: 49.25 ng/ml

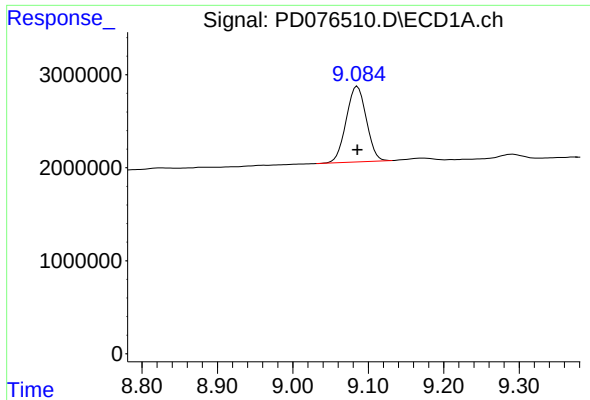

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 15078559
Conc: 6.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

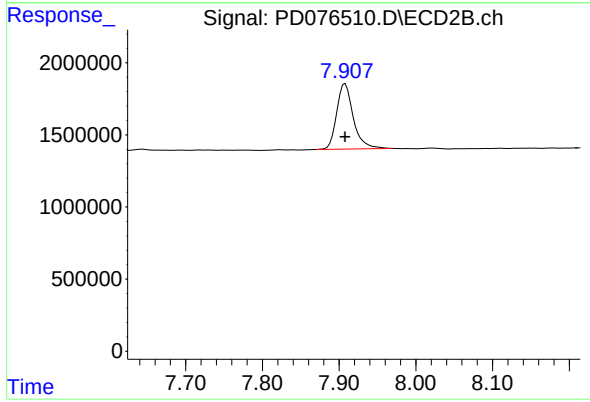

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 6840732
Conc: 5.87 ng/ml