

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 21:12
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD071123

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:04:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 00:56:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.762	110.0E6	169.3E6	50.462	50.989
28)	SA Decachlor...	9.085	7.907	122.1E6	56786860	50.932	49.646
Target Compounds							
23)	Chlordane-1	4.710	3.762	549.0E6	201.1E6	505.462	507.562
24)	Chlordane-2	5.242	4.339	505.5E6	195.2E6	505.415	515.968
25)	Chlordane-3	5.954	4.969	2427.2E6	684.1E6	509.304	502.326
26)	Chlordane-4	6.036	5.032	2846.1E6	671.2E6	509.764	518.869
27)	Chlordane-5	6.887	5.929	486.2E6	242.7E6	511.647	505.069



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 21:12
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD071123

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:04:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 00:56:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

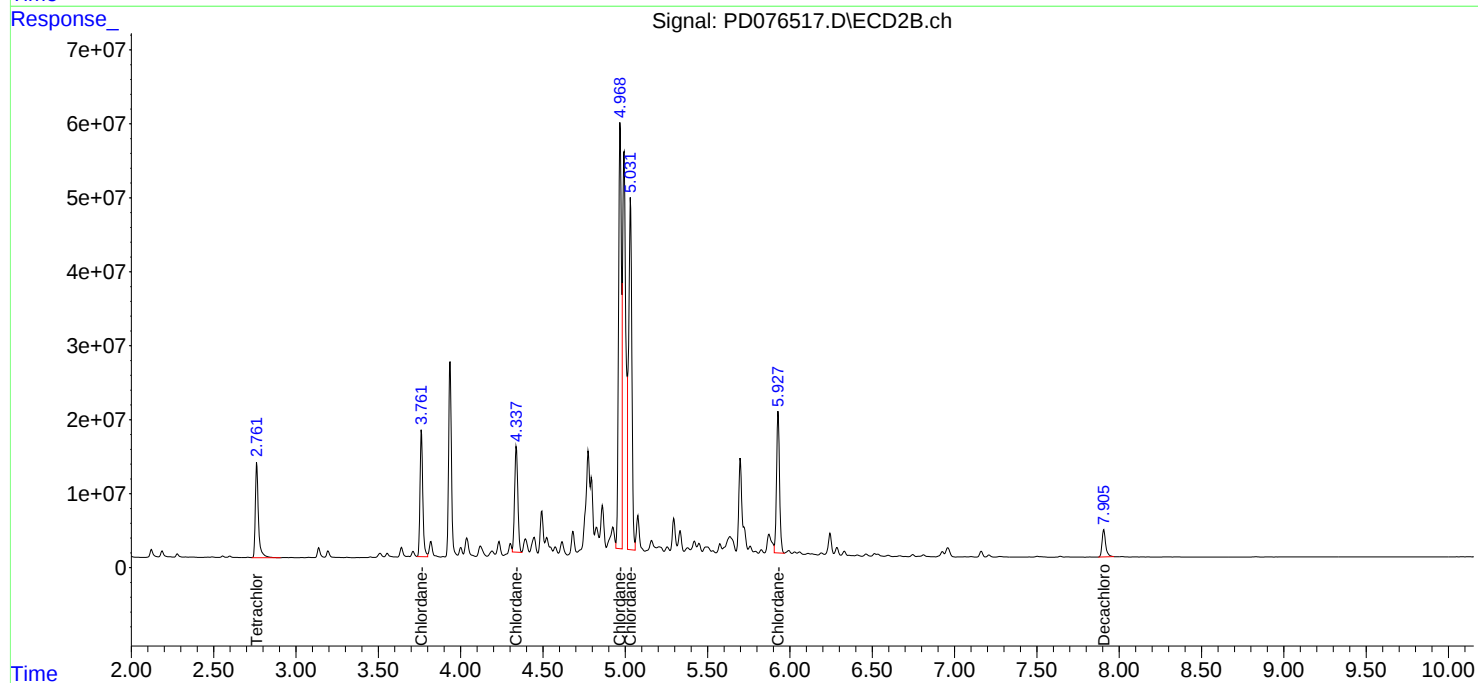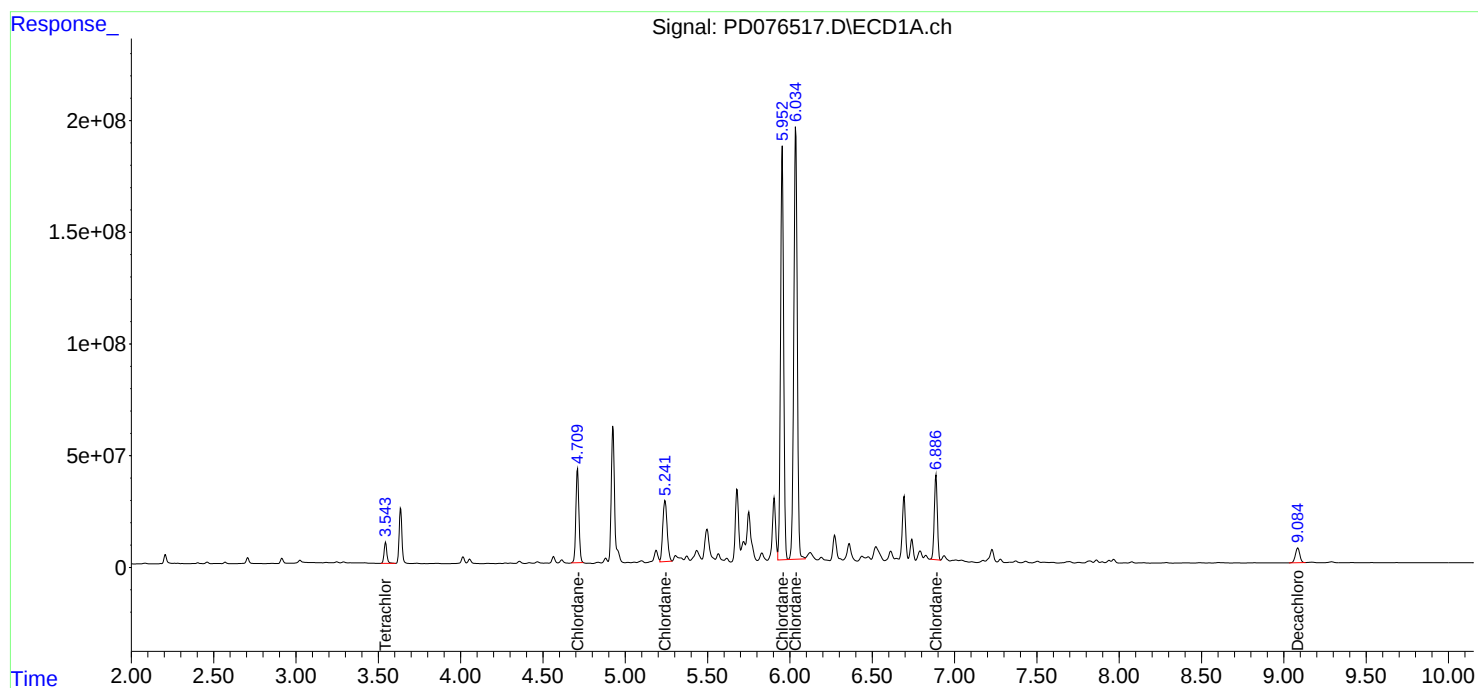


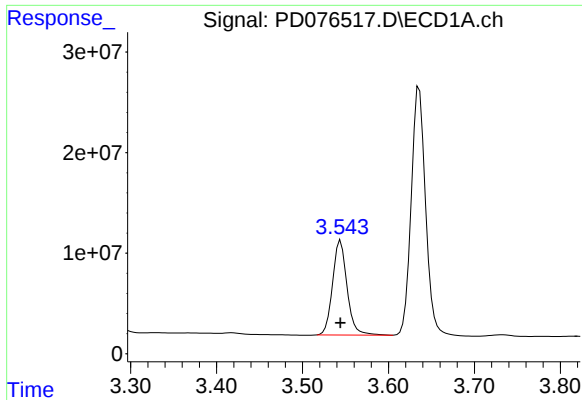

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 109953716
Conc: 50.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071123

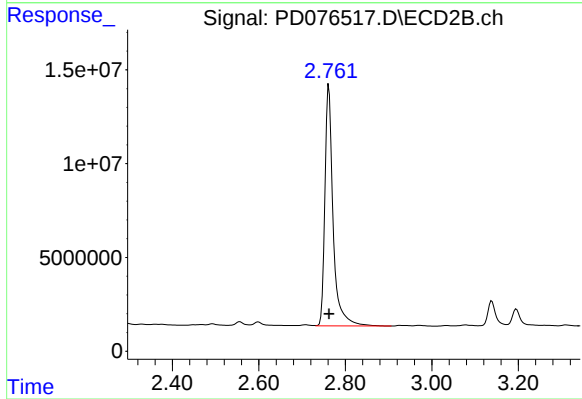


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 169326852
Conc: 50.99 ng/ml

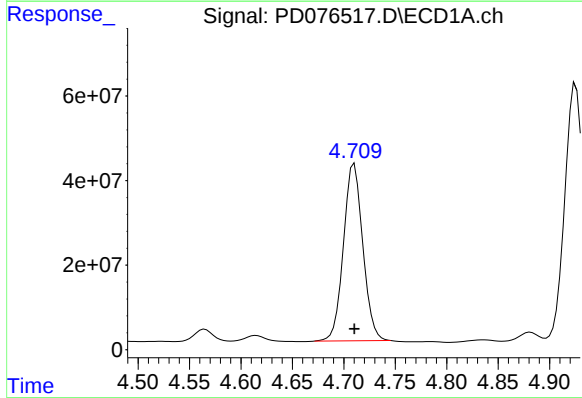


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 548995348
Conc: 505.46 ng/ml

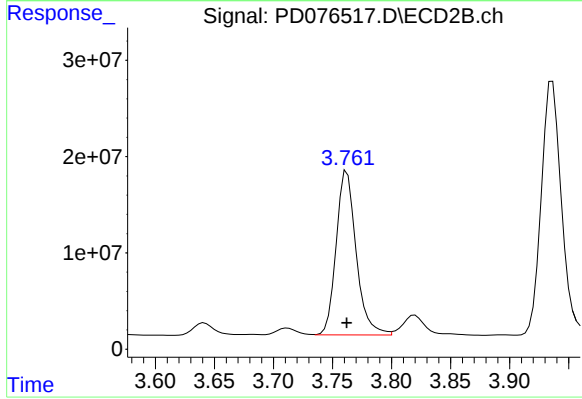

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 201146408
Conc: 507.56 ng/ml

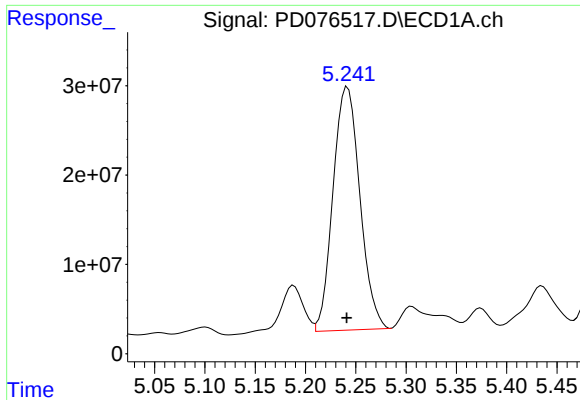

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 505472542
Conc: 505.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071123

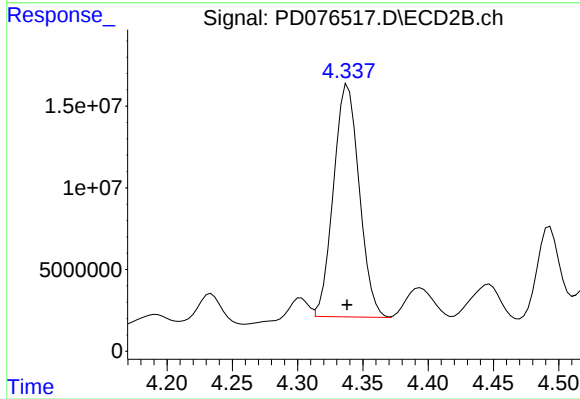


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 195217737
Conc: 515.97 ng/ml

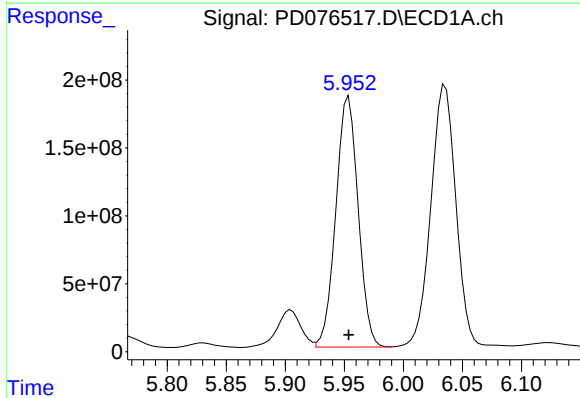


#25 Chlordane-3

R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 2427212552
Conc: 509.30 ng/ml

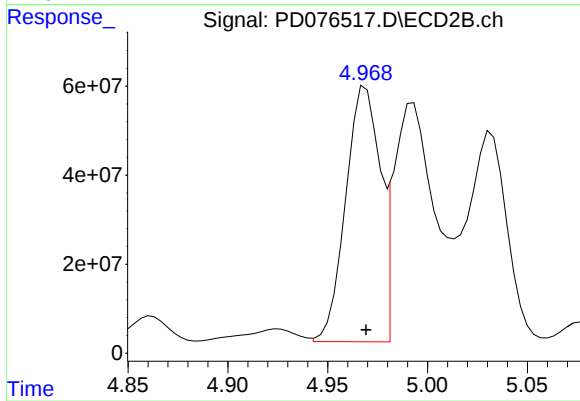

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 684055206
Conc: 502.33 ng/ml

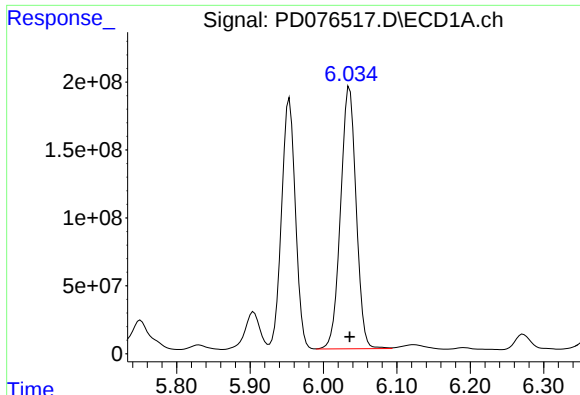

#26 Chlordane-4


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 2846144484
Conc: 509.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071123

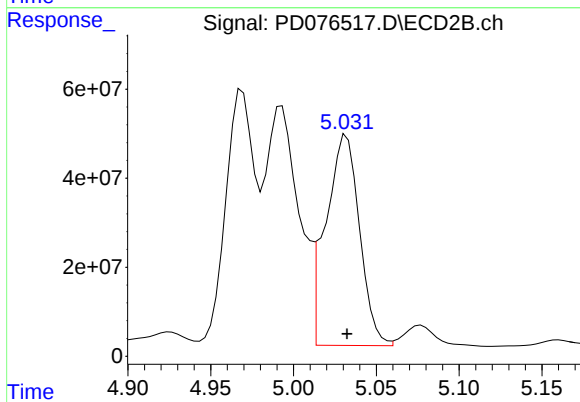


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 671249309
Conc: 518.87 ng/ml

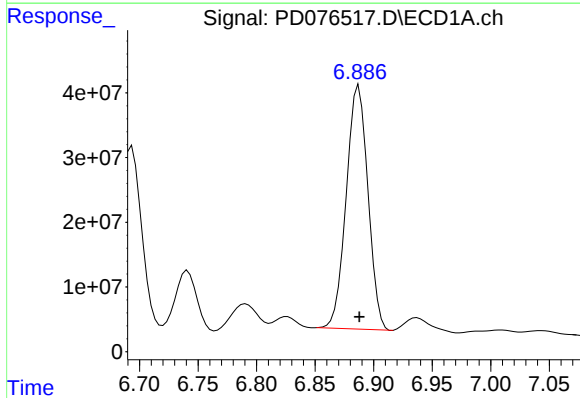


#27 Chlordane-5

R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 486171645
Conc: 511.65 ng/ml

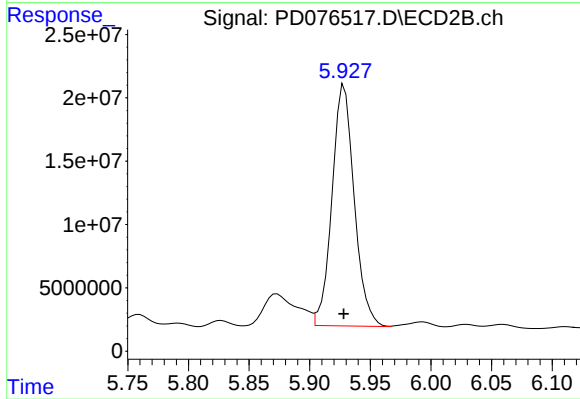

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 242720380
Conc: 505.07 ng/ml

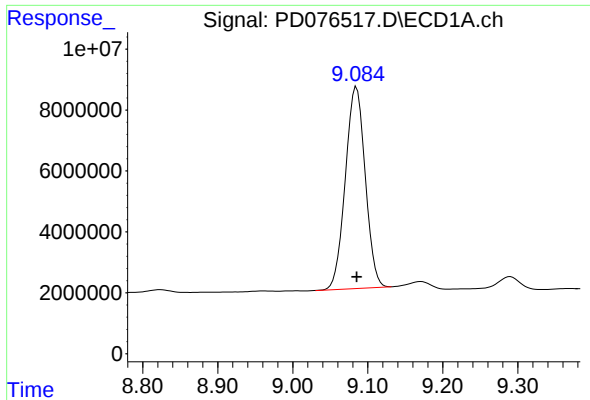

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 122090855
Conc: 50.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071123

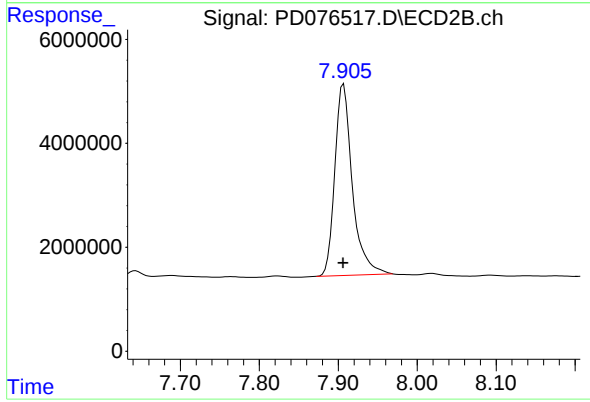

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 56786860
Conc: 49.65 ng/ml