

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 23:26
 Operator : AR\AJ
 Sample : 03570-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EO-01-071023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 02:06:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:40:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.766	21384922	11559672	9.773	10.499
28)	SA Decachlor...	9.086	7.907	23715831	8854684	9.385	8.556
Target Compounds							
12)	B 4,4'-DDE	6.204	5.222	4862562	2790948	1.642	2.321 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 23:26
Operator : AR\AJ
Sample : 03570-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EO-01-071023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 02:06:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:40:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

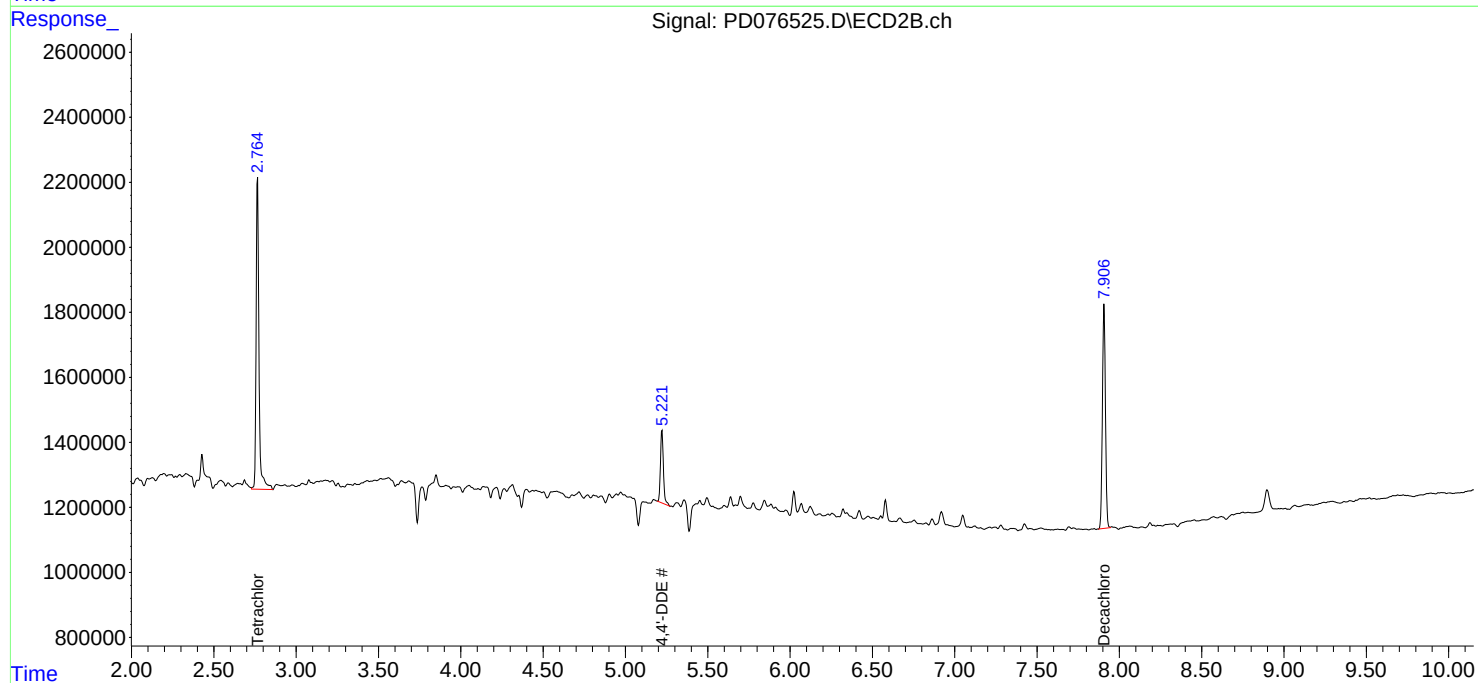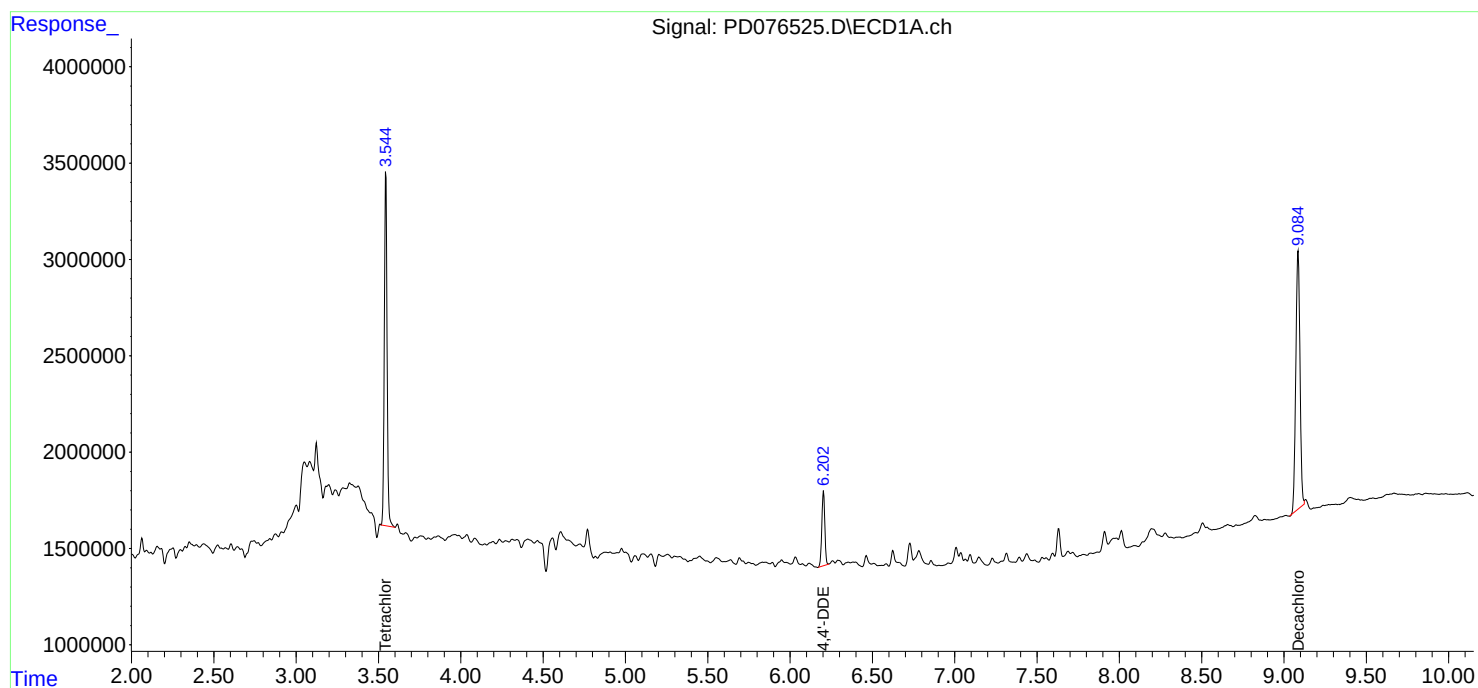


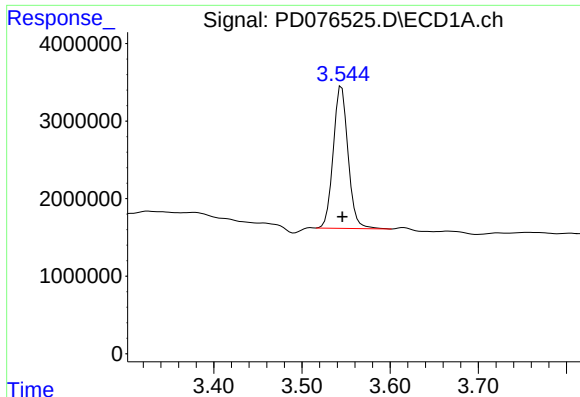

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.001 min
Response: 21384922
Conc: 9.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-01-071023

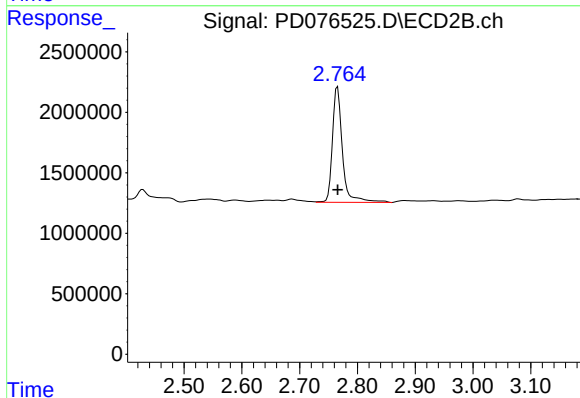


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 11559672
Conc: 10.50 ng/ml

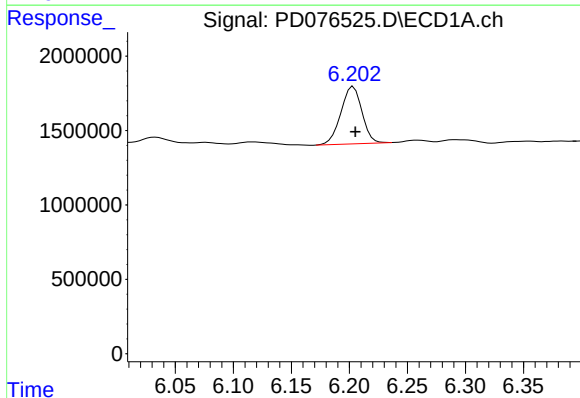


#12 4,4'-DDE

R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 4862562
Conc: 1.64 ng/ml

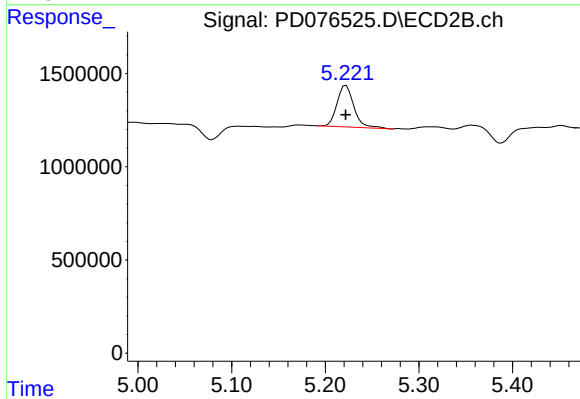

#12 4,4'-DDE


R.T.: 5.222 min
Delta R.T.: 0.000 min
Response: 2790948
Conc: 2.32 ng/ml

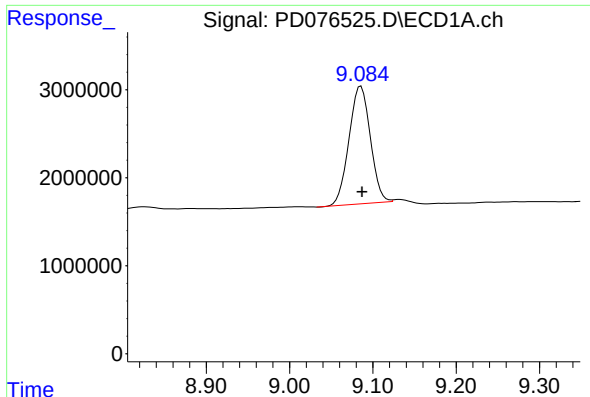

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: -0.002 min
Response: 23715831
Conc: 9.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-01-071023

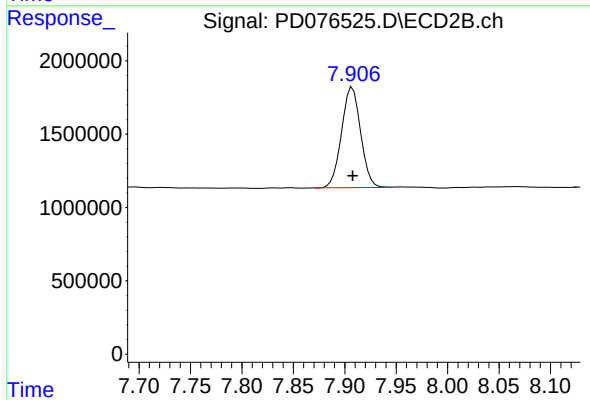

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 8854684
Conc: 8.56 ng/ml