

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
 Data File : PD076526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 23:40
 Operator : AR\AJ
 Sample : 03565-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAT-DIS-01-7-10-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 02:06:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 01:40:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.764	23505904	11704573	10.743	10.630m
28) SA Decachlor...	9.084	7.908	27056879	10007927	10.707m	9.670

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071123\
Data File : PD076526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 23:40
Operator : AR\AJ
Sample : 03565-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PAT-DIS-01-7-10-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 02:06:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071123.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 01:40:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

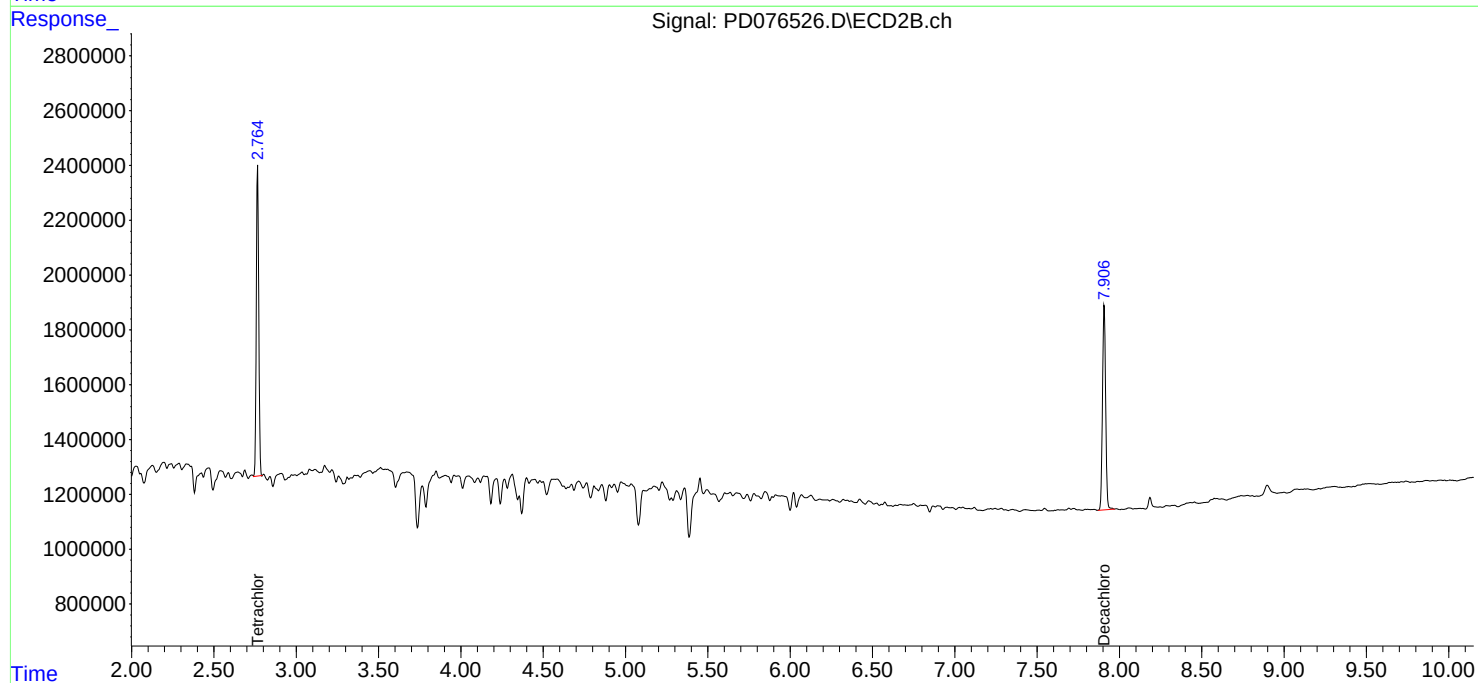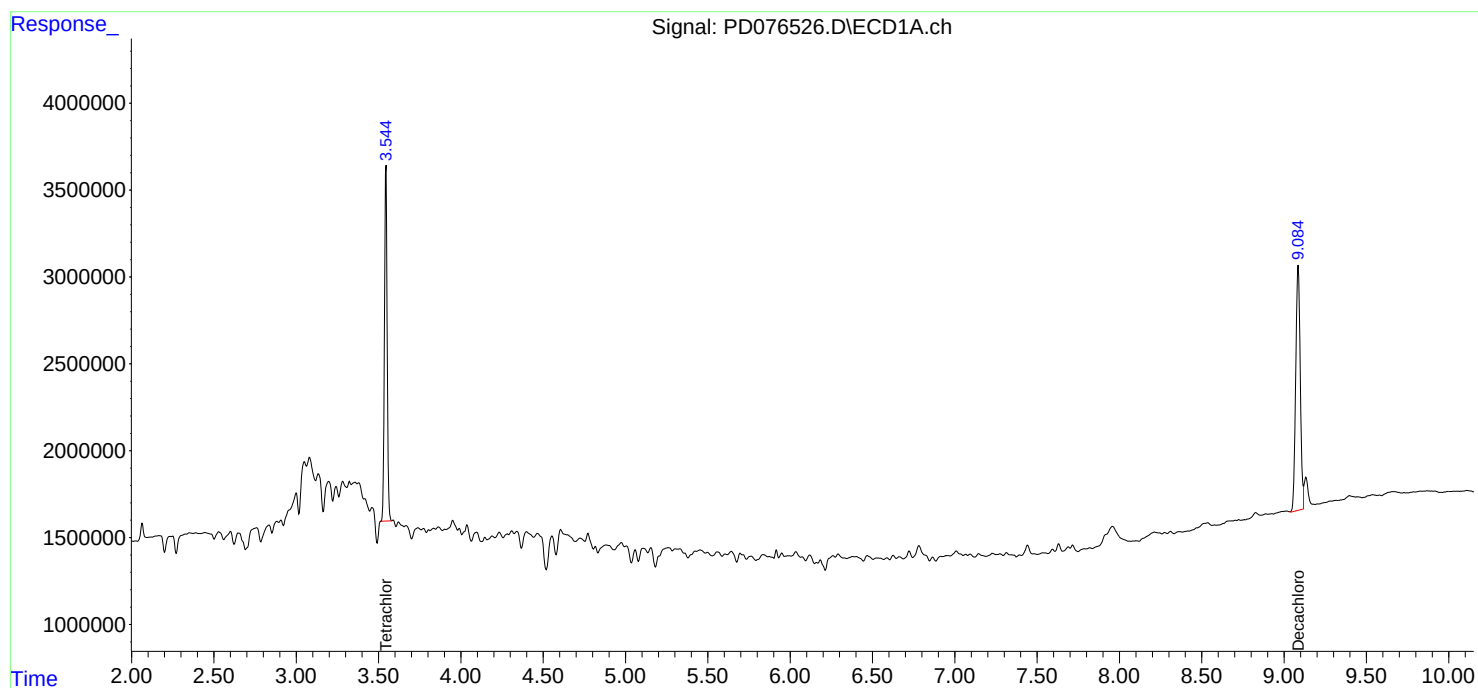


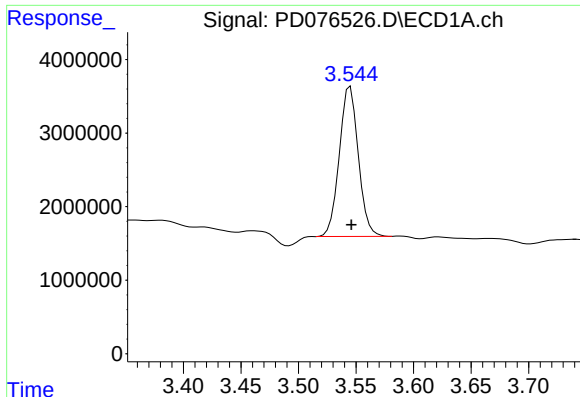

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.001 min
Response: 23505904
Conc: 10.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAT-DIS-01-7-10-2023

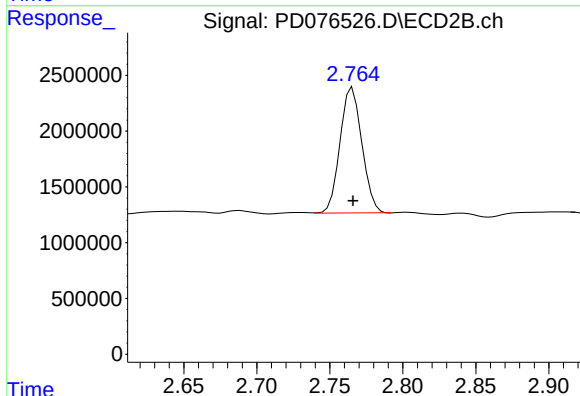


#1 Tetrachloro-m-xylene

R.T.: 2.764 min
Delta R.T.: -0.002 min
Response: 11704573
Conc: 10.63 ng/ml m

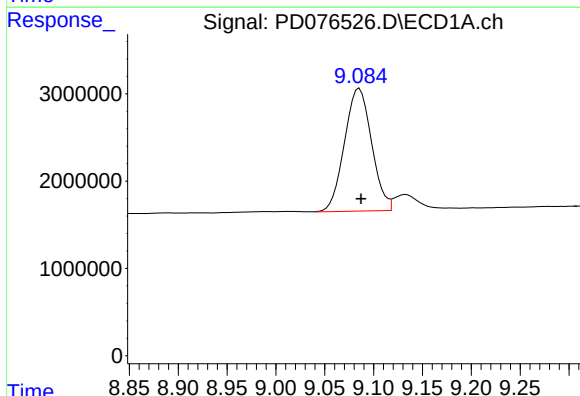

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.003 min
Response: 27056879
Conc: 10.71 ng/ml m

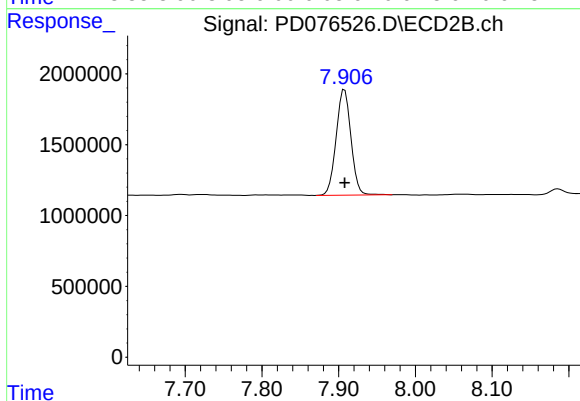

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 10007927
Conc: 9.67 ng/ml