

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 11:49
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:24:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.124	12272688	126.0E6	5.266	5.518
27)	SA Decachlor...	8.246	9.321	27255275	104.9E6	11.363	11.367
Target Compounds							
2)	A alpha-BHC	3.915	4.529	16688116	177.3E6	4.794	5.701
3)	MA gamma-BHC...	4.199	4.823	16942653	149.3E6	5.046	5.790
4)	MA Heptachlor	4.499	5.339	16765839	121.1E6	4.955	5.979
9)	A Endosulfan I	5.533	6.412	14785456	75052913	5.072	5.622
13)	MA Dieldrin	5.777	6.673	31753387	154.2E6	9.613	11.260
14)	MA Endrin	6.036	6.896	26449161	112.2E6	9.661	10.474
16)	A 4,4'-DDD	6.163	7.012	24501166	128.4E6	9.700	11.632
17)	MA 4,4'-DDT	6.405	7.313	25679485	125.9E6	9.728	11.237
20)	A Methoxychlor	6.956	7.773	71648060	299.4E6	52.126	57.154


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 11:49
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:24:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

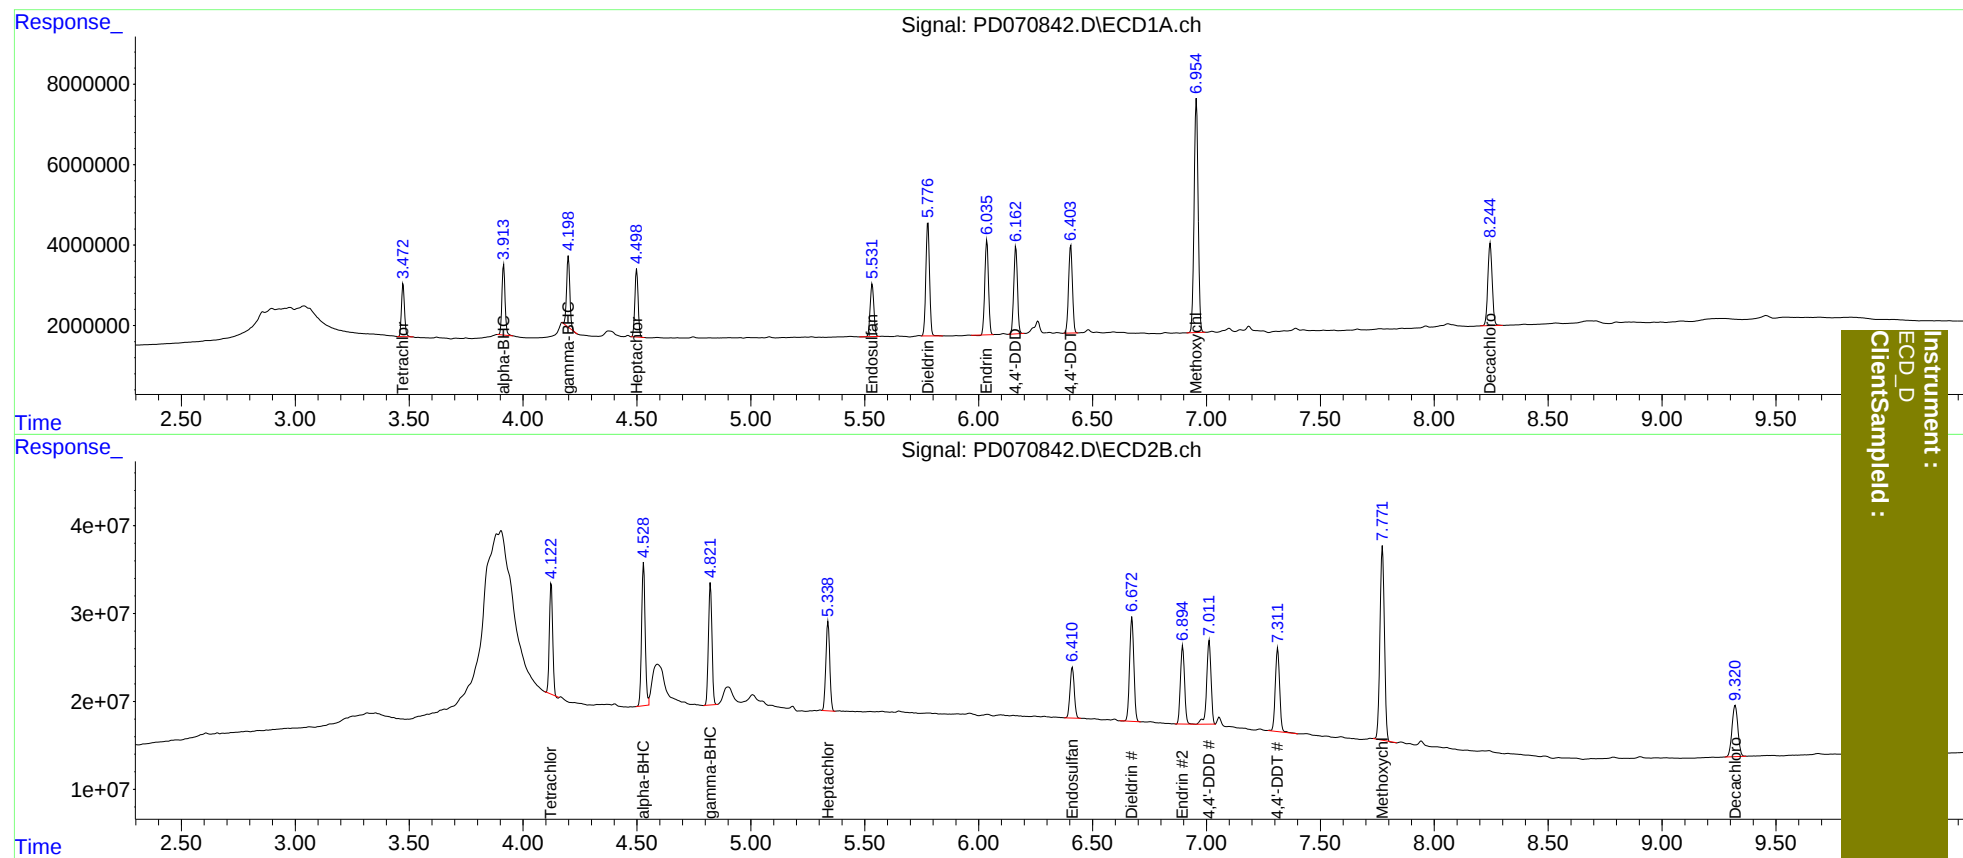


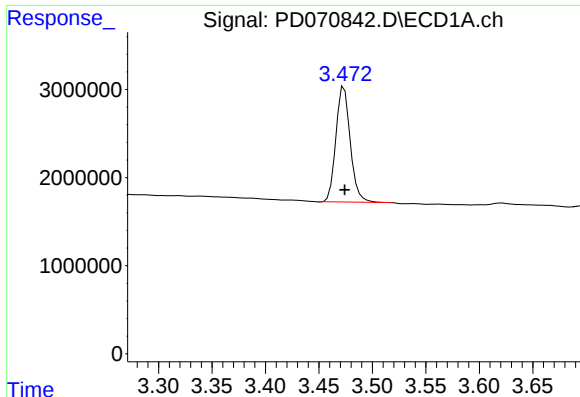

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 12272688
Conc: 5.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

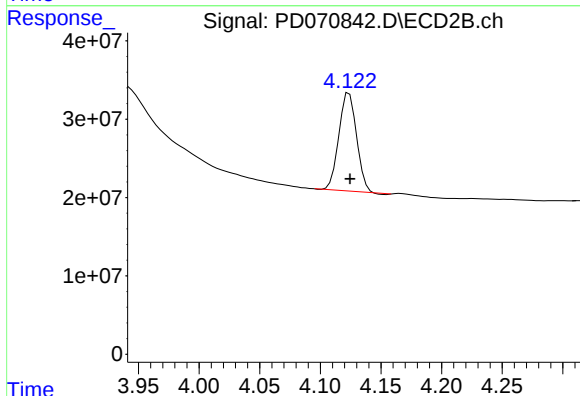


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 126043445
Conc: 5.52 ng/ml

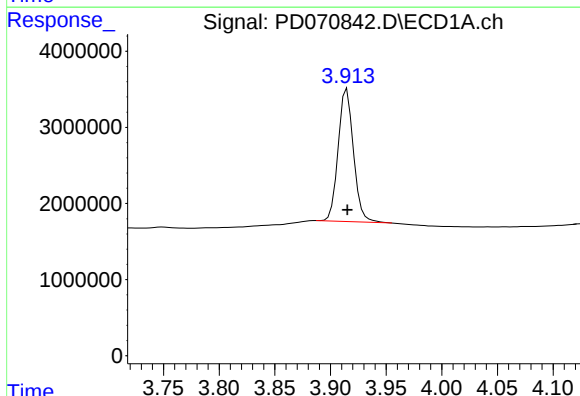


#2 alpha-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 16688116
Conc: 4.79 ng/ml

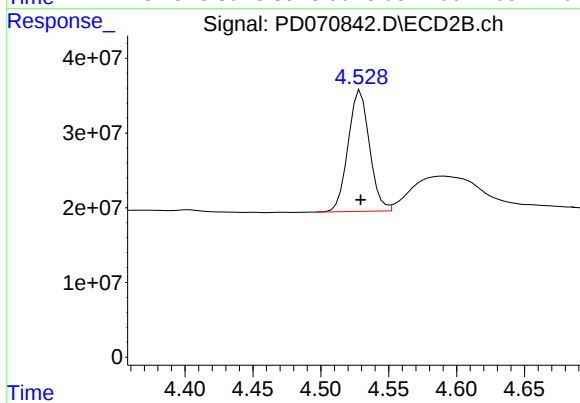

#2 alpha-BHC


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 177289557
Conc: 5.70 ng/ml

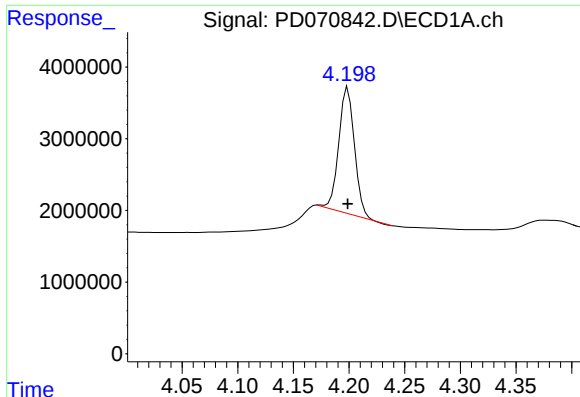

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 16942653
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

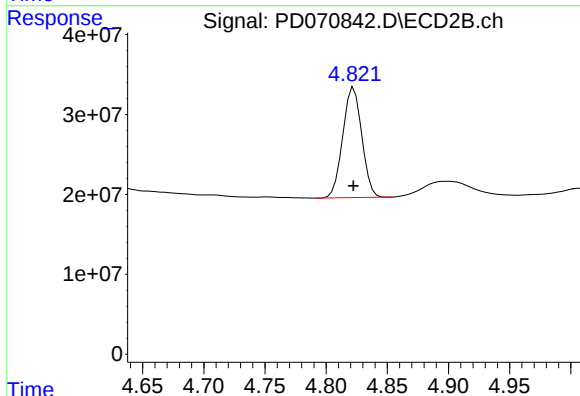


#3 gamma-BHC (Lindane)

R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 149334625
Conc: 5.79 ng/ml

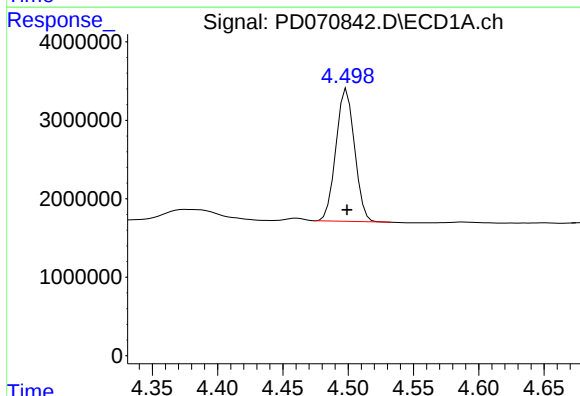


#4 Heptachlor

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 16765839
Conc: 4.96 ng/ml

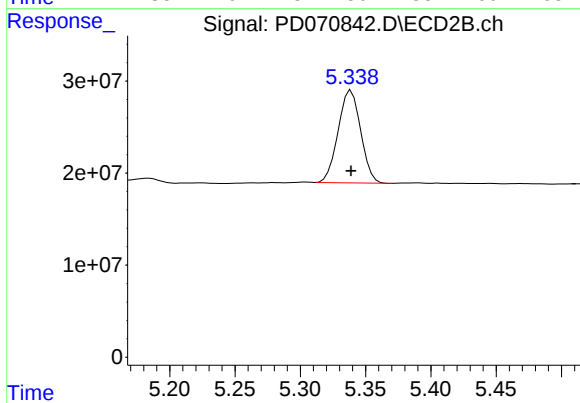

#4 Heptachlor


R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 121104900
Conc: 5.98 ng/ml

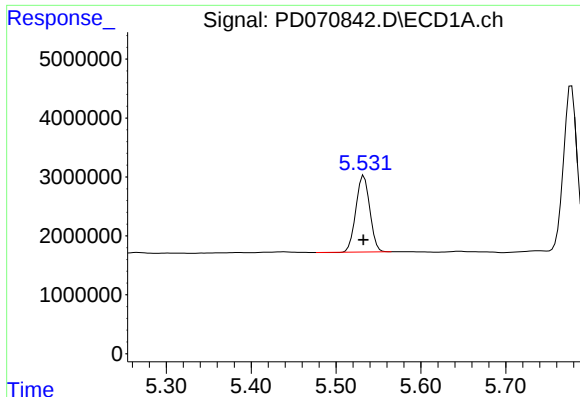

#9 Endosulfan I


R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 14785456
Conc: 5.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

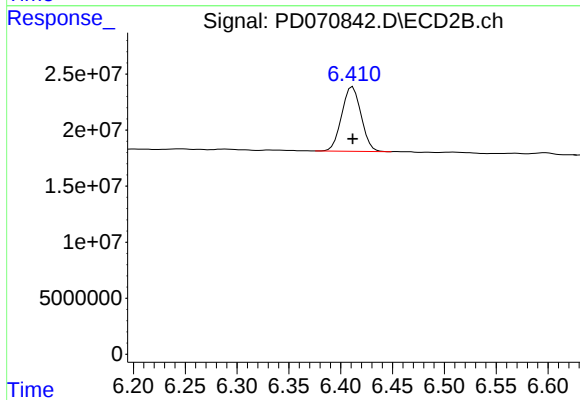


#9 Endosulfan I

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 75052913
Conc: 5.62 ng/ml

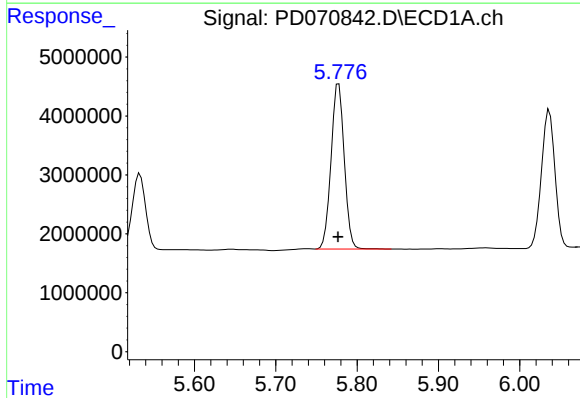


#13 Dieldrin

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 31753387
Conc: 9.61 ng/ml

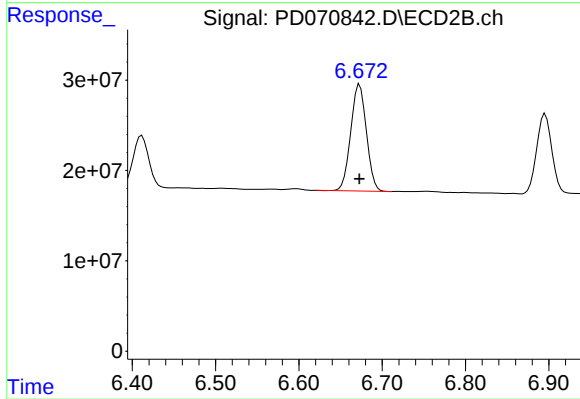

#13 Dieldrin


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 154150377
Conc: 11.26 ng/ml

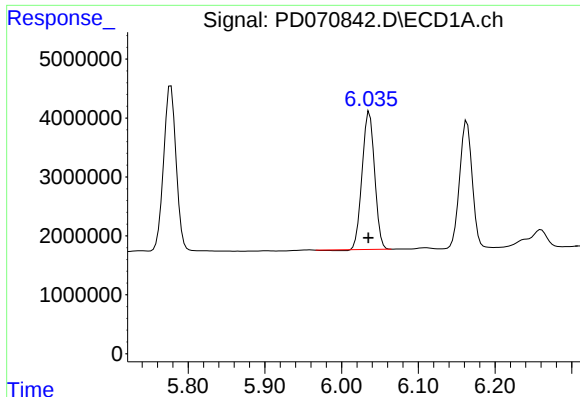

#14 Endrin


R.T.: 6.036 min
Delta R.T.: 0.001 min
Response: 26449161
Conc: 9.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

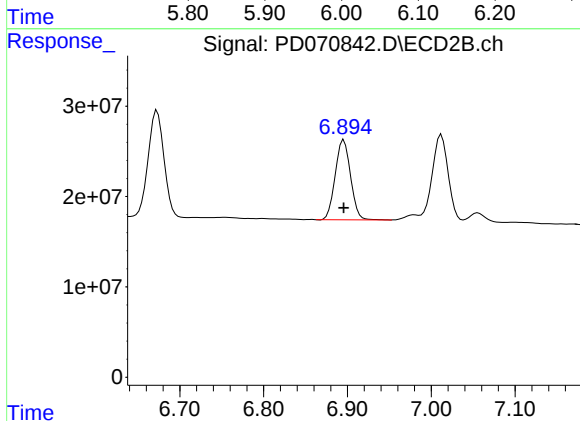


#14 Endrin

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 112173114
Conc: 10.47 ng/ml

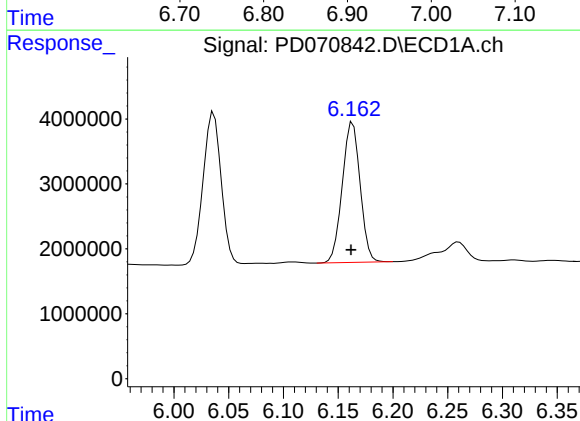


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.001 min
Response: 24501166
Conc: 9.70 ng/ml

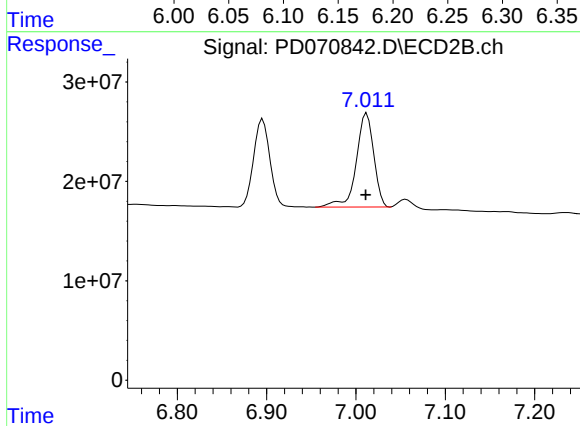

#16 4,4'-DDD


R.T.: 7.012 min
Delta R.T.: 0.001 min
Response: 128422723
Conc: 11.63 ng/ml

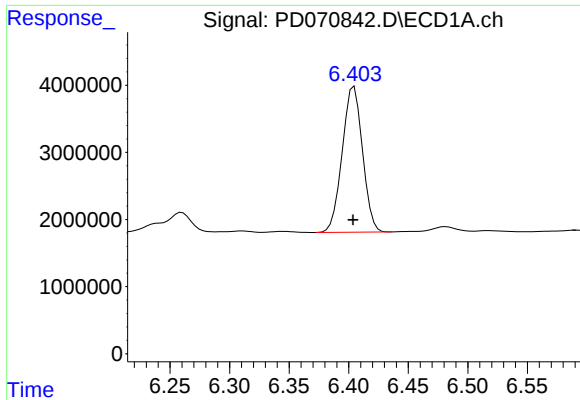

#17 4,4'-DDT


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 25679485
Conc: 9.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

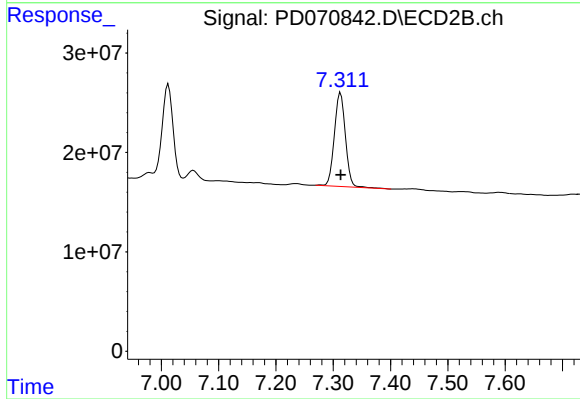


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: 0.000 min
Response: 125891162
Conc: 11.24 ng/ml

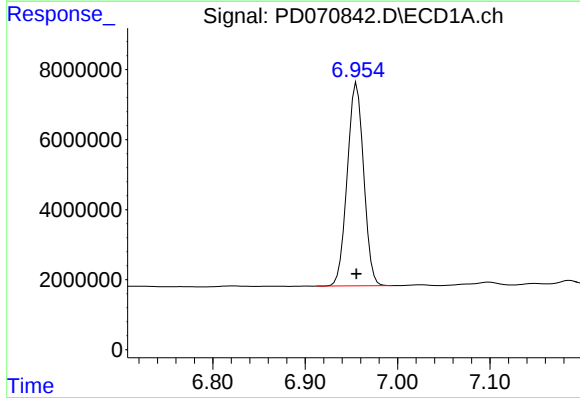


#20 Methoxychlor

R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 71648060
Conc: 52.13 ng/ml

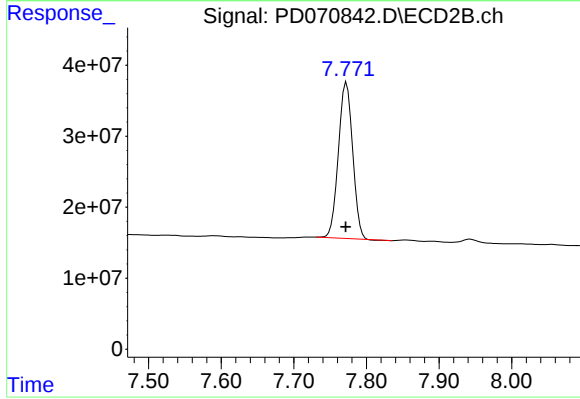

#20 Methoxychlor


R.T.: 7.773 min
Delta R.T.: 0.000 min
Response: 299426430
Conc: 57.15 ng/ml

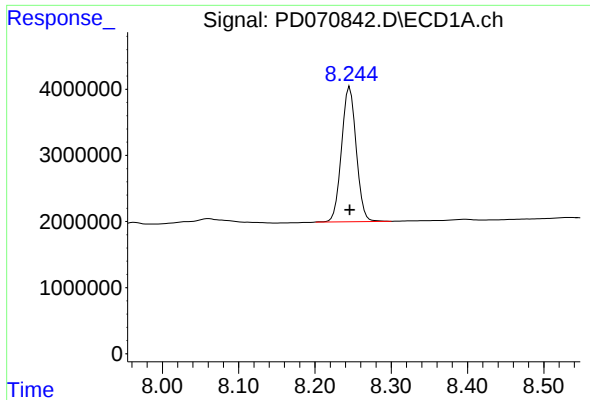

#27 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: 0.000 min
Response: 27255275
Conc: 11.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

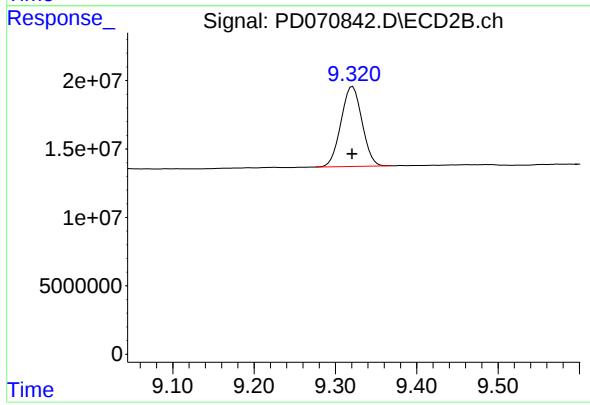

#27 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.000 min
Response: 104855708
Conc: 11.37 ng/ml