

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 12:18
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:24:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.124	24597822	262.4E6	10.554	11.486
27)	SA Decachlor...	8.245	9.320	51119162	198.4E6	21.313	21.512
Target Compounds							
2)	A alpha-BHC	3.915	4.529	34863618	356.0E6	10.015	11.450
3)	MA gamma-BHC...	4.199	4.823	34656225	289.8E6	10.321	11.234
4)	MA Heptachlor	4.499	5.339	34261071	229.2E6	10.126	11.313
9)	A Endosulfan I	5.532	6.411	29755667	144.3E6	10.207	10.811
13)	MA Dieldrin	5.777	6.673	65348963	294.1E6	19.783	21.483
14)	MA Endrin	6.035	6.896	54007917	222.7E6	19.727	20.794
16)	A 4,4'-DDD	6.162	7.011	49950102	238.8E6	19.776	21.629
17)	MA 4,4'-DDT	6.403	7.312	52015536	237.8E6	19.704	21.227
20)	A Methoxychlor	6.955	7.772	140.1E6	563.7E6	101.944	107.593


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 12:18
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:24:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

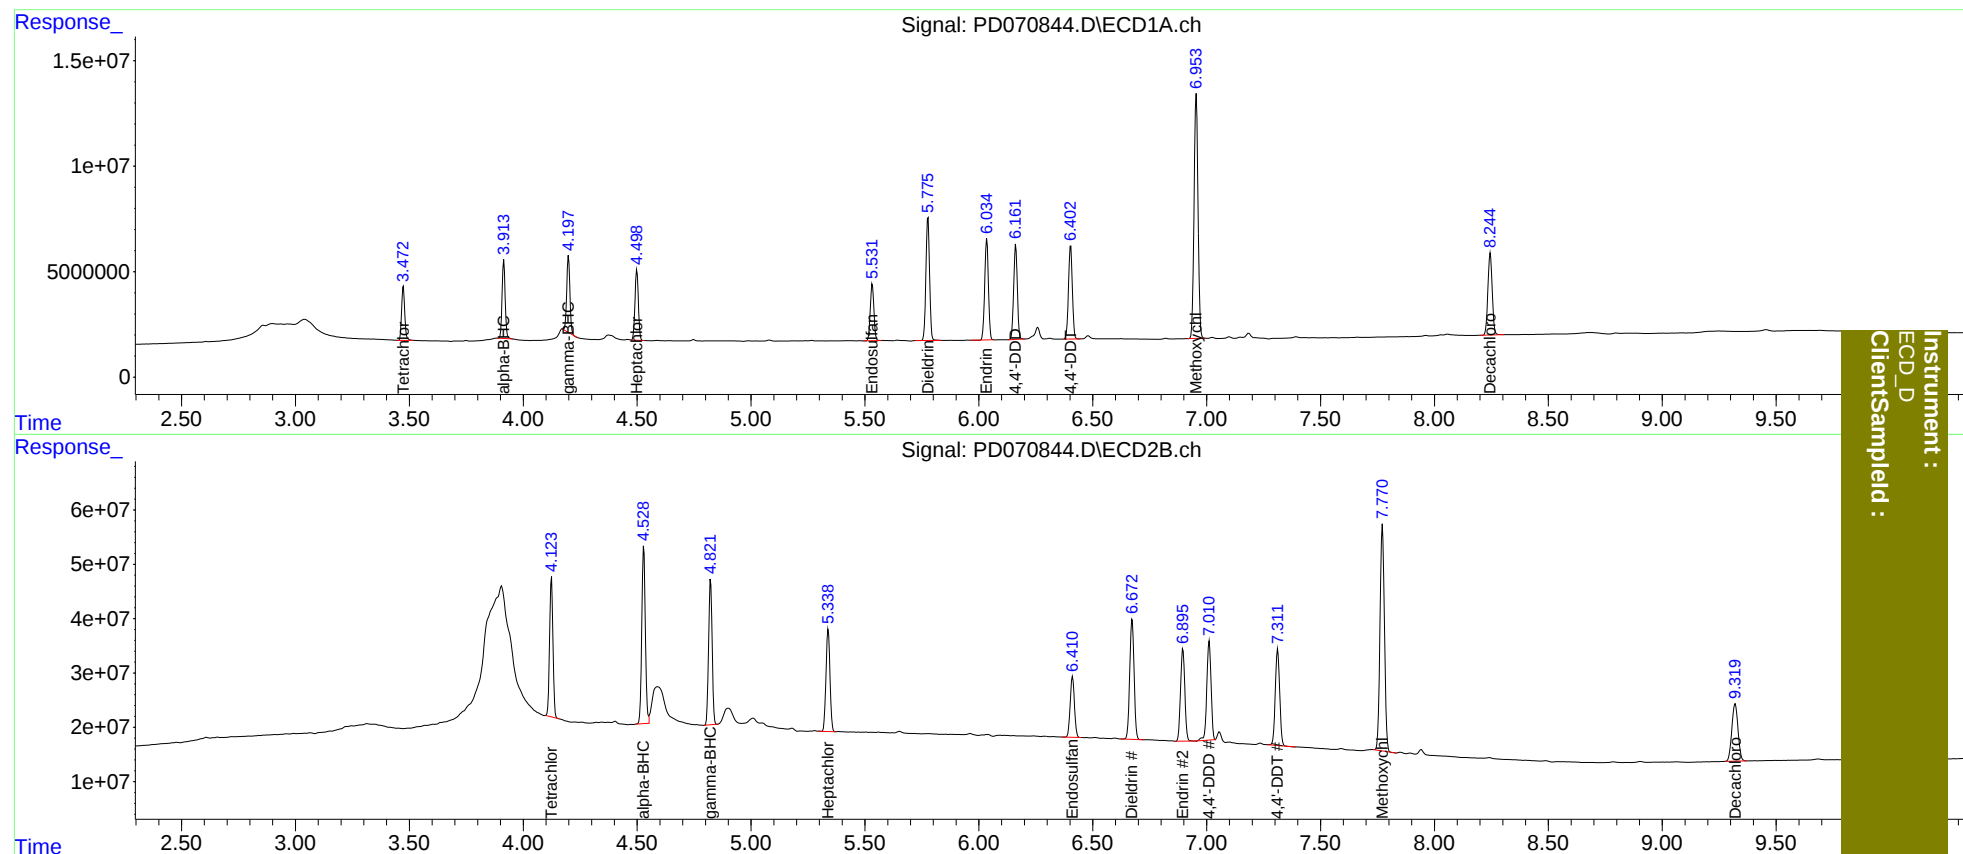


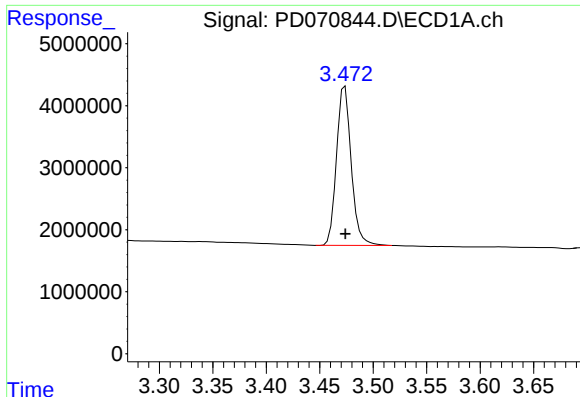

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 24597822
Conc: 10.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

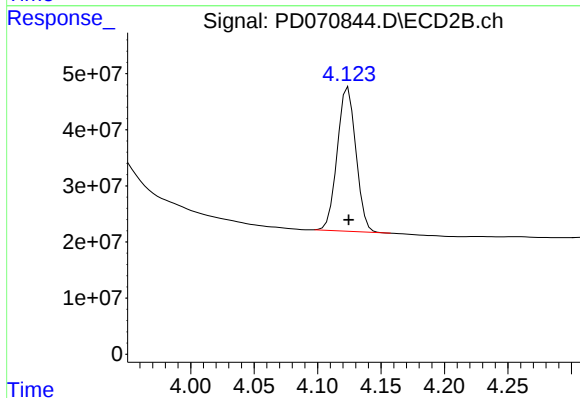


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 262374470
Conc: 11.49 ng/ml

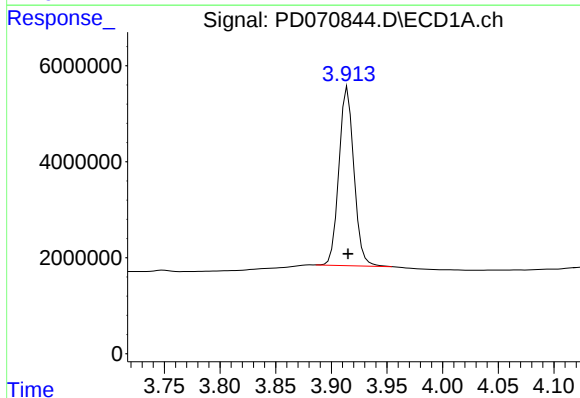


#2 alpha-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 34863618
Conc: 10.02 ng/ml

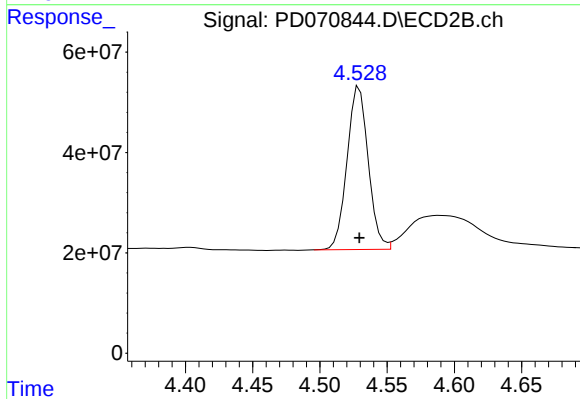

#2 alpha-BHC


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 356044352
Conc: 11.45 ng/ml

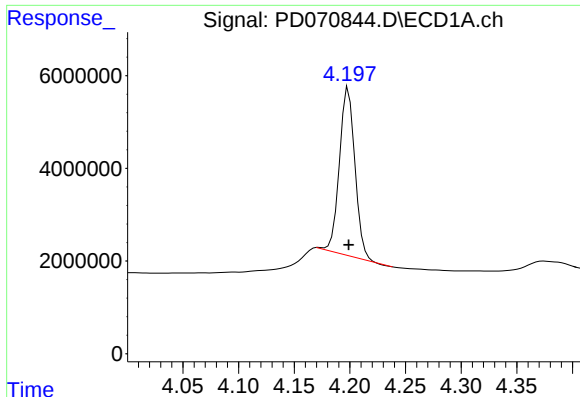

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 34656225
Conc: 10.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

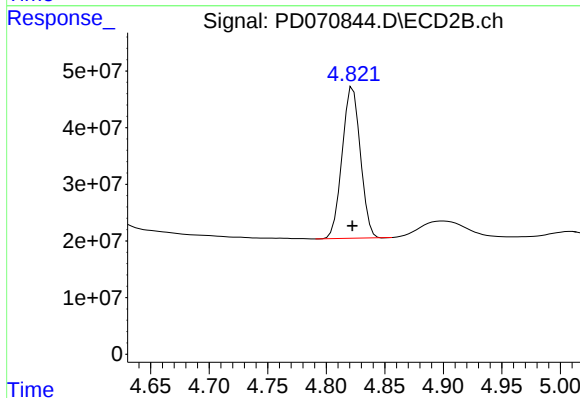


#3 gamma-BHC (Lindane)

R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 289772477
Conc: 11.23 ng/ml

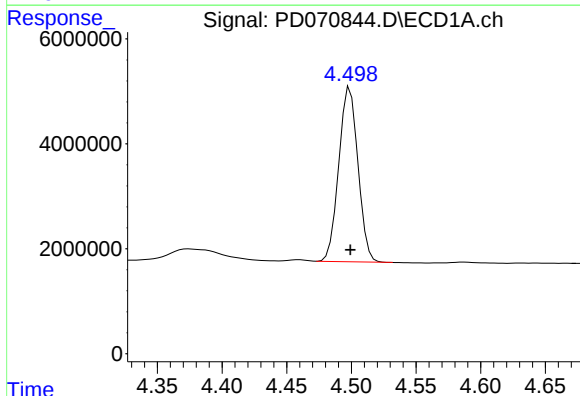


#4 Heptachlor

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 34261071
Conc: 10.13 ng/ml

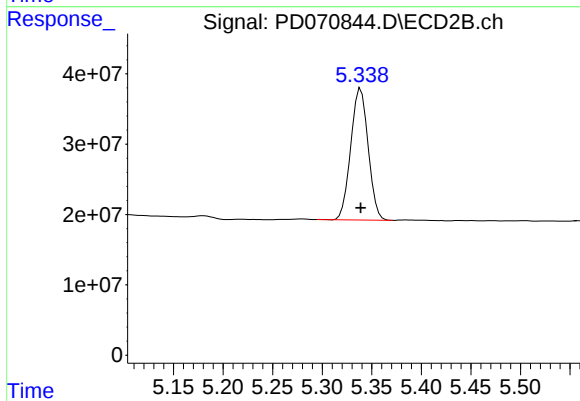

#4 Heptachlor


R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 229151140
Conc: 11.31 ng/ml

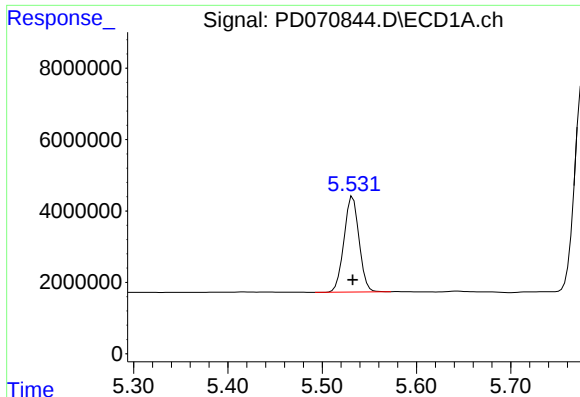

#9 Endosulfan I


R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 29755667
Conc: 10.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

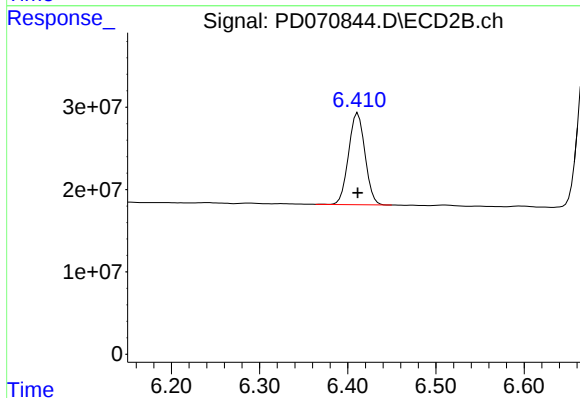


#9 Endosulfan I

R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 144331203
Conc: 10.81 ng/ml

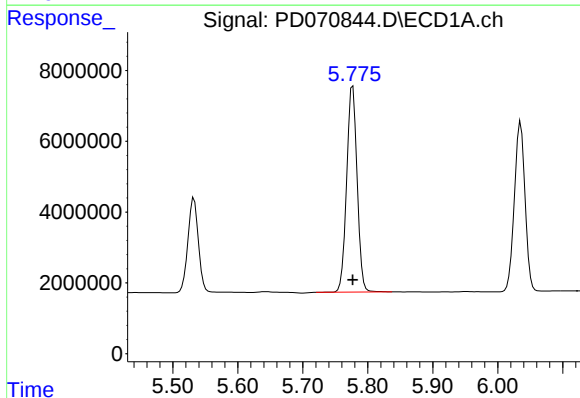


#13 Dieldrin

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 65348963
Conc: 19.78 ng/ml

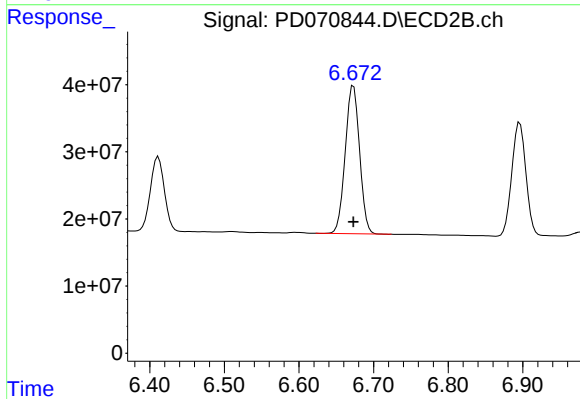

#13 Dieldrin


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 294099347
Conc: 21.48 ng/ml

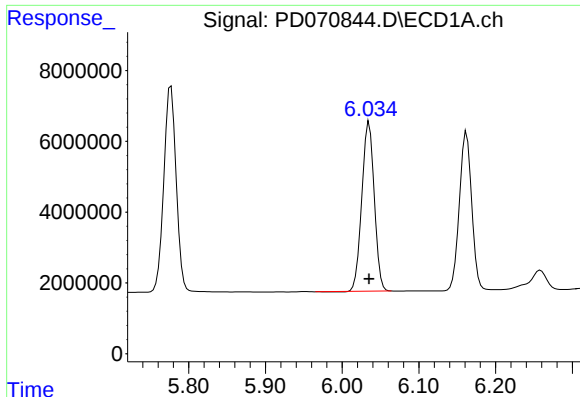

#14 Endrin


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 54007917
Conc: 19.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

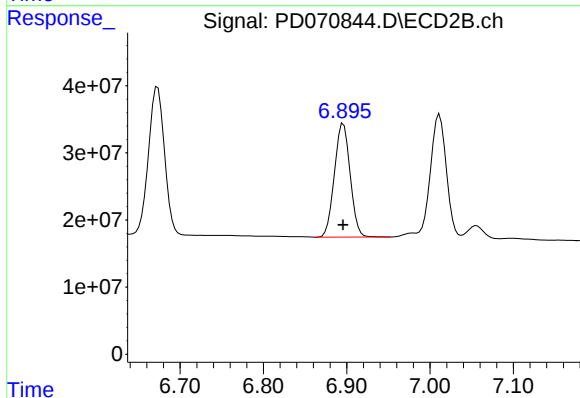


#14 Endrin

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 222689690
Conc: 20.79 ng/ml

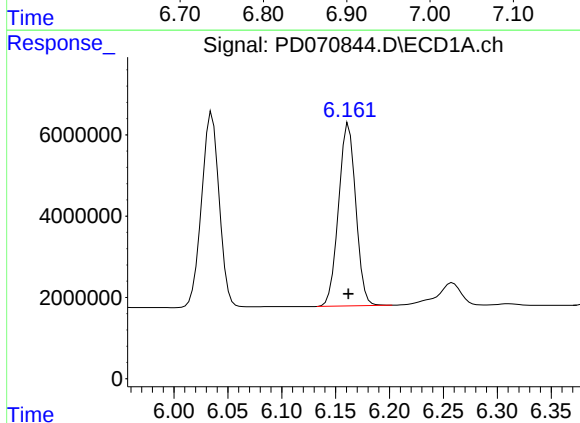


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 49950102
Conc: 19.78 ng/ml

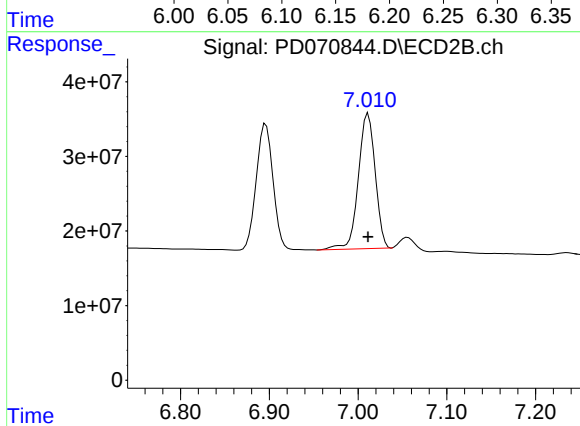

#16 4,4'-DDD


R.T.: 7.011 min
Delta R.T.: 0.000 min
Response: 238801772
Conc: 21.63 ng/ml

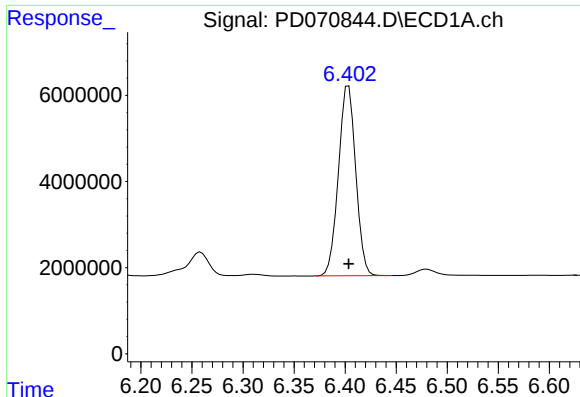

#17 4,4'-DDT


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 52015536
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

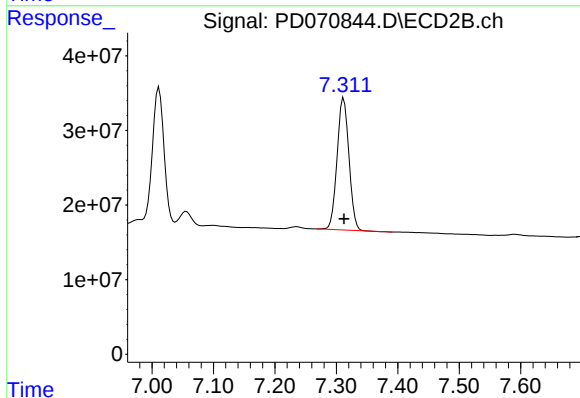


#17 4,4'-DDT

R.T.: 7.312 min
Delta R.T.: 0.000 min
Response: 237822903
Conc: 21.23 ng/ml

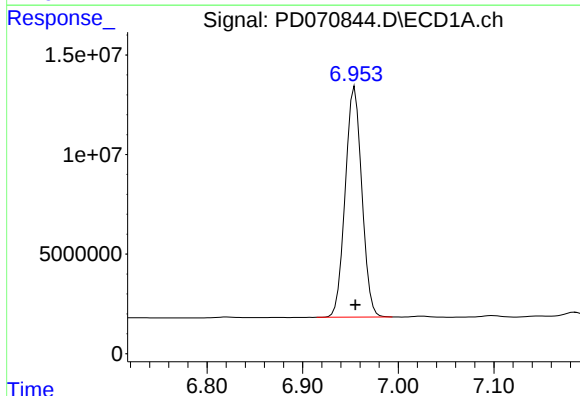


#20 Methoxychlor

R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 140123397
Conc: 101.94 ng/ml

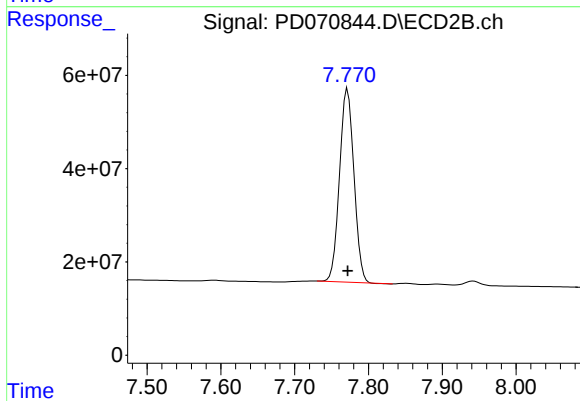

#20 Methoxychlor


R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 563678627
Conc: 107.59 ng/ml

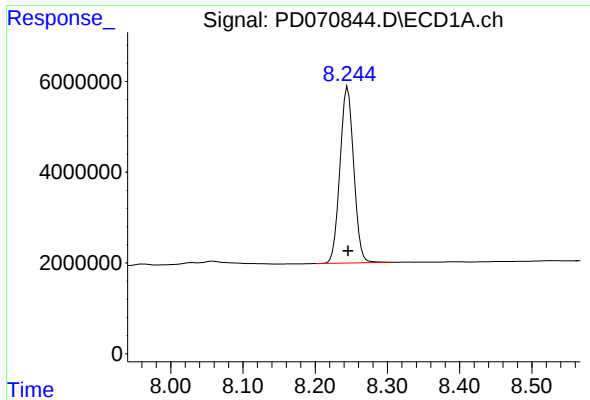

#27 Decachlorobiphenyl

R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 51119162
Conc: 21.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

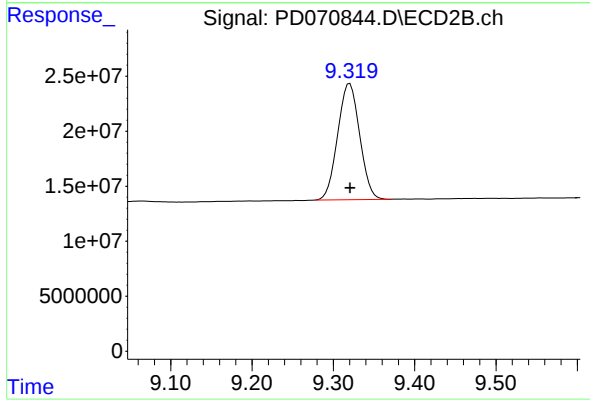

#27 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: 0.000 min
Response: 198437293
Conc: 21.51 ng/ml