

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 12:46
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:24:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	46612302	456.9E6	20.000	20.000
27)	SA Decachlor...	8.246	9.320	95941356	369.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.915	4.529	69620318	621.9E6	20.000	20.000
3)	MA gamma-BHC...	4.199	4.822	67154149	515.9E6	20.000	20.000
4)	MA Heptachlor	4.499	5.339	67671136	405.1E6	20.000	20.000
9)	A Endosulfan I	5.532	6.411	58302973	267.0E6	20.000	20.000
13)	MA Dieldrin	5.777	6.673	132.1E6	547.6E6	40.000	40.000
14)	MA Endrin	6.035	6.896	109.5E6	428.4E6	40.000	40.000
16)	A 4,4'-DDD	6.162	7.011	101.0E6	441.6E6	40.000	40.000
17)	MA 4,4'-DDT	6.404	7.313	105.6E6	448.1E6	40.000	40.000
20)	A Methoxychlor	6.955	7.772	274.9E6	1047.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 12:46
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:24:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

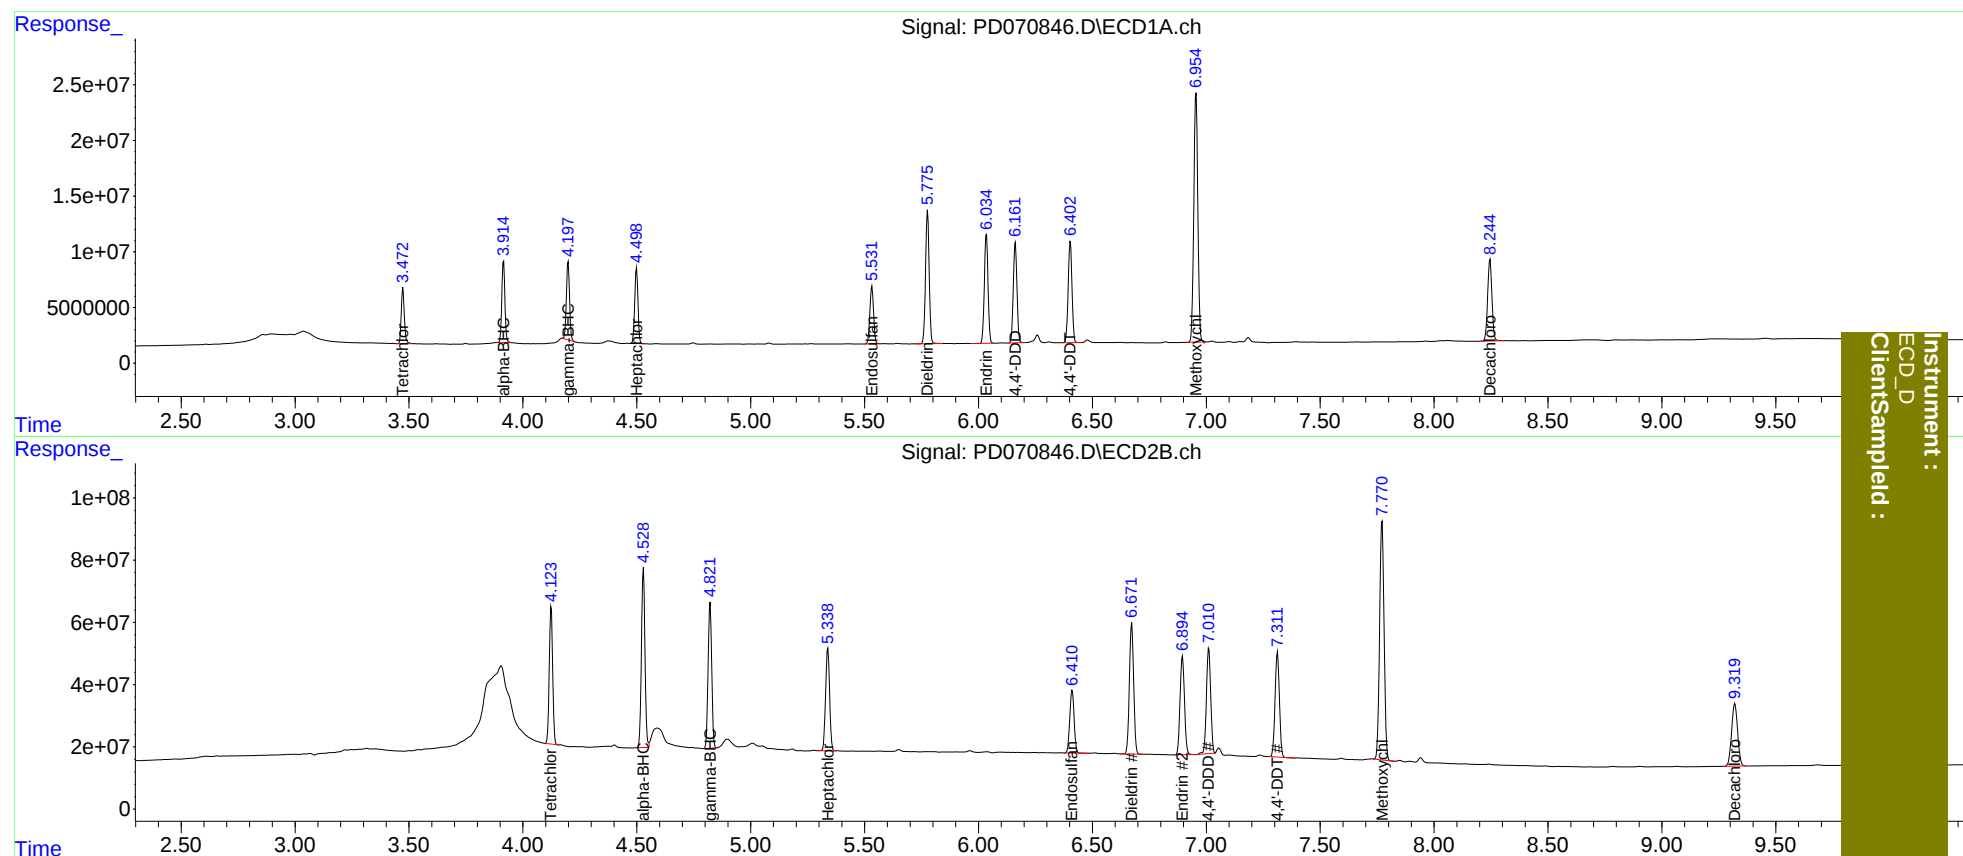


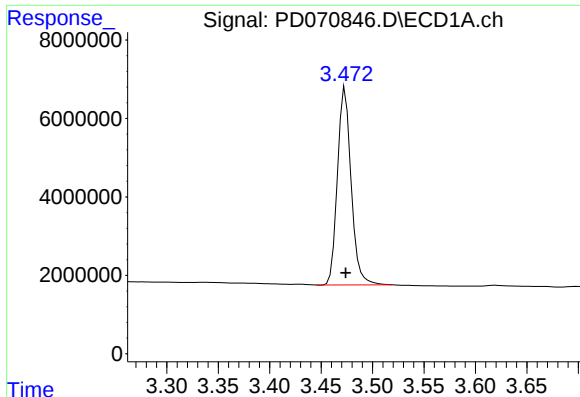

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 46612302
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

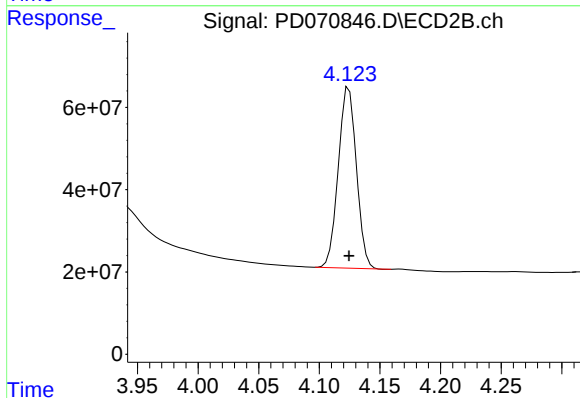


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 456879348
Conc: 20.00 ng/ml

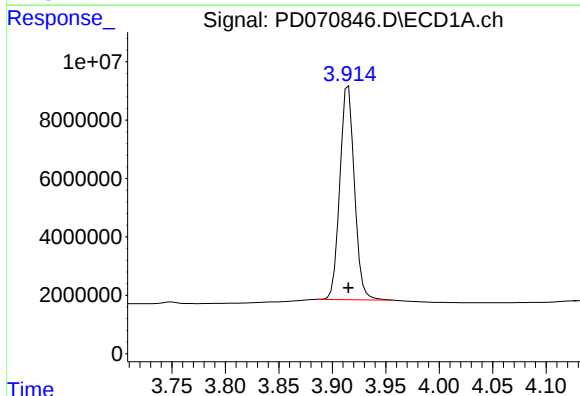


#2 alpha-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 69620318
Conc: 20.00 ng/ml

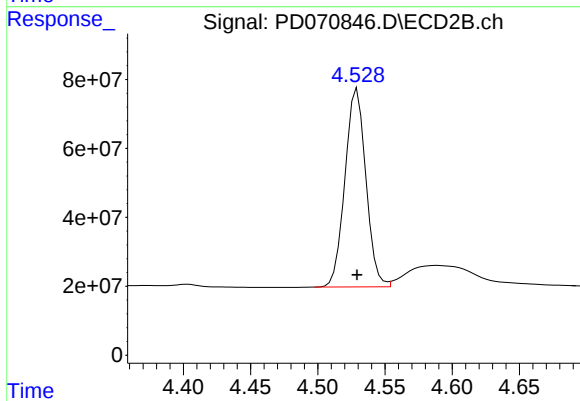

#2 alpha-BHC


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 621937887
Conc: 20.00 ng/ml

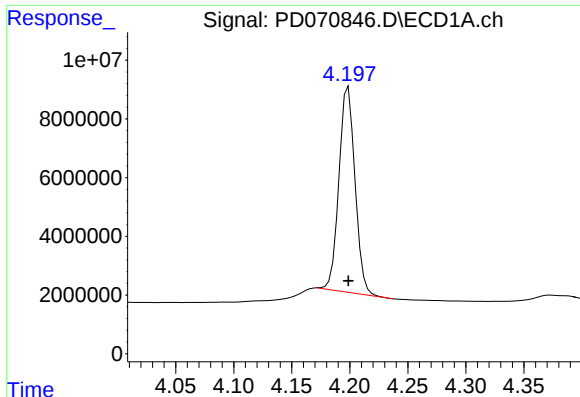

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 67154149
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

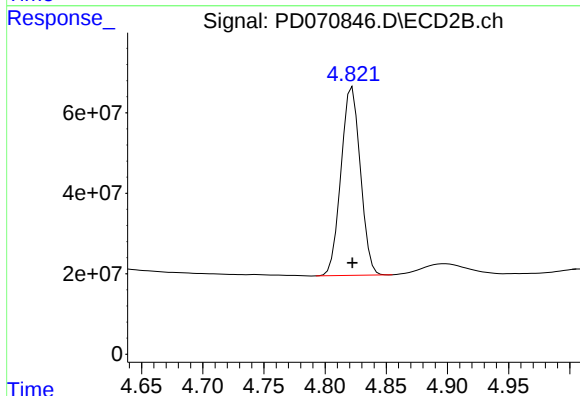


#3 gamma-BHC (Lindane)

R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 515877494
Conc: 20.00 ng/ml

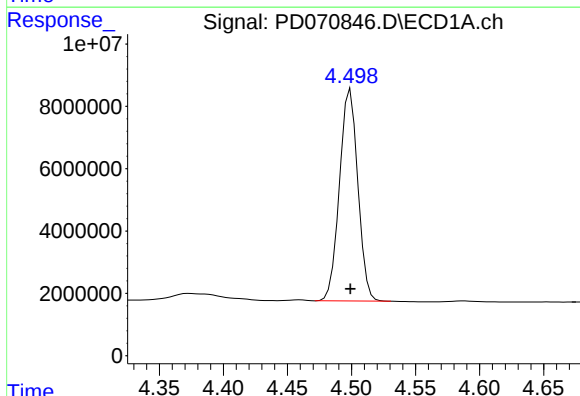


#4 Heptachlor

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 67671136
Conc: 20.00 ng/ml

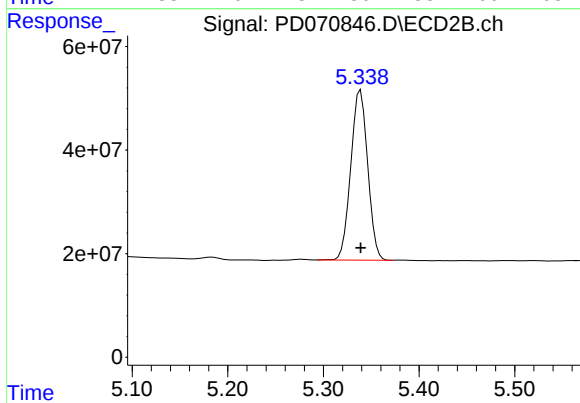

#4 Heptachlor


R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 405104120
Conc: 20.00 ng/ml

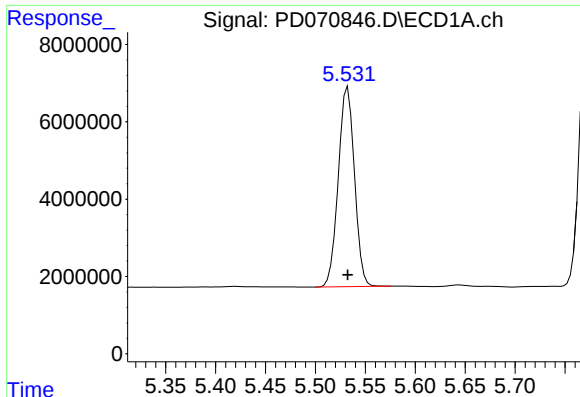

#9 Endosulfan I


R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 58302973
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

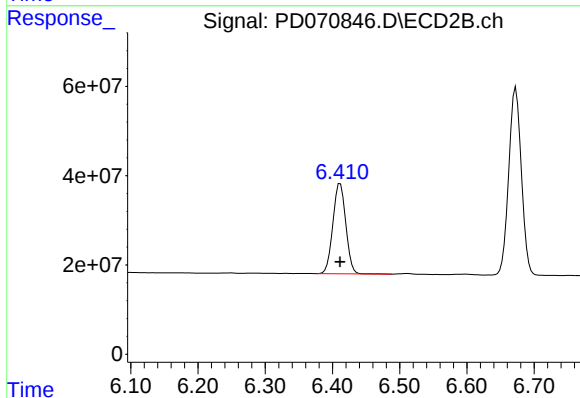


#9 Endosulfan I

R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 267005223
Conc: 20.00 ng/ml

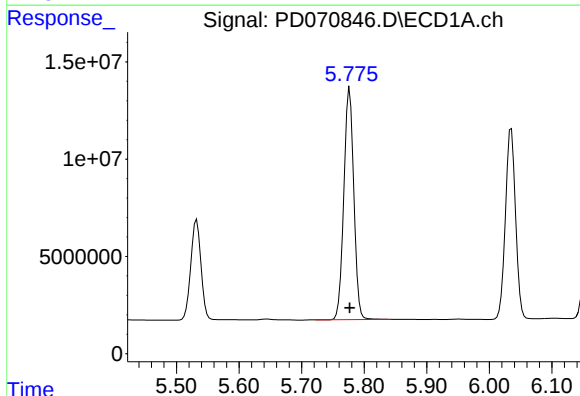


#13 Dieldrin

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 132129834
Conc: 40.00 ng/ml

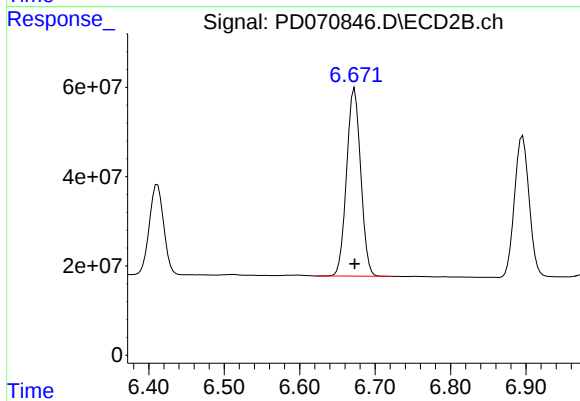

#13 Dieldrin


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 547605222
Conc: 40.00 ng/ml

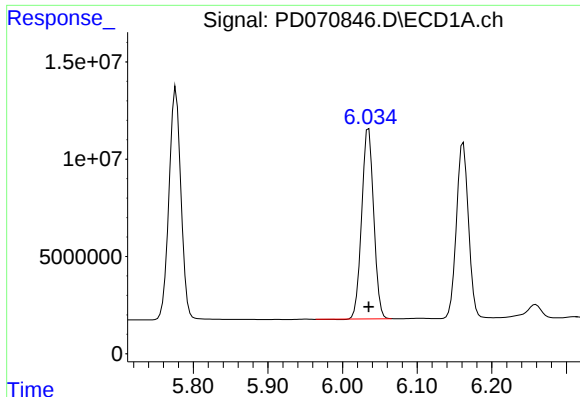

#14 Endrin


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 109508377
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

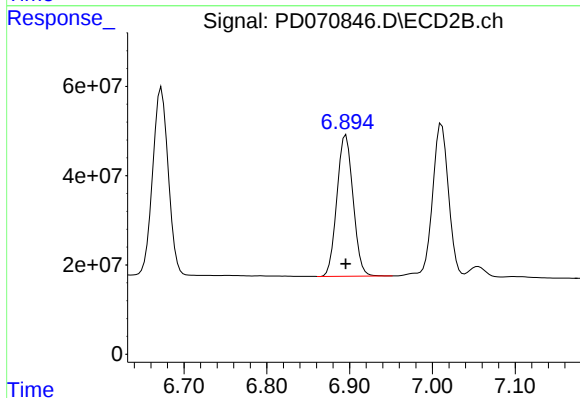


#14 Endrin

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 428380081
Conc: 40.00 ng/ml

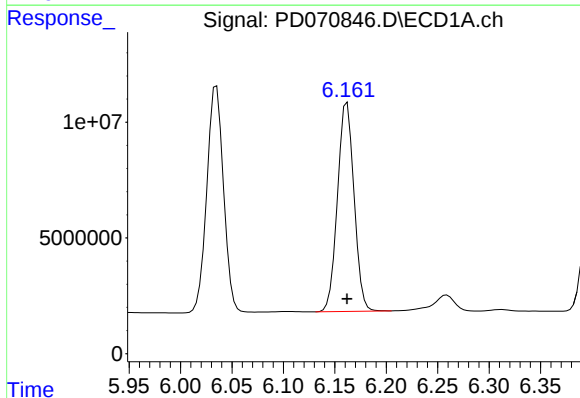


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 101032988
Conc: 40.00 ng/ml

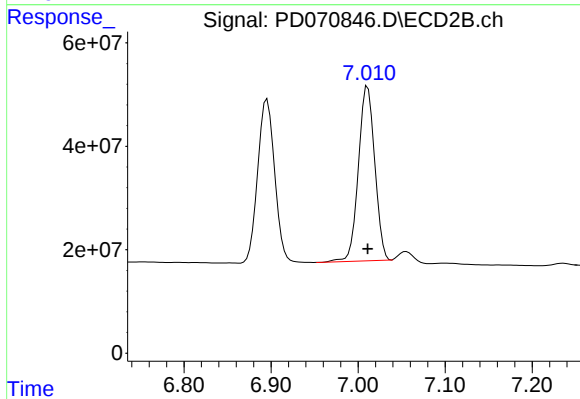

#16 4,4'-DDD


R.T.: 7.011 min
Delta R.T.: 0.000 min
Response: 441626722
Conc: 40.00 ng/ml

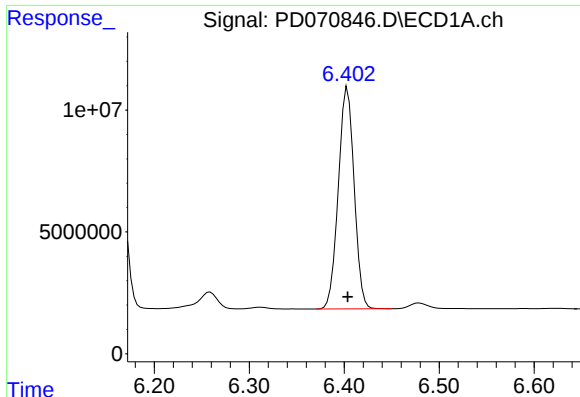

#17 4,4'-DDT


R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 105595004
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

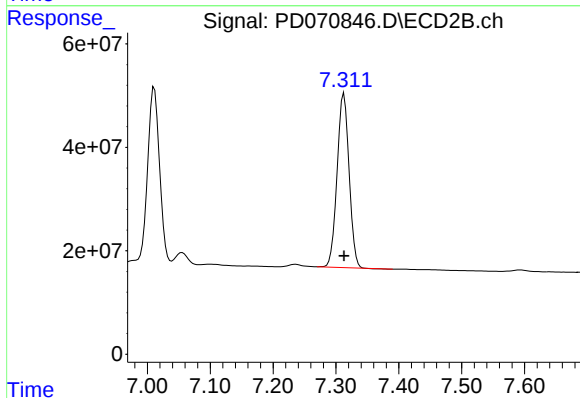


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: 0.000 min
Response: 448141915
Conc: 40.00 ng/ml

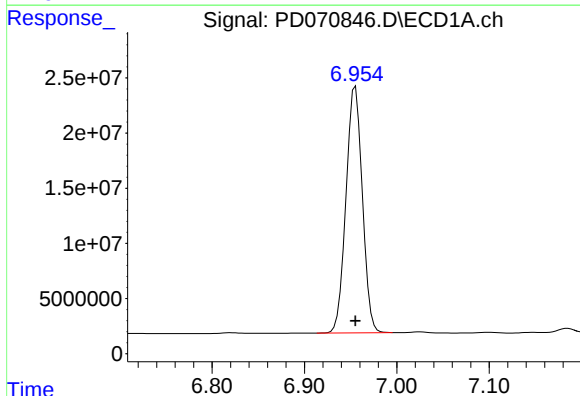


#20 Methoxychlor

R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 274903759
Conc: 200.00 ng/ml

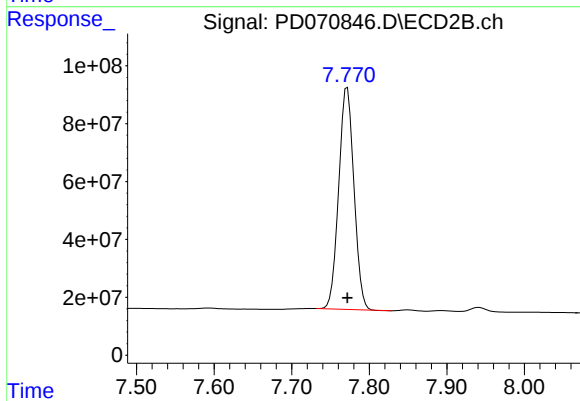

#20 Methoxychlor


R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 1047794164
Conc: 200.00 ng/ml

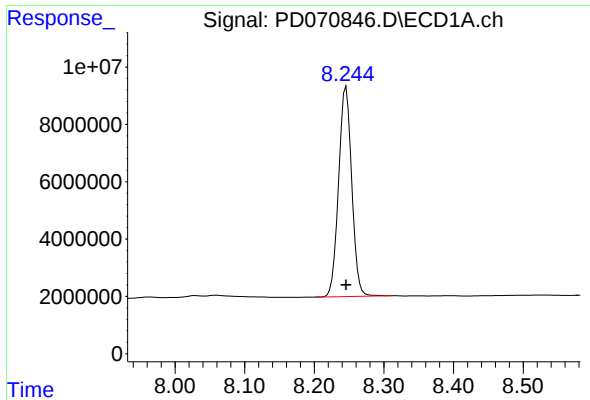

#27 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: 0.000 min
Response: 95941356
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

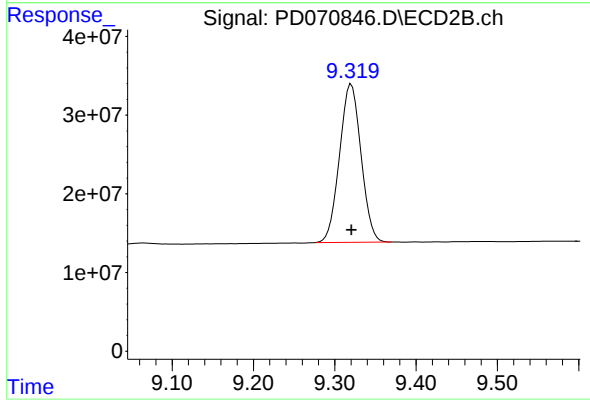

#27 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: 0.000 min
Response: 368986961
Conc: 40.00 ng/ml