

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 13:14
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:24:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	88683980	848.6E6	38.052	37.147
27)	SA Decachlor...	8.245	9.319	178.5E6	650.9E6	74.408	70.564
Target Compounds							
2)	A alpha-BHC	3.915	4.529	139.9E6	1138.5E6	40.185	36.611
3)	MA gamma-BHC...	4.199	4.822	129.1E6	938.7E6	38.454	36.391
4)	MA Heptachlor	4.499	5.338	131.3E6	714.5E6	38.814	35.276
9)	A Endosulfan I	5.532	6.410	110.3E6	464.1E6	37.850	34.767
13)	MA Dieldrin	5.776	6.673	252.5E6	967.4E6	76.436	70.664
14)	MA Endrin	6.034	6.895	207.8E6	766.2E6	75.892	71.540
16)	A 4,4'-DDD	6.162	7.011	191.8E6	806.1E6	75.938	73.014
17)	MA 4,4'-DDT	6.403	7.312	202.4E6	808.5E6	76.683	72.161
20)	A Methoxychlor	6.955	7.771	504.0E6	1850.2E6	366.684	353.165


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 13:14
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:24:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

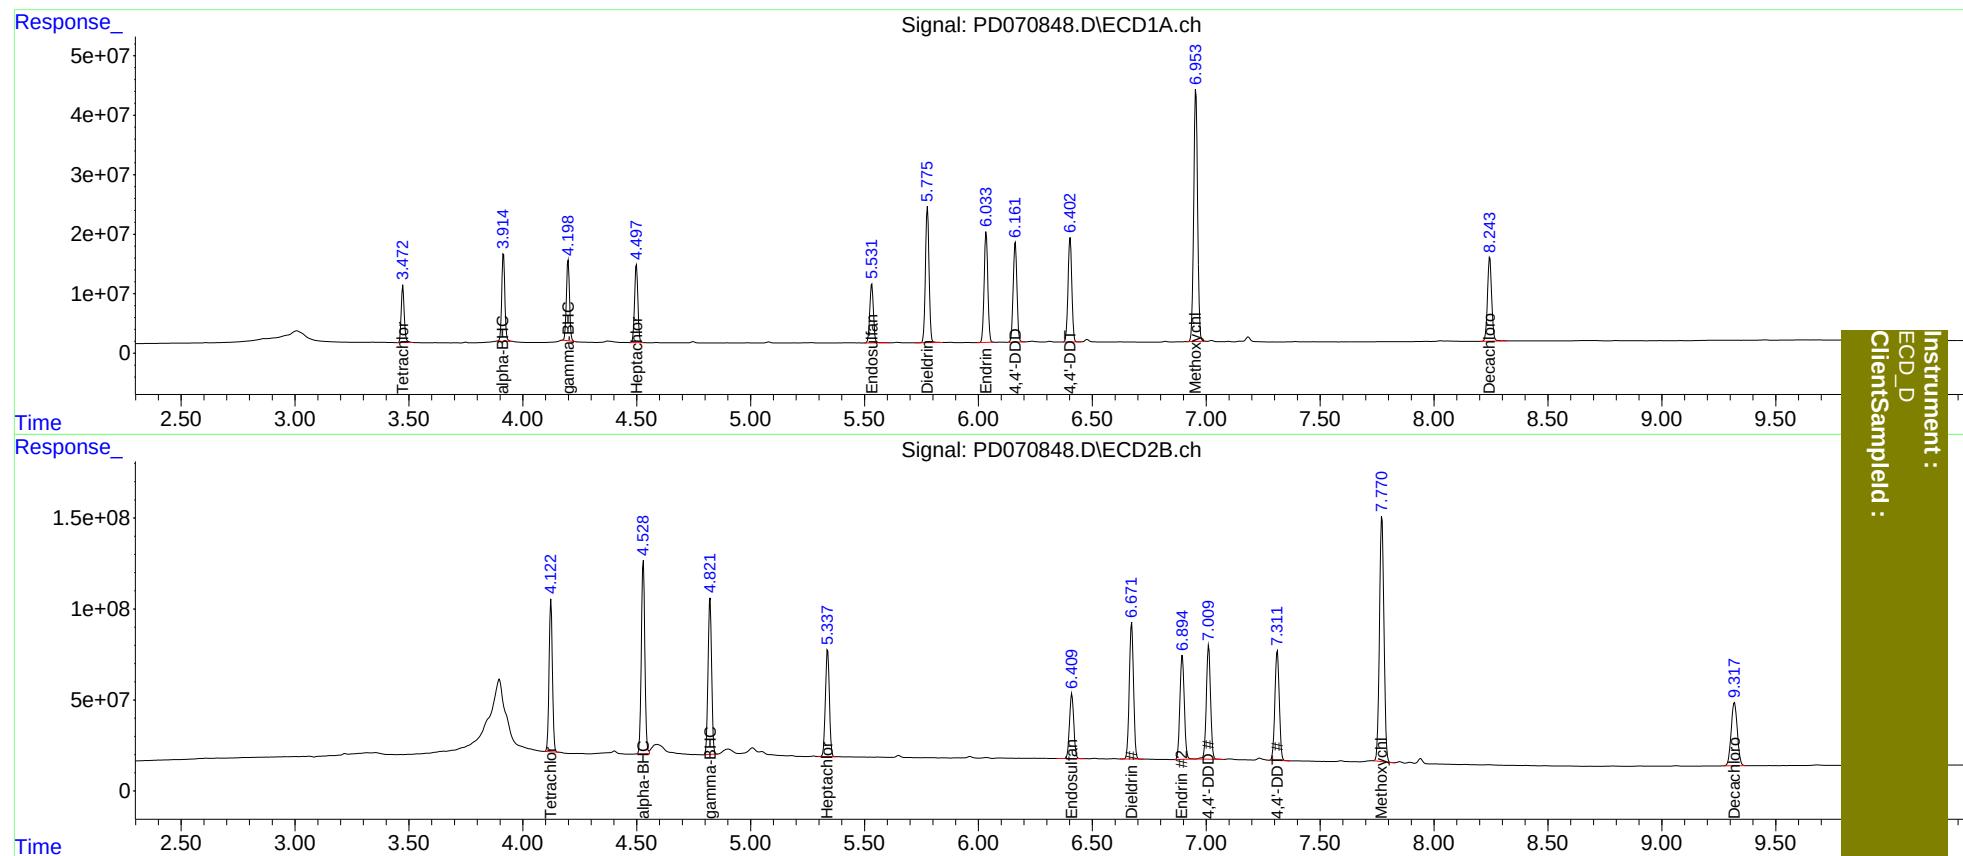


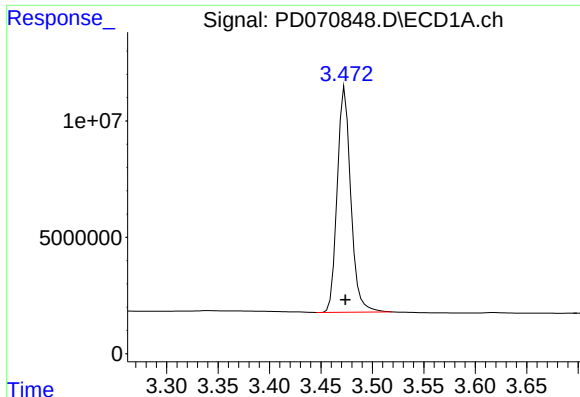

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 88683980
Conc: 38.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

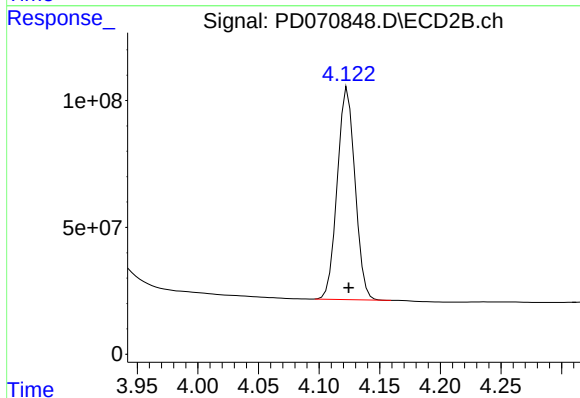


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 848595429
Conc: 37.15 ng/ml

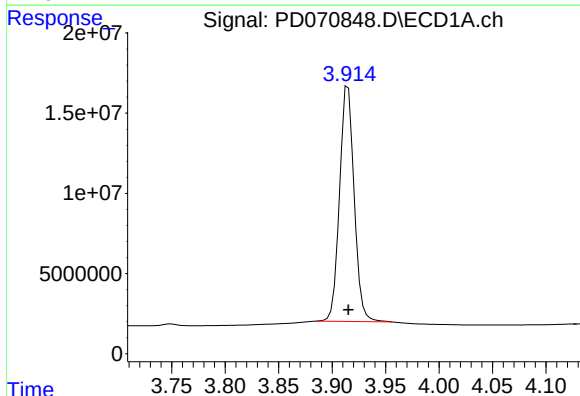


#2 alpha-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 139885604
Conc: 40.19 ng/ml

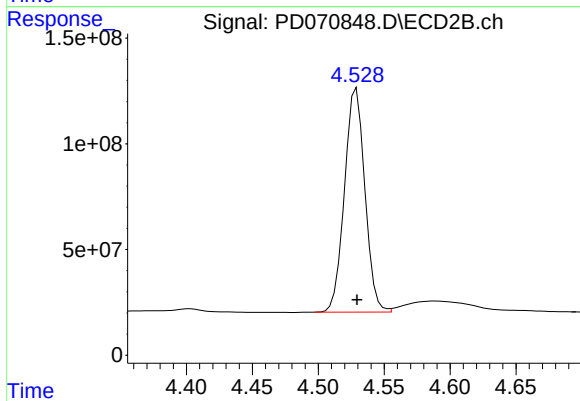

#2 alpha-BHC


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 1138476894
Conc: 36.61 ng/ml

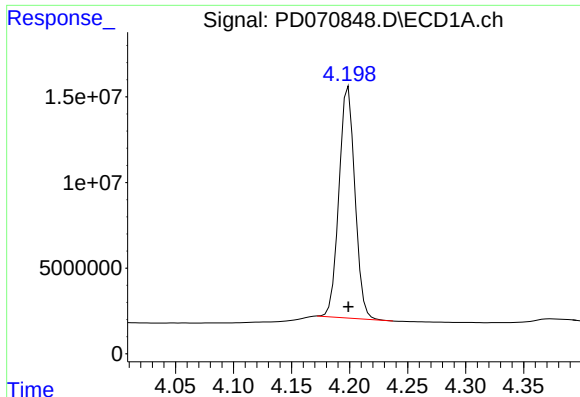

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 129118704
Conc: 38.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

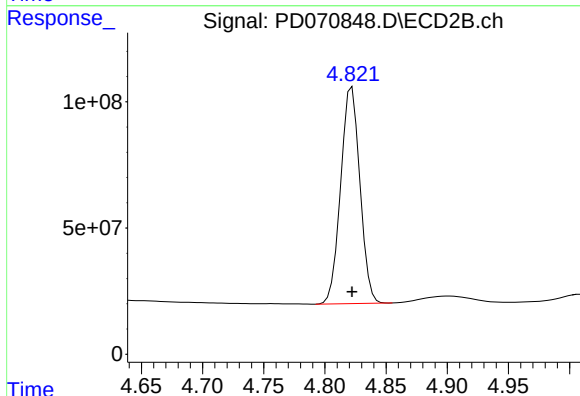


#3 gamma-BHC (Lindane)

R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 938659478
Conc: 36.39 ng/ml

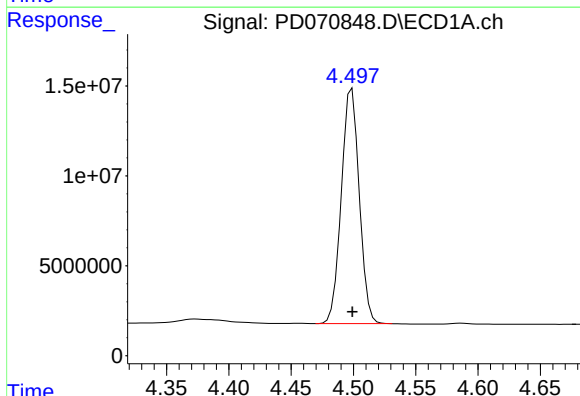


#4 Heptachlor

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 131329899
Conc: 38.81 ng/ml

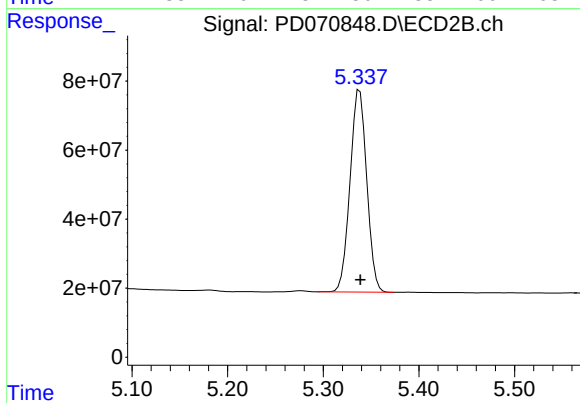

#4 Heptachlor


R.T.: 5.338 min
Delta R.T.: 0.000 min
Response: 714528306
Conc: 35.28 ng/ml

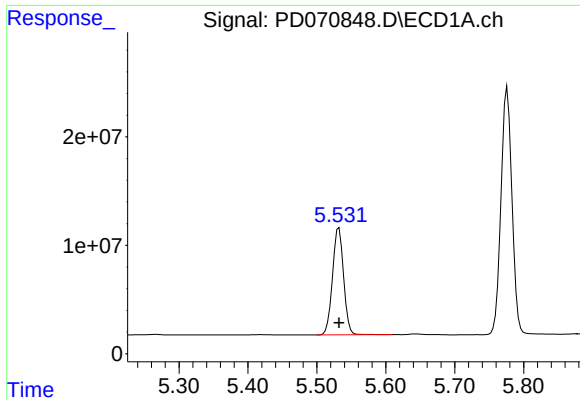

#9 Endosulfan I


R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 110338835
Conc: 37.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

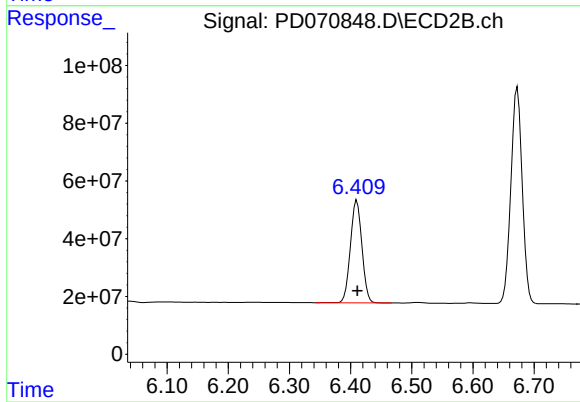


#9 Endosulfan I

R.T.: 6.410 min
Delta R.T.: -0.001 min
Response: 464143147
Conc: 34.77 ng/ml

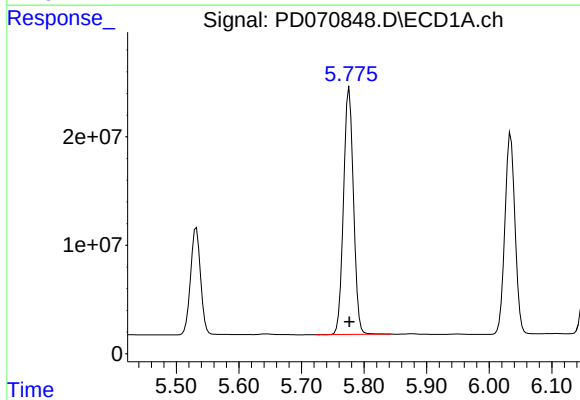


#13 Dieldrin

R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 252487688
Conc: 76.44 ng/ml

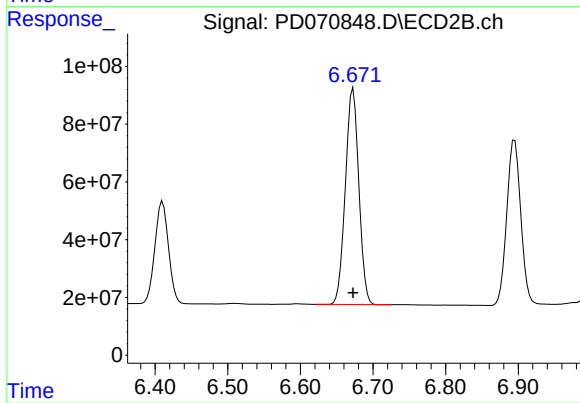

#13 Dieldrin


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 967397165
Conc: 70.66 ng/ml

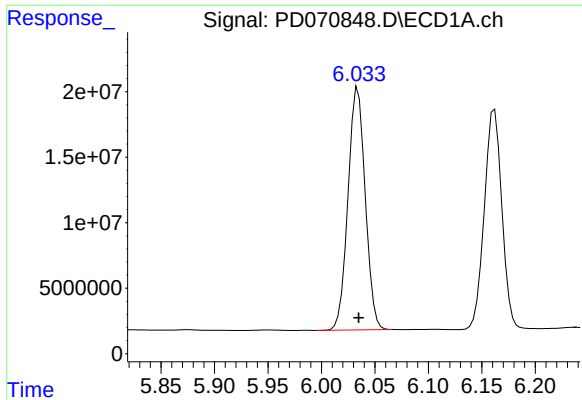

#14 Endrin


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 207769419
Conc: 75.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

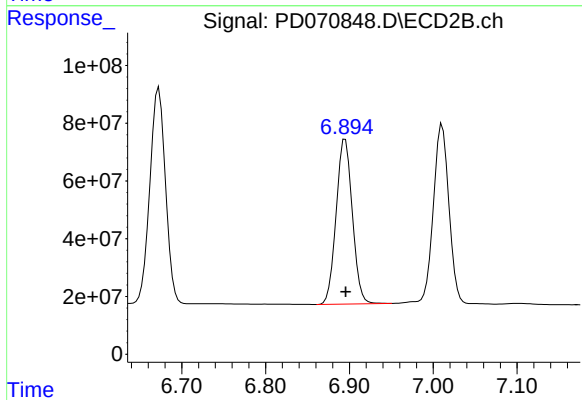


#14 Endrin

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 766153989
Conc: 71.54 ng/ml

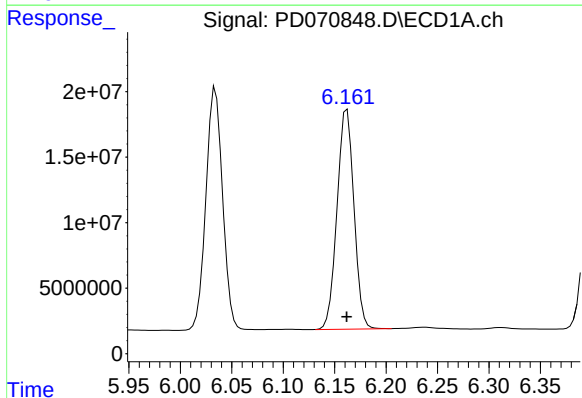


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 191805837
Conc: 75.94 ng/ml

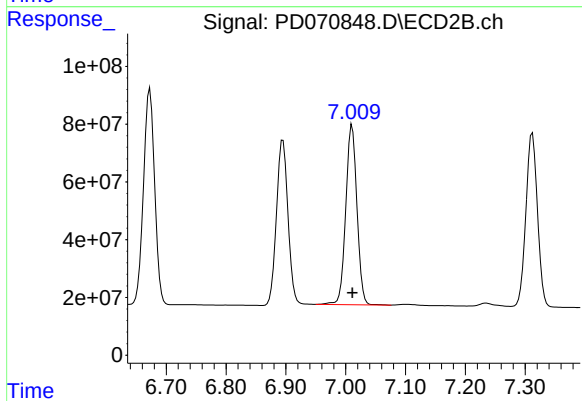

#16 4,4'-DDD


R.T.: 7.011 min
Delta R.T.: 0.000 min
Response: 806119158
Conc: 73.01 ng/ml

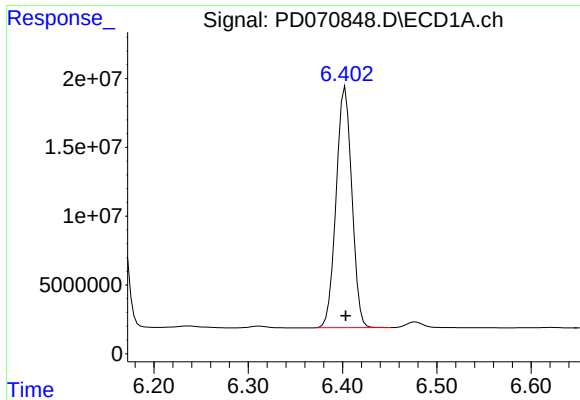

#17 4,4'-DDT


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 202432454
Conc: 76.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

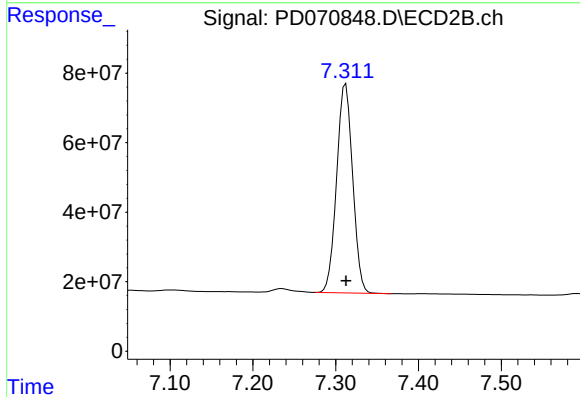


#17 4,4'-DDT

R.T.: 7.312 min
Delta R.T.: 0.000 min
Response: 808455616
Conc: 72.16 ng/ml

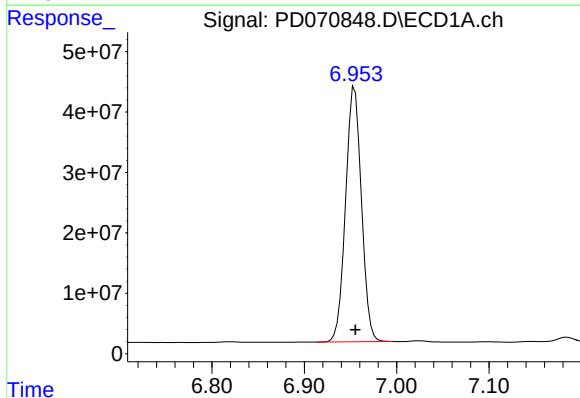


#20 Methoxychlor

R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 504014092
Conc: 366.68 ng/ml

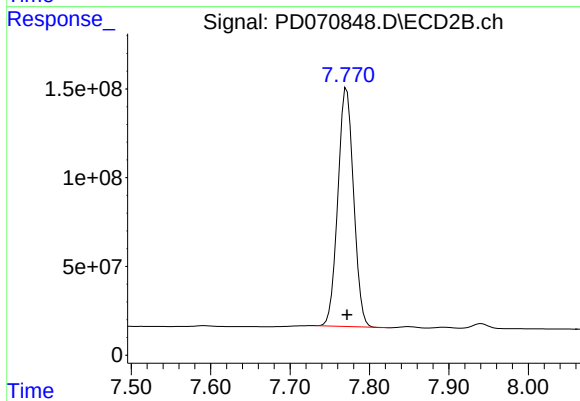

#20 Methoxychlor


R.T.: 7.771 min
Delta R.T.: 0.000 min
Response: 1850223521
Conc: 353.17 ng/ml

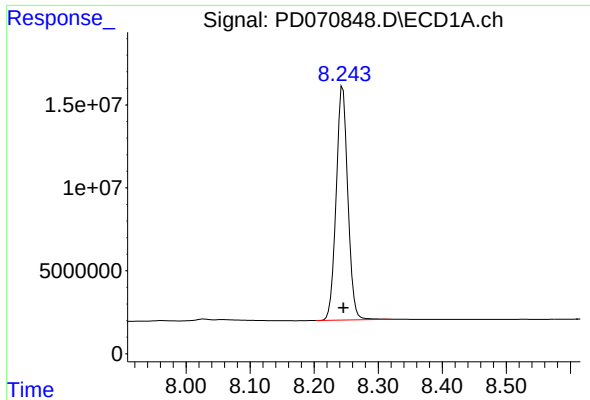

#27 Decachlorobiphenyl

R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 178470533
Conc: 74.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

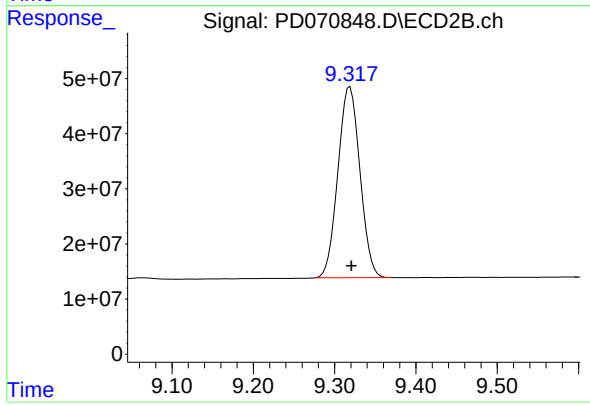

#27 Decachlorobiphenyl

R.T.: 9.319 min
Delta R.T.: -0.002 min
Response: 650929645
Conc: 70.56 ng/ml