

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 13:44
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:24:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.124	182.4E6	1655.3E6	78.278	72.462
27)	SA Decachlor...	8.245	9.320	365.6E6	1267.5E6	152.437	137.403
Target Compounds							
2)	A alpha-BHC	3.915	4.529	297.5E6	2258.7E6	85.470	72.633
3)	MA gamma-BHC...	4.199	4.823	275.1E6	1849.4E6	81.941	71.698
4)	MA Heptachlor	4.500	5.339	281.2E6	1381.2E6	83.101	68.191
9)	A Endosulfan I	5.533	6.411	232.6E6	898.3E6	79.794	67.291
13)	MA Dieldrin	5.777	6.672	537.1E6	1922.6E6	162.609	140.438
14)	MA Endrin	6.036	6.896	440.4E6	1525.7E6	160.882	142.460
16)	A 4,4'-DDD	6.163	7.011	409.8E6	1586.8E6	162.232	143.721
17)	MA 4,4'-DDT	6.404	7.312	437.4E6	1608.5E6	165.704	143.571
20)	A Methoxychlor	6.956	7.772	1022.6E6	3581.4E6	743.974	683.603


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 13:44
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:24:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

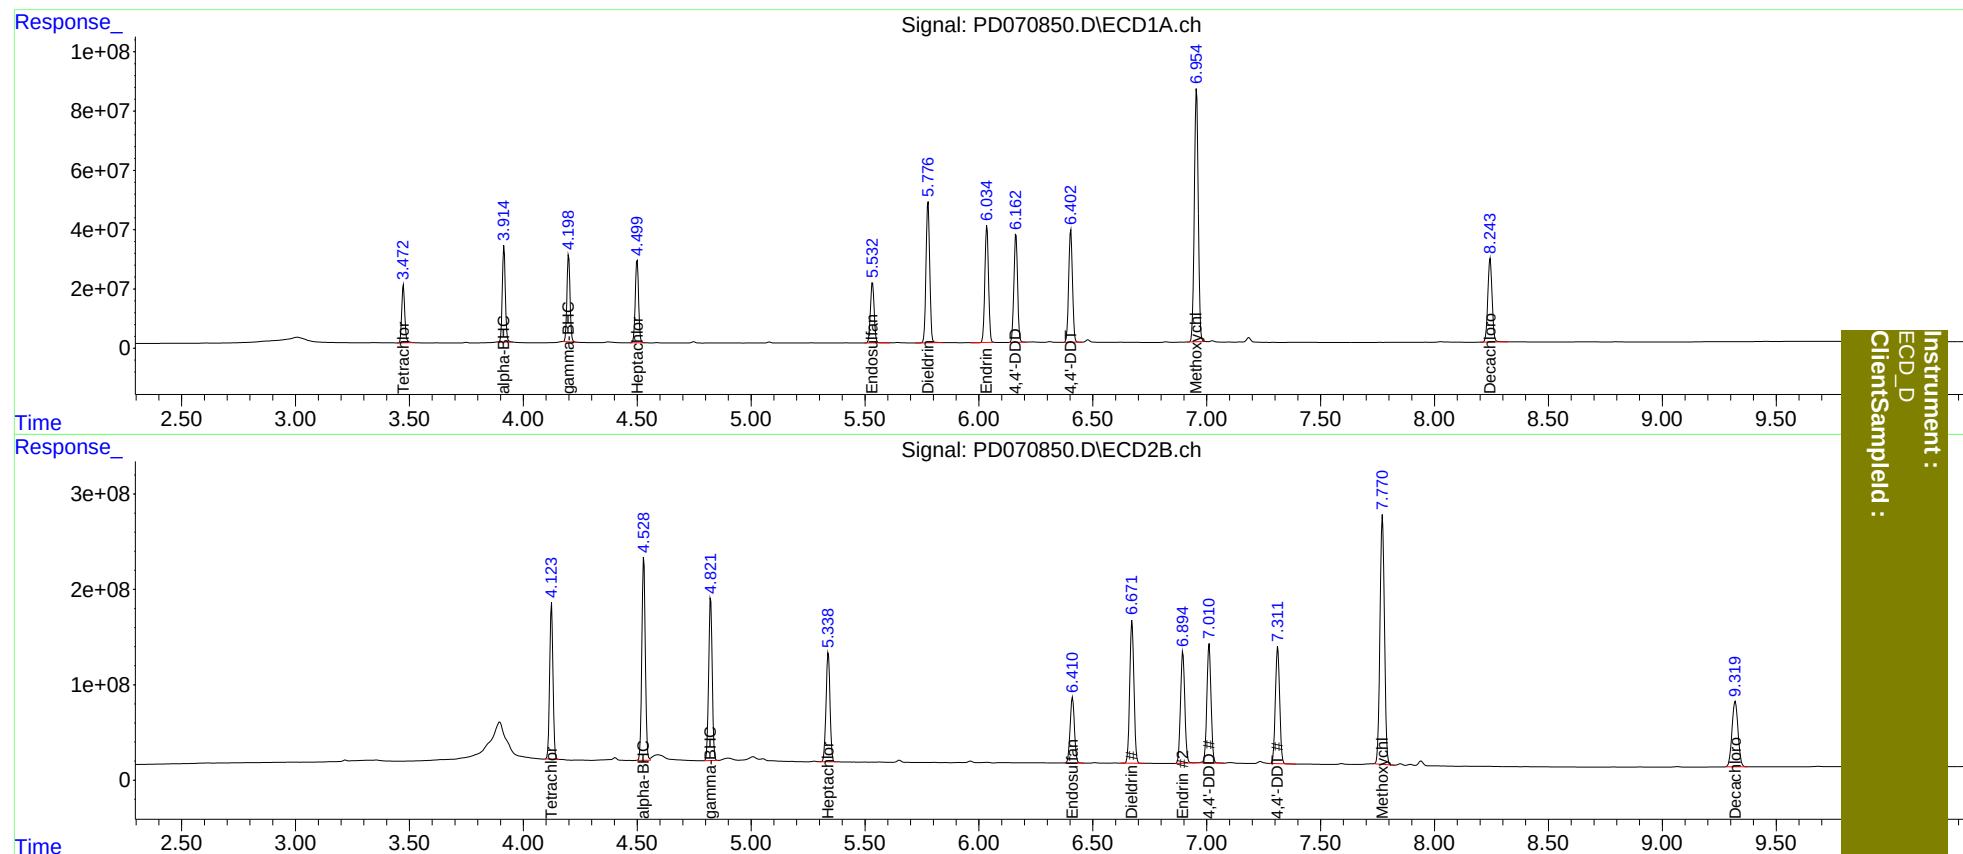


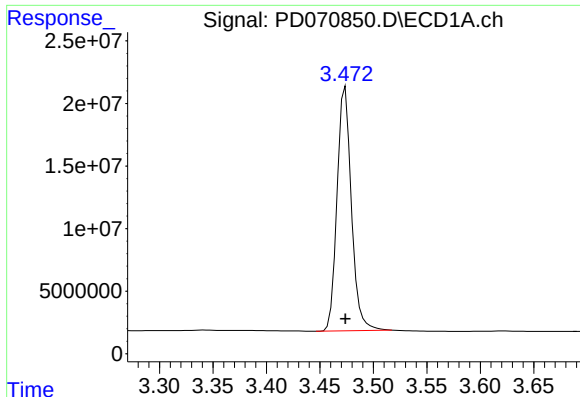

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 182435882
Conc: 78.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

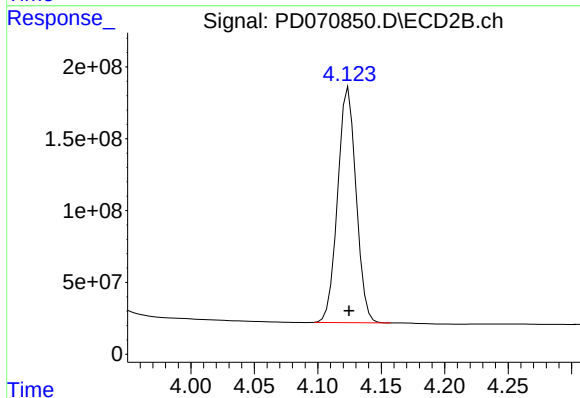


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 1655329456
Conc: 72.46 ng/ml

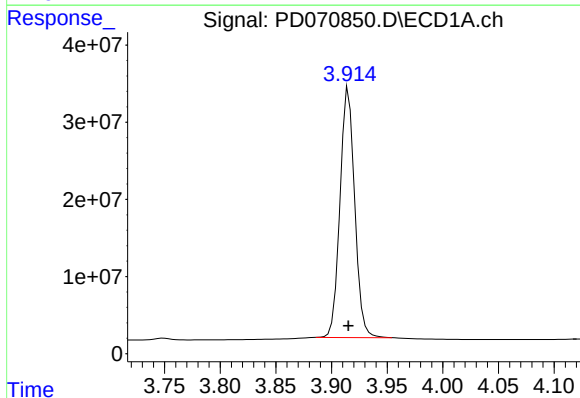


#2 alpha-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 297522270
Conc: 85.47 ng/ml

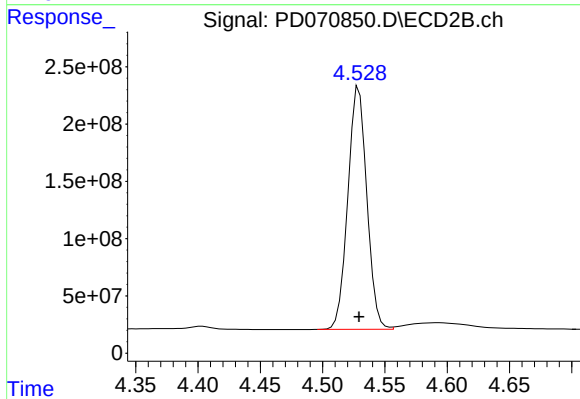

#2 alpha-BHC


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 2258661082
Conc: 72.63 ng/ml

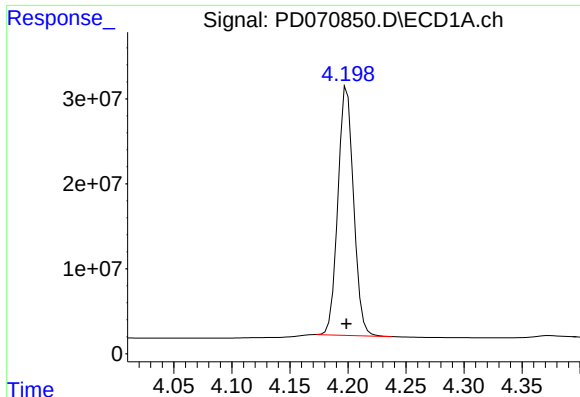

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 275135358
Conc: 81.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

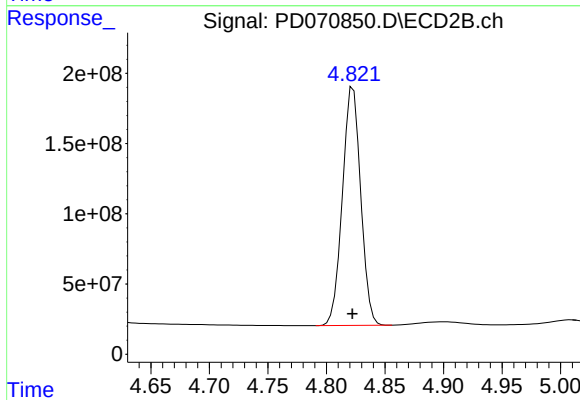


#3 gamma-BHC (Lindane)

R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 1849376662
Conc: 71.70 ng/ml

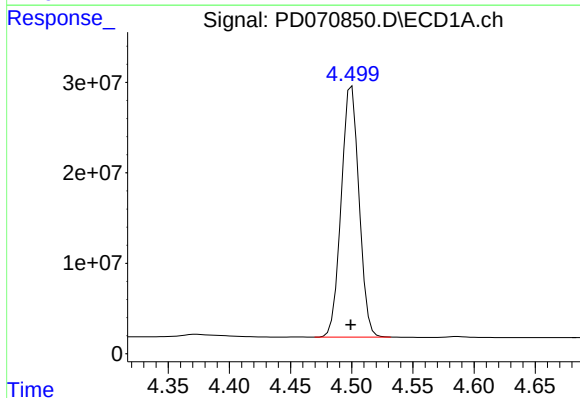


#4 Heptachlor

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 281176441
Conc: 83.10 ng/ml

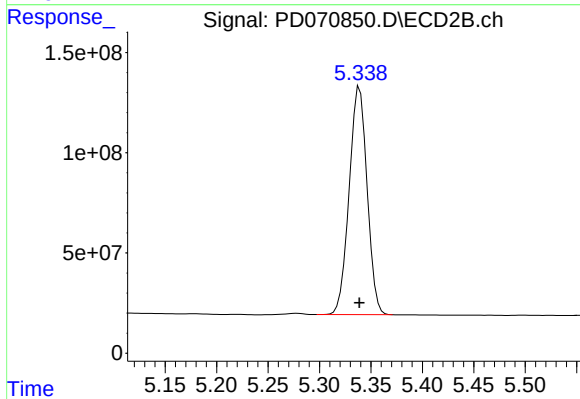

#4 Heptachlor


R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 1381221001
Conc: 68.19 ng/ml

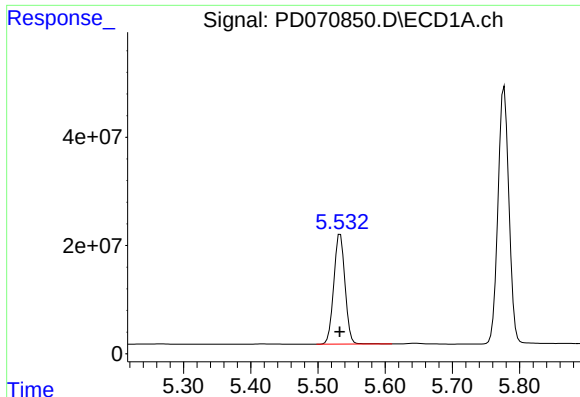

#9 Endosulfan I


R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 232612158
Conc: 79.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

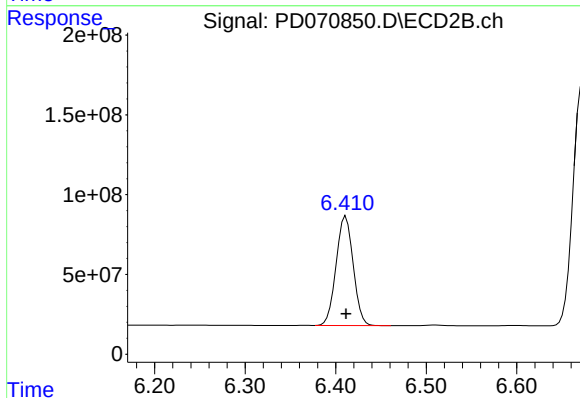


#9 Endosulfan I

R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 898346106
Conc: 67.29 ng/ml

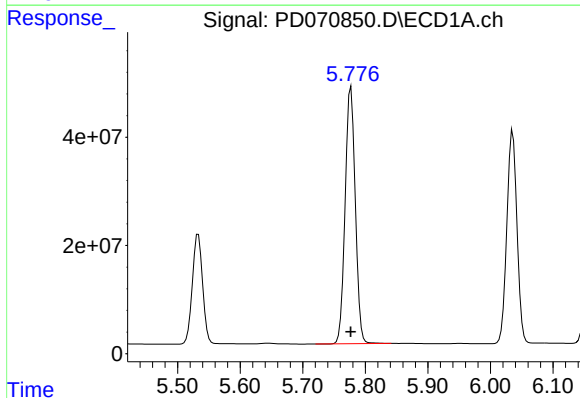


#13 Dieldrin

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 537138012
Conc: 162.61 ng/ml

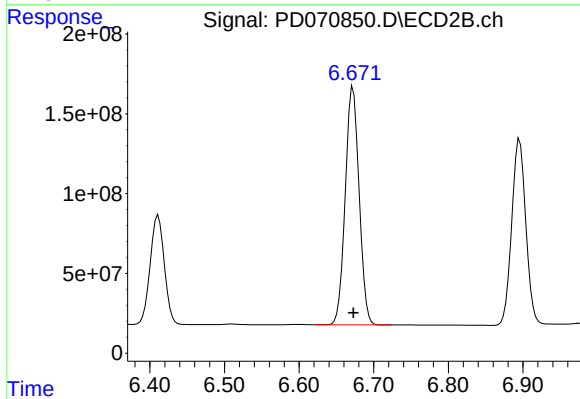

#13 Dieldrin


R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 1922615151
Conc: 140.44 ng/ml

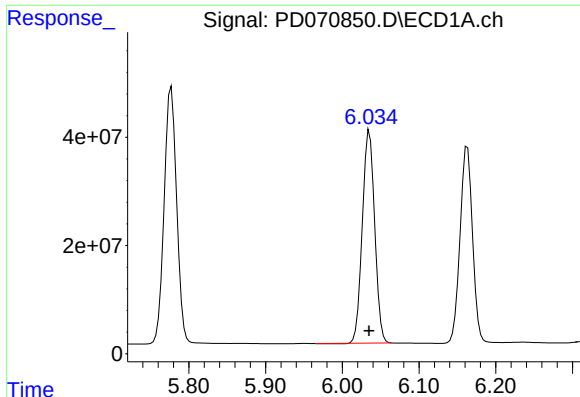

#14 Endrin


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 440448167
Conc: 160.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

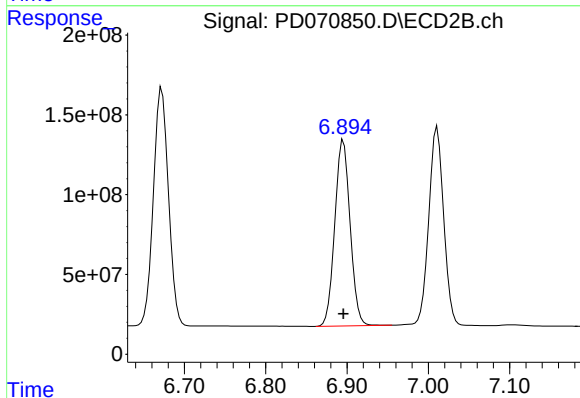


#14 Endrin

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 1525678895
Conc: 142.46 ng/ml

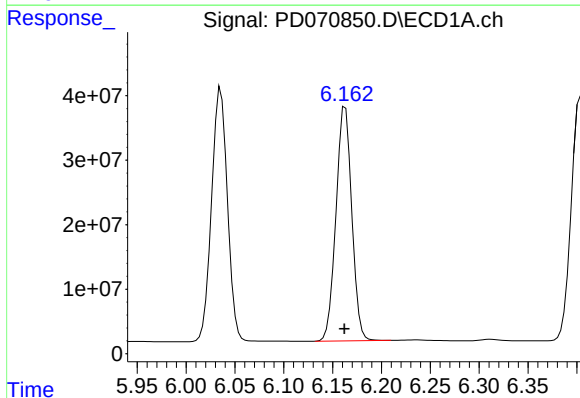


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.001 min
Response: 409768512
Conc: 162.23 ng/ml

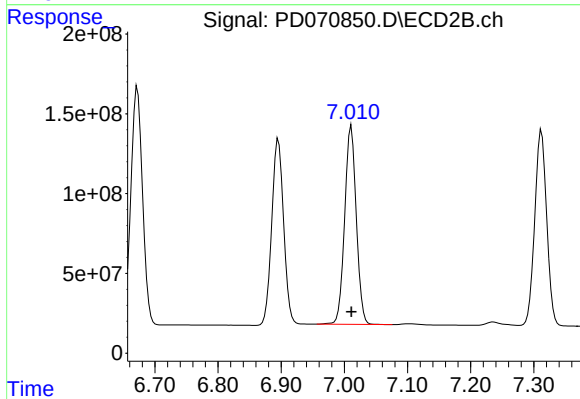

#16 4,4'-DDD


R.T.: 7.011 min
Delta R.T.: 0.000 min
Response: 1586776744
Conc: 143.72 ng/ml

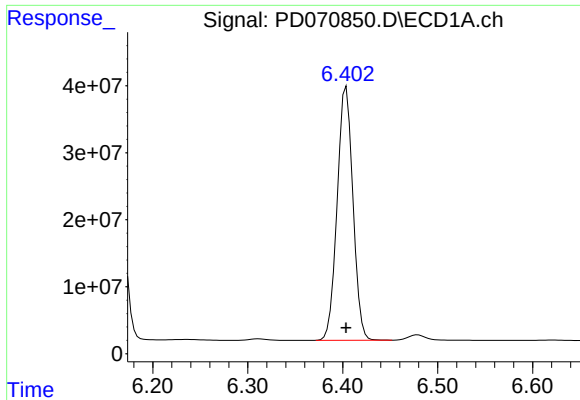

#17 4,4'-DDT


R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 437438309
Conc: 165.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

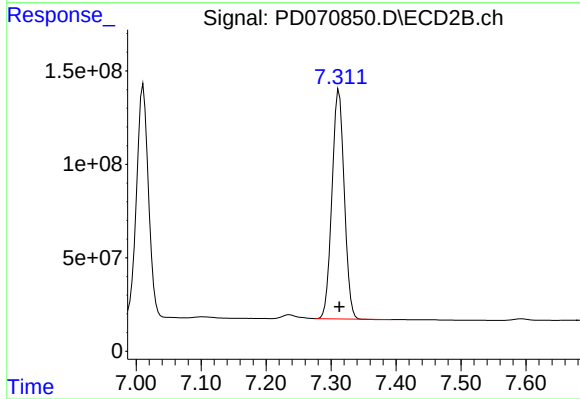


#17 4,4'-DDT

R.T.: 7.312 min
Delta R.T.: 0.000 min
Response: 1608508659
Conc: 143.57 ng/ml

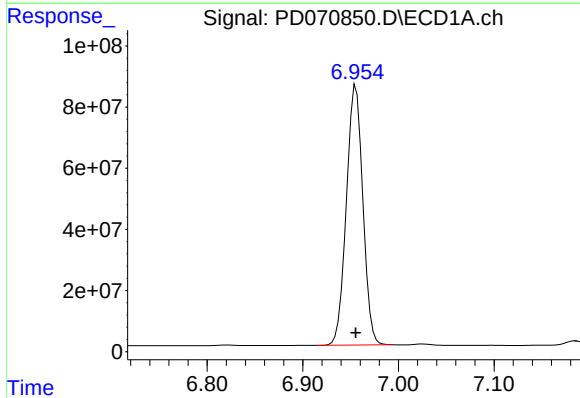


#20 Methoxychlor

R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 1022605701
Conc: 743.97 ng/ml

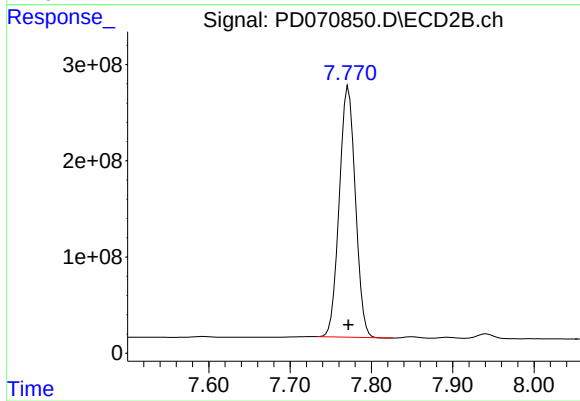

#20 Methoxychlor


R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 3581378747
Conc: 683.60 ng/ml

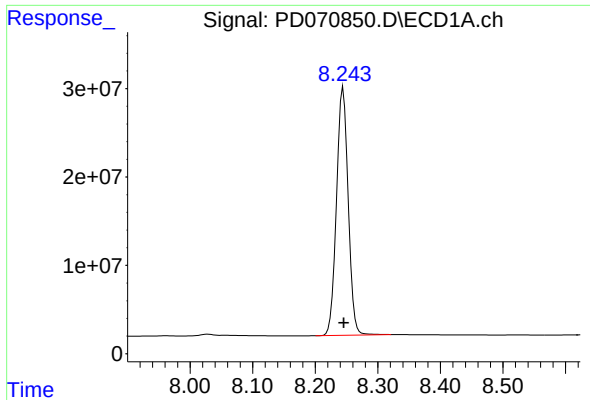

#27 Decachlorobiphenyl

R.T.: 8.245 min
Delta R.T.: -0.001 min
Response: 365625871
Conc: 152.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

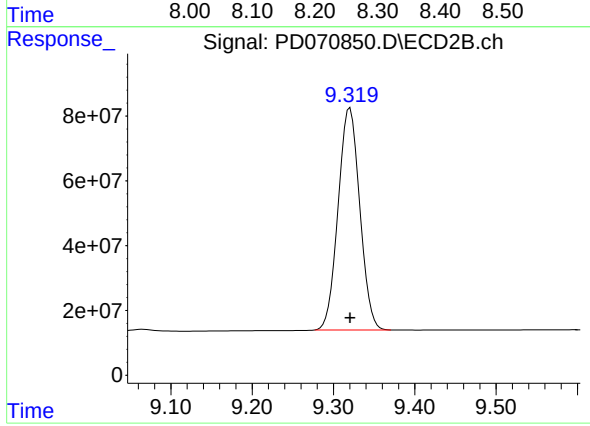

#27 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: 0.000 min
Response: 1267494683
Conc: 137.40 ng/ml