

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 14:12
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:33:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 14:22:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	354.9E6	3069.8E6	152.286	134.381
27)	SA Decachlor...	8.245	9.322	709.7E6	2379.6E6	295.898	257.964
Target Compounds							
2)	A alpha-BHC	3.916	4.530	586.1E6	4253.1E6	168.360	136.769
3)	MA gamma-BHC...	4.200	4.824	543.1E6	3458.8E6	161.751	134.092
4)	MA Heptachlor	4.500	5.340	557.2E6	2533.9E6	164.691	125.099
9)	A Endosulfan I	5.533	6.412	458.0E6	1652.4E6	157.103	123.773
13)	MA Dieldrin	5.778	6.673	1054.2E6	3614.1E6	319.126	263.995
14)	MA Endrin	6.036	6.896	861.1E6	2873.8E6	314.547	268.341
16)	A 4,4'-DDD	6.163	7.012	805.3E6	2969.5E6	318.824	268.959
17)	MA 4,4'-DDT	6.405	7.313	869.8E6	3048.3E6	329.472	272.082
20)	A Methoxychlor	6.955	7.772	1934.2E6	6464.0E6	1407.185	1233.823


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 14:12
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:33:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 14:22:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

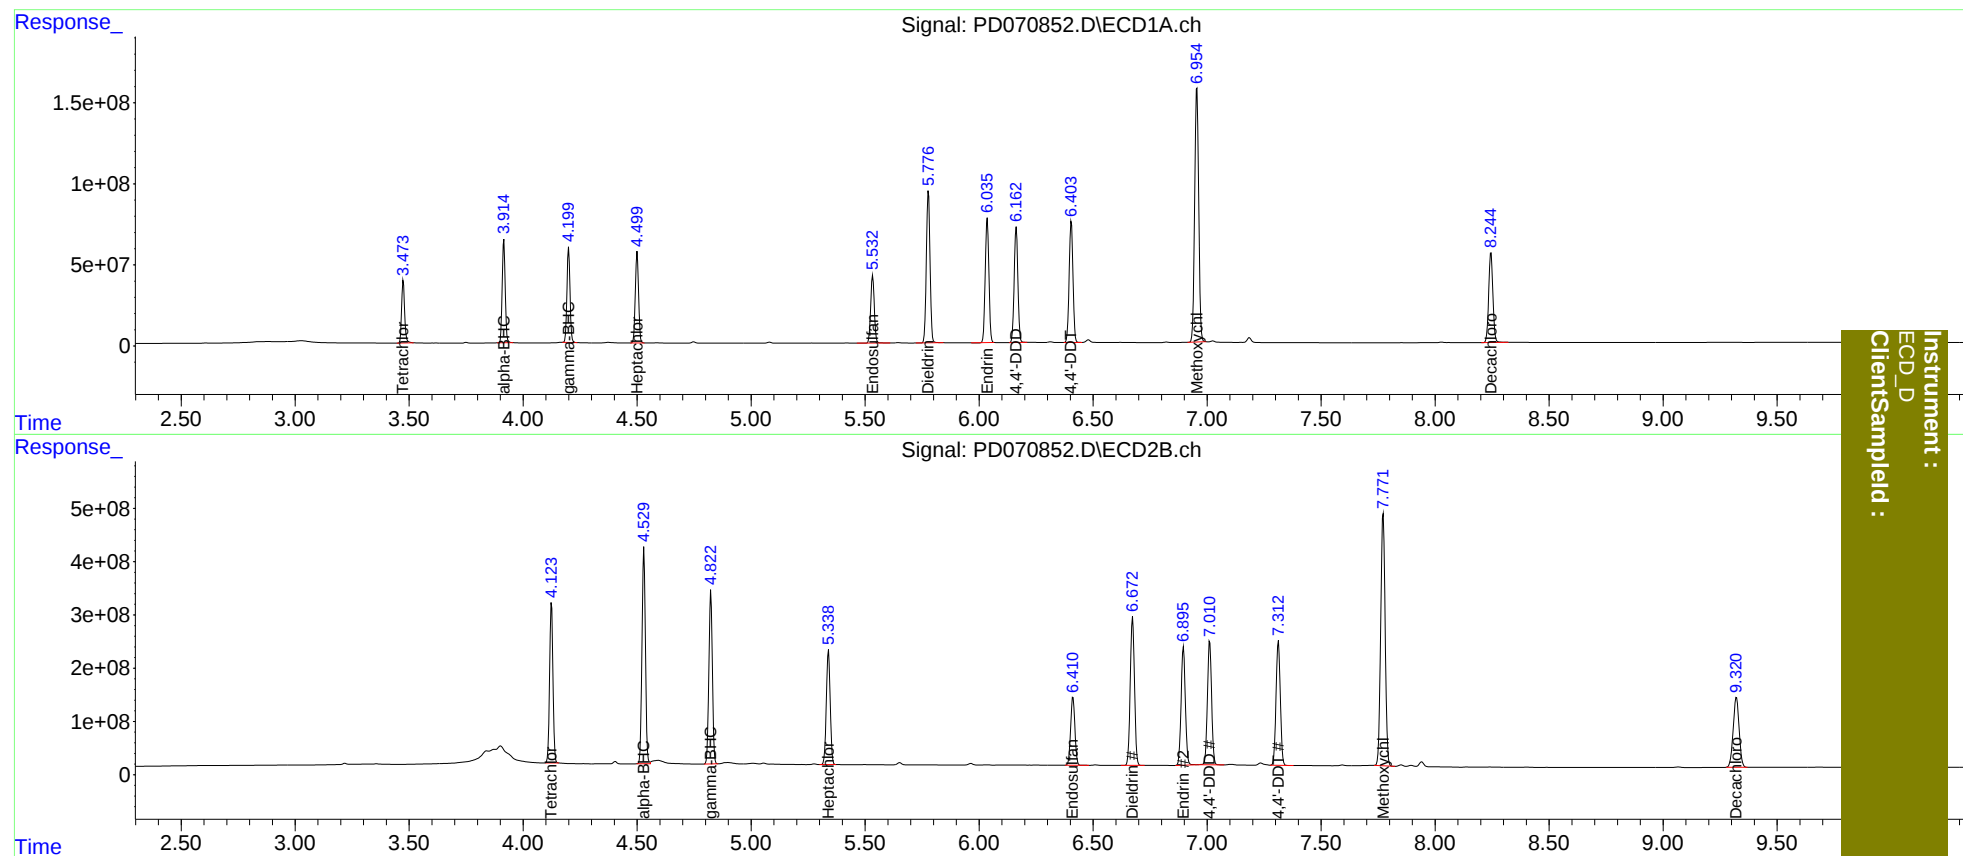


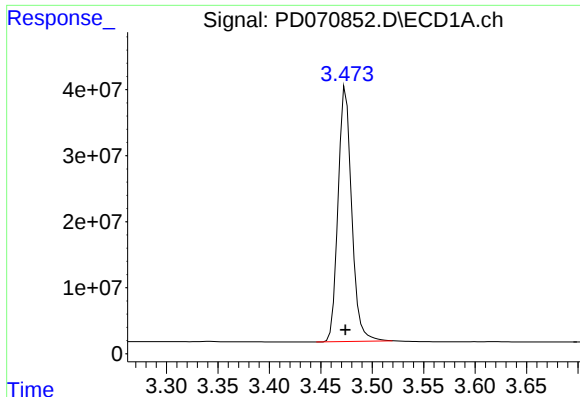

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 354919614
Conc: 152.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

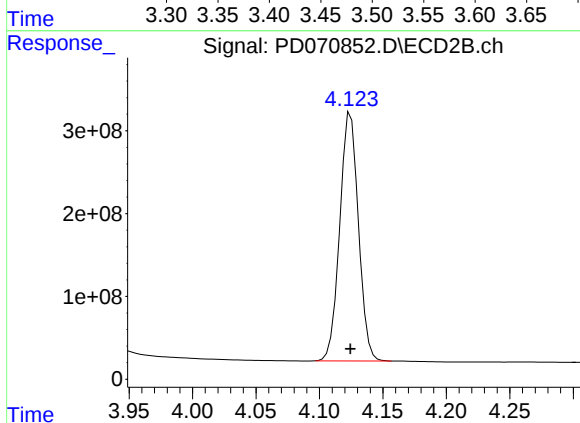


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 3069786956
Conc: 134.38 ng/ml

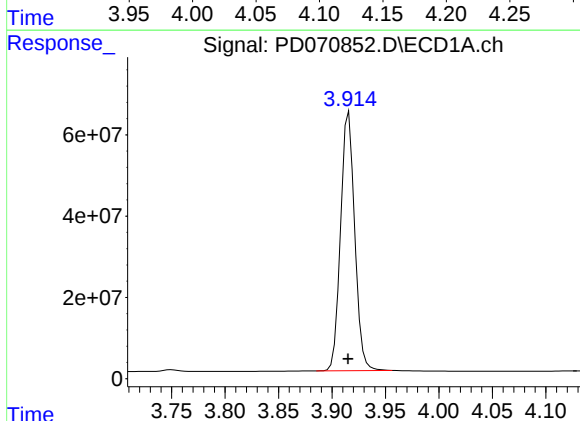


#2 alpha-BHC

R.T.: 3.916 min
Delta R.T.: 0.000 min
Response: 586063704
Conc: 168.36 ng/ml

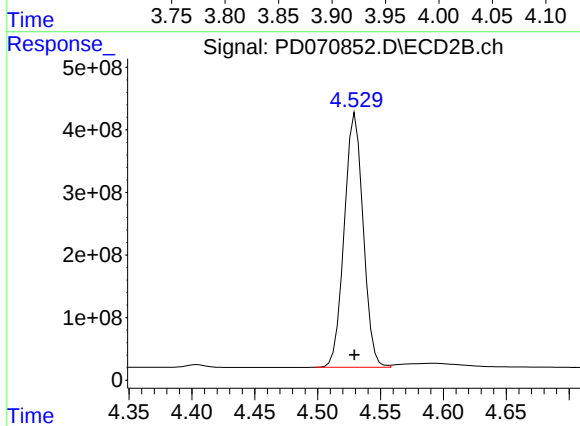

#2 alpha-BHC


R.T.: 4.530 min
Delta R.T.: 0.000 min
Response: 4253079529
Conc: 136.77 ng/ml

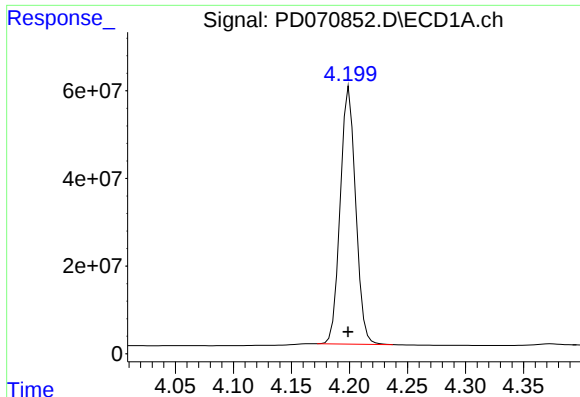

#3 gamma-BHC (Lindane)


R.T.: 4.200 min
Delta R.T.: 0.001 min
Response: 543112878
Conc: 161.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

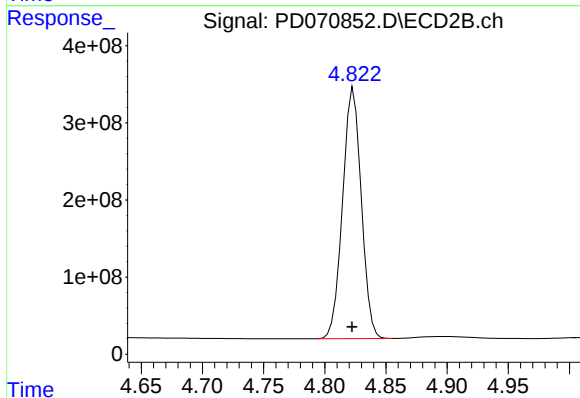


#3 gamma-BHC (Lindane)

R.T.: 4.824 min
Delta R.T.: 0.001 min
Response: 3458752879
Conc: 134.09 ng/ml

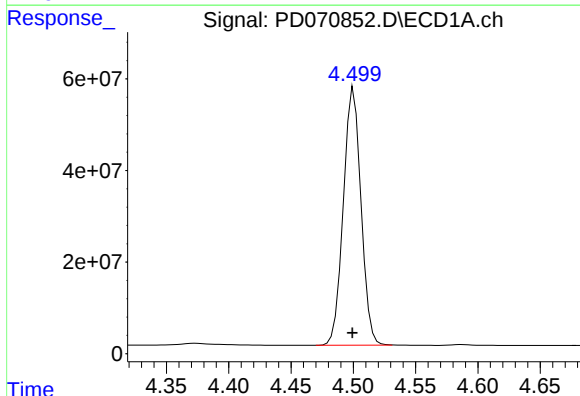


#4 Heptachlor

R.T.: 4.500 min
Delta R.T.: 0.001 min
Response: 557242034
Conc: 164.69 ng/ml

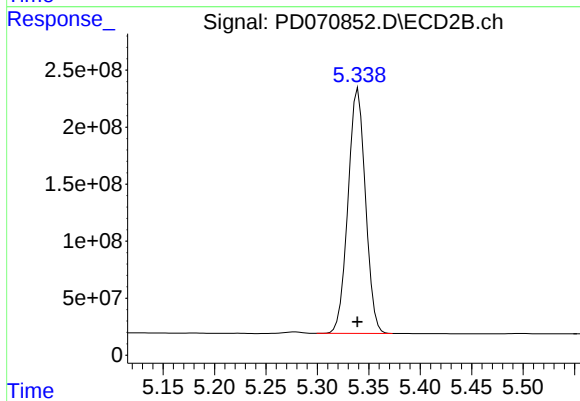

#4 Heptachlor


R.T.: 5.340 min
Delta R.T.: 0.000 min
Response: 2533904870
Conc: 125.10 ng/ml

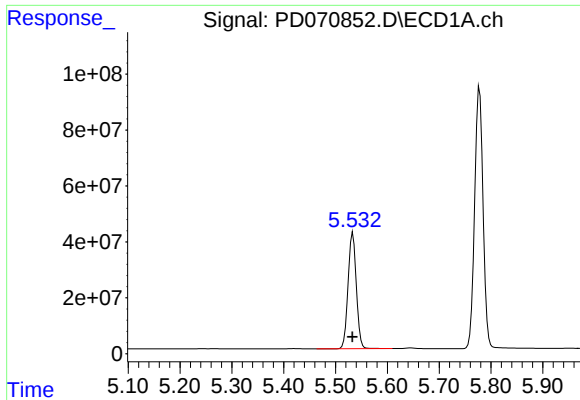

#9 Endosulfan I


R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 457977392
Conc: 157.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

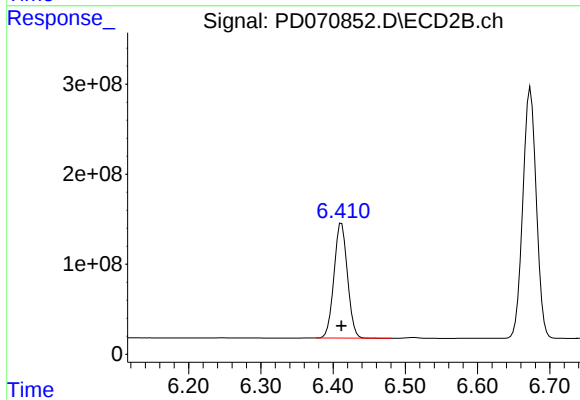


#9 Endosulfan I

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 1652401927
Conc: 123.77 ng/ml

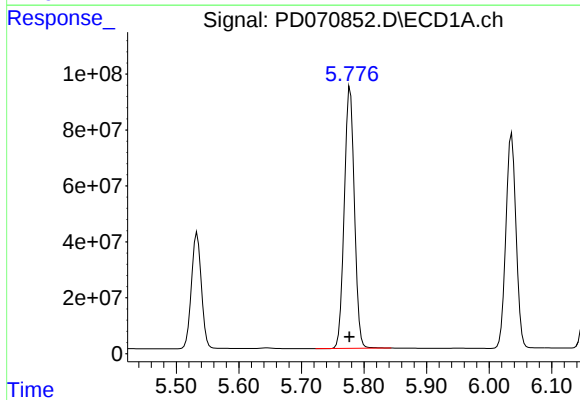


#13 Dieldrin

R.T.: 5.778 min
Delta R.T.: 0.001 min
Response: 1054151686
Conc: 319.13 ng/ml

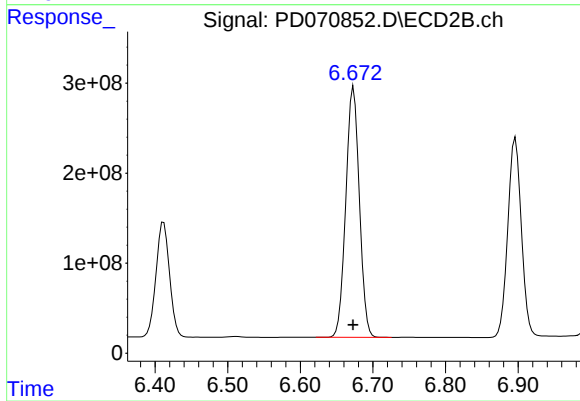

#13 Dieldrin


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 3614125155
Conc: 263.99 ng/ml

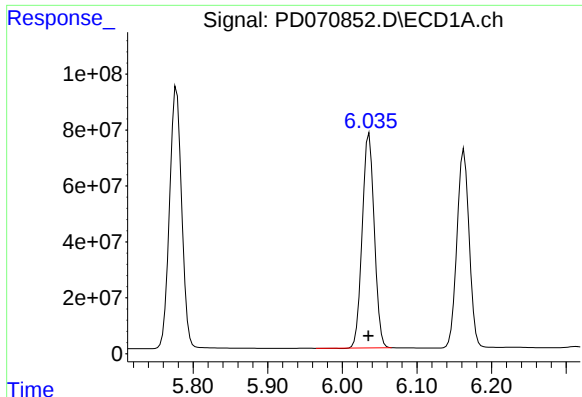

#14 Endrin


R.T.: 6.036 min
Delta R.T.: 0.001 min
Response: 861138396
Conc: 314.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

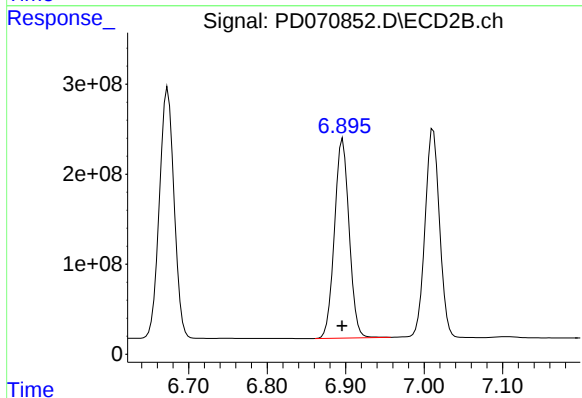


#14 Endrin

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 2873796454
Conc: 268.34 ng/ml

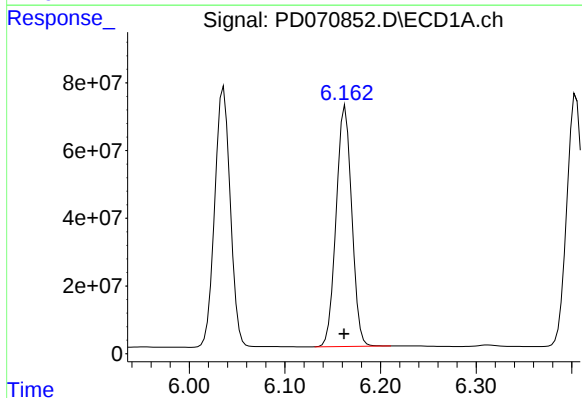


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.001 min
Response: 805293330
Conc: 318.82 ng/ml

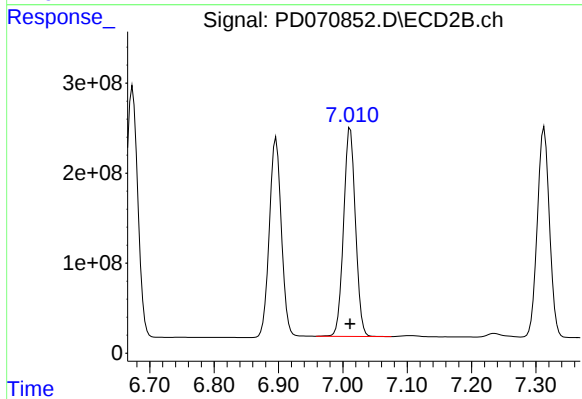

#16 4,4'-DDD


R.T.: 7.012 min
Delta R.T.: 0.000 min
Response: 2969489880
Conc: 268.96 ng/ml

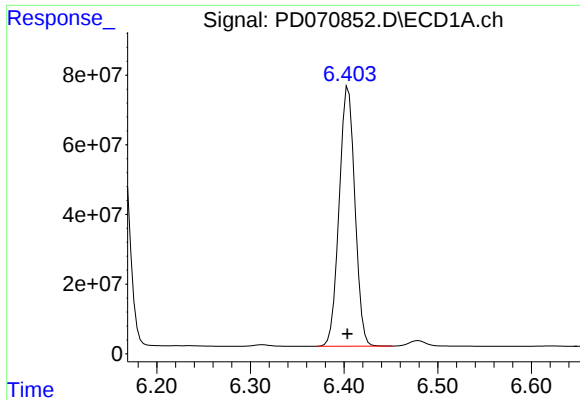

#17 4,4'-DDT


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 869764473
Conc: 329.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

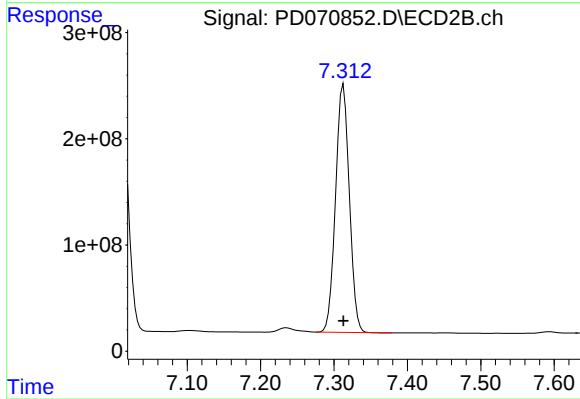


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: 0.000 min
Response: 3048289028
Conc: 272.08 ng/ml

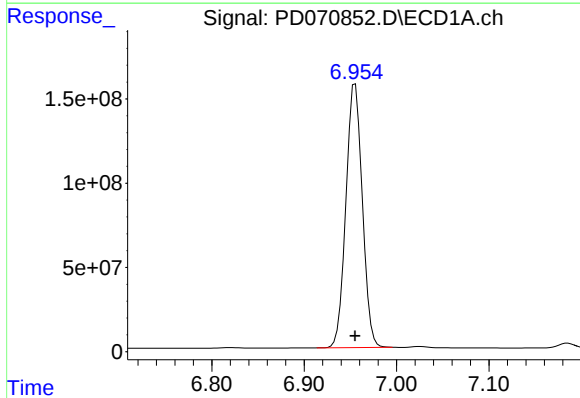


#20 Methoxychlor

R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 1934202095
Conc: 1407.18 ng/ml

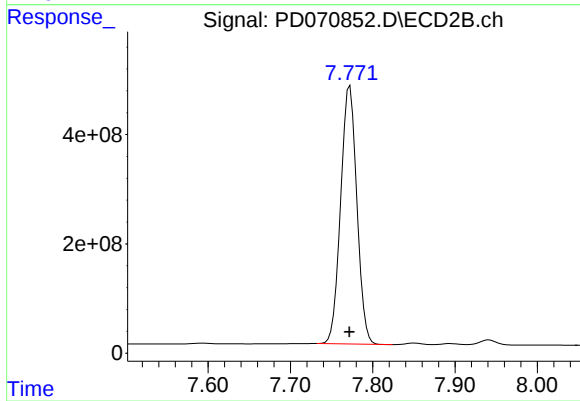

#20 Methoxychlor


R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 6463963138
Conc: 1233.82 ng/ml

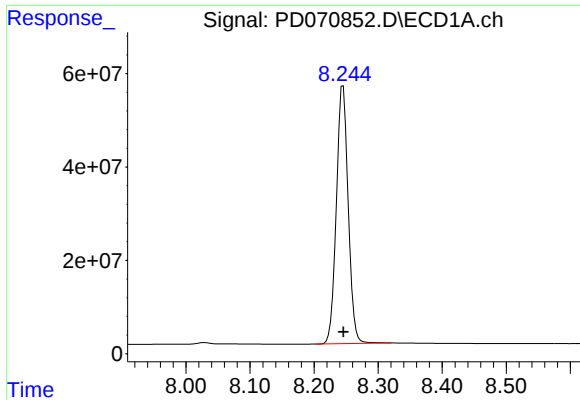

#27 Decachlorobiphenyl

R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 709722133
Conc: 295.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

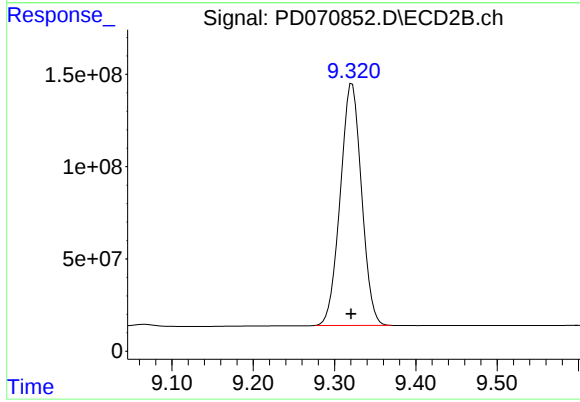

#27 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: 0.001 min
Response: 2379629338
Conc: 257.96 ng/ml