

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
 Data File : PD070834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 09:41
 Operator : AR\AJ
 Sample : RESC032
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC034

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 15:38:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 15:03:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.124	48991588	535.3E6	21.055	23.726
27)	SA Decachlor...	8.246	9.319	98666691	384.8E6	41.071	43.459
Target Compounds							
2)	A alpha-BHC	3.915	4.529	35565174	364.1E6	10.073	11.781
3)	MA gamma-BHC...	4.199	4.822	34260261	304.3E6	10.139	11.948
4)	MA Heptachlor	4.500	5.338	34153975	235.3E6	10.024	11.928
5)	MB Aldrin	4.748	5.651	38597221	212.9E6	10.965	12.592
6)	B beta-BHC	4.449	4.998	17328304	164.9E6	11.668	13.673
7)	B delta-BHC	4.654	5.223	36364325	275.6E6	10.759	12.561
8)	B Heptachlo...	5.194	6.046	35167559	175.9E6	10.983	12.359
9)	A Endosulfan I	5.534	6.411	29082892	141.1E6	10.042	11.144
10)	B trans-Chl...	5.420	6.283	35999783	172.9E6	10.862	12.070
11)	B cis-Chlor...	5.480	6.356	34951541	163.6E6	10.821	11.794
12)	B 4,4'-DDE	5.646	6.511	65968315	312.5E6	21.231	23.755
13)	MA Dieldrin	5.778	6.673	64030450	292.0E6	19.648	22.119
14)	MA Endrin	6.036	6.895	53903561	223.3E6	20.058	21.905
15)	B Endosulfa...	6.310	7.109	57246656	260.3E6	21.670	23.873
16)	A 4,4'-DDD	6.163	7.010	49475089	244.6E6	19.858	22.546
17)	MA 4,4'-DDT	6.405	7.312	50557349	236.9E6	19.210	21.742
18)	B Endrin al...	6.480	7.235	50252723	220.7E6	22.411	23.859
19)	B Endosulfa...	6.693	7.460	57546043	253.0E6	21.710	23.519
20)	A Methoxychlor	6.956	7.771	137.6E6	555.7E6	103.786	111.115
21)	B Endrin ke...	7.187	7.941	66276829	282.5E6	22.493	24.156

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 09:41
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 15:38:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 15:03:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

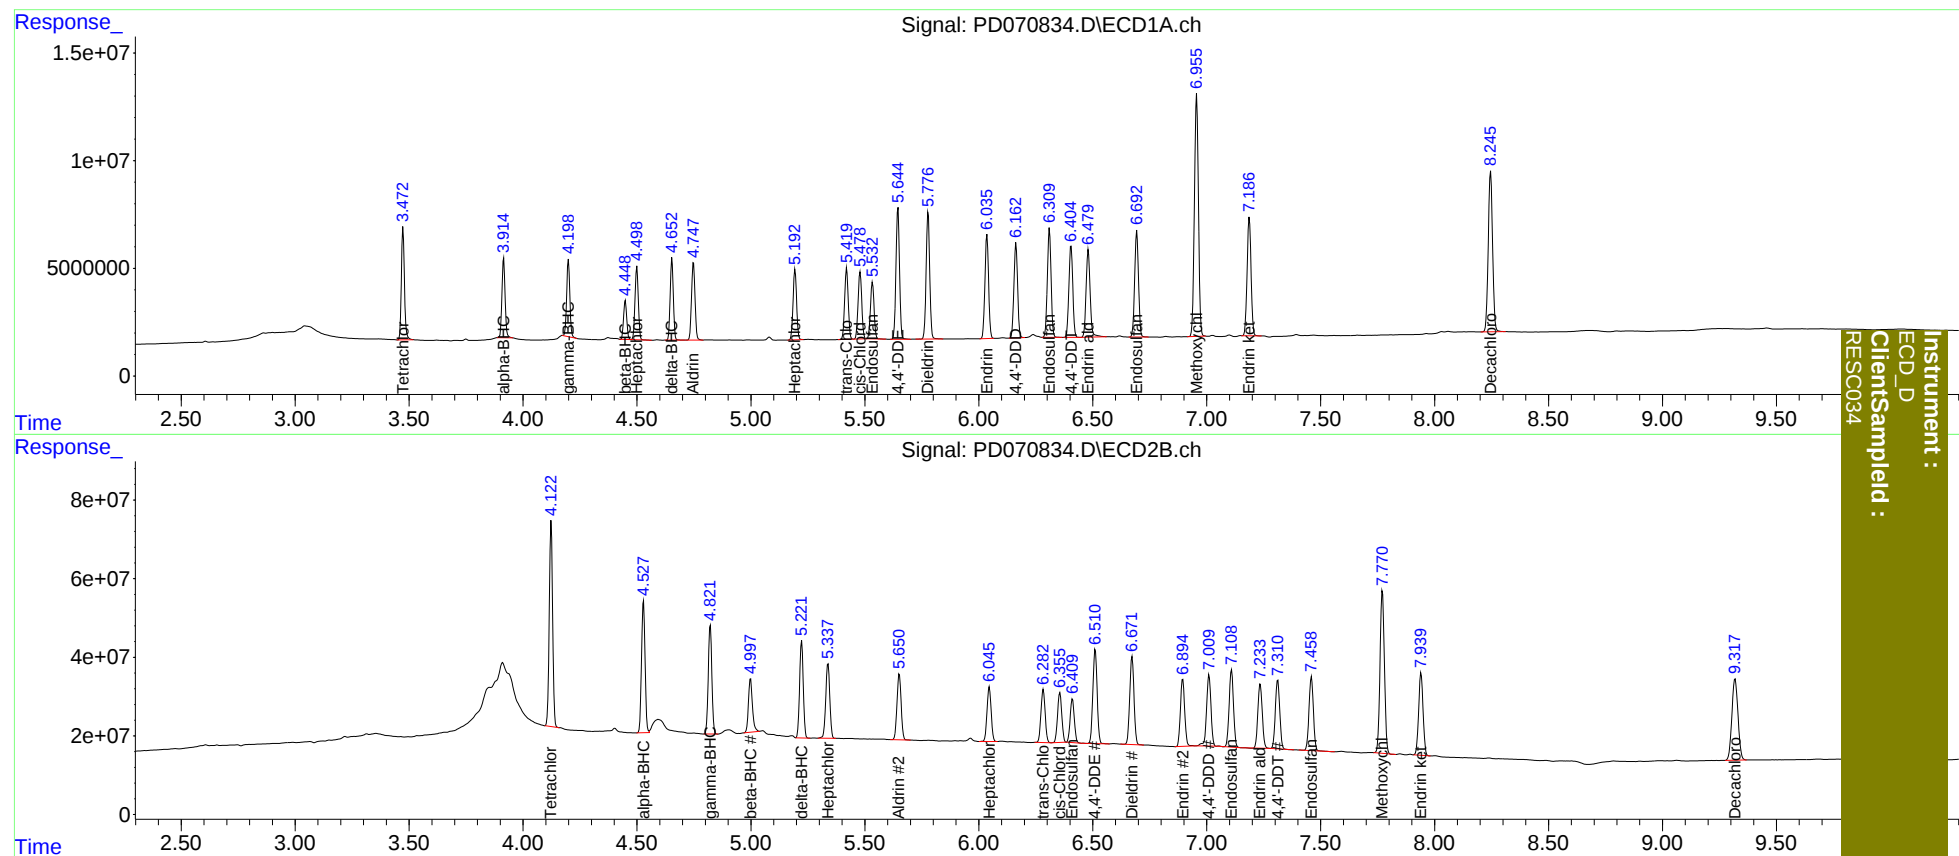

Instrument :
ECD_D
ClientSampled :
RESC034

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071322\
Data File : PD070834.D
Acq On : 13 Jul 2022 09:41
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC034

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Title : GC Extractables
Last Update : Wed Jul 13 15:03:36 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
3.474	3.915	100.00%
3.915	4.199	100.00%
4.199	4.449	100.00%
4.449	4.500	100.00%
4.500	4.654	100.00%
4.654	4.748	100.00%
4.748	5.194	100.00%
5.194	5.420	100.00%
5.420	5.480	100.00%
5.480	5.534	100.00%
5.534	5.646	100.00%
5.646	5.778	100.00%
5.778	6.036	100.00%
6.036	6.163	100.00%
6.163	6.310	100.00%
6.310	6.405	100.00%
6.405	6.480	100.00%
6.480	6.693	100.00%
6.693	6.956	100.00%
6.956	7.187	100.00%
7.187	8.246	100.00%

Signal #2

4.124	4.529	100.00%
4.529	4.822	100.00%
4.822	4.998	100.00%
4.998	5.223	100.00%
5.223	5.338	100.00%
5.338	5.651	100.00%
5.651	6.046	100.00%
6.046	6.283	100.00%
6.283	6.356	100.00%
6.356	6.411	100.00%
6.411	6.511	100.00%
6.511	6.673	100.00%
6.673	6.895	100.00%
6.895	7.010	100.00%
7.010	7.109	100.00%
7.109	7.235	100.00%
7.235	7.312	100.00%
7.312	7.460	100.00%
7.460	7.771	100.00%
7.771	7.941	100.00%
7.941	9.319	100.00%