

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071421\
 Data File : PD064250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 08:30
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 05:37:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
8) B	Heptachlo...	5.951	5.169f	1182526	472397	0.776	<MDL #
10) B	trans-Chl...	0.000	5.486f	0	1661552	N.D.	0.179
11) B	cis-Chlor...	0.000	5.486	0	1661552	N.D.	0.184
14) MA	Endrin	0.000	6.066	0	2963694	N.D.	0.407
15) B	Endosulfa...	0.000	6.300	0	1033008	N.D.	0.159
16) A	4,4'-DDD	6.889f	6.116f	2245169	182512	1.972	<MDL #
18) B	Endrin al...	7.091f	0.000	2320469	0	2.254	N.D. #
19) B	Endosulfa...	0.000	6.760f	0	1053413	N.D.	0.171
26)	Toxaphene-5	0.000	7.114	0	488583	N.D.	3.926


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071421\
Data File : PD064250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 08:30
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 05:37:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

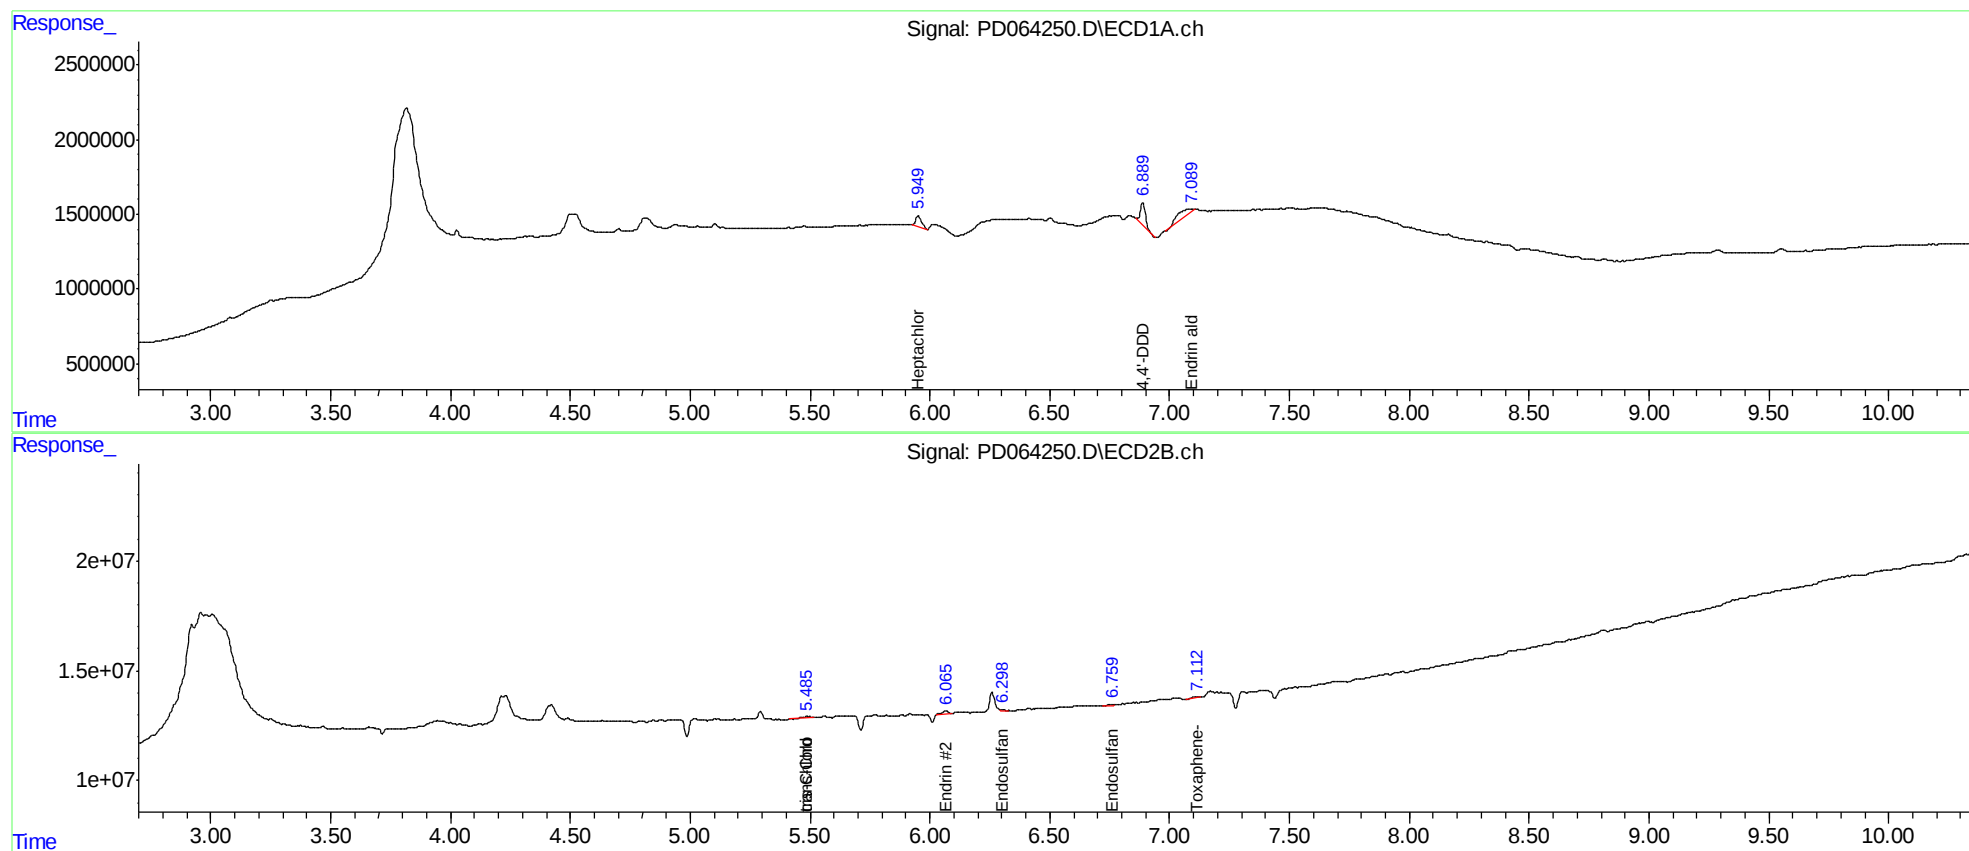


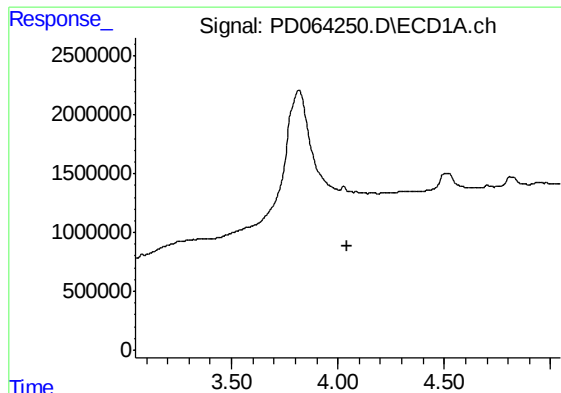

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

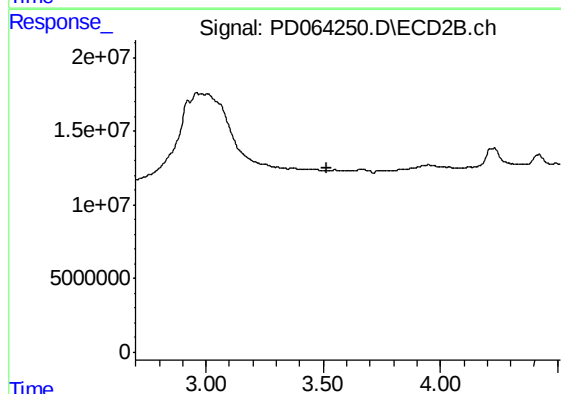


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.513 min
Response: 0
Conc: N.D.

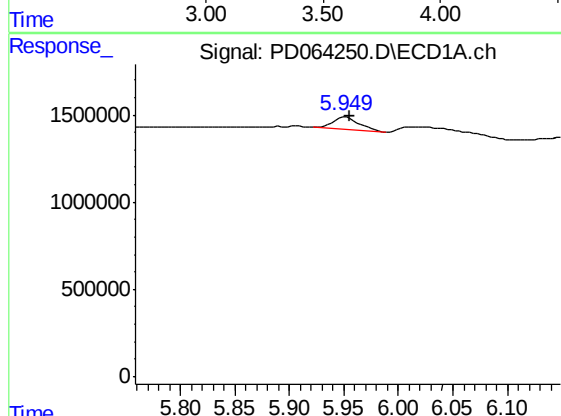


#8 Heptachlor epoxide

R.T.: 5.951 min
Delta R.T.: -0.005 min
Response: 1182526
Conc: 0.78 ng/ml

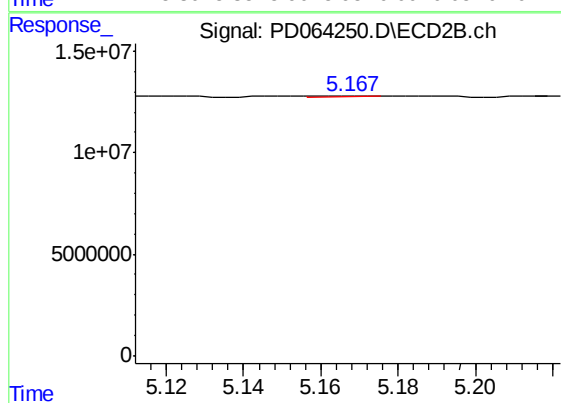

#8 Heptachlor epoxide


R.T.: 5.169 min
Delta R.T.: -0.055 min
Response: 472397
Conc: N.D.

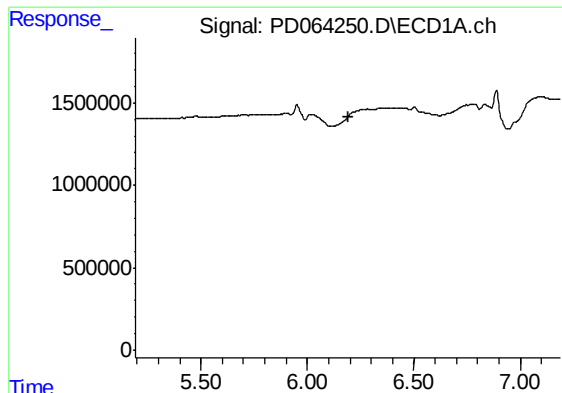

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

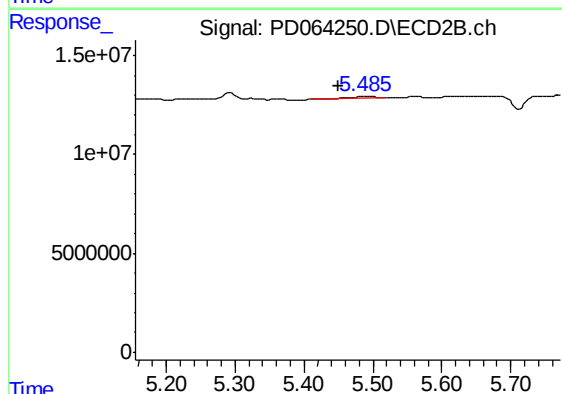


#10 trans-Chlordane

R.T.: 5.486 min
Delta R.T.: 0.037 min
Response: 1661552
Conc: 0.18 ng/ml

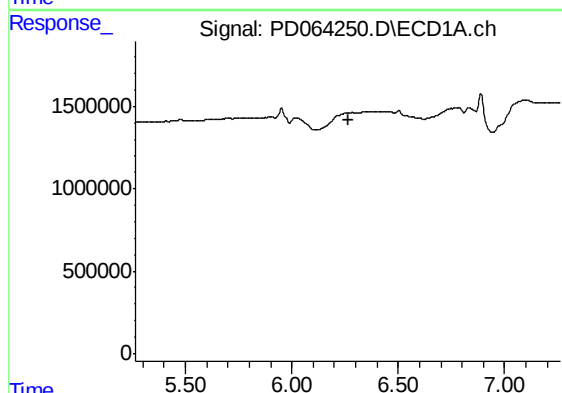


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.265 min
Response: 0
Conc: N.D.

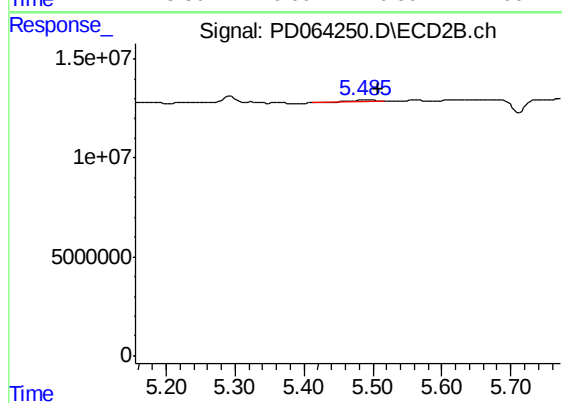

#11 cis-Chlordane


R.T.: 5.486 min
Delta R.T.: -0.022 min
Response: 1661552
Conc: 0.18 ng/ml

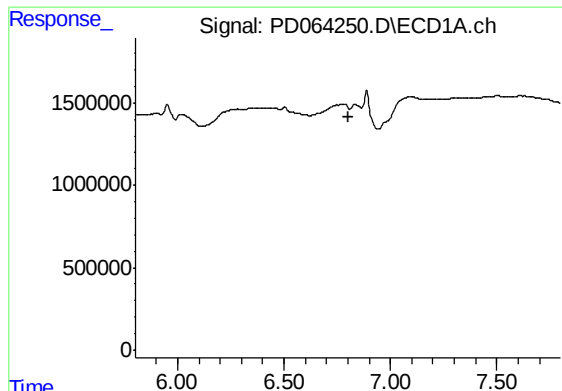

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

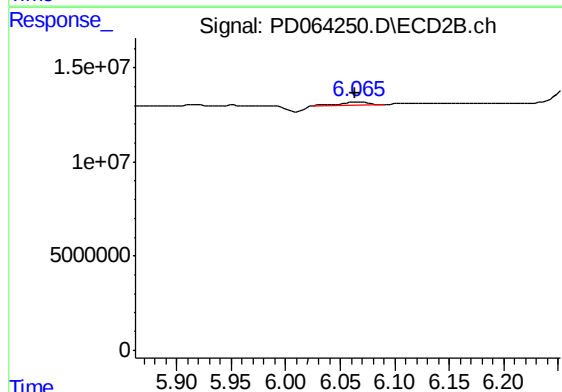


#14 Endrin

R.T.: 6.066 min
Delta R.T.: 0.003 min
Response: 2963694
Conc: 0.41 ng/ml

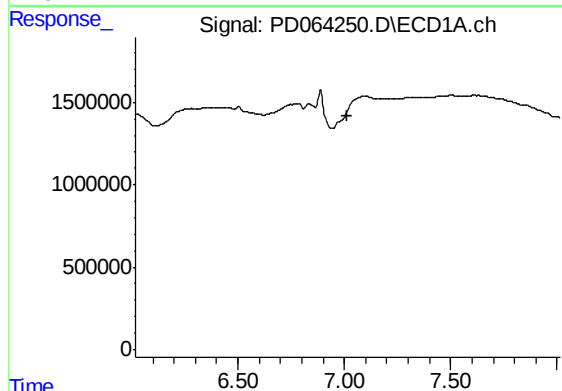


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 7.016 min
Response: 0
Conc: N.D.

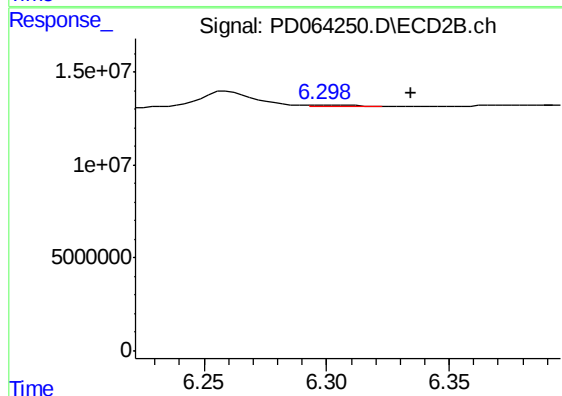

#15 Endosulfan II


R.T.: 6.300 min
Delta R.T.: -0.035 min
Response: 1033008
Conc: 0.16 ng/ml

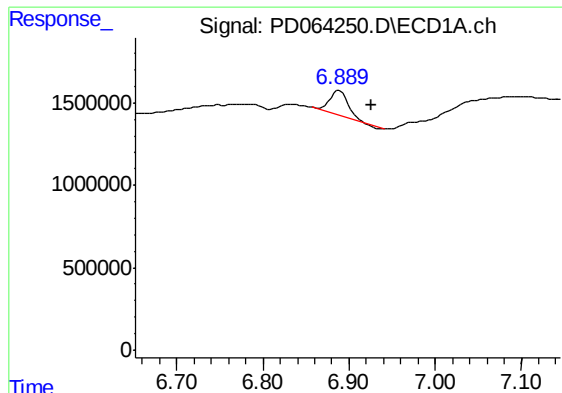

#16 4,4'-DDD


R.T.: 6.889 min
Delta R.T.: -0.037 min
Response: 2245169
Conc: 1.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

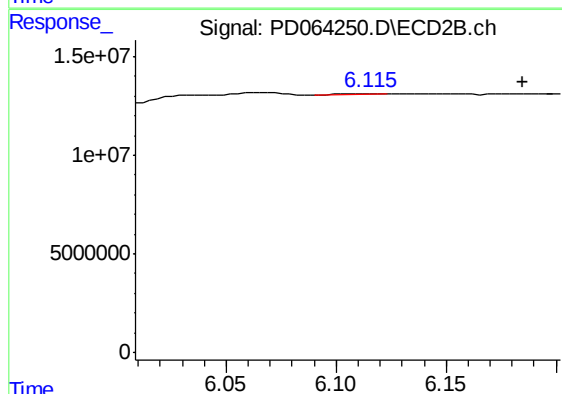


#16 4,4'-DDD

R.T.: 6.116 min
Delta R.T.: -0.069 min
Response: 182512
Conc: N.D.

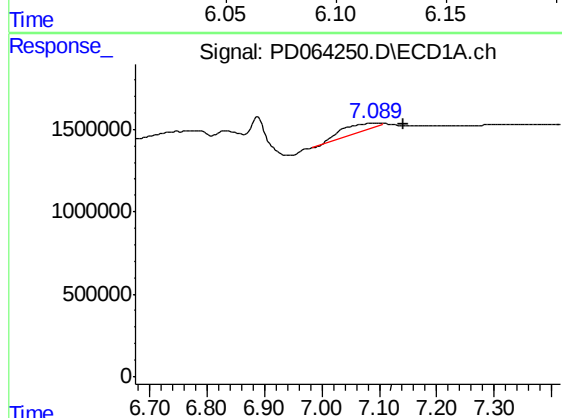


#18 Endrin aldehyde

R.T.: 7.091 min
Delta R.T.: -0.051 min
Response: 2320469
Conc: 2.25 ng/ml

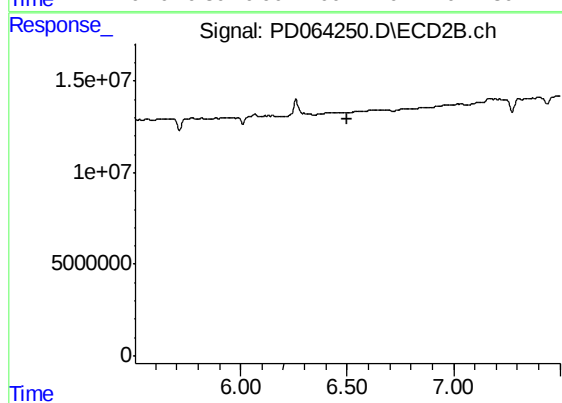

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.503 min
Response: 0
Conc: N.D.

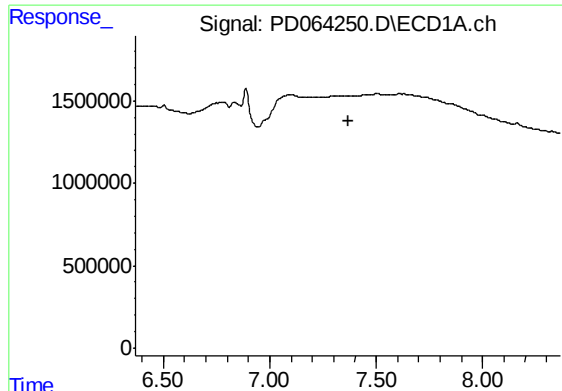

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

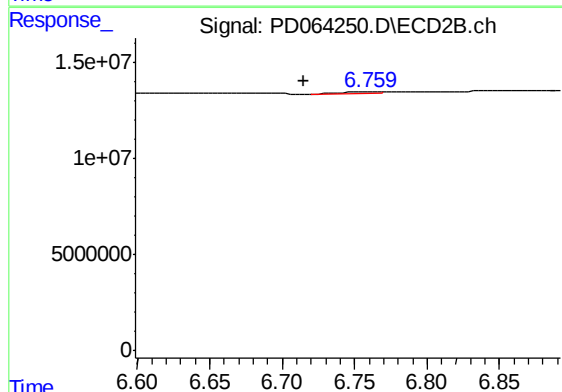


#19 Endosulfan Sulfate

R.T.: 6.760 min
Delta R.T.: 0.045 min
Response: 1053413
Conc: 0.17 ng/ml

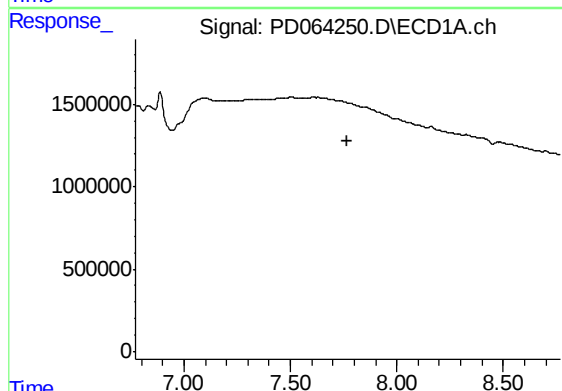


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.769 min
Response: 0
Conc: N.D.

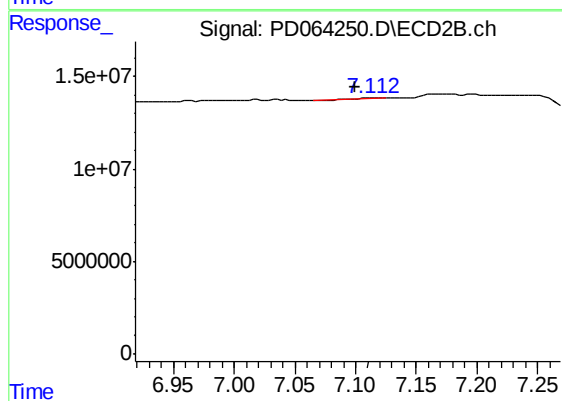

#26 Toxaphene-5


R.T.: 7.114 min
Delta R.T.: 0.014 min
Response: 488583
Conc: 3.93 ng/ml

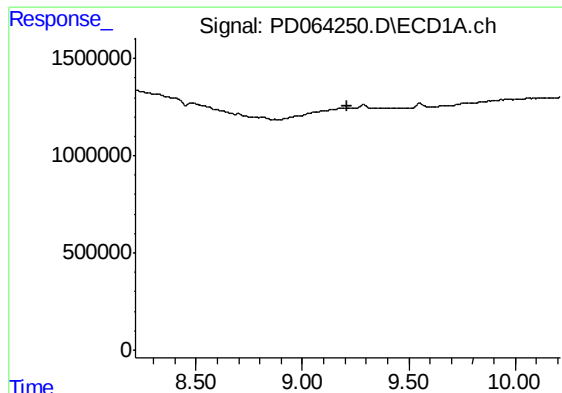

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

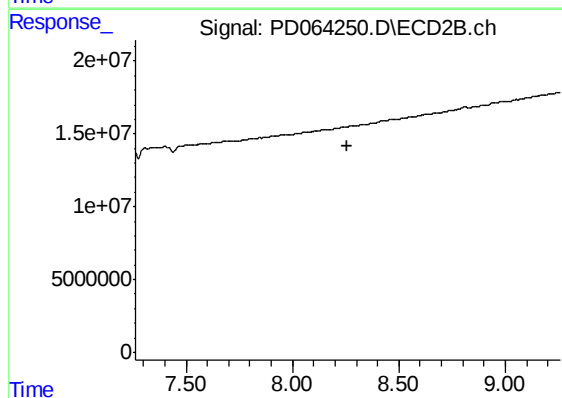

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.259 min
Response: 0
Conc: N.D.